

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL021523\
 Data File : PL080939.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Feb 2023 15:03
 Operator : AR\AJ
 Sample : 01552-12 10X
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 SB-06-4.0-6.0

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 02/16/2023
 Supervised By : Ankita Jodhani 02/16/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 15 20:36:44 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012023.M
 Quant Title : GC Extractables
 QLast Update : Sun Jan 22 23:56:48 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.351	2.688	3983112	3972042	1.857m	1.808
28) SA Decachlor...	8.791	7.834	5417704	5458374	3.094	2.291 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL021523\
Data File : PL080939.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Feb 2023 15:03
Operator : AR\AJ
Sample : 01552-12 10X
Misc :
ALS Vial : 15 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
SB-06-4.0-6.0


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 02/16/2023
Supervised By : Ankita Jodhani 02/16/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 15 20:36:44 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012023.M
Quant Title : GC Extractables
QLast Update : Sun Jan 22 23:56:48 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

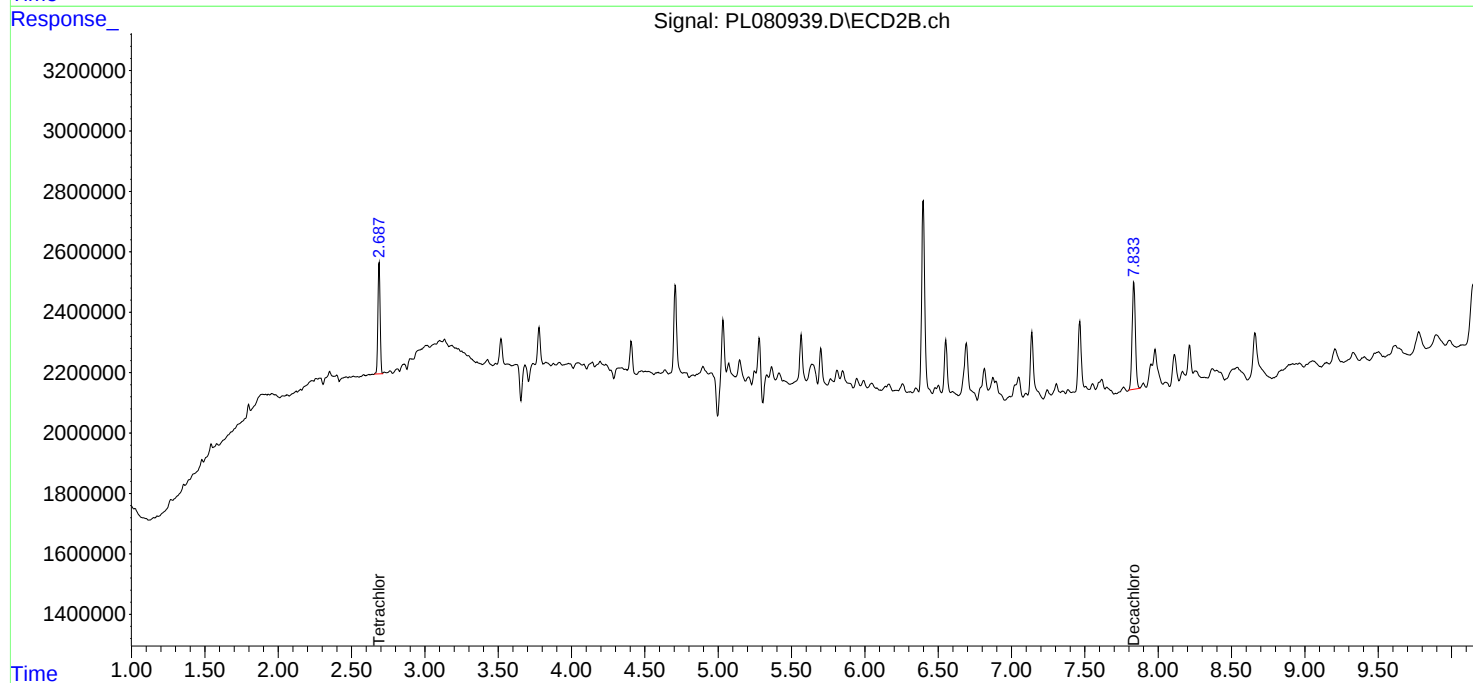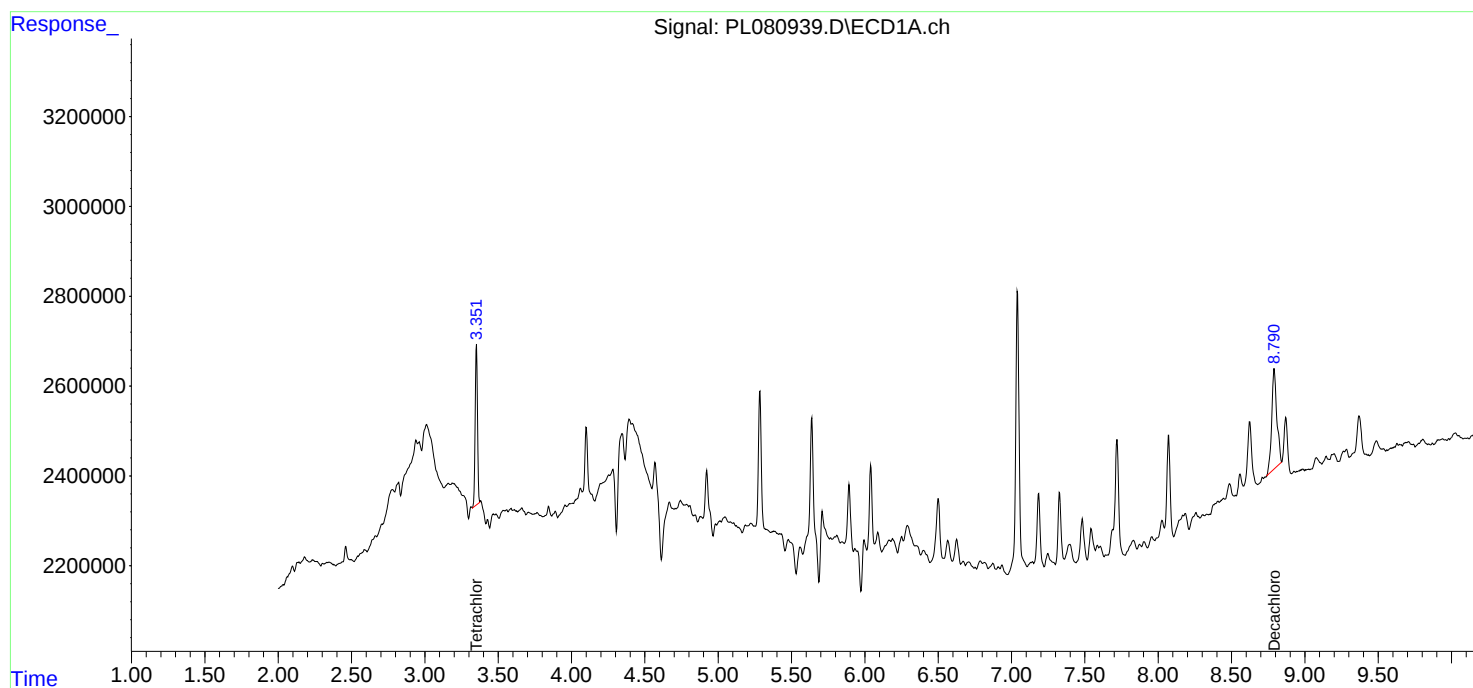

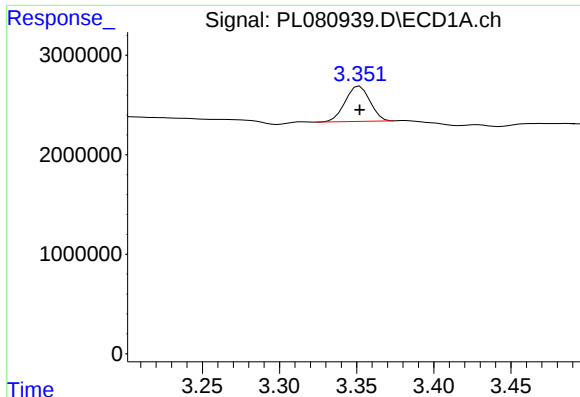


#1 Tetrachloro-m-xylene

R.T.: 3.351 min
Delta R.T.: -0.001 min
Response: 3983112
Conc: 1.86 ng/ml

Instrument :
ECD_L
ClientSampleId :
SB-06-4.0-6.0


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 02/16/2023
Supervised By :Ankita Jodhani 02/16/2023

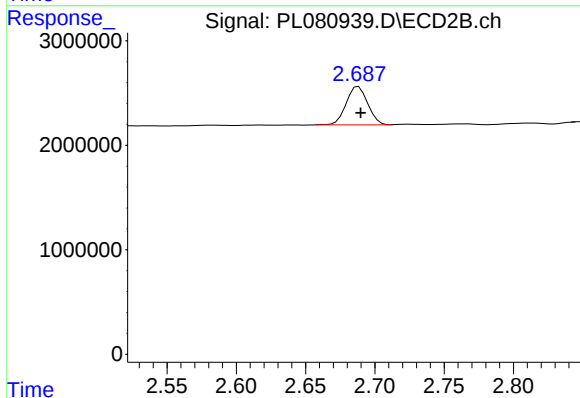


#1 Tetrachloro-m-xylene

R.T.: 2.688 min
Delta R.T.: -0.001 min
Response: 3972042
Conc: 1.81 ng/ml

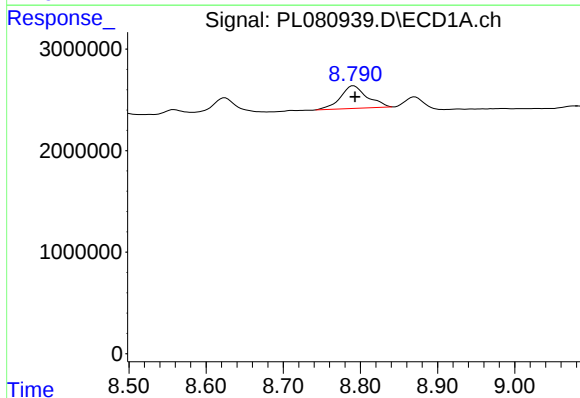

#28 Decachlorobiphenyl

R.T.: 8.791 min
Delta R.T.: -0.002 min
Response: 5417704
Conc: 3.09 ng/ml

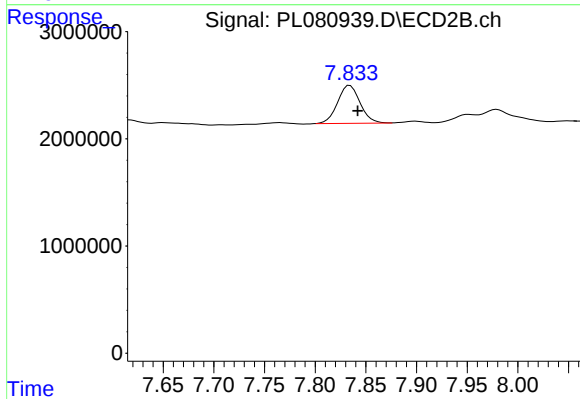

#28 Decachlorobiphenyl

R.T.: 7.834 min
Delta R.T.: -0.008 min
Response: 5458374
Conc: 2.29 ng/ml