

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL021524\
 Data File : PL088107.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Feb 2024 21:27
 Operator : AR\AJ
 Sample : PCHLORICC250
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 16 10:25:06 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL021524.M
 Quant Title : GC Extractables
 QLast Update : Fri Feb 16 10:23:37 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.635	2.853	70901681	42764955	24.503	24.271
28)	SA Decachlor...	9.303	8.086	54789584	35038124	24.959	25.249
Target Compounds							
23)	Chlordane-1	4.820	3.877	30807532	12514398	249.934	244.723
24)	Chlordane-2	5.357	4.464	33468488	16032167	254.619	256.814
25)	Chlordane-3	6.078	5.106	122.5E6	44582848	240.915	238.135
26)	Chlordane-4	6.161	5.170	149.0E6	41744976	243.952	242.149
27)	Chlordane-5	7.021	5.847	24758260	12960572	244.076	250.499



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL021524\
Data File : PL088107.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Feb 2024 21:27
Operator : AR\AJ
Sample : PCHLORICC250
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 16 10:25:06 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL021524.M
Quant Title : GC Extractables
QLast Update : Fri Feb 16 10:23:37 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

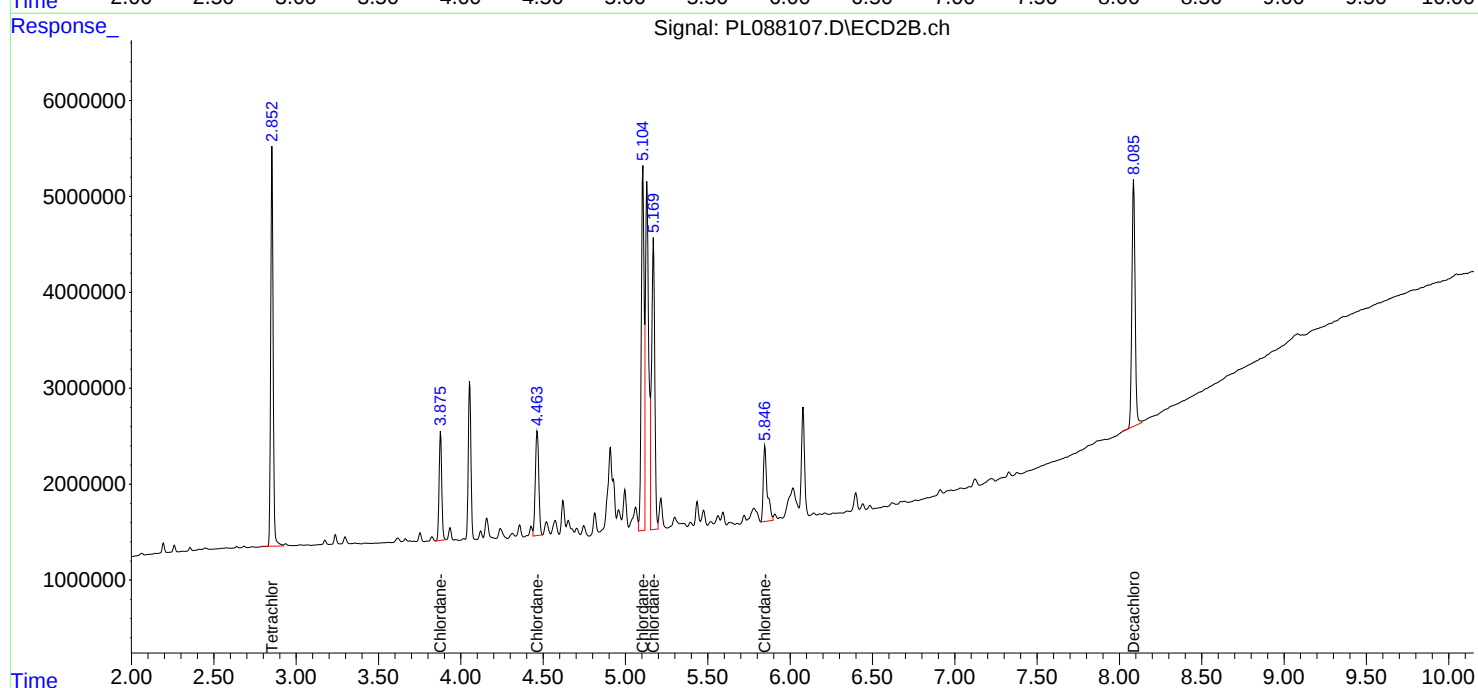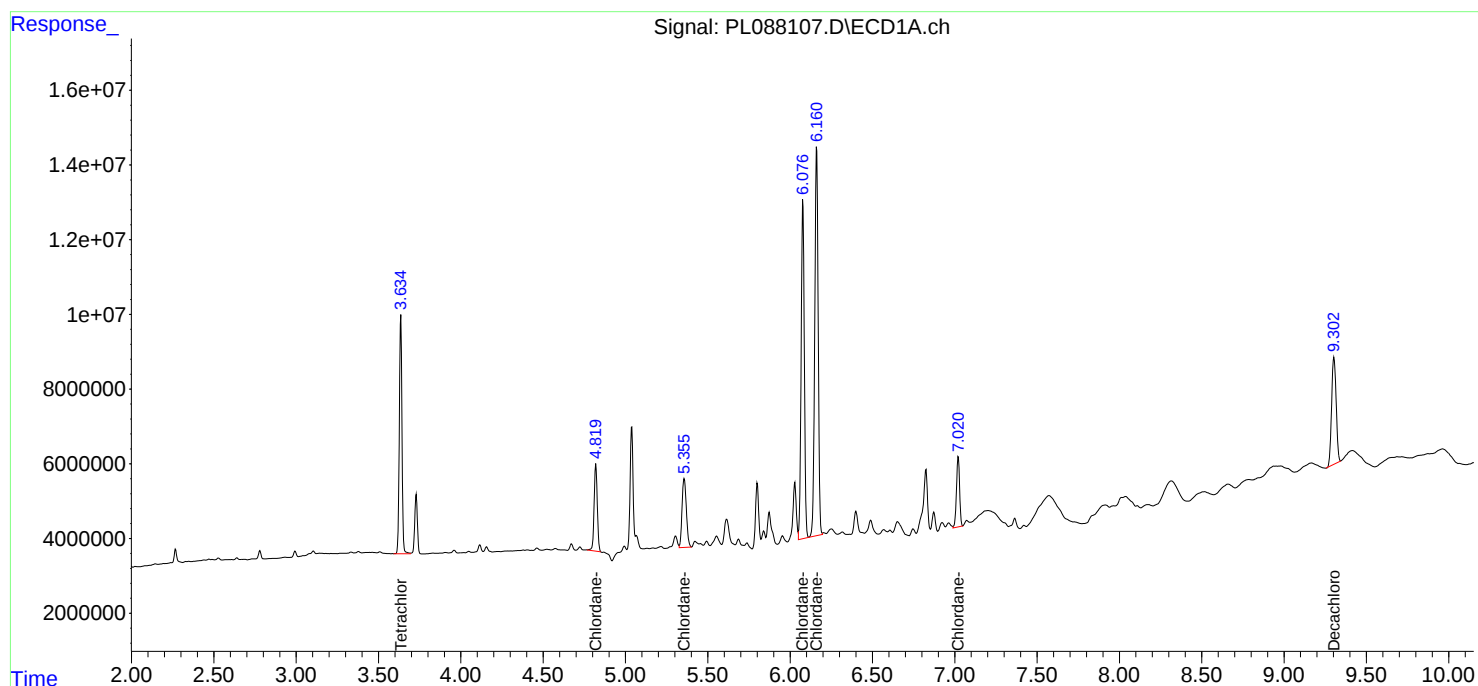


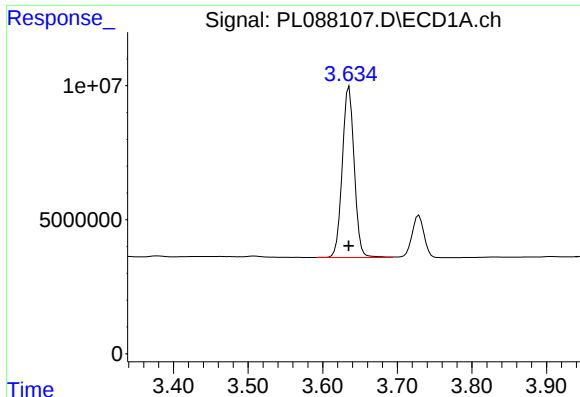

#1 Tetrachloro-m-xylene


R.T.: 3.635 min
Delta R.T.: 0.000 min
Response: 70901681
Conc: 24.50 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

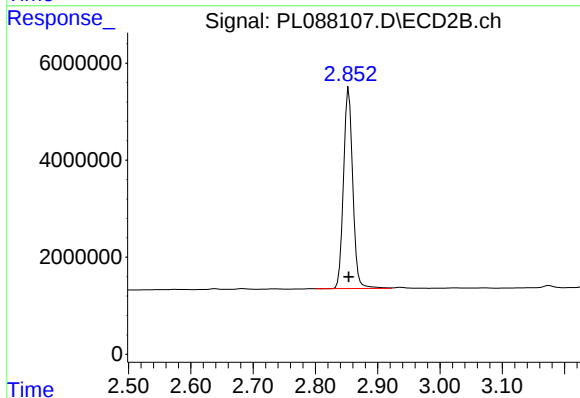


#1 Tetrachloro-m-xylene

R.T.: 2.853 min
Delta R.T.: 0.000 min
Response: 42764955
Conc: 24.27 ng/ml

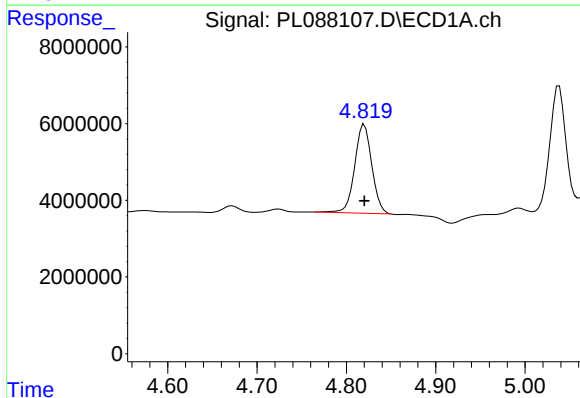


#23 Chlordane-1

R.T.: 4.820 min
Delta R.T.: 0.000 min
Response: 30807532
Conc: 249.93 ng/ml

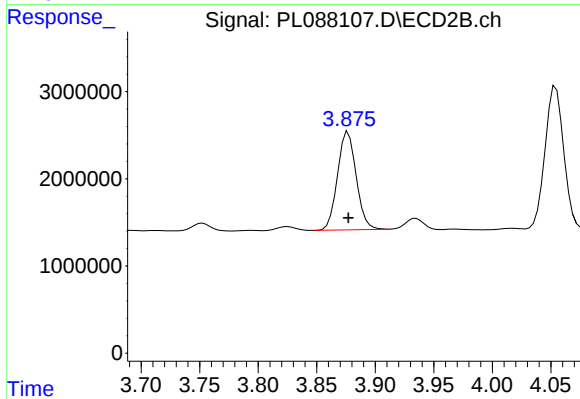

#23 Chlordane-1


R.T.: 3.877 min
Delta R.T.: 0.000 min
Response: 12514398
Conc: 244.72 ng/ml

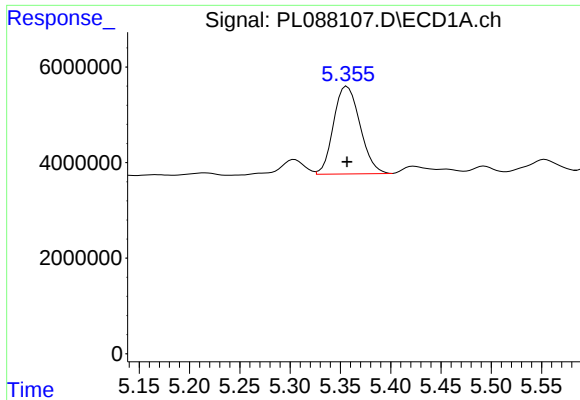

#24 Chlordane-2


R.T.: 5.357 min
Delta R.T.: 0.000 min
Response: 33468488
Conc: 254.62 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

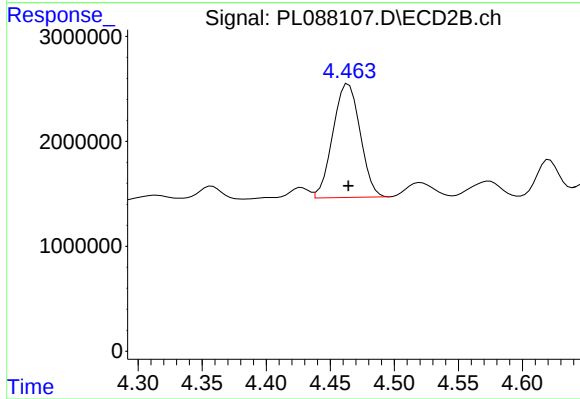


#24 Chlordane-2

R.T.: 4.464 min
Delta R.T.: 0.000 min
Response: 16032167
Conc: 256.81 ng/ml

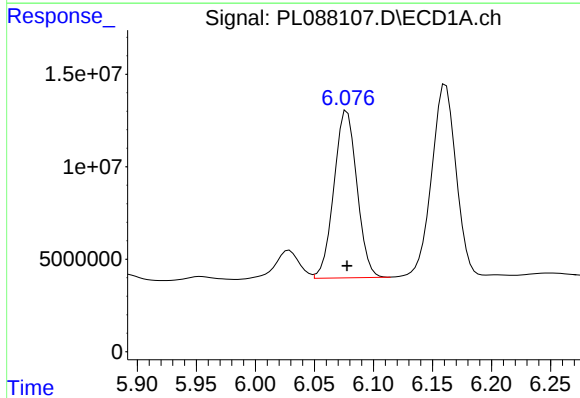


#25 Chlordane-3

R.T.: 6.078 min
Delta R.T.: 0.000 min
Response: 122484353
Conc: 240.91 ng/ml

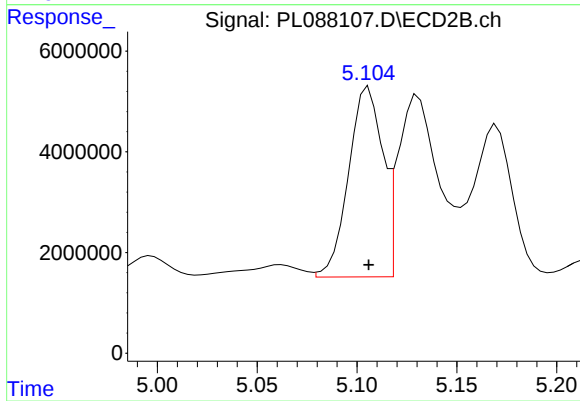

#25 Chlordane-3


R.T.: 5.106 min
Delta R.T.: 0.000 min
Response: 44582848
Conc: 238.13 ng/ml

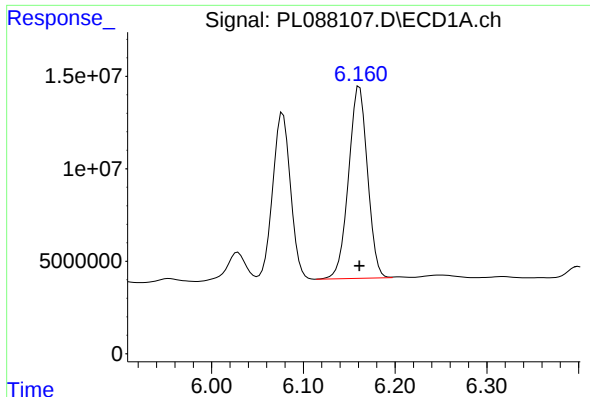

#26 Chlordane-4


R.T.: 6.161 min
Delta R.T.: 0.000 min
Response: 149013187
Conc: 243.95 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

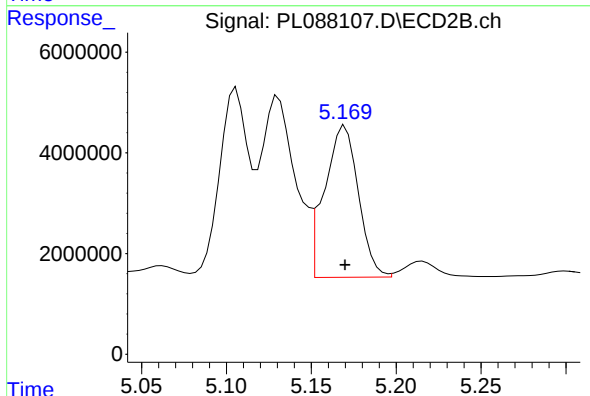


#26 Chlordane-4

R.T.: 5.170 min
Delta R.T.: 0.000 min
Response: 41744976
Conc: 242.15 ng/ml

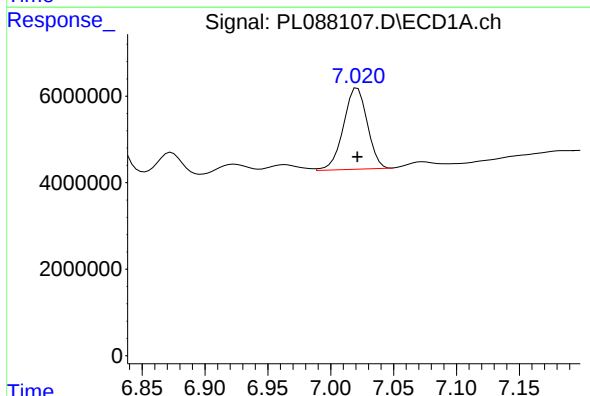


#27 Chlordane-5

R.T.: 7.021 min
Delta R.T.: 0.000 min
Response: 24758260
Conc: 244.08 ng/ml

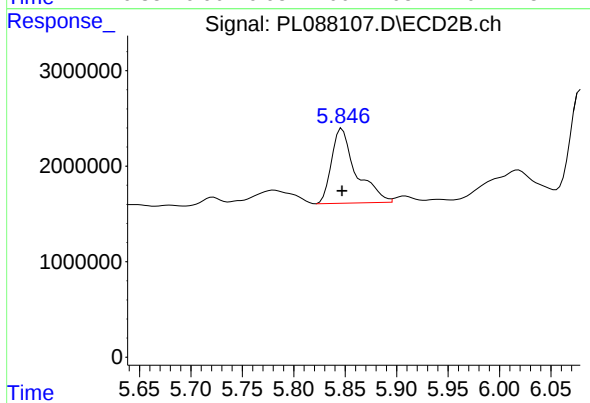

#27 Chlordane-5


R.T.: 5.847 min
Delta R.T.: 0.000 min
Response: 12960572
Conc: 250.50 ng/ml

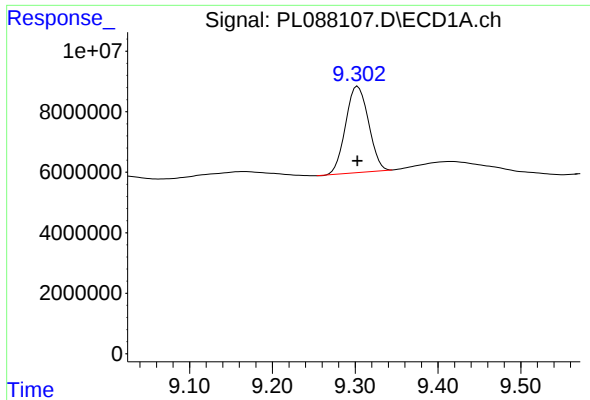

#28 Decachlorobiphenyl

R.T.: 9.303 min
Delta R.T.: 0.000 min
Response: 54789584
Conc: 24.96 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

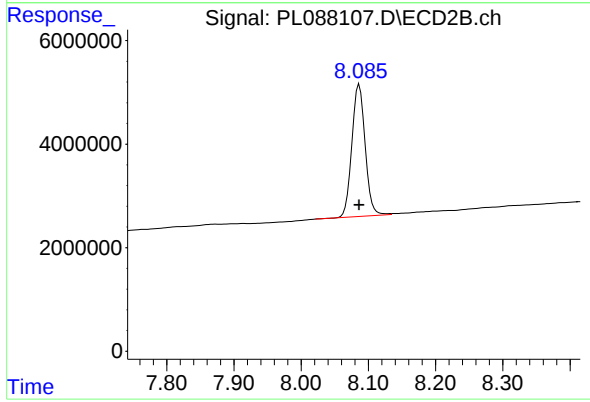

#28 Decachlorobiphenyl

R.T.: 8.086 min
Delta R.T.: 0.000 min
Response: 35038124
Conc: 25.25 ng/ml