

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL021524\
 Data File : PL088098.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Feb 2024 19:23
 Operator : AR\AJ
 Sample : RESCHK
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 RESCHK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 16 11:41:39 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL021524.M
 Quant Title : GC Extractables
 QLast Update : Fri Feb 16 11:40:19 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.636	2.853	52926508	26133312	19.269	18.633
28)	SA Decachlor...	9.304	8.084	43169817	24441952	22.415	19.196
Target Compounds							
9)	A Endosulfan I	6.208	5.226	26959434	13328304	8.614	8.283
10)	B gamma-Chl...	6.077	5.105	30799443	16028963	9.063	8.986
12)	B 4,4'-DDE	6.332	5.363	55865994	28363414	18.420	17.845
13)	MA Dieldrin	6.487	5.496	59050675	30282231	17.959	17.551
19)	B Endosulfa...	7.308	6.480	49915192	25918245	19.160	18.455
20)	A Methoxychlor	7.654	6.764	133.8E6	71286292	101.050	90.955
21)	B Endrin ke...	7.800	6.993	54720338	29644100	19.535	17.706



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL021524\
Data File : PL088098.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Feb 2024 19:23
Operator : AR\AJ
Sample : RESCHK
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
RESCHK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 16 11:41:39 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL021524.M
Quant Title : GC Extractables
QLast Update : Fri Feb 16 11:40:19 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

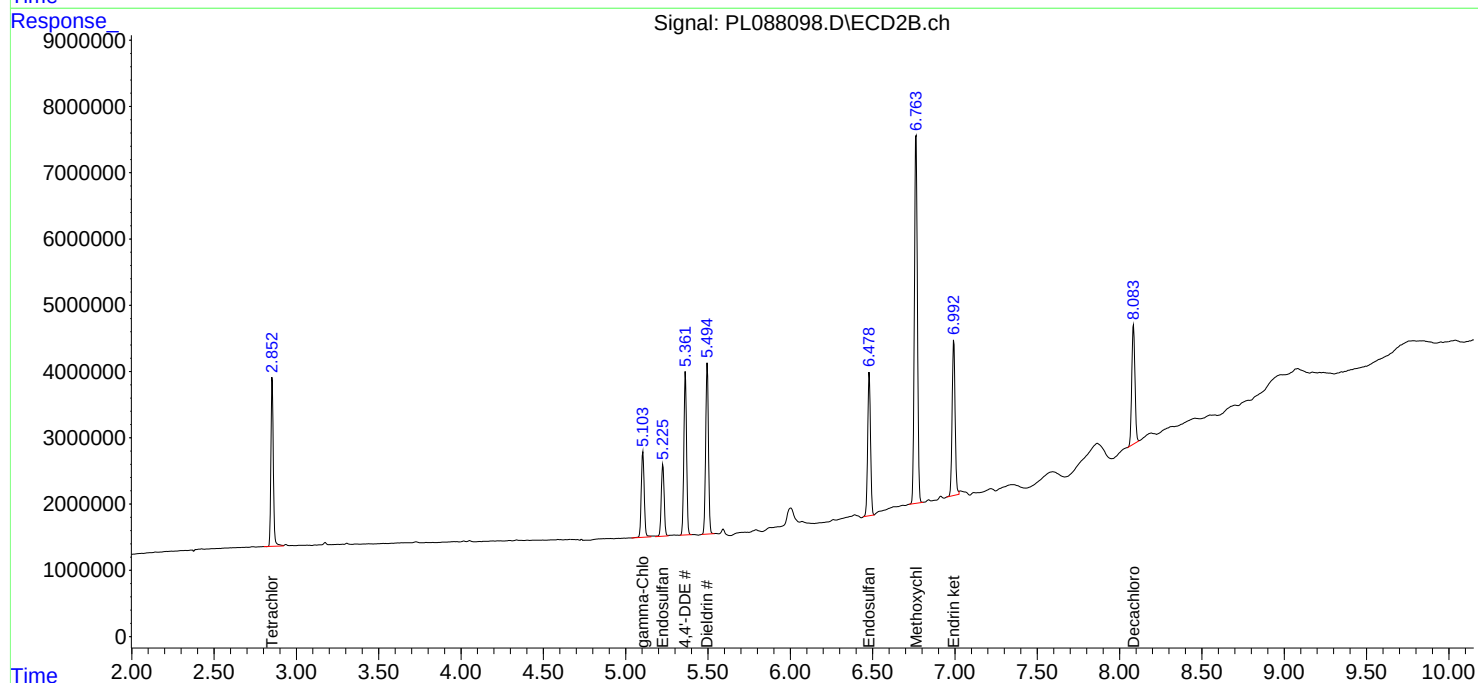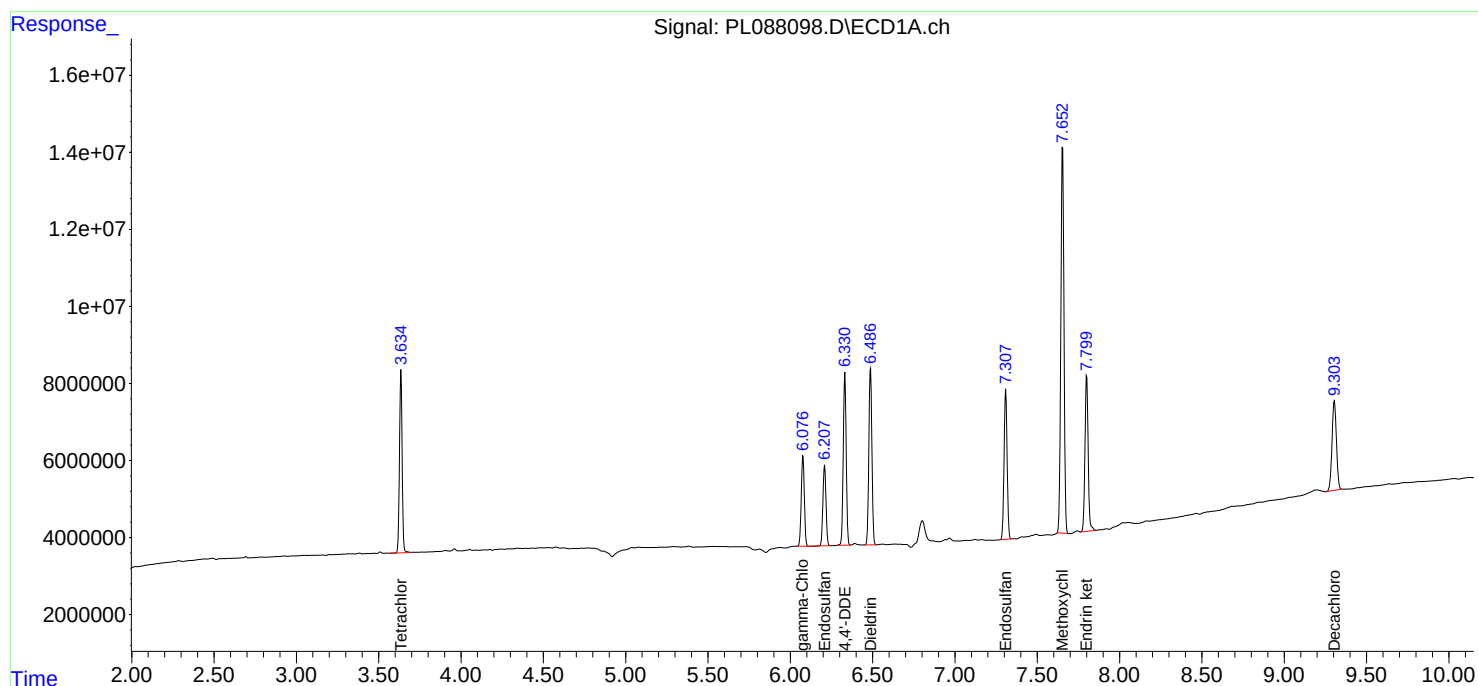


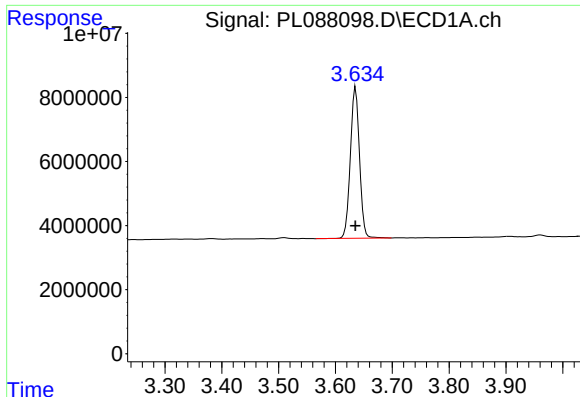

#1 Tetrachloro-m-xylene


R.T.: 3.636 min
Delta R.T.: 0.000 min
Response: 52926508
Conc: 19.27 ng/ml

Instrument :
ECD_L
ClientSampleId :
RESCHK

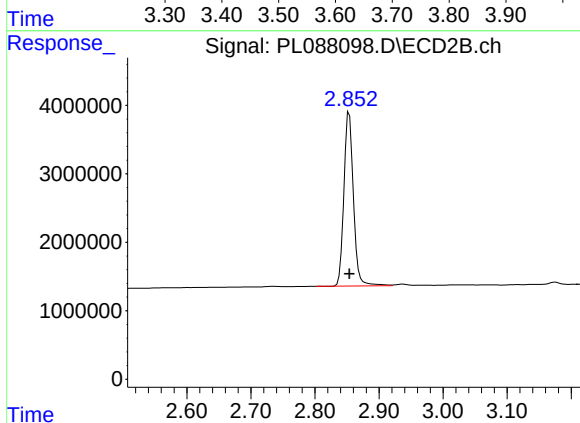


#1 Tetrachloro-m-xylene

R.T.: 2.853 min
Delta R.T.: 0.000 min
Response: 26133312
Conc: 18.63 ng/ml

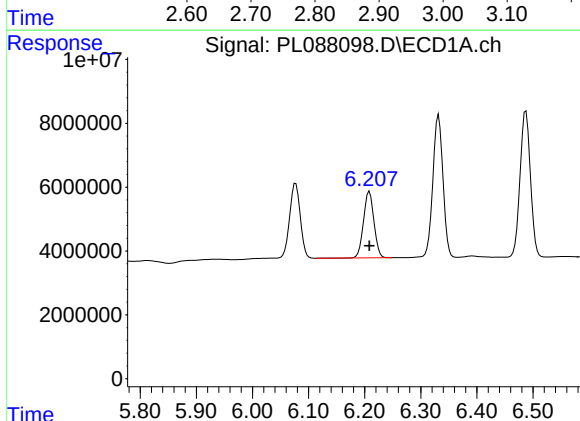


#9 Endosulfan I

R.T.: 6.208 min
Delta R.T.: 0.000 min
Response: 26959434
Conc: 8.61 ng/ml

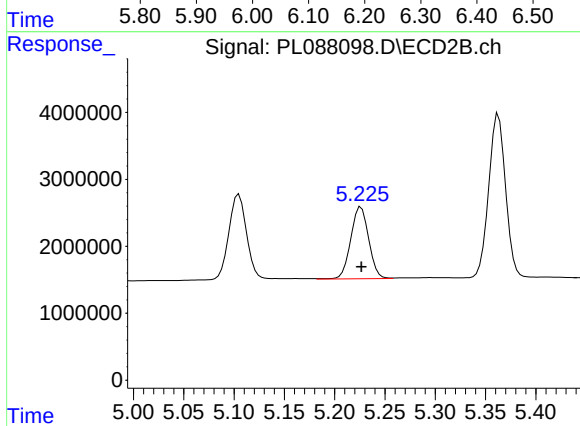

#9 Endosulfan I


R.T.: 5.226 min
Delta R.T.: 0.000 min
Response: 13328304
Conc: 8.28 ng/ml

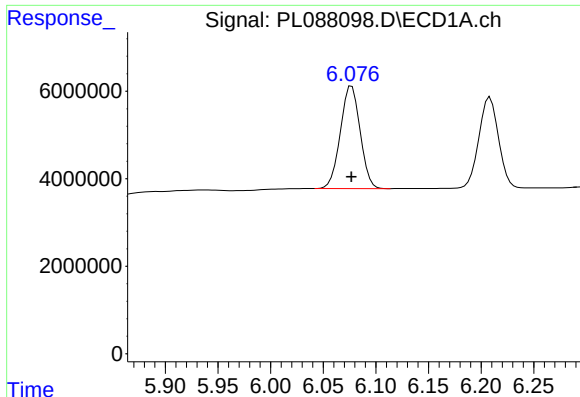

#10 gamma-Chlordane


R.T.: 6.077 min
Delta R.T.: 0.000 min
Response: 30799443
Conc: 9.06 ng/ml

Instrument :
ECD_L
ClientSampleId :
RESCHK

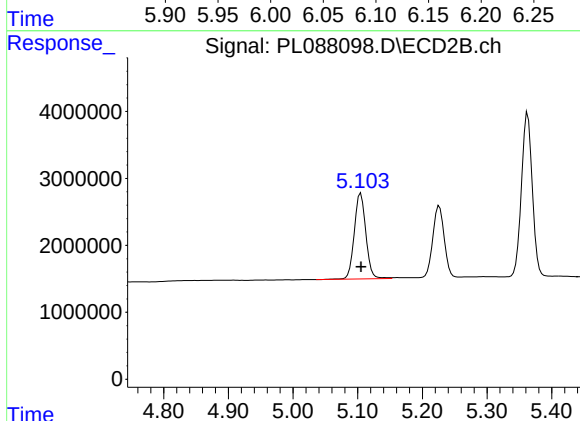


#10 gamma-Chlordane

R.T.: 5.105 min
Delta R.T.: 0.000 min
Response: 16028963
Conc: 8.99 ng/ml

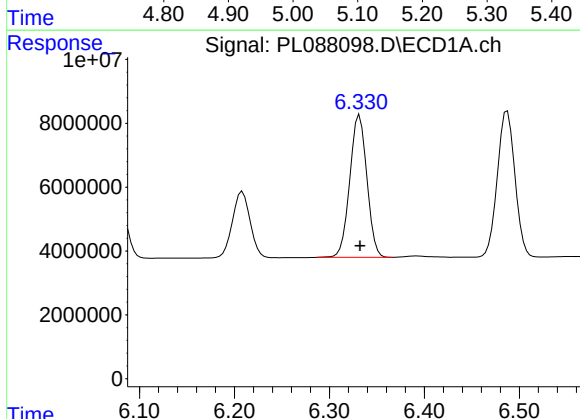


#12 4,4'-DDE

R.T.: 6.332 min
Delta R.T.: 0.000 min
Response: 55865994
Conc: 18.42 ng/ml

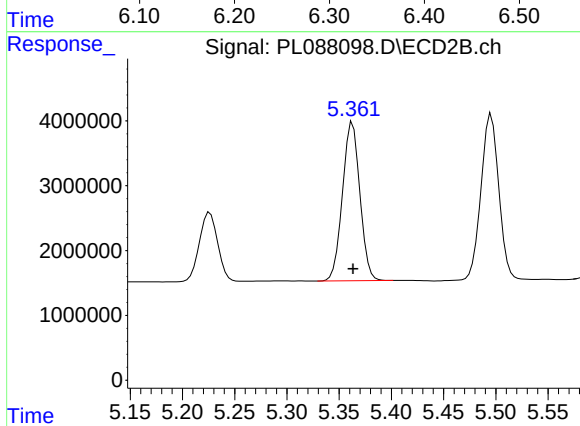

#12 4,4'-DDE


R.T.: 5.363 min
Delta R.T.: 0.000 min
Response: 28363414
Conc: 17.85 ng/ml

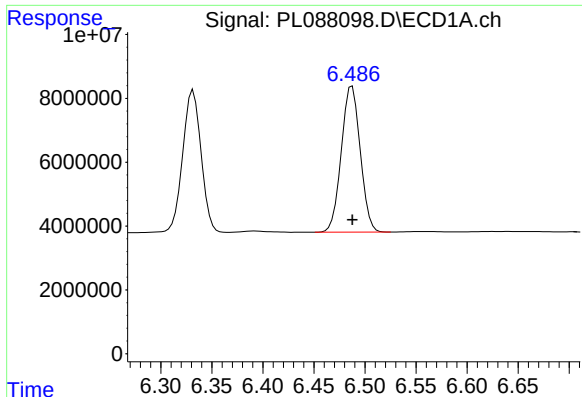

#13 Dieldrin


R.T.: 6.487 min
Delta R.T.: 0.000 min
Response: 59050675
Conc: 17.96 ng/ml

Instrument :
ECD_L
ClientSampleId :
RESCHK

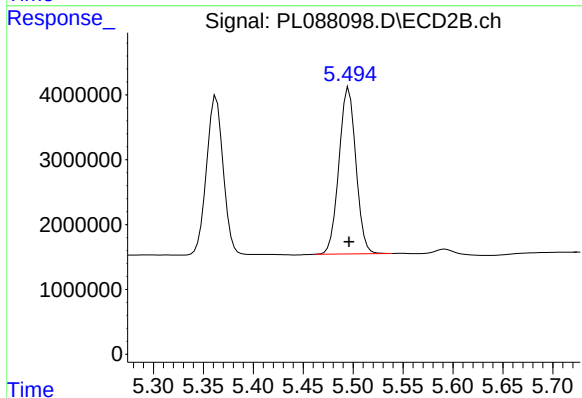


#13 Dieldrin

R.T.: 5.496 min
Delta R.T.: 0.000 min
Response: 30282231
Conc: 17.55 ng/ml

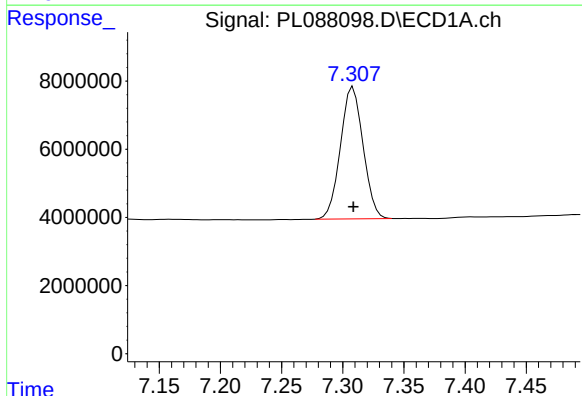


#19 Endosulfan Sulfate

R.T.: 7.308 min
Delta R.T.: 0.000 min
Response: 49915192
Conc: 19.16 ng/ml

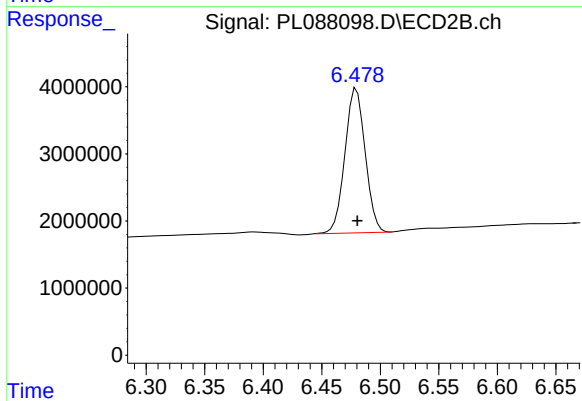

#19 Endosulfan Sulfate


R.T.: 6.480 min
Delta R.T.: 0.000 min
Response: 25918245
Conc: 18.45 ng/ml

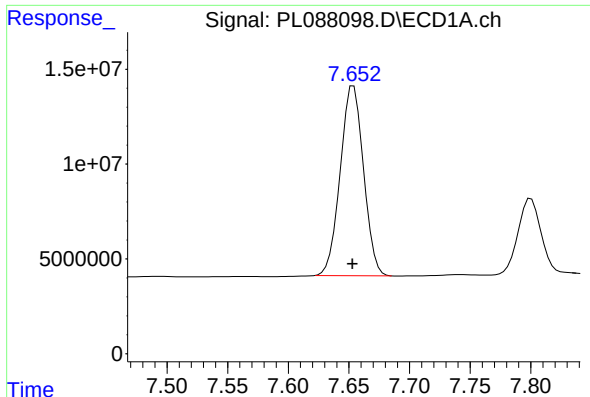

#20 Methoxychlor


R.T.: 7.654 min
Delta R.T.: 0.001 min
Response: 133761704
Conc: 101.05 ng/ml

Instrument :
ECD_L
ClientSampleId :
RESCHK

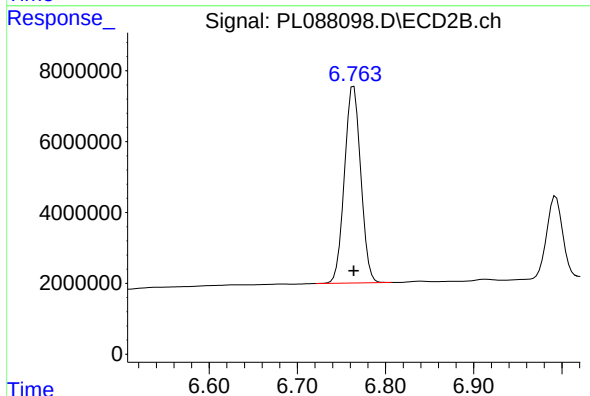


#20 Methoxychlor

R.T.: 6.764 min
Delta R.T.: 0.000 min
Response: 71286292
Conc: 90.95 ng/ml

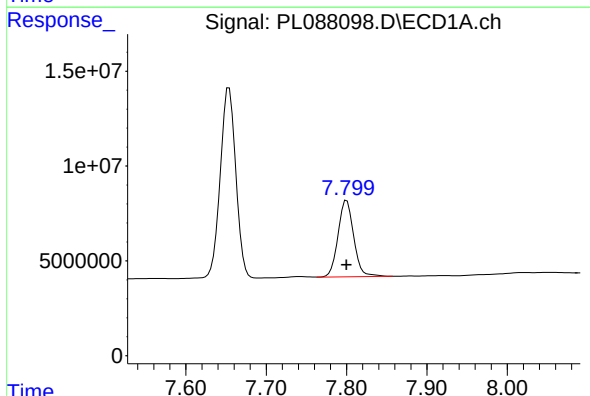


#21 Endrin ketone

R.T.: 7.800 min
Delta R.T.: 0.000 min
Response: 54720338
Conc: 19.53 ng/ml

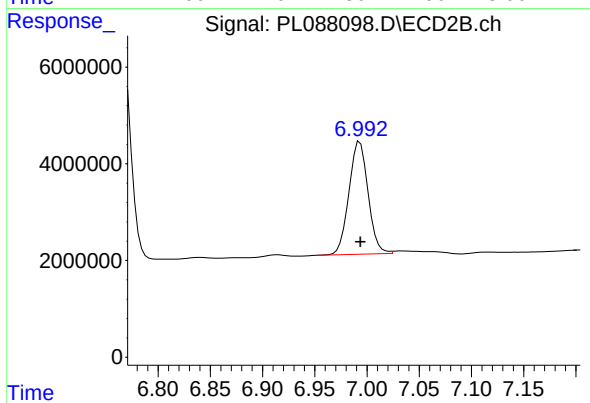

#21 Endrin ketone


R.T.: 6.993 min
Delta R.T.: 0.000 min
Response: 29644100
Conc: 17.71 ng/ml

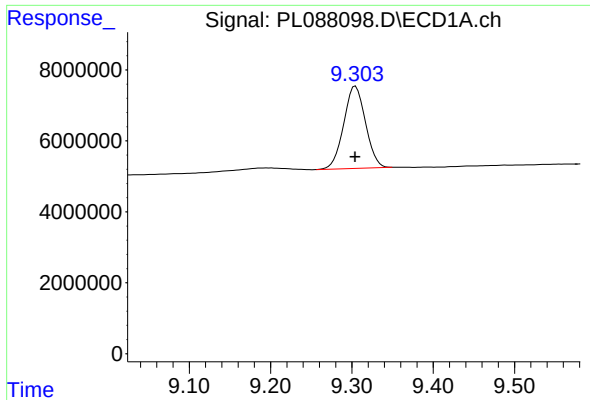

#28 Decachlorobiphenyl

R.T.: 9.304 min
Delta R.T.: 0.000 min
Response: 43169817
Conc: 22.42 ng/ml

Instrument :
ECD_L
ClientSampleId :
RESCHK

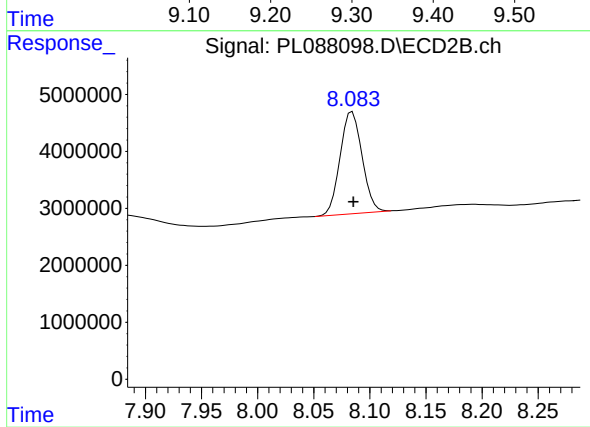

#28 Decachlorobiphenyl

R.T.: 8.084 min
Delta R.T.: 0.000 min
Response: 24441952
Conc: 19.20 ng/ml