

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL021524\
 Data File : PL088104.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Feb 2024 20:46
 Operator : AR\AJ
 Sample : PCHLORICC1000
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 16 05:45:23 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL021524.M
 Quant Title : GC Extractables
 QLast Update : Fri Feb 16 05:43:44 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.635	2.853	296.7E6	182.3E6	103.109	103.984
28)	SA Decachlor...	9.304	8.085	222.6E6	138.9E6	102.689	101.156
Target Compounds							
23)	Chlordane-1	4.820	3.876	124.7E6	52825917	1023.589	1045.493
24)	Chlordane-2	5.357	4.464	129.4E6	61315073	987.975	991.553
25)	Chlordane-3	6.077	5.106	531.3E6	197.3E6	1054.064	1061.184
26)	Chlordane-4	6.162	5.170	630.1E6	178.4E6	1039.226	1038.975
27)	Chlordane-5	7.022	5.846	104.5E6	52344356	1037.294	1025.749



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL021524\
Data File : PL088104.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Feb 2024 20:46
Operator : AR\AJ
Sample : PCHLORICC1000
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 16 05:45:23 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL021524.M
Quant Title : GC Extractables
QLast Update : Fri Feb 16 05:43:44 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

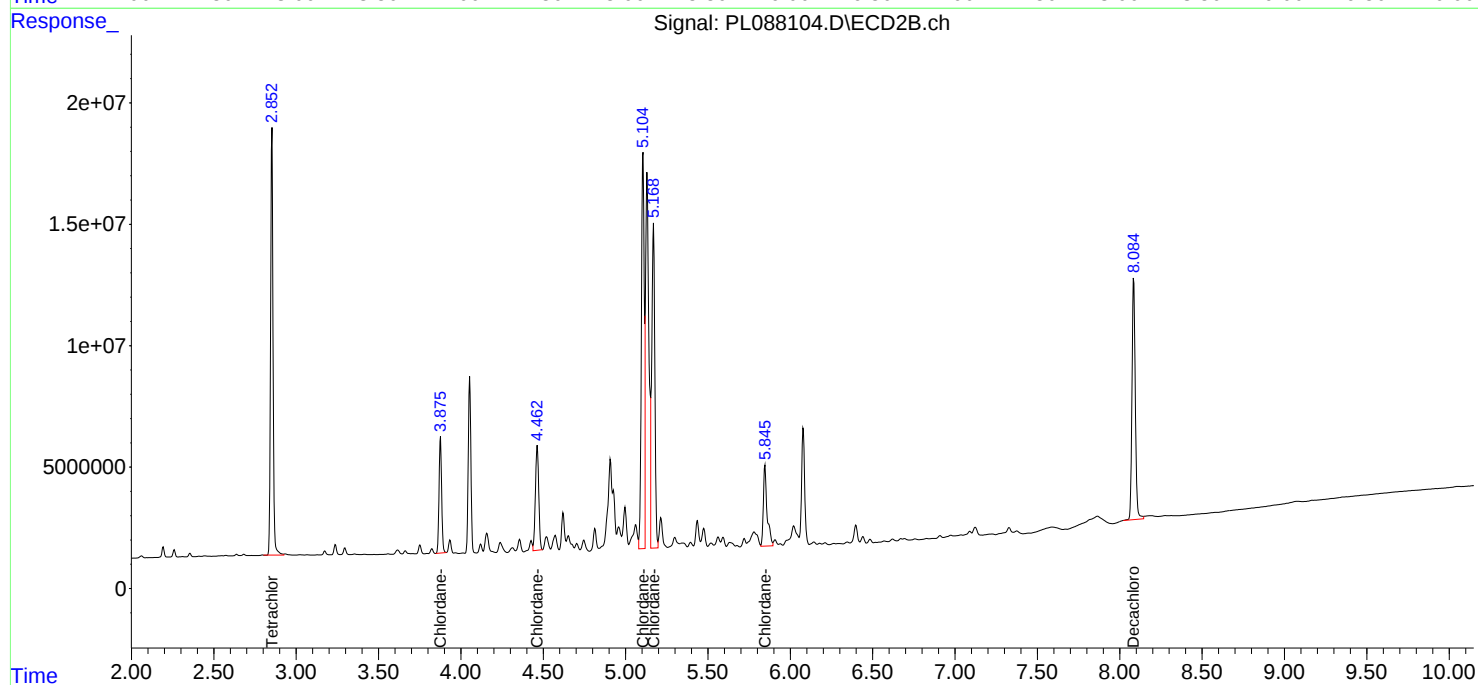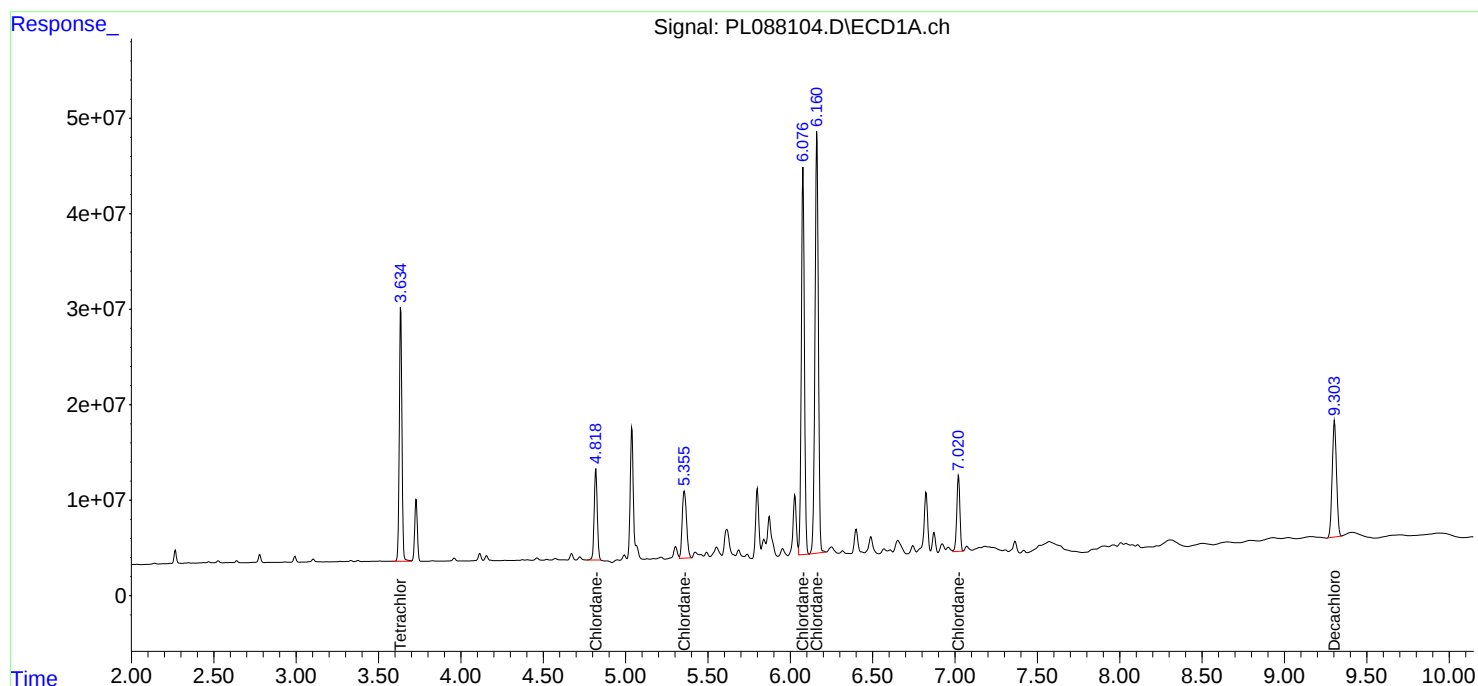


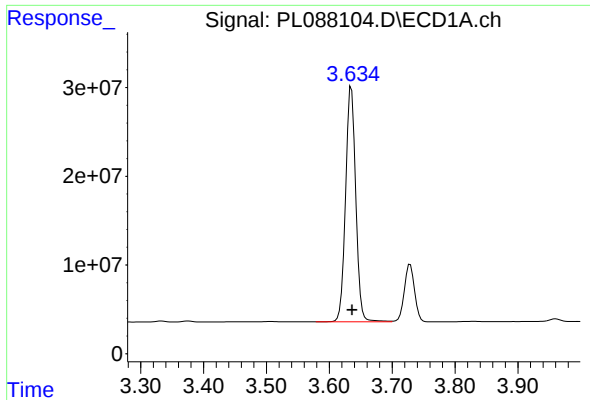

#1 Tetrachloro-m-xylene


R.T.: 3.635 min
Delta R.T.: 0.000 min
Response: 296703447
Conc: 103.11 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

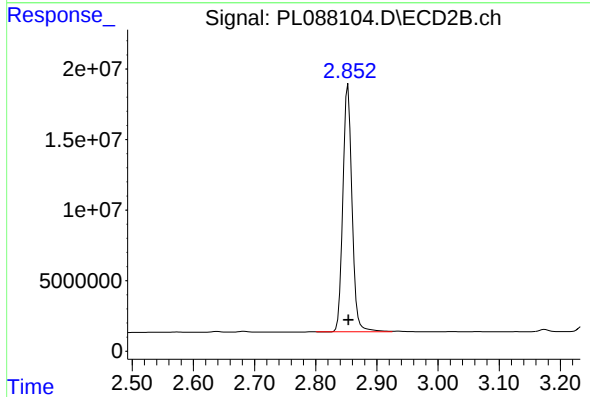


#1 Tetrachloro-m-xylene

R.T.: 2.853 min
Delta R.T.: 0.000 min
Response: 182258706
Conc: 103.98 ng/ml

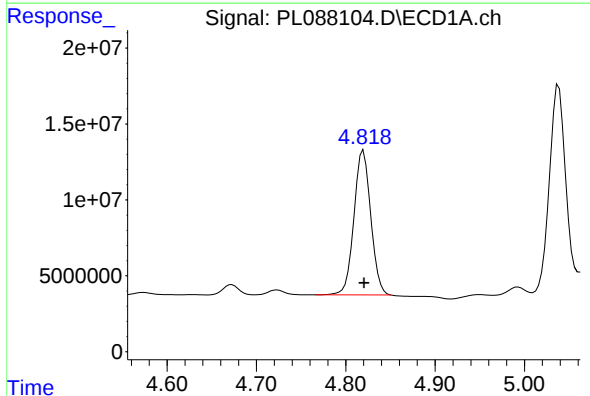


#23 Chlordane-1

R.T.: 4.820 min
Delta R.T.: 0.000 min
Response: 124715743
Conc: 1023.59 ng/ml

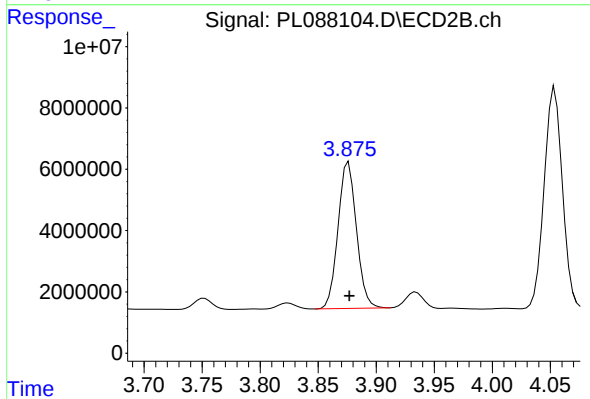

#23 Chlordane-1


R.T.: 3.876 min
Delta R.T.: 0.000 min
Response: 52825917
Conc: 1045.49 ng/ml

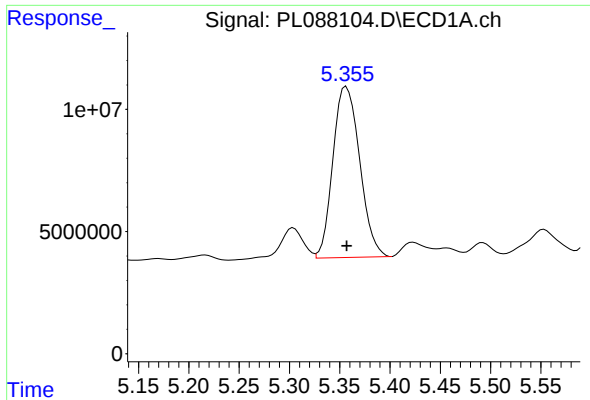

#24 Chlordane-2


R.T.: 5.357 min
Delta R.T.: 0.000 min
Response: 129443185
Conc: 987.97 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

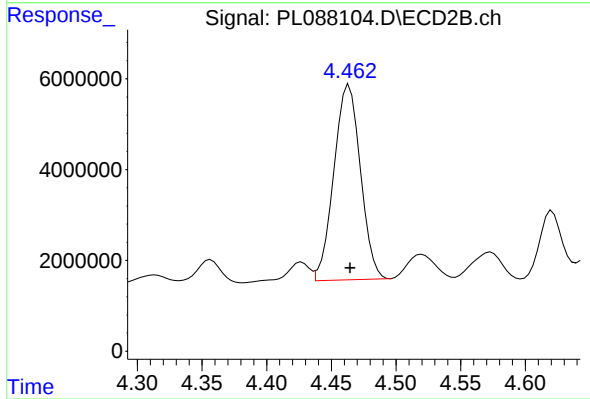


#24 Chlordane-2

R.T.: 4.464 min
Delta R.T.: 0.000 min
Response: 61315073
Conc: 991.55 ng/ml

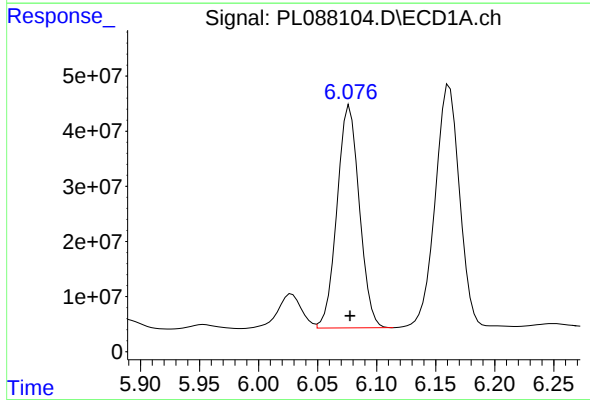


#25 Chlordane-3

R.T.: 6.077 min
Delta R.T.: 0.000 min
Response: 531276635
Conc: 1054.06 ng/ml

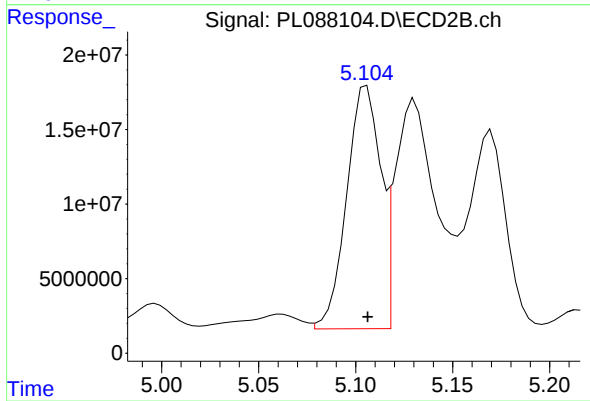

#25 Chlordane-3


R.T.: 5.106 min
Delta R.T.: 0.000 min
Response: 197349099
Conc: 1061.18 ng/ml

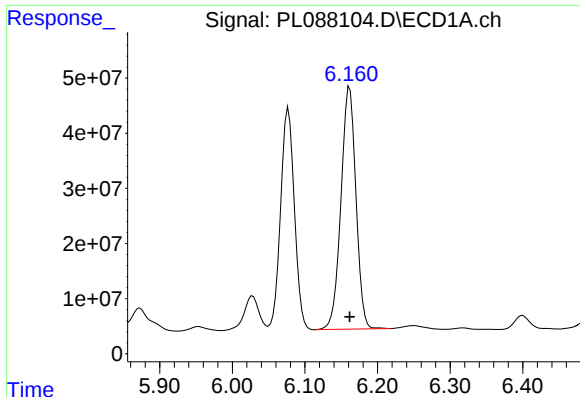

#26 Chlordane-4


R.T.: 6.162 min
Delta R.T.: 0.000 min
Response: 630108808
Conc: 1039.23 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

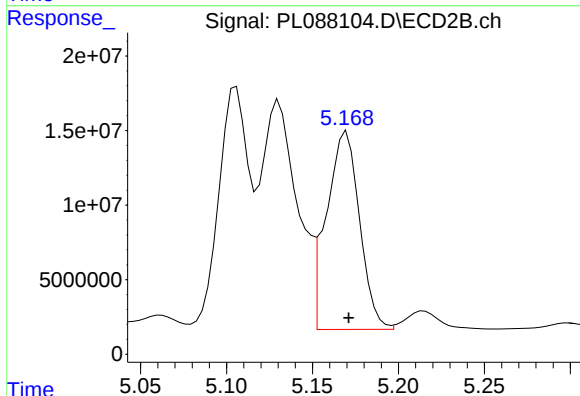


#26 Chlordane-4

R.T.: 5.170 min
Delta R.T.: -0.001 min
Response: 178447948
Conc: 1038.98 ng/ml

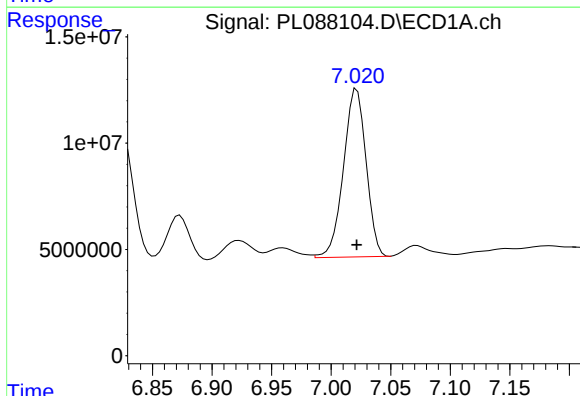


#27 Chlordane-5

R.T.: 7.022 min
Delta R.T.: 0.000 min
Response: 104517038
Conc: 1037.29 ng/ml

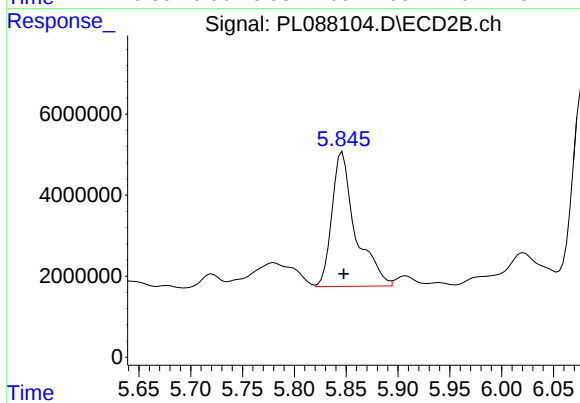

#27 Chlordane-5


R.T.: 5.846 min
Delta R.T.: -0.001 min
Response: 52344356
Conc: 1025.75 ng/ml

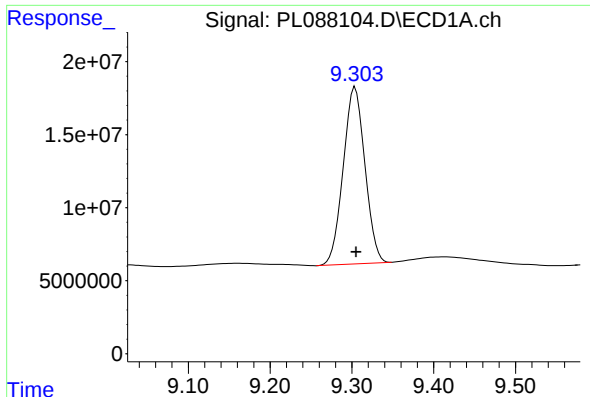

#28 Decachlorobiphenyl

R.T.: 9.304 min
Delta R.T.: -0.001 min
Response: 222612843
Conc: 102.69 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

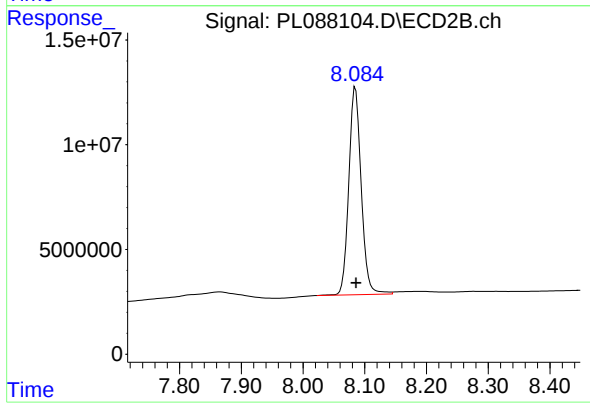

#28 Decachlorobiphenyl

R.T.: 8.085 min
Delta R.T.: 0.000 min
Response: 138873470
Conc: 101.16 ng/ml