

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL021524\
 Data File : PL088105.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Feb 2024 21:00
 Operator : AR\AJ
 Sample : PCHLORICC750
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 16 10:31:09 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL021524.M
 Quant Title : GC Extractables
 QLast Update : Fri Feb 16 10:30:57 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.636	2.873	212.0E6	130.9E6	73.089	73.769
28)	SA Decachlor...	9.306	8.106	159.1E6	99611871	73.316	70.947
Target Compounds							
23)	Chlordane-1	4.821	3.897	88041187	37305246	685.637	724.753
24)	Chlordane-2	5.358	4.485	93984606	44857140	700.230	706.008
25)	Chlordane-3	6.078	5.126	375.1E6	138.4E6	742.591	743.160
26)	Chlordane-4	6.162	5.191	448.5E6	128.5E6	730.550	742.835
27)	Chlordane-5	7.021	5.867	73834071	37333297	729.472	705.700



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL021524\
Data File : PL088105.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Feb 2024 21:00
Operator : AR\AJ
Sample : PCHLORICC750
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 16 10:31:09 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL021524.M
Quant Title : GC Extractables
QLast Update : Fri Feb 16 10:30:57 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

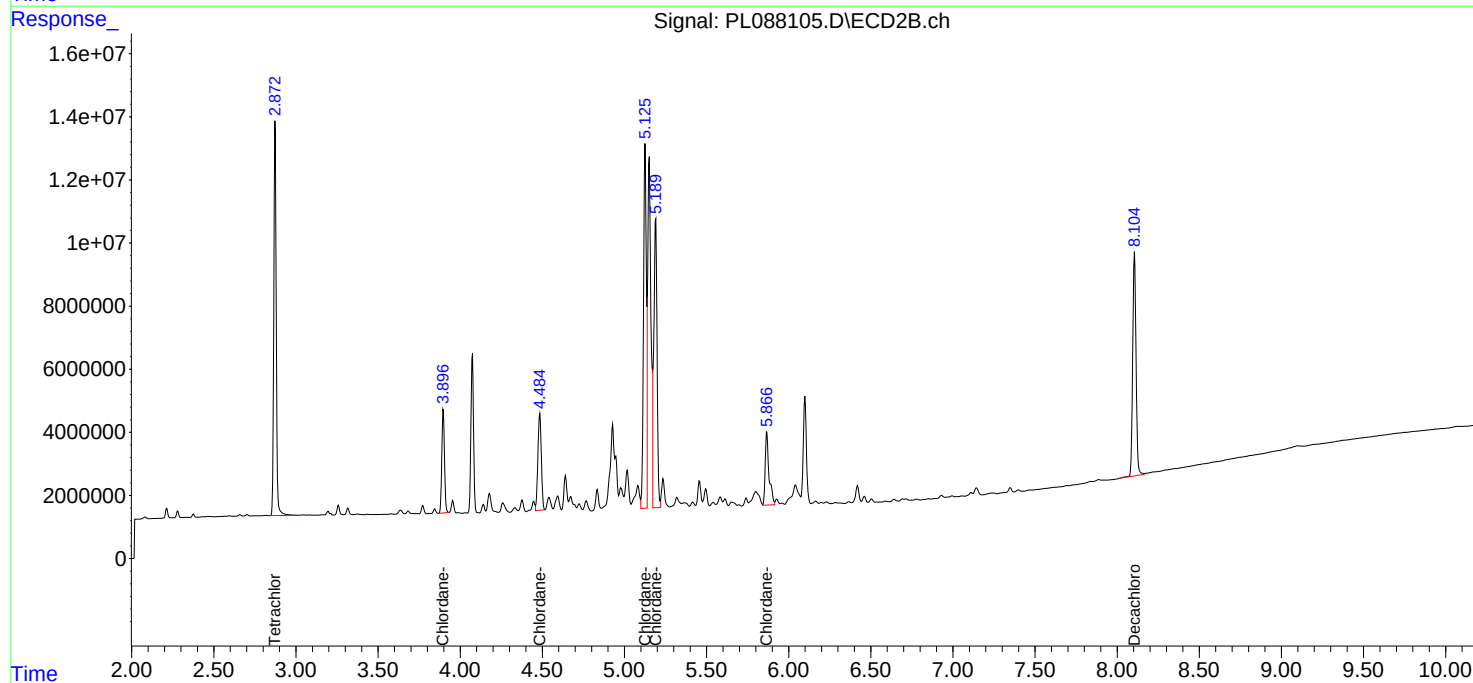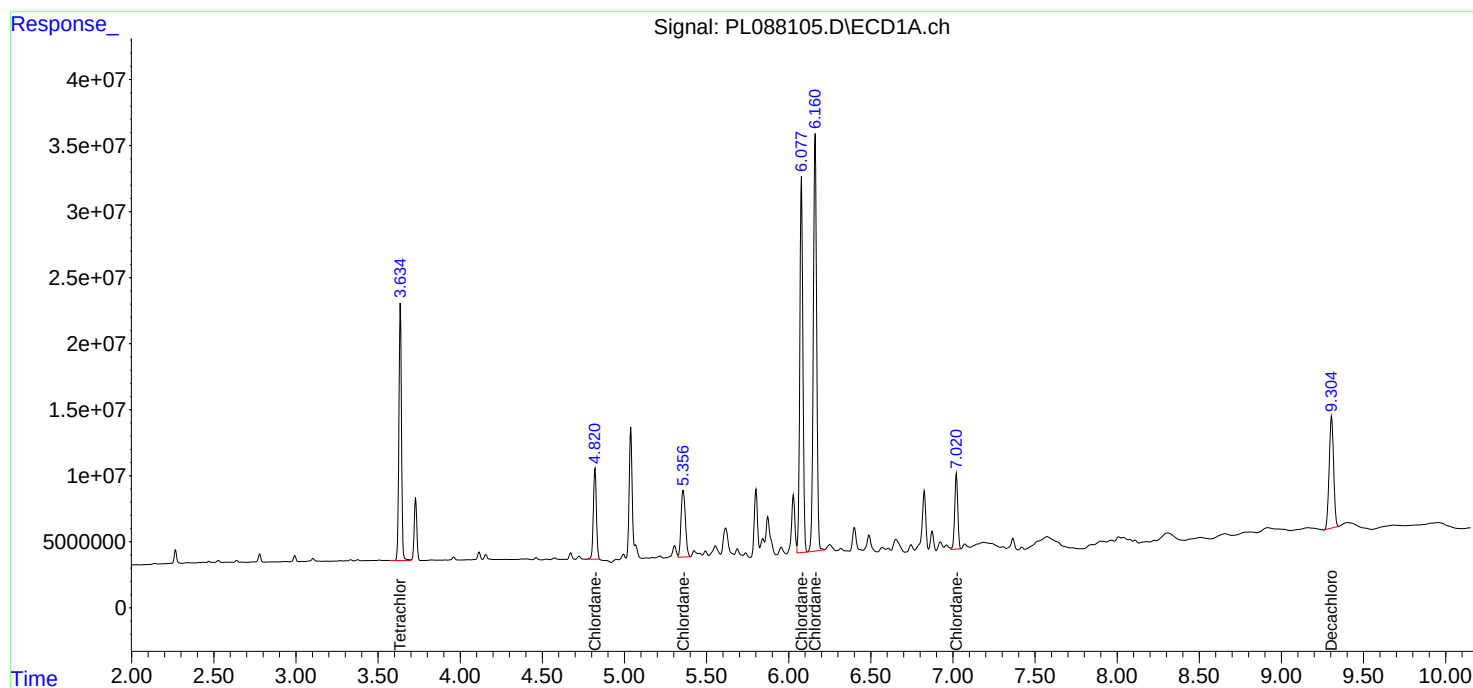


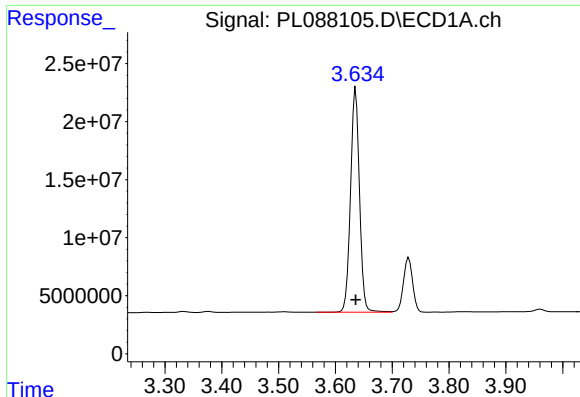

#1 Tetrachloro-m-xylene


R.T.: 3.636 min
Delta R.T.: 0.000 min
Response: 211964342
Conc: 73.09 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

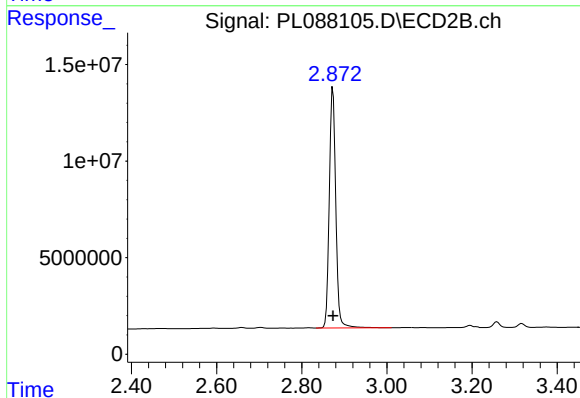


#1 Tetrachloro-m-xylene

R.T.: 2.873 min
Delta R.T.: 0.000 min
Response: 130930118
Conc: 73.77 ng/ml

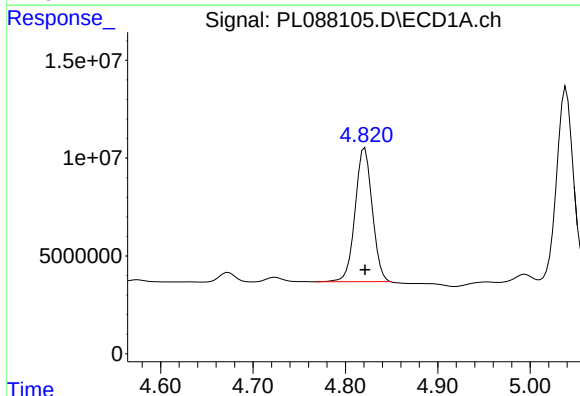


#23 Chlordane-1

R.T.: 4.821 min
Delta R.T.: 0.000 min
Response: 88041187
Conc: 685.64 ng/ml

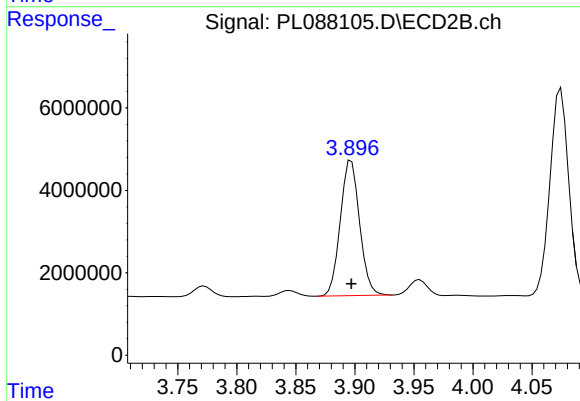

#23 Chlordane-1


R.T.: 3.897 min
Delta R.T.: 0.000 min
Response: 37305246
Conc: 724.75 ng/ml

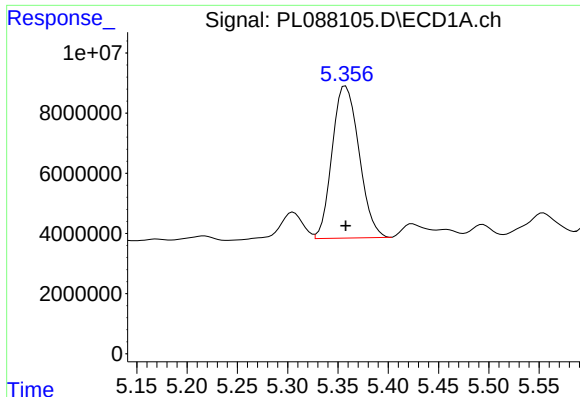

#24 Chlordane-2


R.T.: 5.358 min
Delta R.T.: 0.000 min
Response: 93984606
Conc: 700.23 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

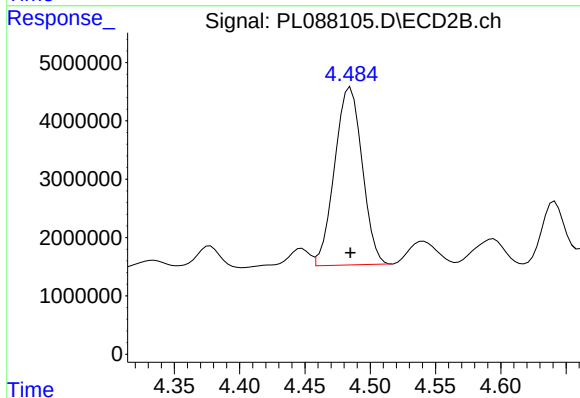


#24 Chlordane-2

R.T.: 4.485 min
Delta R.T.: 0.000 min
Response: 44857140
Conc: 706.01 ng/ml

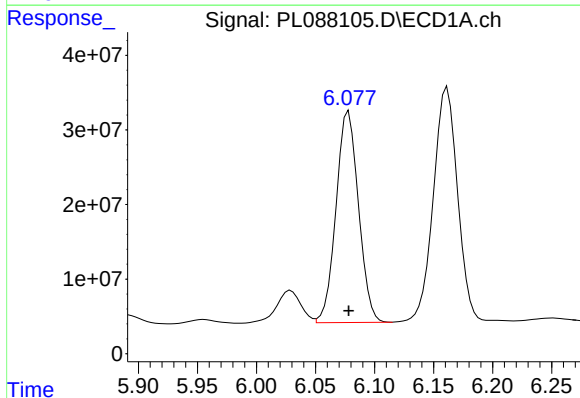


#25 Chlordane-3

R.T.: 6.078 min
Delta R.T.: 0.000 min
Response: 375061756
Conc: 742.59 ng/ml

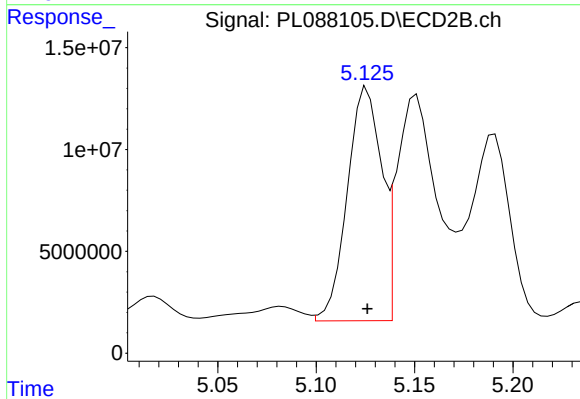

#25 Chlordane-3


R.T.: 5.126 min
Delta R.T.: 0.000 min
Response: 138374052
Conc: 743.16 ng/ml

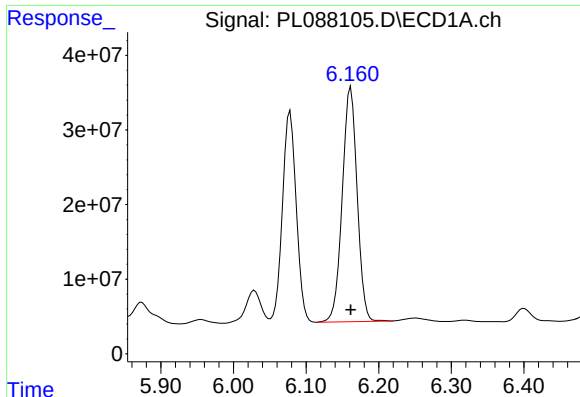

#26 Chlordane-4


R.T.: 6.162 min
Delta R.T.: 0.000 min
Response: 448526371
Conc: 730.55 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

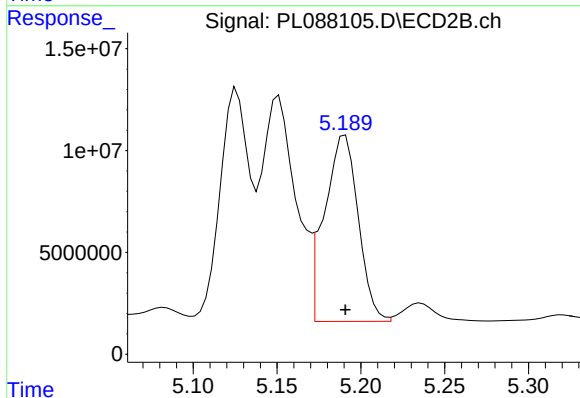


#26 Chlordane-4

R.T.: 5.191 min
Delta R.T.: 0.000 min
Response: 128453470
Conc: 742.83 ng/ml

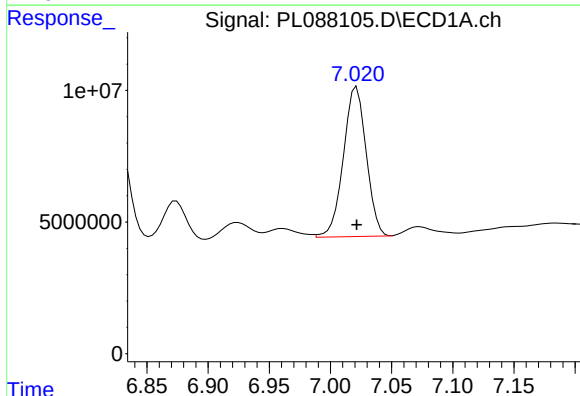


#27 Chlordane-5

R.T.: 7.021 min
Delta R.T.: 0.000 min
Response: 73834071
Conc: 729.47 ng/ml

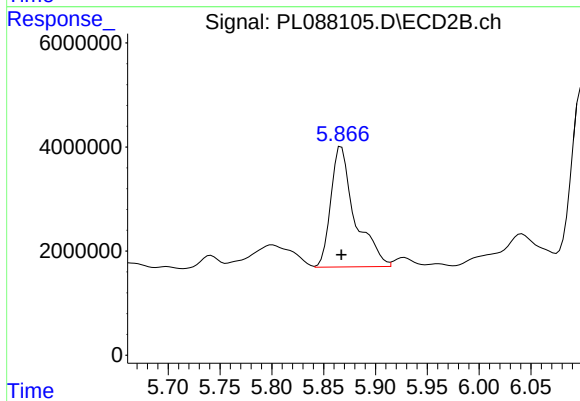

#27 Chlordane-5

R.T.: 5.867 min
Delta R.T.: 0.000 min
Response: 37333297
Conc: 705.70 ng/ml

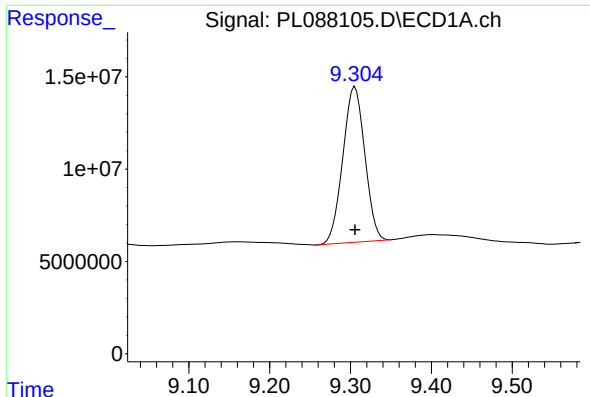

#28 Decachlorobiphenyl


R.T.: 9.306 min

Delta R.T.: 0.000 min

Response: 159058884

Conc: 73.32 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

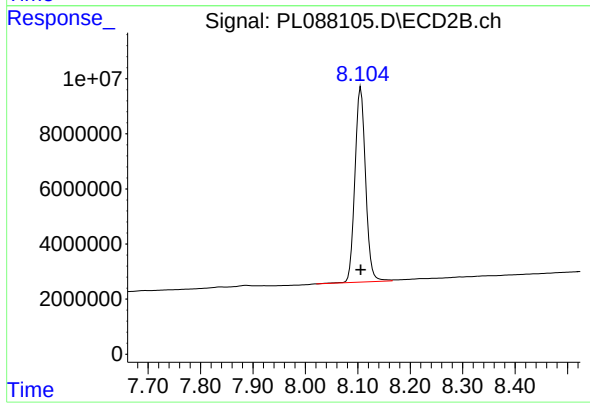

#28 Decachlorobiphenyl

R.T.: 8.106 min

Delta R.T.: 0.000 min

Response: 99611871

Conc: 70.95 ng/ml