

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL021524\
 Data File : PL088106.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Feb 2024 21:13
 Operator : AR\AJ
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 16 05:46:00 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL021524.M
 Quant Title : GC Extractables
 QLast Update : Fri Feb 16 05:43:44 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.636	2.854	143.9E6	87638000	50.000	50.000
28)	SA Decachlor...	9.305	8.086	108.4E6	68643456	50.000	50.000
Target Compounds							
23)	Chlordane-1	4.821	3.877	60920827	25263629	500.000	500.000
24)	Chlordane-2	5.357	4.464	65509355	30918701	500.000	500.000
25)	Chlordane-3	6.078	5.106	252.0E6	92985363	500.000	500.000
26)	Chlordane-4	6.162	5.171	303.2E6	85876898	500.000	500.000
27)	Chlordane-5	7.022	5.848	50379677	25515188	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL021524\
Data File : PL088106.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Feb 2024 21:13
Operator : AR\AJ
Sample : PCHLORICC500
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 16 05:46:00 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL021524.M
Quant Title : GC Extractables
QLast Update : Fri Feb 16 05:43:44 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

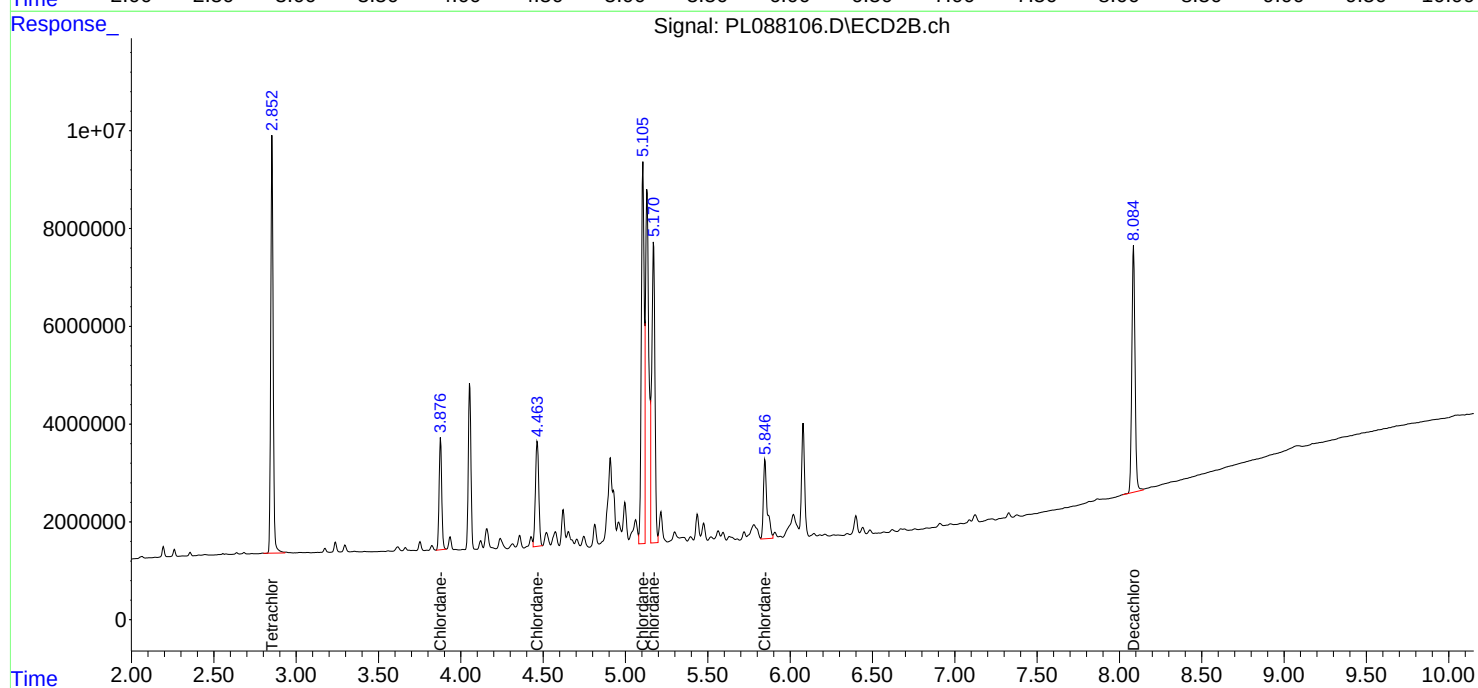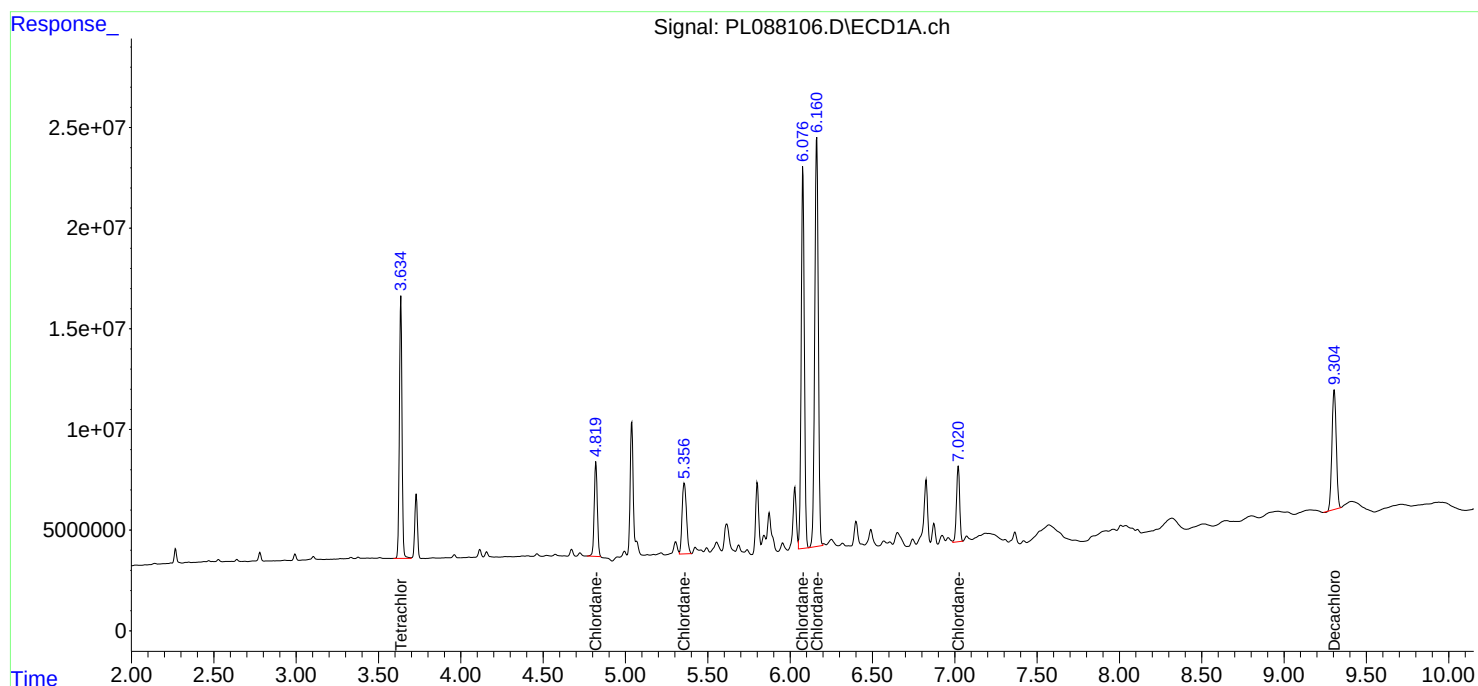


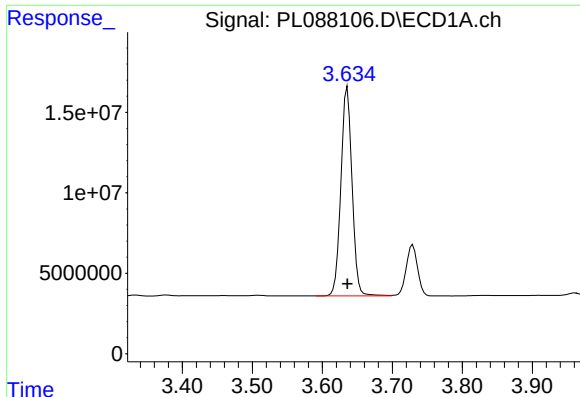

#1 Tetrachloro-m-xylene


R.T.: 3.636 min
Delta R.T.: 0.000 min
Response: 143878865
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

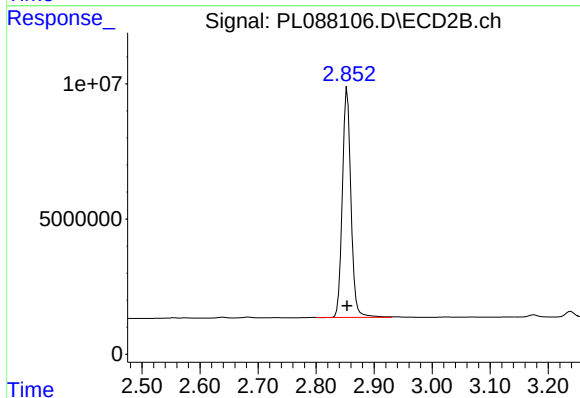


#1 Tetrachloro-m-xylene

R.T.: 2.854 min
Delta R.T.: 0.000 min
Response: 87638000
Conc: 50.00 ng/ml

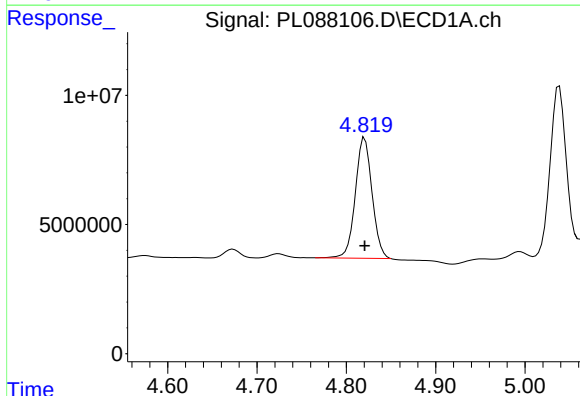


#23 Chlordane-1

R.T.: 4.821 min
Delta R.T.: 0.000 min
Response: 60920827
Conc: 500.00 ng/ml

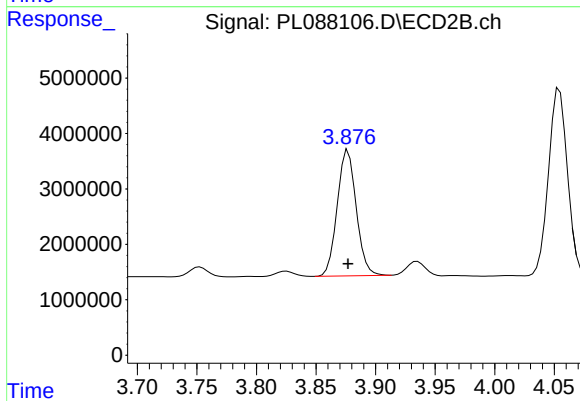

#23 Chlordane-1


R.T.: 3.877 min
Delta R.T.: 0.000 min
Response: 25263629
Conc: 500.00 ng/ml

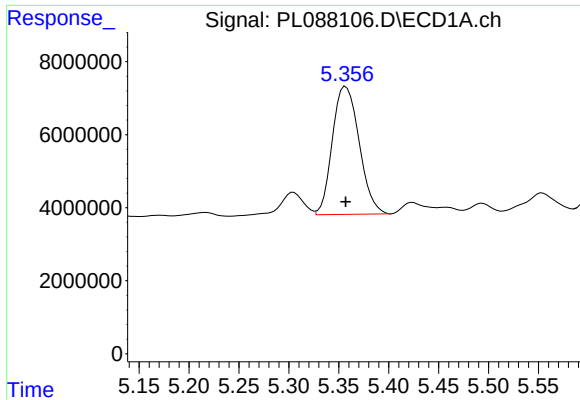

#24 Chlordane-2


R.T.: 5.357 min
Delta R.T.: 0.000 min
Response: 65509355
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

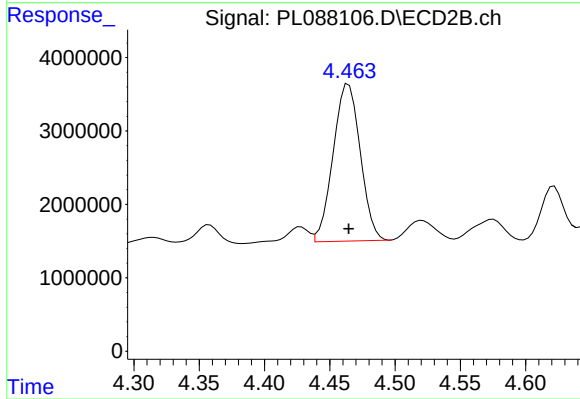


#24 Chlordane-2

R.T.: 4.464 min
Delta R.T.: 0.000 min
Response: 30918701
Conc: 500.00 ng/ml

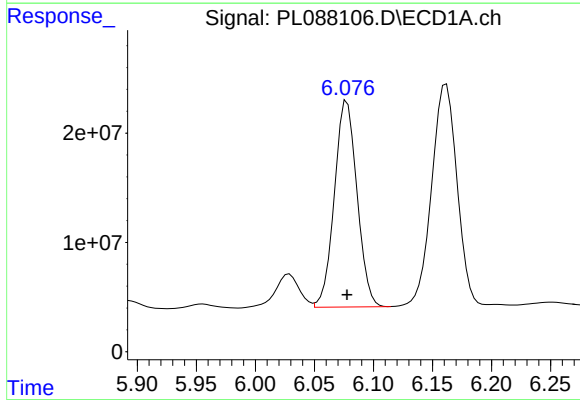


#25 Chlordane-3

R.T.: 6.078 min
Delta R.T.: 0.000 min
Response: 252013369
Conc: 500.00 ng/ml

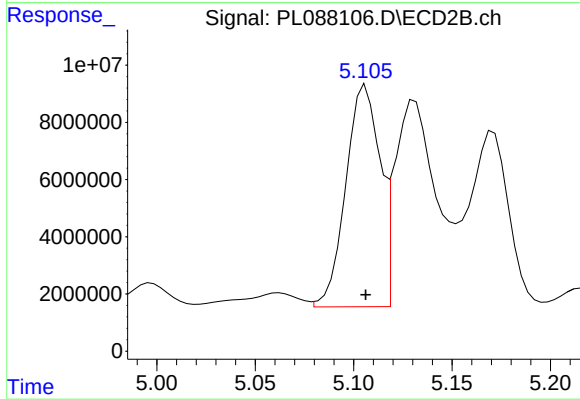

#25 Chlordane-3


R.T.: 5.106 min
Delta R.T.: 0.000 min
Response: 92985363
Conc: 500.00 ng/ml

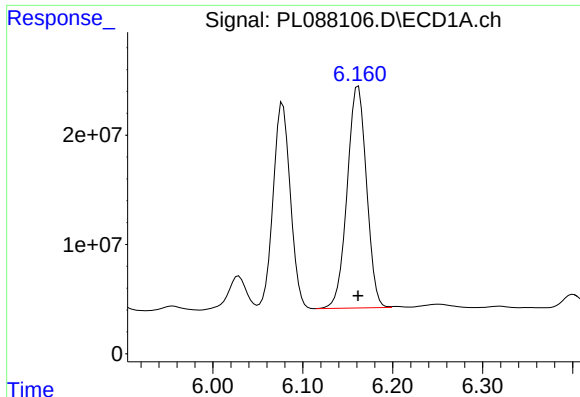

#26 Chlordane-4


R.T.: 6.162 min
Delta R.T.: 0.000 min
Response: 303162605
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

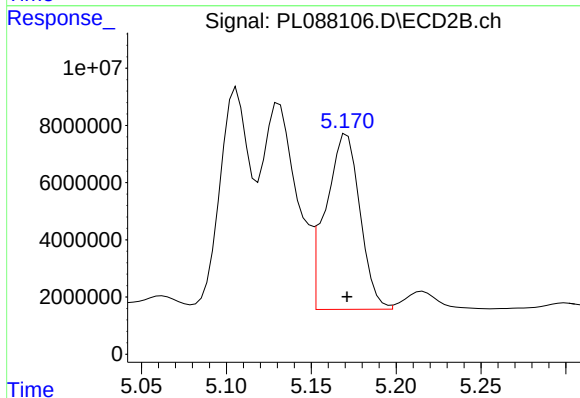


#26 Chlordane-4

R.T.: 5.171 min
Delta R.T.: 0.000 min
Response: 85876898
Conc: 500.00 ng/ml

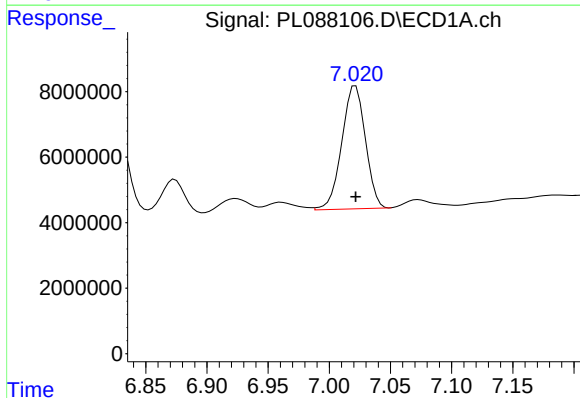


#27 Chlordane-5

R.T.: 7.022 min
Delta R.T.: 0.000 min
Response: 50379677
Conc: 500.00 ng/ml

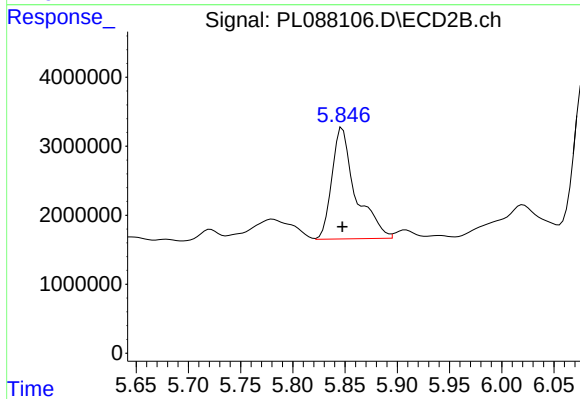

#27 Chlordane-5


R.T.: 5.848 min
Delta R.T.: 0.000 min
Response: 25515188
Conc: 500.00 ng/ml

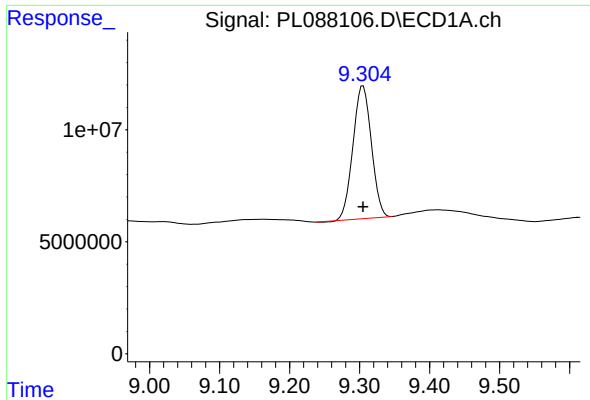

#28 Decachlorobiphenyl

R.T.: 9.305 min
Delta R.T.: 0.000 min
Response: 108392137
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

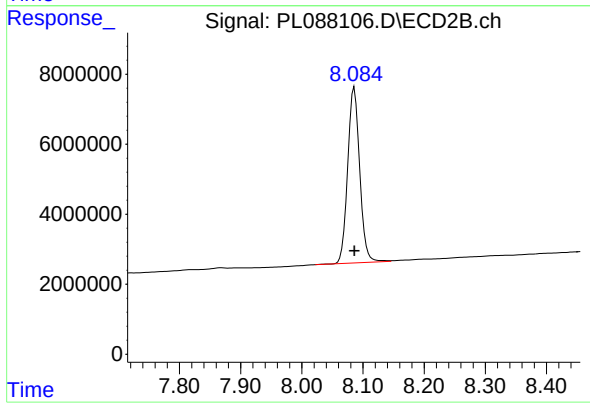

#28 Decachlorobiphenyl

R.T.: 8.086 min
Delta R.T.: 0.000 min
Response: 68643456
Conc: 50.00 ng/ml