

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL021524\
 Data File : PL088115.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Feb 2024 23:17
 Operator : AR\AJ
 Sample : PCHLORICV500
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 ICVPL021524CHLOR

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 16 10:47:26 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL021524.M
 Quant Title : GC Extractables
 QLast Update : Fri Feb 16 10:31:48 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.636	2.854	141.9E6	87132885	48.928	49.092
28)	SA Decachlor...	9.307	8.086	114.4E6	68833331	52.711	49.026
Target Compounds							
23)	Chlordane-1	4.820	3.877	61493160	25575948	478.889	496.880
24)	Chlordane-2	5.357	4.465	65835101	31233519	490.502	491.585
25)	Chlordane-3	6.078	5.106	255.5E6	93549609	505.882	502.423
26)	Chlordane-4	6.161	5.170	307.9E6	87298900	501.527	504.842
27)	Chlordane-5	7.021	5.847	52207466	25778914	515.804	487.291



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL021524\
Data File : PL088115.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Feb 2024 23:17
Operator : AR\AJ
Sample : PCHLORICV500
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
ICVPL021524CHLOR

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 16 10:47:26 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL021524.M
Quant Title : GC Extractables
QLast Update : Fri Feb 16 10:31:48 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

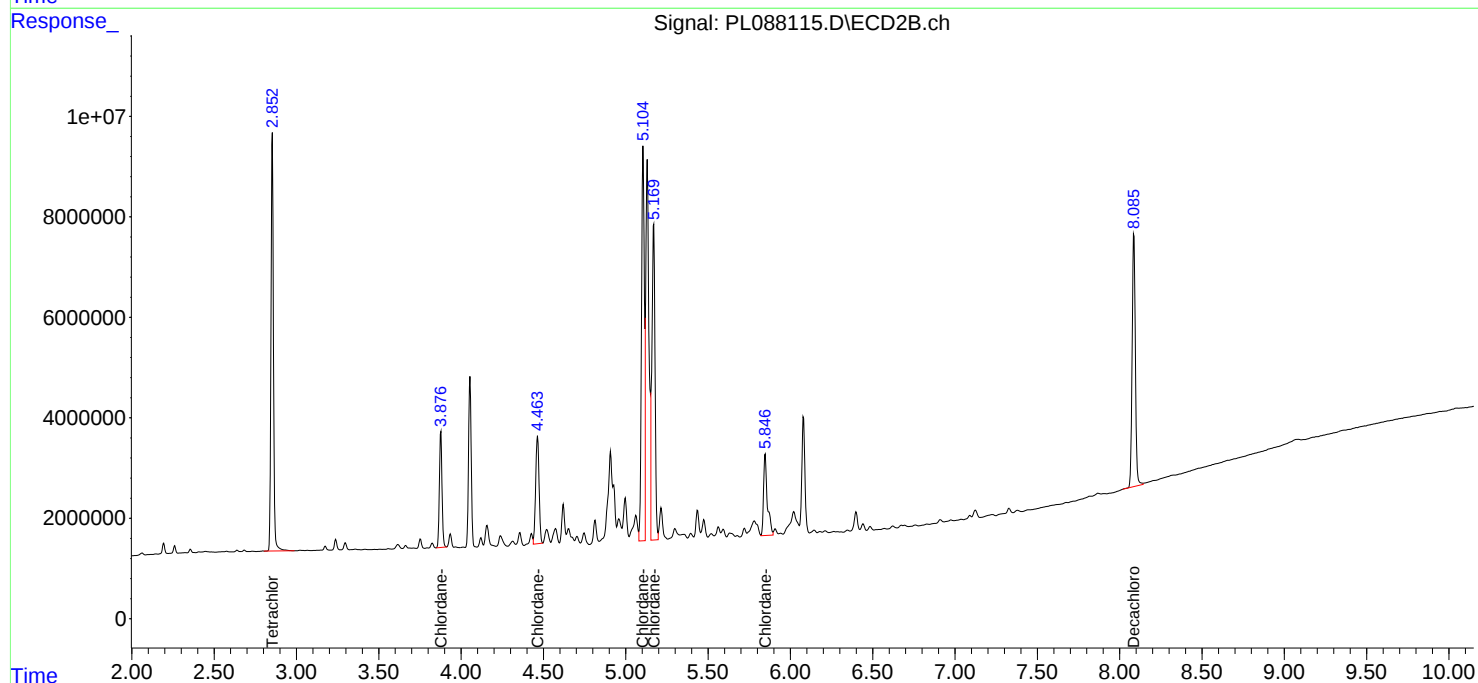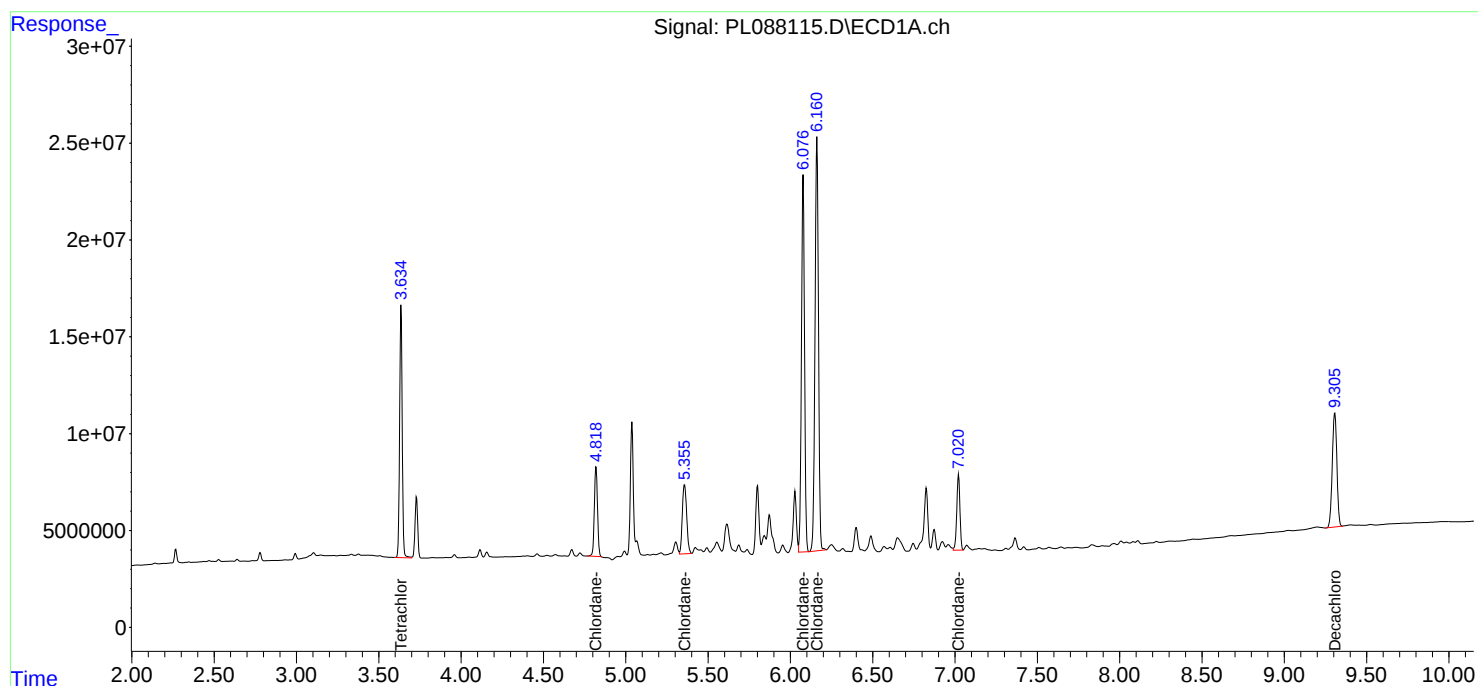


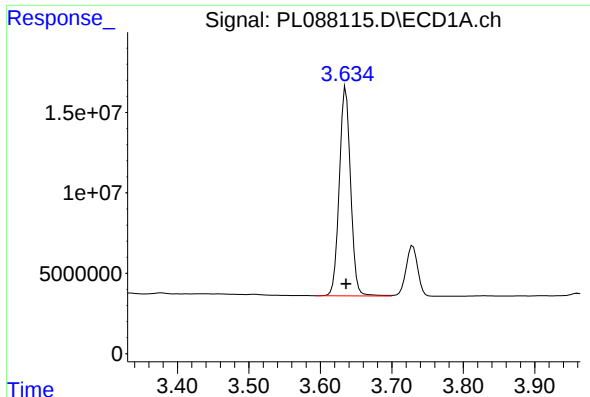

#1 Tetrachloro-m-xylene


R.T.: 3.636 min
Delta R.T.: 0.000 min
Response: 141896079
Conc: 48.93 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL021524CHLOR

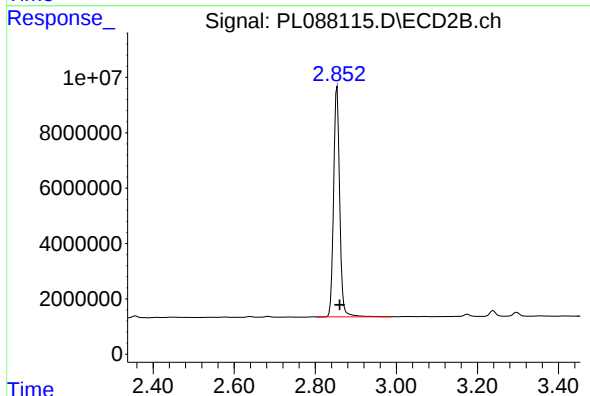


#1 Tetrachloro-m-xylene

R.T.: 2.854 min
Delta R.T.: -0.006 min
Response: 87132885
Conc: 49.09 ng/ml

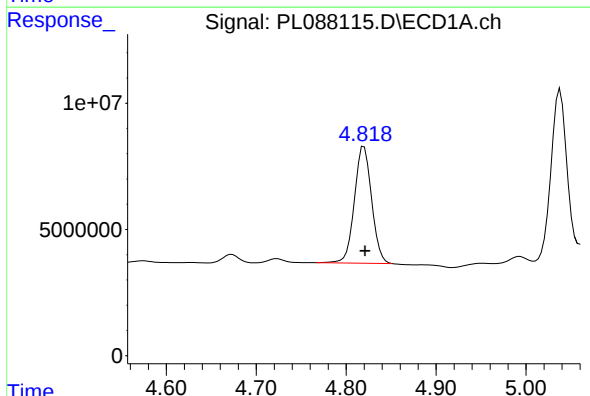


#23 Chlordane-1

R.T.: 4.820 min
Delta R.T.: -0.001 min
Response: 61493160
Conc: 478.89 ng/ml

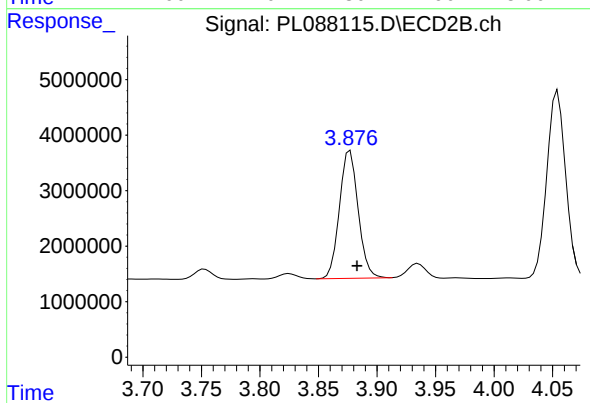

#23 Chlordane-1


R.T.: 3.877 min
Delta R.T.: -0.006 min
Response: 25575948
Conc: 496.88 ng/ml

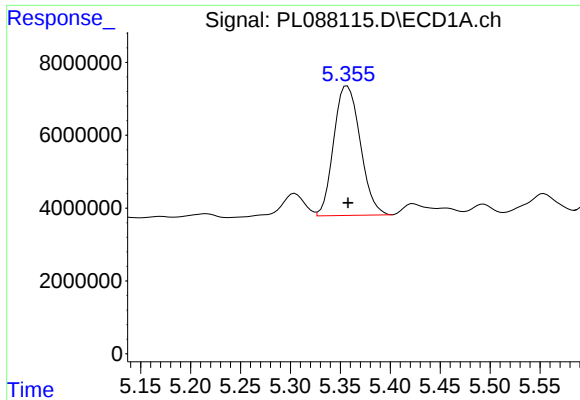

#24 Chlordane-2


R.T.: 5.357 min
Delta R.T.: 0.000 min
Response: 65835101
Conc: 490.50 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL021524CHLOR

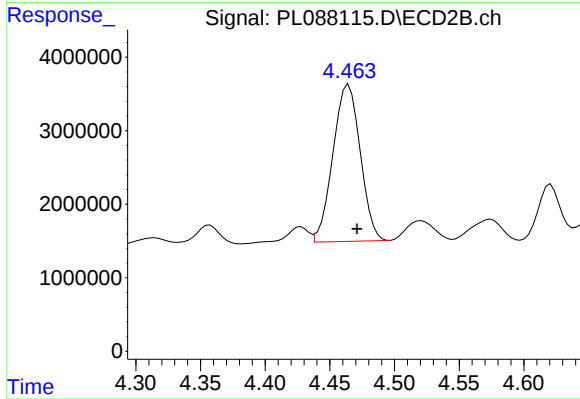


#24 Chlordane-2

R.T.: 4.465 min
Delta R.T.: -0.006 min
Response: 31233519
Conc: 491.59 ng/ml

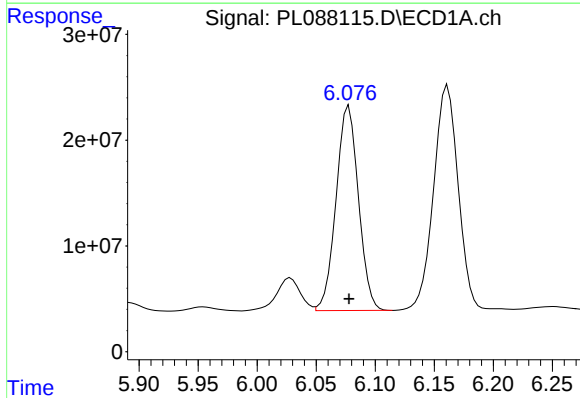


#25 Chlordane-3

R.T.: 6.078 min
Delta R.T.: 0.000 min
Response: 255507044
Conc: 505.88 ng/ml

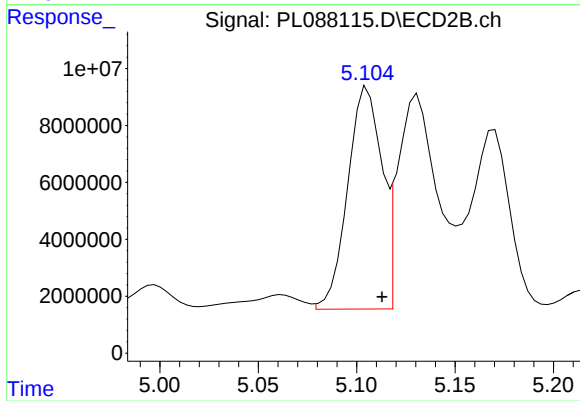

#25 Chlordane-3


R.T.: 5.106 min
Delta R.T.: -0.007 min
Response: 93549609
Conc: 502.42 ng/ml

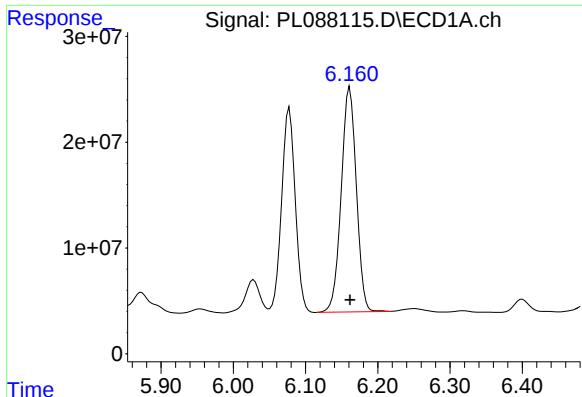

#26 Chlordane-4


R.T.: 6.161 min
Delta R.T.: 0.000 min
Response: 307916390
Conc: 501.53 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL021524CHLOR

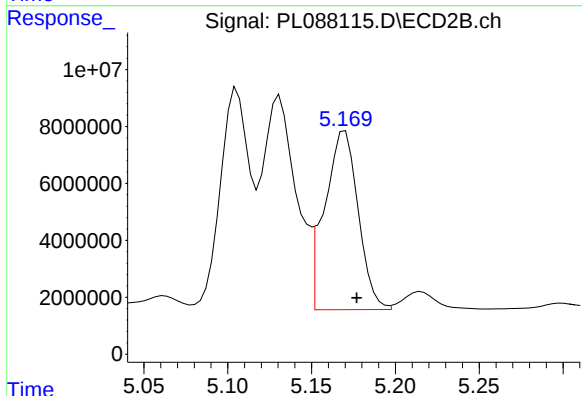


#26 Chlordane-4

R.T.: 5.170 min
Delta R.T.: -0.007 min
Response: 87298900
Conc: 504.84 ng/ml

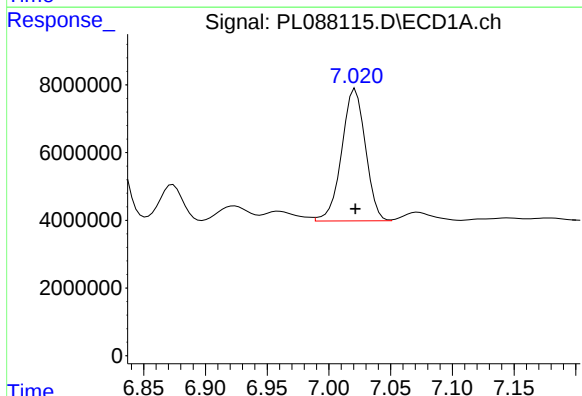


#27 Chlordane-5

R.T.: 7.021 min
Delta R.T.: 0.000 min
Response: 52207466
Conc: 515.80 ng/ml

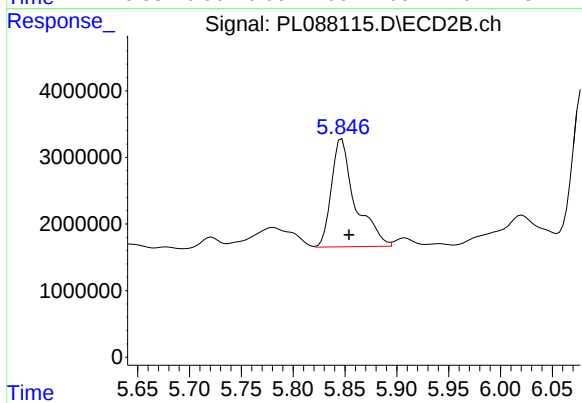

#27 Chlordane-5


R.T.: 5.847 min
Delta R.T.: -0.007 min
Response: 25778914
Conc: 487.29 ng/ml

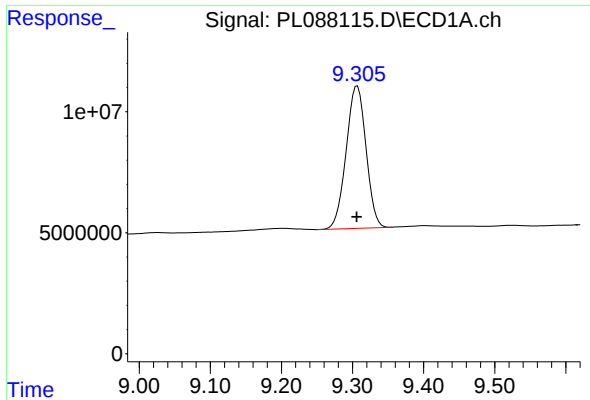

#28 Decachlorobiphenyl

R.T.: 9.307 min
Delta R.T.: 0.001 min
Response: 114355926
Conc: 52.71 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL021524CHLOR

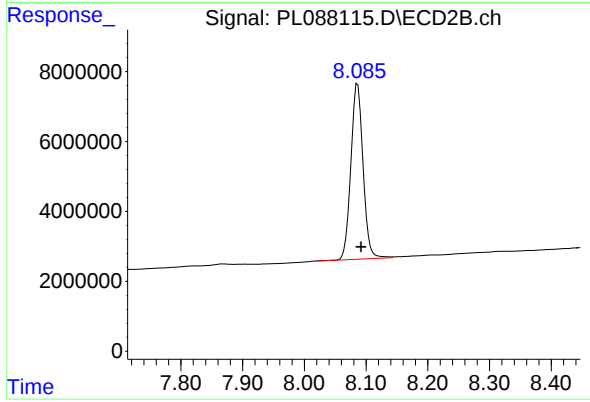

#28 Decachlorobiphenyl

R.T.: 8.086 min
Delta R.T.: -0.006 min
Response: 68833331
Conc: 49.03 ng/ml