

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL021623\
 Data File : PL080981.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Feb 2023 14:46
 Operator : AR\AJ
 Sample : 01553-01
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TWP-01

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 02/17/2023
 Supervised By :Ankita Jodhani 02/17/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 16 20:44:33 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012023.M
 Quant Title : GC Extractables
 QLast Update : Sun Jan 22 23:56:48 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.353	2.690	32715451	32642213	15.253	14.861
28) SA Decachlor...	8.790	7.834	18170214	20905565	10.379m	8.774

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL021623\
Data File : PL080981.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Feb 2023 14:46
Operator : AR\AJ
Sample : 01553-01
Misc :
ALS Vial : 18 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
TWP-01


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 02/17/2023
Supervised By : Ankita Jodhani 02/17/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 16 20:44:33 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012023.M
Quant Title : GC Extractables
QLast Update : Sun Jan 22 23:56:48 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

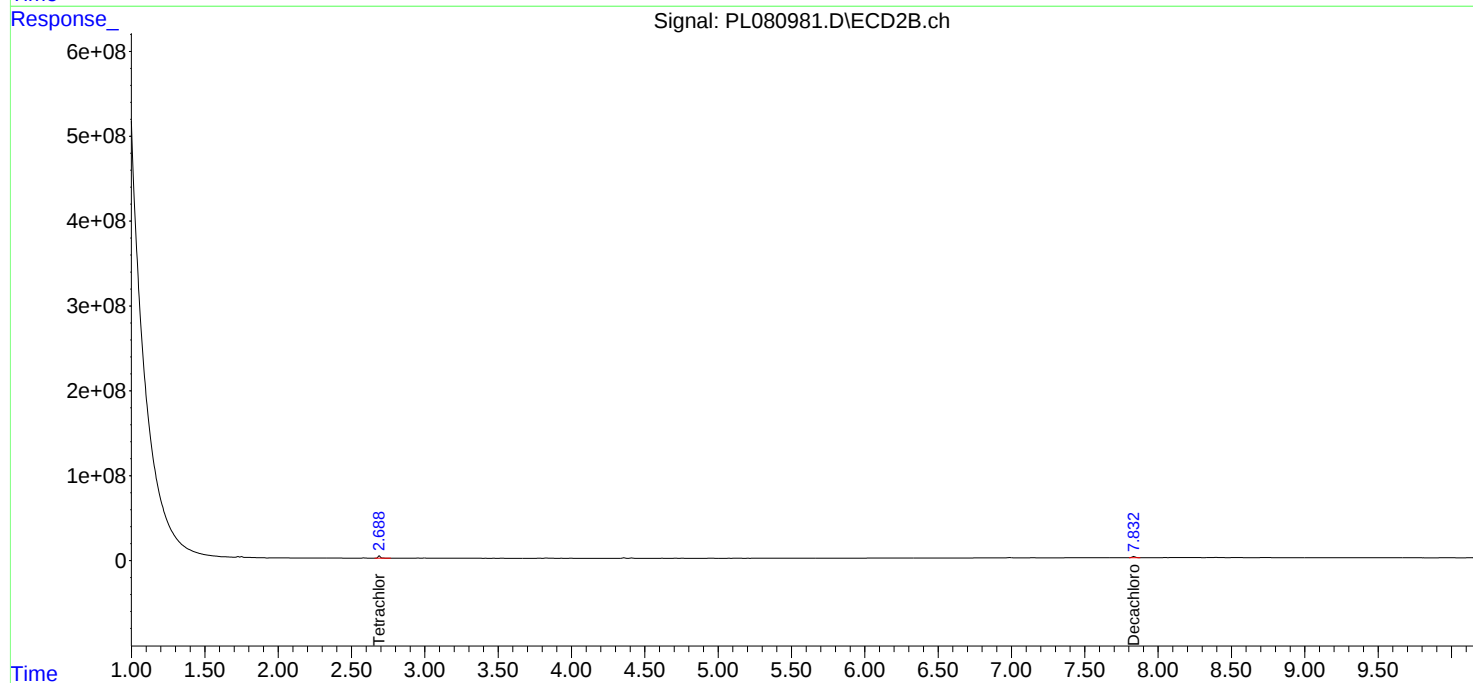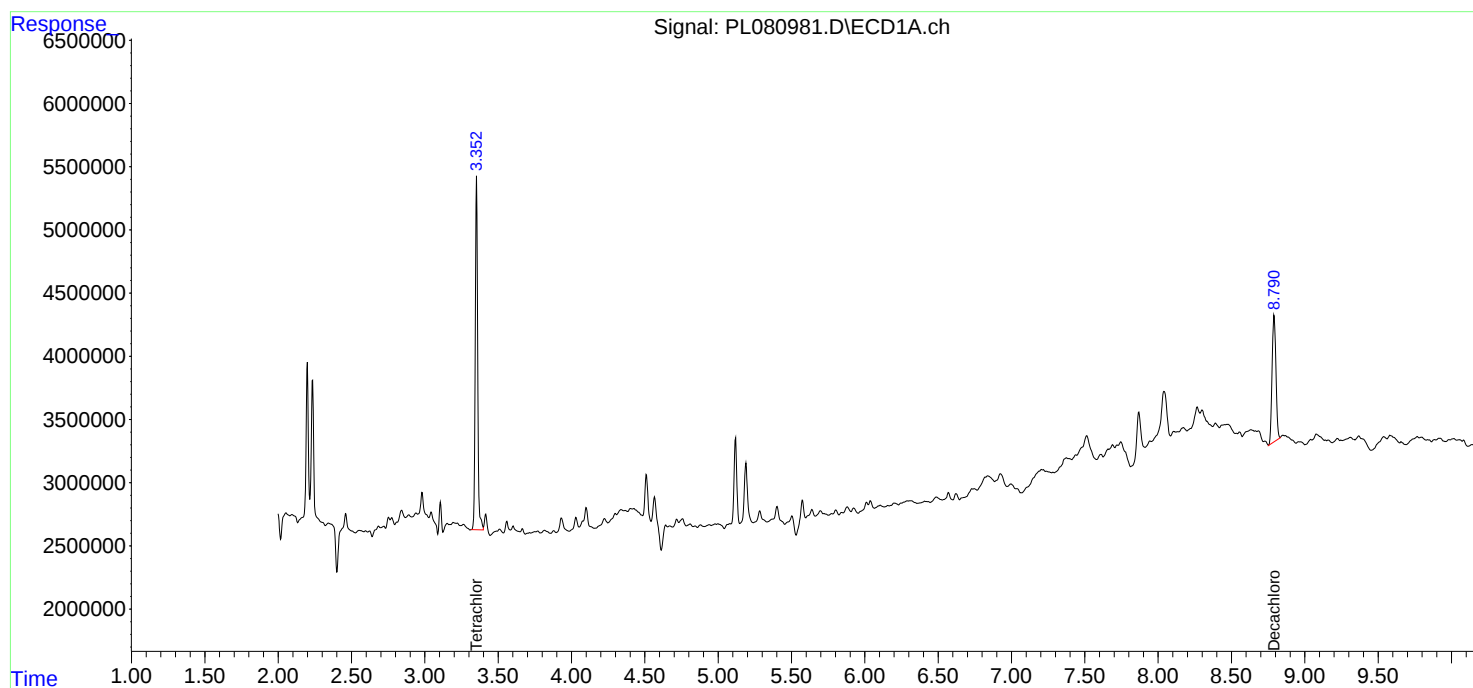

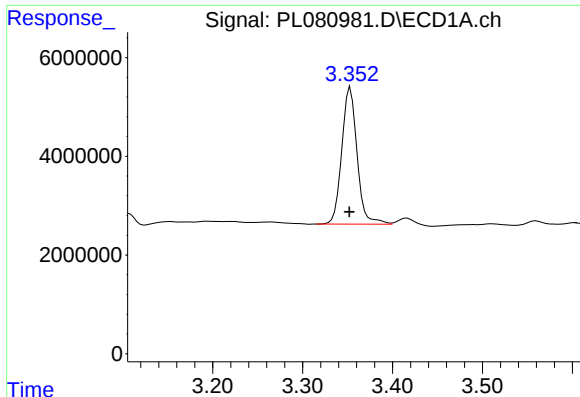


#1 Tetrachloro-m-xylene

R.T.: 3.353 min
Delta R.T.: 0.001 min
Response: 32715451
Conc: 15.25 ng/ml

Instrument :
ECD_L
ClientSampleId :
TWP-01


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 02/17/2023
Supervised By :Ankita Jodhani 02/17/2023

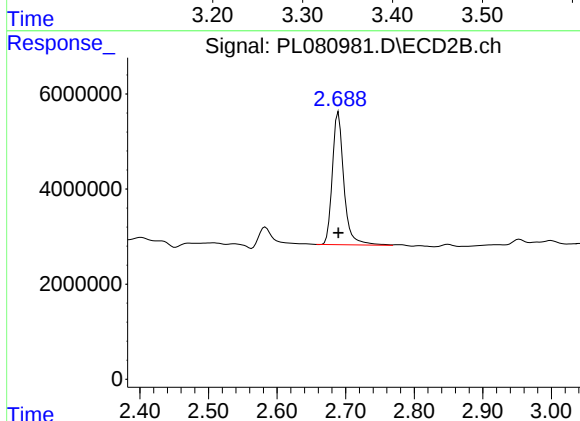


#1 Tetrachloro-m-xylene

R.T.: 2.690 min
Delta R.T.: 0.000 min
Response: 32642213
Conc: 14.86 ng/ml

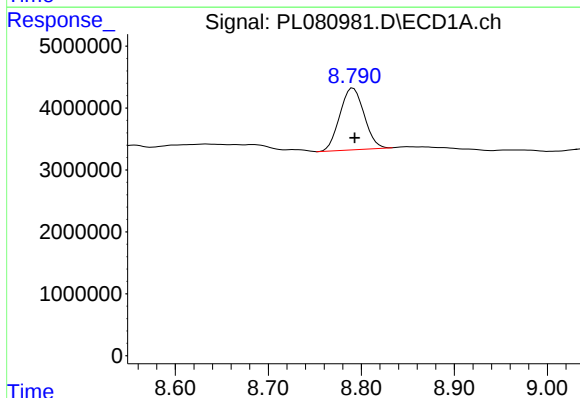

#28 Decachlorobiphenyl

R.T.: 8.790 min
Delta R.T.: -0.003 min
Response: 18170214
Conc: 10.38 ng/ml m

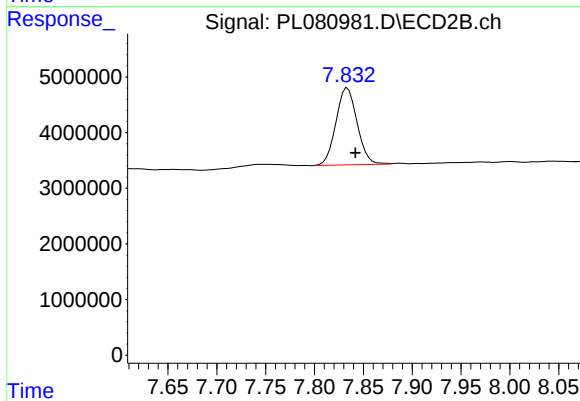

#28 Decachlorobiphenyl

R.T.: 7.834 min
Delta R.T.: -0.008 min
Response: 20905565
Conc: 8.77 ng/ml