

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL021720\
 Data File : PL056587.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Feb 2020 14:25
 Operator : AJ\MA
 Sample : L1545-01
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 18 01:00:52 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL021220.M
 Quant Title : GC Extractables
 QLast Update : Thu Feb 13 05:32:36 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.496	4.020	127.1E6	41475998	14.406	15.246
28)	SA Decachlor...	8.249	9.091	142.9E6	30873170	14.914	15.136
Target Compounds							
10)	B gamma-Chl...	5.459f	0.000	19742347	0	1.435	N.D. #
11)	B alpha-Chl...	0.000	6.201	0	8946034	N.D.	3.046 #
12)	B 4,4'-DDE	5.659	6.358	43357572	12062217	3.410	4.305 #
16)	A 4,4'-DDD	0.000	6.855	0	8621496	N.D.	3.812 #
17)	MA 4,4'-DDT	6.413	7.121f	40204286	8740540	4.242	4.138
20)	A Methoxychlor	6.945	0.000	45928610	0	9.334	N.D. #
25)	Chlordane-3	5.459f	0.000	19742347	0	15.036	N.D. #
26)	Chlordane-4	0.000	6.201	0	8946034	N.D.	19.657 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL021720\
Data File : PL056587.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Feb 2020 14:25
Operator : AJ\MA
Sample : L1545-01
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 18 01:00:52 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL021220.M
Quant Title : GC Extractables
QLast Update : Thu Feb 13 05:32:36 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

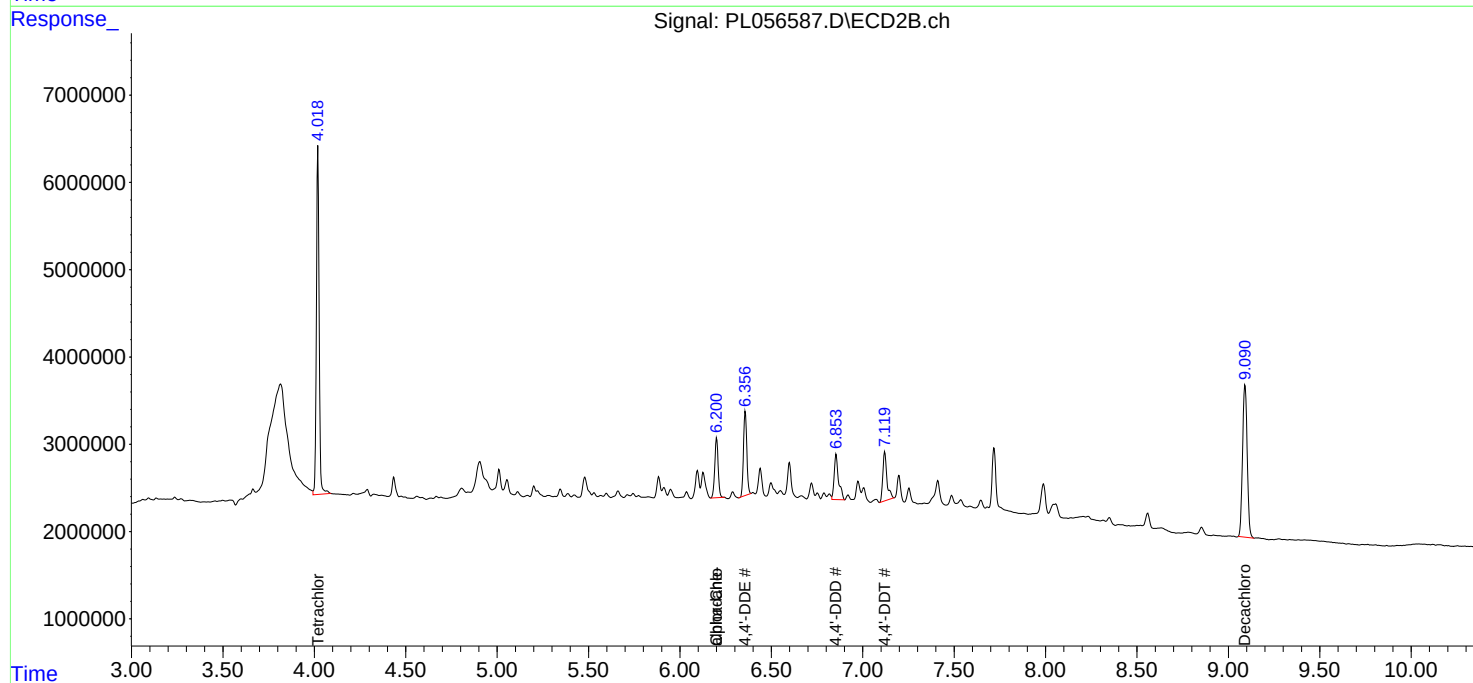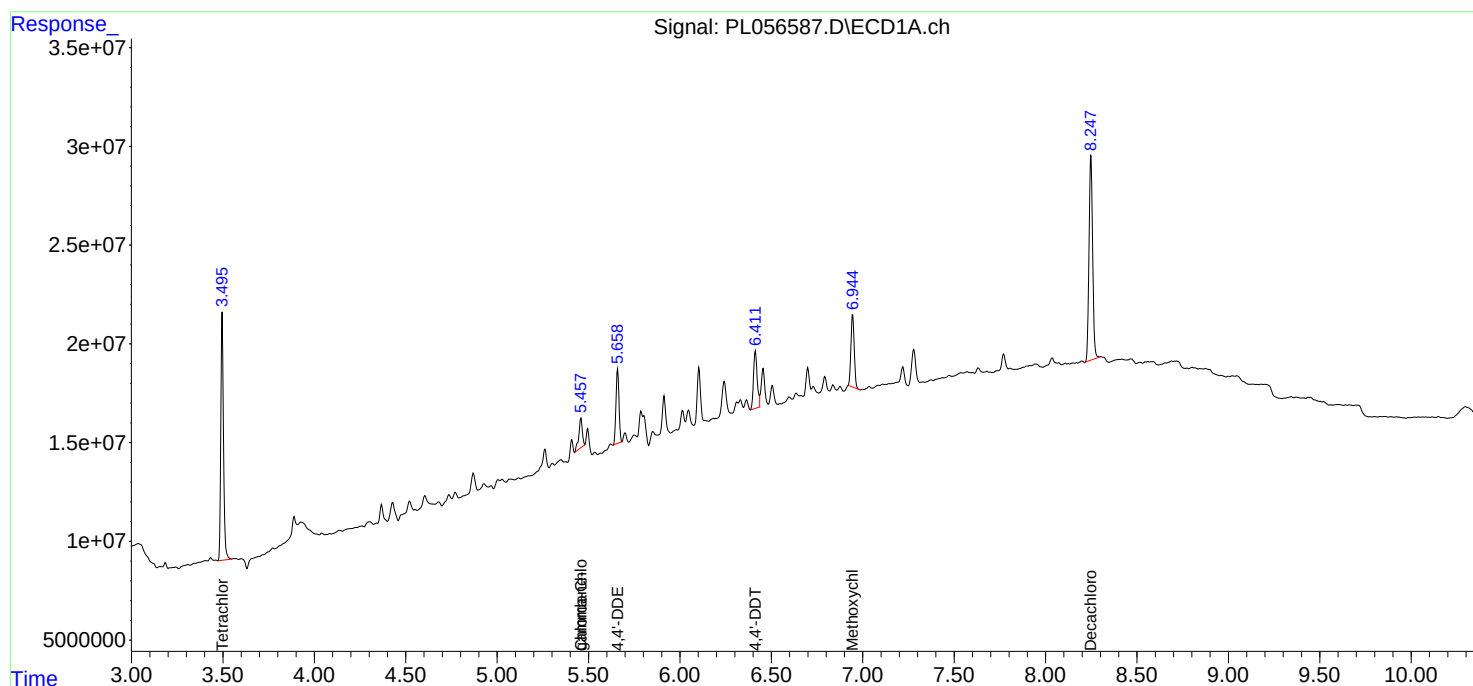


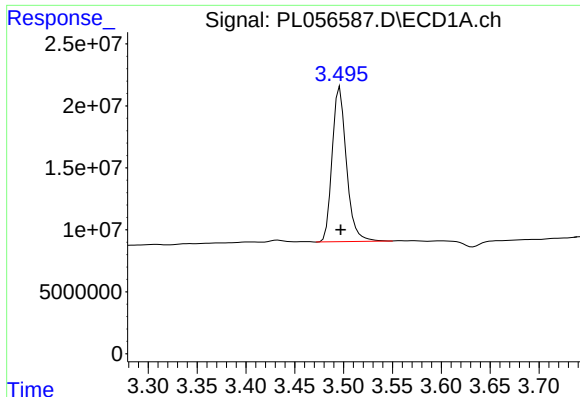

#1 Tetrachloro-m-xylene


R.T.: 3.496 min
Delta R.T.: 0.000 min
Response: 127109065
Conc: 14.41 ng/ml

Instrument :
ECD_L
ClientSampleId :

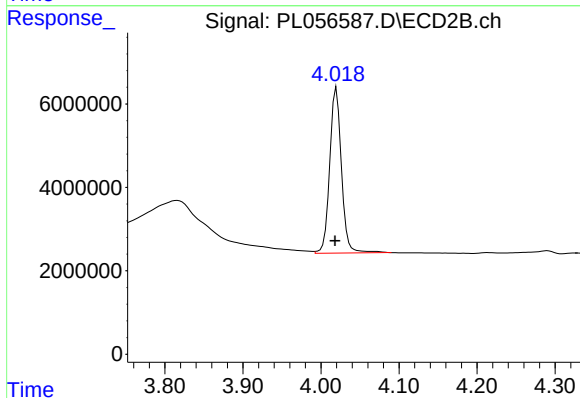


#1 Tetrachloro-m-xylene

R.T.: 4.020 min
Delta R.T.: 0.002 min
Response: 41475998
Conc: 15.25 ng/ml

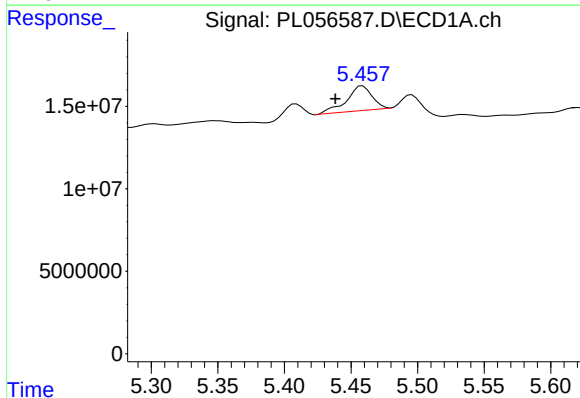


#10 gamma-Chlordane

R.T.: 5.459 min
Delta R.T.: 0.020 min
Response: 19742347
Conc: 1.44 ng/ml

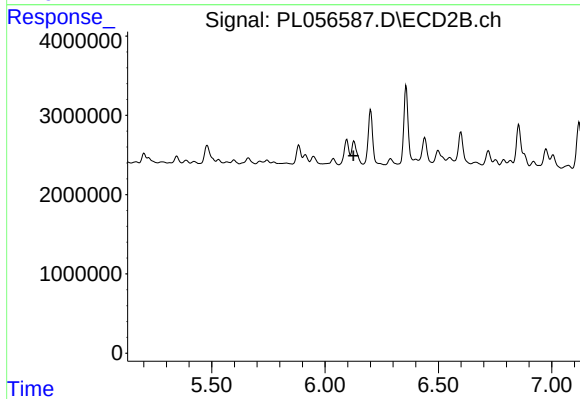

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 6.126 min
Response: 0
Conc: N.D.

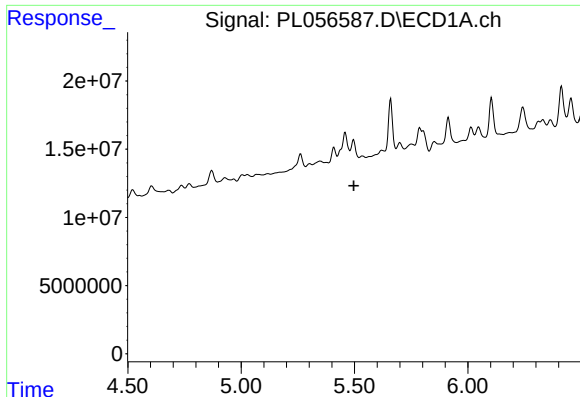

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.497 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

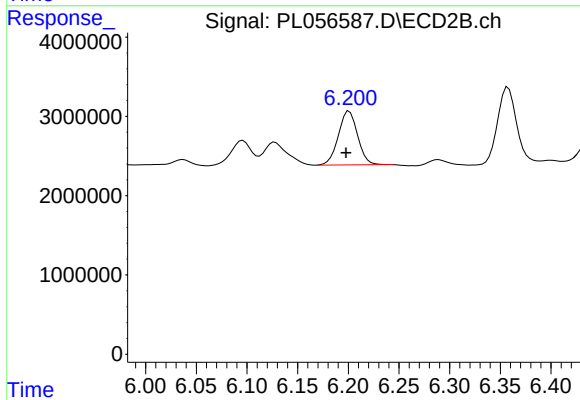


#11 alpha-Chlordane

R.T.: 6.201 min
Delta R.T.: 0.003 min
Response: 8946034
Conc: 3.05 ng/ml

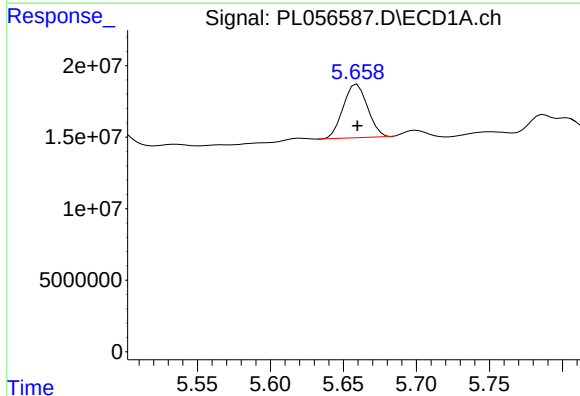


#12 4,4'-DDE

R.T.: 5.659 min
Delta R.T.: 0.000 min
Response: 43357572
Conc: 3.41 ng/ml

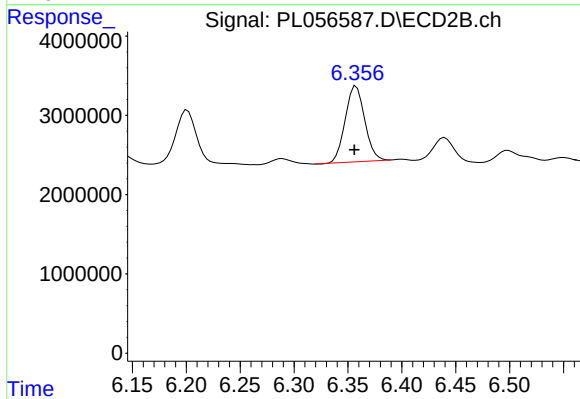

#12 4,4'-DDE


R.T.: 6.358 min
Delta R.T.: 0.002 min
Response: 12062217
Conc: 4.30 ng/ml

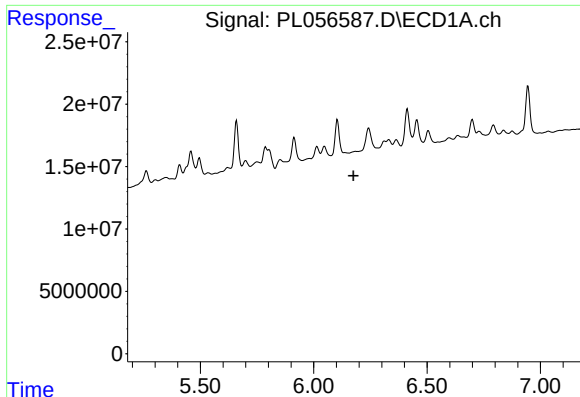

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 6.176 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

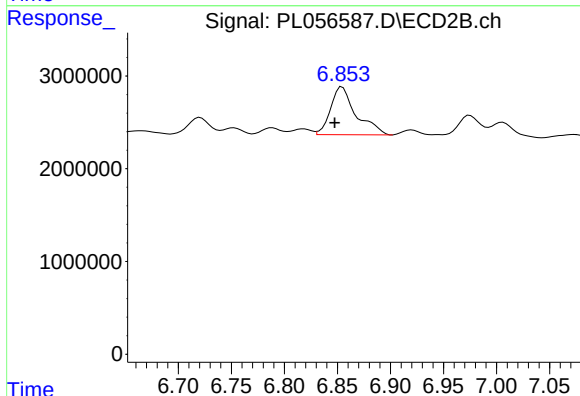


#16 4,4'-DDD

R.T.: 6.855 min
Delta R.T.: 0.007 min
Response: 8621496
Conc: 3.81 ng/ml

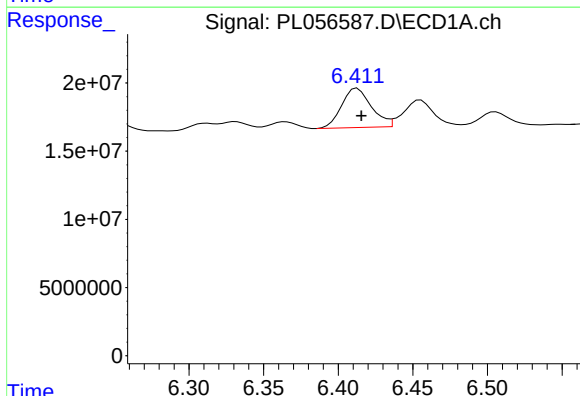


#17 4,4'-DDT

R.T.: 6.413 min
Delta R.T.: -0.003 min
Response: 40204286
Conc: 4.24 ng/ml

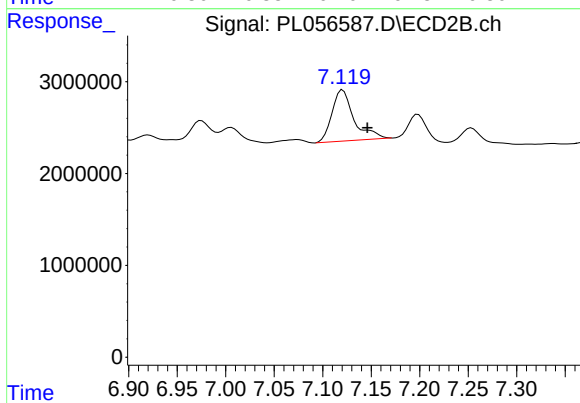

#17 4,4'-DDT


R.T.: 7.121 min
Delta R.T.: -0.025 min
Response: 8740540
Conc: 4.14 ng/ml

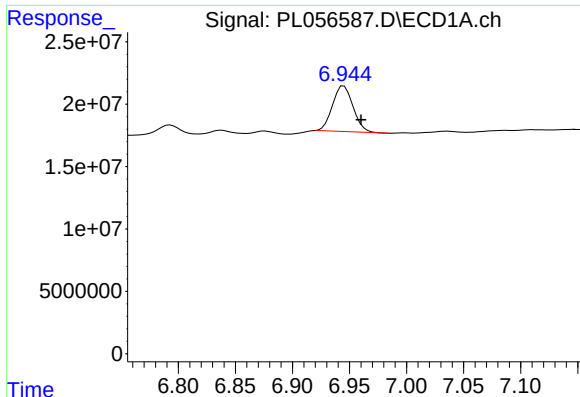

#20 Methoxychlor


R.T.: 6.945 min
Delta R.T.: -0.015 min
Response: 45928610
Conc: 9.33 ng/ml

Instrument :
ECD_L
ClientSampleId :

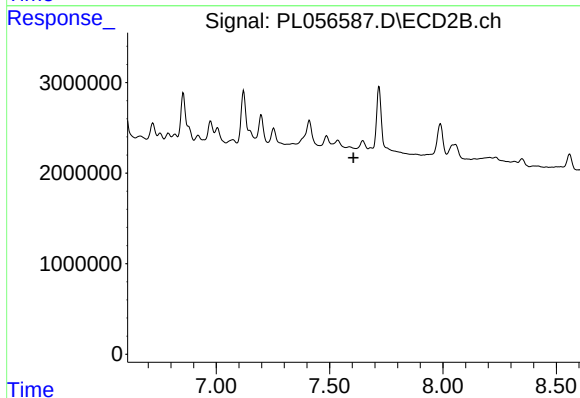


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 7.606 min
Response: 0
Conc: N.D.

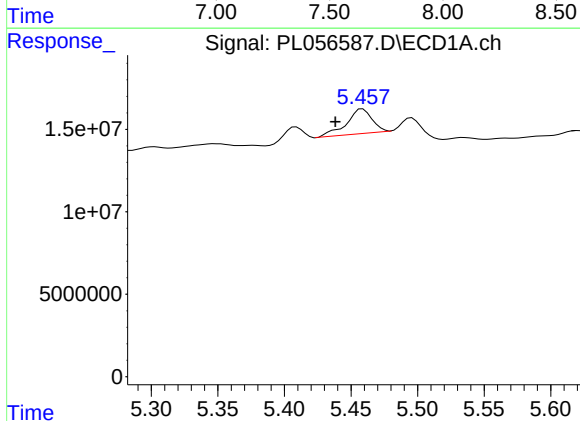


#25 Chlordane-3

R.T.: 5.459 min
Delta R.T.: 0.020 min
Response: 19742347
Conc: 15.04 ng/ml

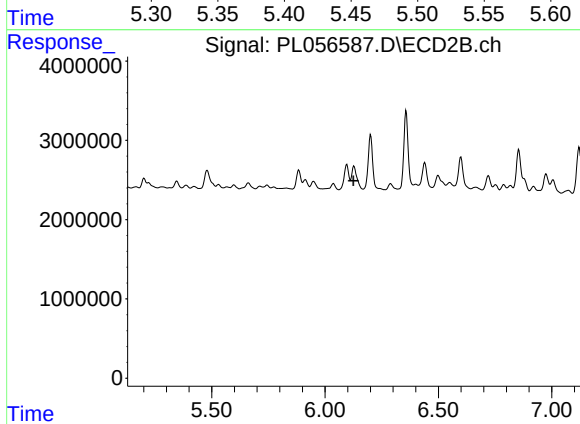

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T. : 6.126 min
Response: 0
Conc: N.D.

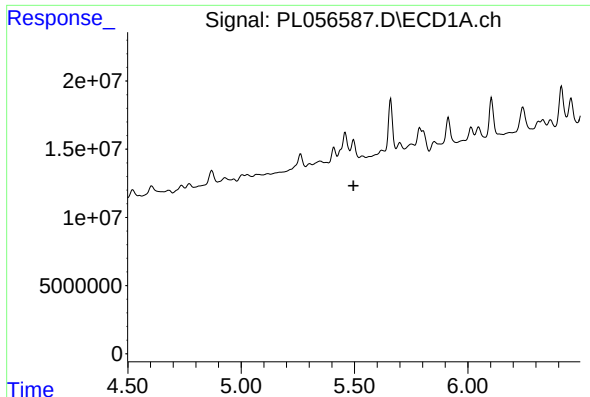

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 5.496 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

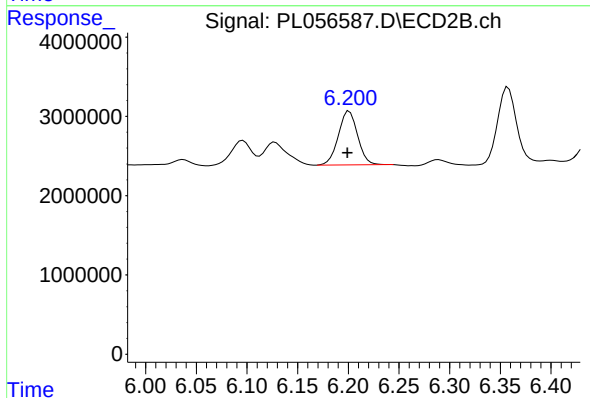


#26 Chlordane-4

R.T.: 6.201 min
Delta R.T.: 0.002 min
Response: 8946034
Conc: 19.66 ng/ml

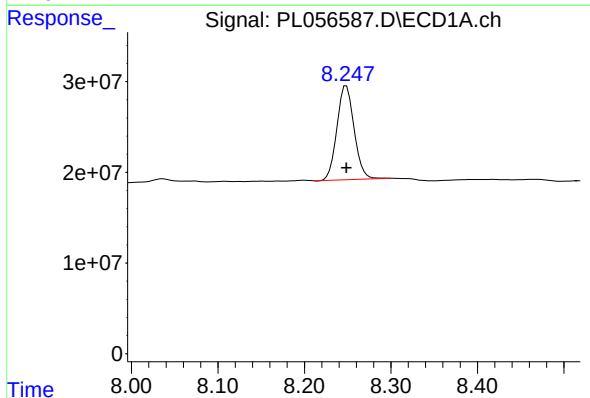

#28 Decachlorobiphenyl

R.T.: 8.249 min
Delta R.T.: 0.000 min
Response: 142867828
Conc: 14.91 ng/ml

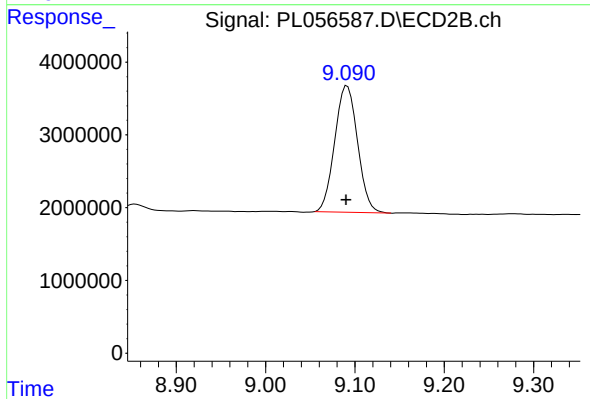

#28 Decachlorobiphenyl

R.T.: 9.091 min
Delta R.T.: 0.001 min
Response: 30873170
Conc: 15.14 ng/ml