

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL021720\
 Data File : PL056598.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Feb 2020 17:04
 Operator : AJ\MA
 Sample : L1548-01
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 18 01:02:52 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL021220.M
 Quant Title : GC Extractables
 QLast Update : Thu Feb 13 05:32:36 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.497	4.020	127.9E6	43042188	14.490	15.822
28)	SA Decachlor...	8.248	9.091	133.0E6	28715909	13.879	14.078
Target Compounds							
11)	B alpha-Chl...	0.000	6.201	0	6434675	N.D.	2.191 #
26)	Chlordane-4	0.000	6.201	0	6434675	N.D.	14.139 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL021720\
Data File : PL056598.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Feb 2020 17:04
Operator : AJ\MA
Sample : L1548-01
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 18 01:02:52 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL021220.M
Quant Title : GC Extractables
QLast Update : Thu Feb 13 05:32:36 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

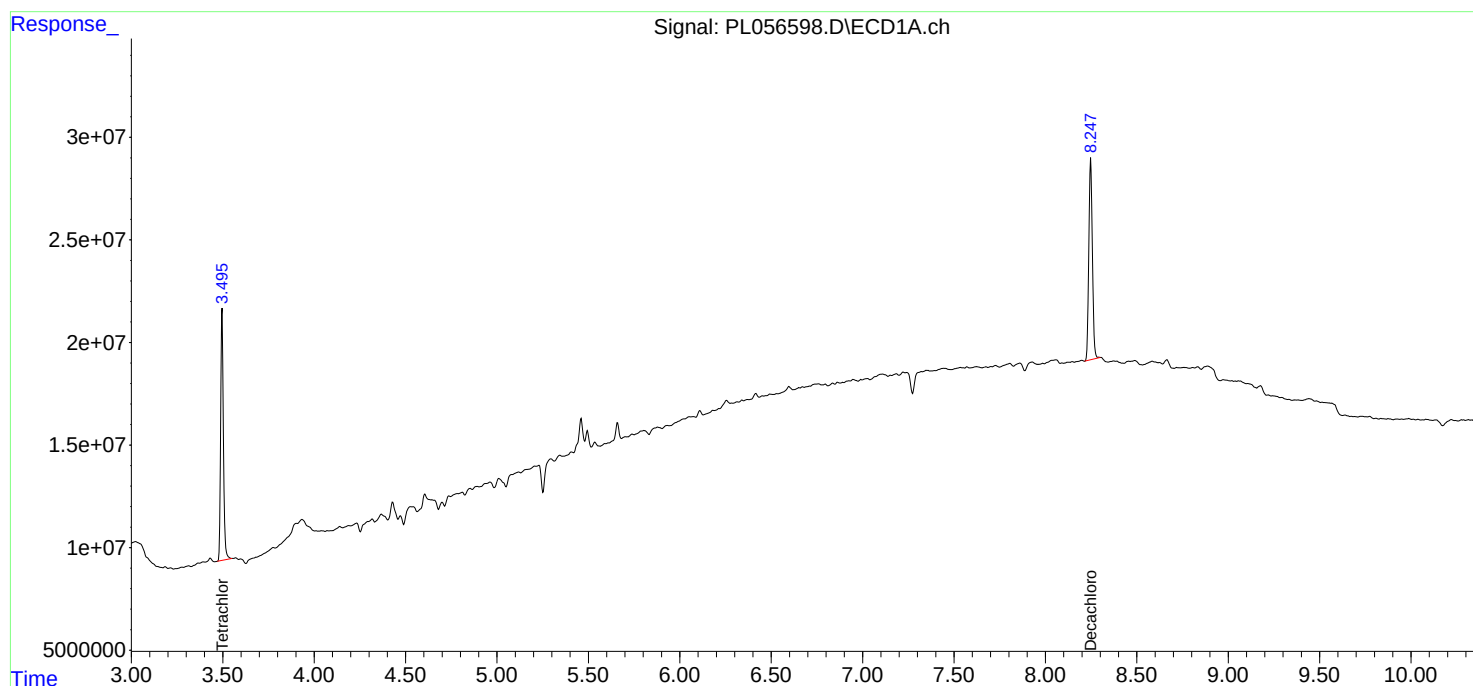


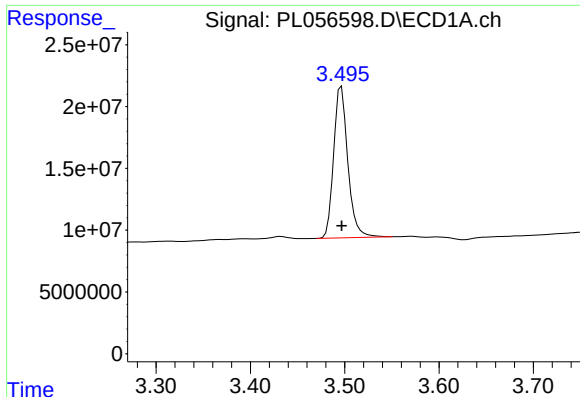

#1 Tetrachloro-m-xylene


R.T.: 3.497 min
Delta R.T.: 0.000 min
Response: 127850648
Conc: 14.49 ng/ml

Instrument :
ECD_L
ClientSampleId :

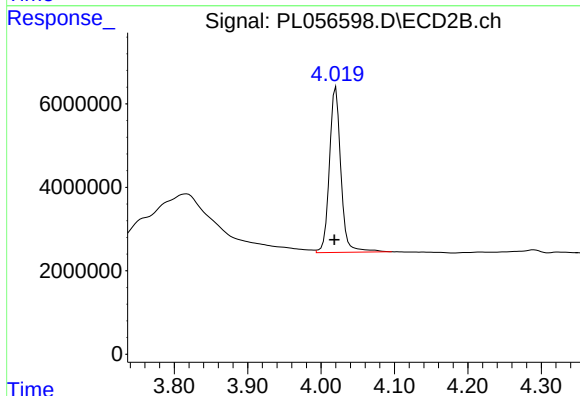


#1 Tetrachloro-m-xylene

R.T.: 4.020 min
Delta R.T.: 0.002 min
Response: 43042188
Conc: 15.82 ng/ml

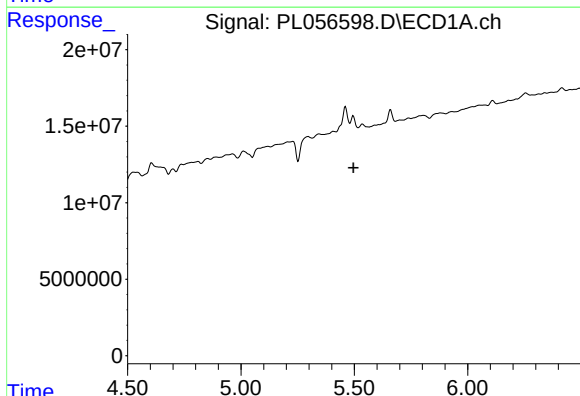


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.497 min
Response: 0
Conc: N.D.

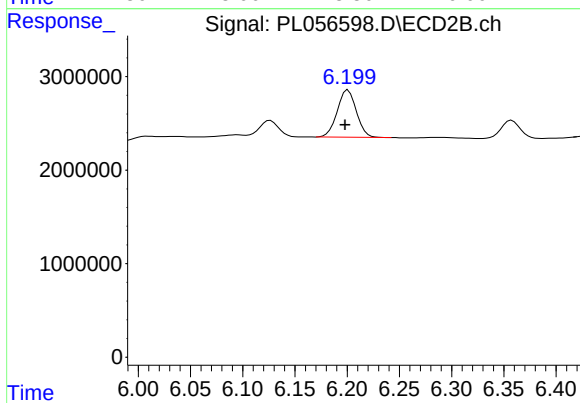

#11 alpha-Chlordane


R.T.: 6.201 min
Delta R.T.: 0.003 min
Response: 6434675
Conc: 2.19 ng/ml

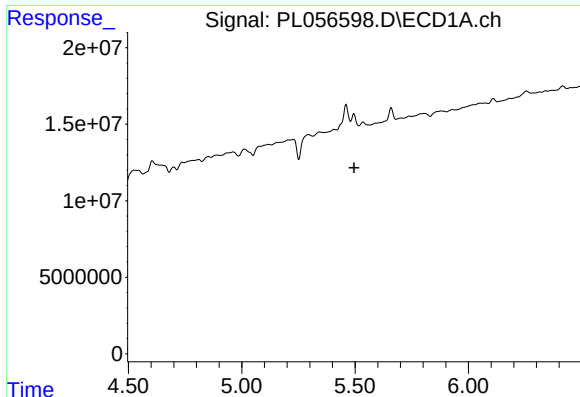

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 5.496 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

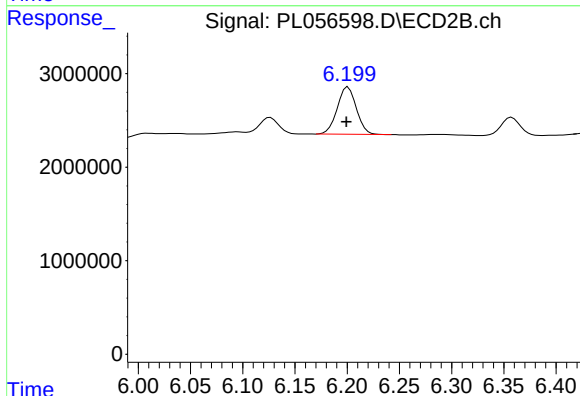


#26 Chlordane-4

R.T.: 6.201 min
Delta R.T.: 0.002 min
Response: 6434675
Conc: 14.14 ng/ml

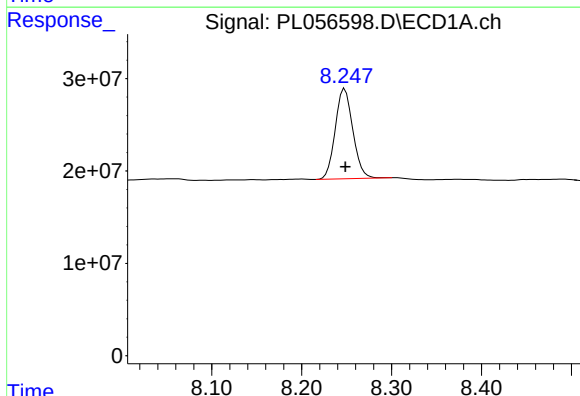

#28 Decachlorobiphenyl

R.T.: 8.248 min
Delta R.T.: 0.000 min
Response: 132951890
Conc: 13.88 ng/ml

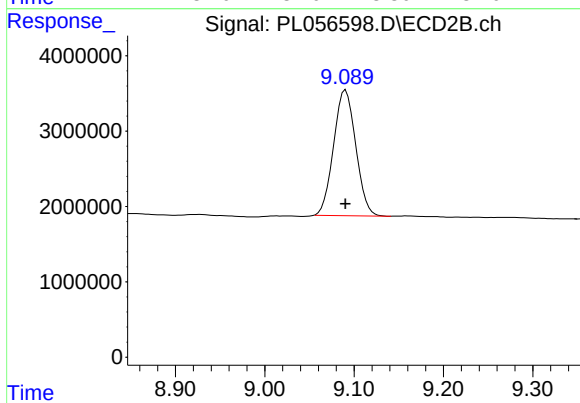

#28 Decachlorobiphenyl

R.T.: 9.091 min
Delta R.T.: 0.000 min
Response: 28715909
Conc: 14.08 ng/ml