

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL021723\
 Data File : PL081003.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Feb 2023 15:13
 Operator : AR\AJ
 Sample : 01576-01
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 RE137-BAGFILTER-20220215

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 02/20/2023
 Supervised By : Ankita Jodhani 02/20/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 17 22:10:48 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012023.M
 Quant Title : GC Extractables
 QLast Update : Sun Jan 22 23:56:48 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.359	2.686	32388271	30252914	15.101m	13.774
2) SA Decachlor...	8.800	7.835	26002707	31703923	14.852	13.307

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL021723\
Data File : PL081003.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Feb 2023 15:13
Operator : AR\AJ
Sample : 01576-01
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
RE137-BAGFILTER-20220215


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 02/20/2023
Supervised By : Ankita Jodhani 02/20/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 17 22:10:48 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012023.M
Quant Title : GC Extractables
QLast Update : Sun Jan 22 23:56:48 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

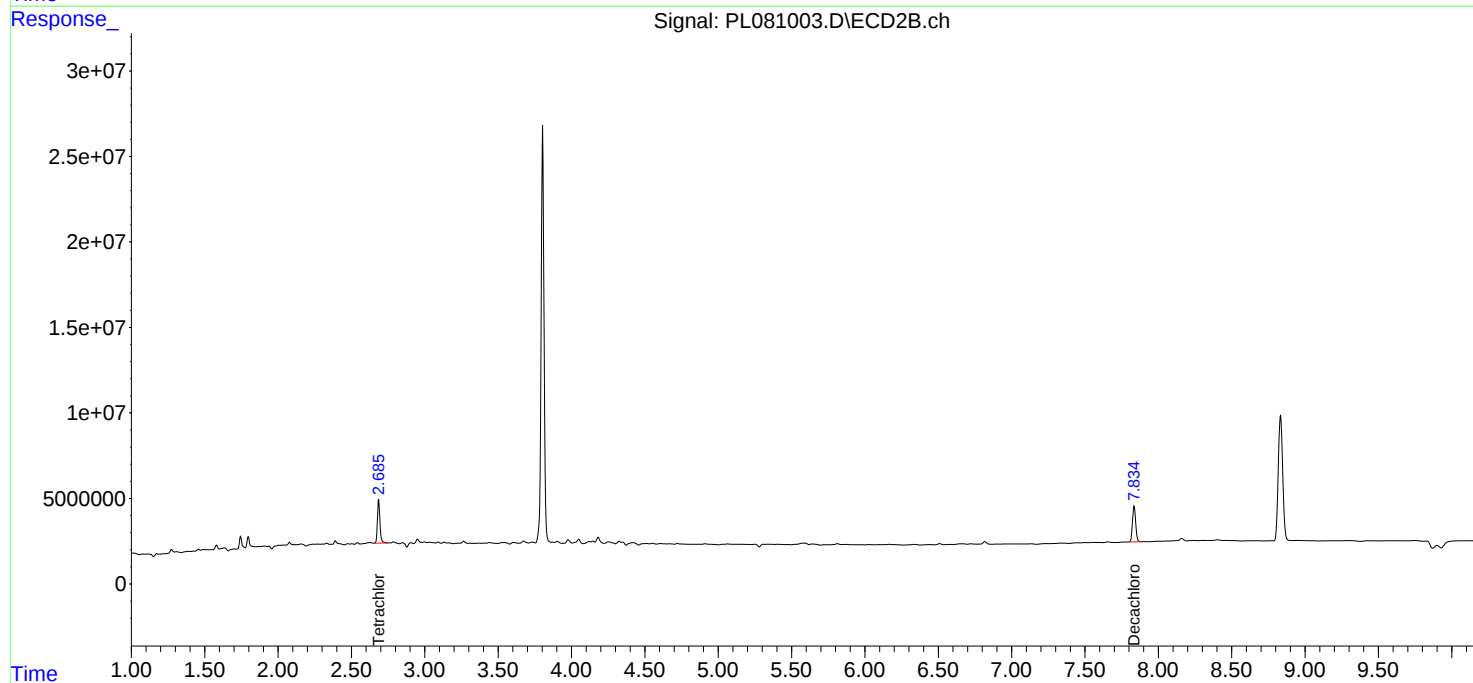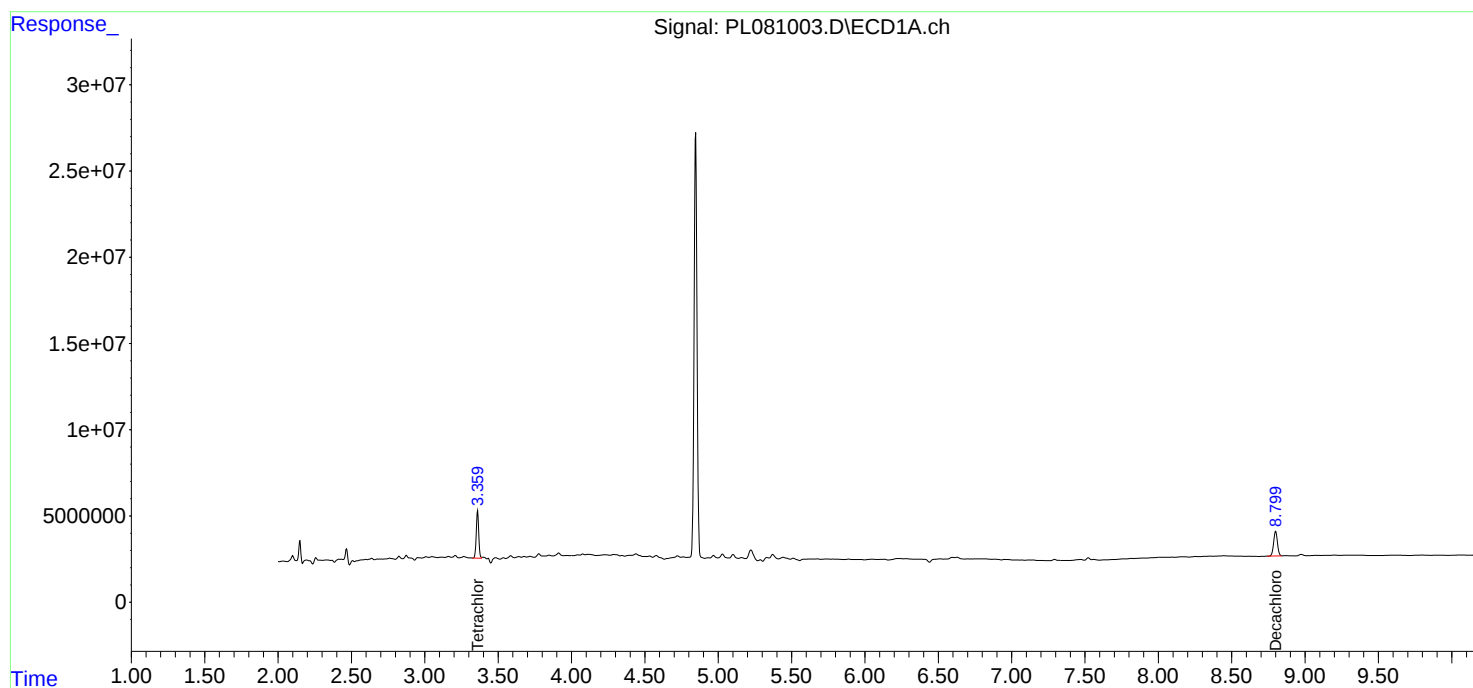

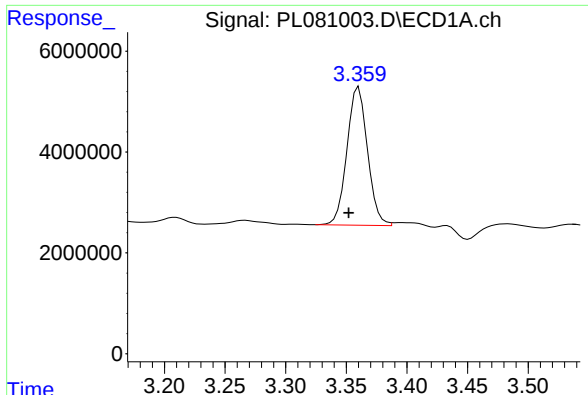


#1 Tetrachloro-m-xylene

R.T.: 3.359 min
Delta R.T.: 0.007 min
Response: 32388271
Conc: 15.10 ng/ml

Instrument :
ECD_L
ClientSampleId :
RE137-BAGFILTER-20220215


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 02/20/2023
Supervised By :Ankita Jodhani 02/20/2023

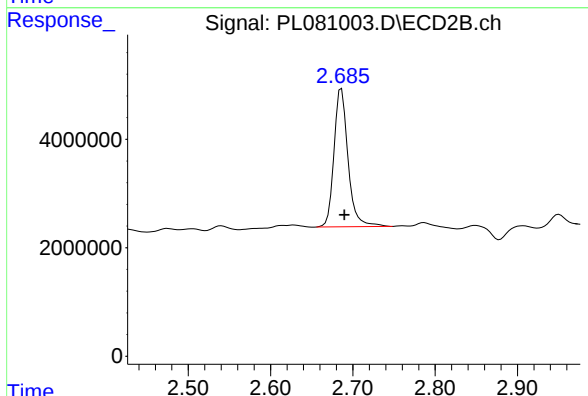


#1 Tetrachloro-m-xylene

R.T.: 2.686 min
Delta R.T.: -0.004 min
Response: 30252914
Conc: 13.77 ng/ml

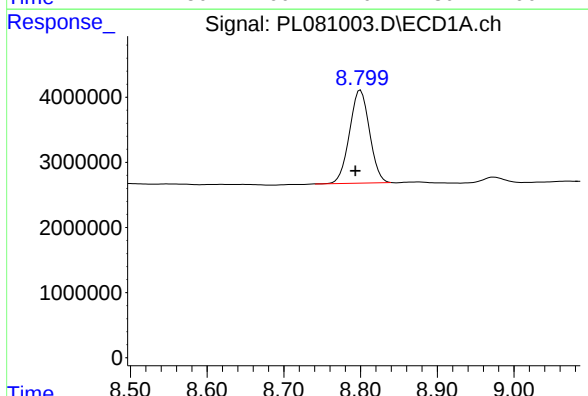

#28 Decachlorobiphenyl

R.T.: 8.800 min
Delta R.T.: 0.007 min
Response: 26002707
Conc: 14.85 ng/ml

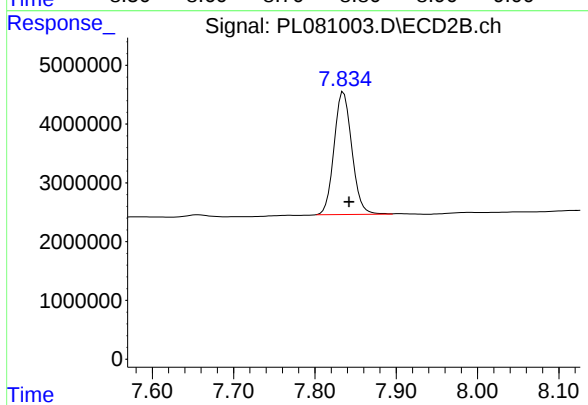

#28 Decachlorobiphenyl

R.T.: 7.835 min
Delta R.T.: -0.007 min
Response: 31703923
Conc: 13.31 ng/ml