

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL021723\
 Data File : PL081010.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Feb 2023 17:31
 Operator : AR\AJ
 Sample : 01582-01
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 LEONIA-TRENCH-LINE

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 02/20/2023
 Supervised By :Ankita Jodhani 02/20/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 17 22:14:24 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012023.M
 Quant Title : GC Extractables
 QLast Update : Sun Jan 22 23:56:48 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.358	2.685	41882064	42170656	19.527m	19.199
28)	SA Decachlor...	8.800	7.835	28030253	35138304	16.010	14.748

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL021723\
Data File : PL081010.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Feb 2023 17:31
Operator : AR\AJ
Sample : 01582-01
Misc :
ALS Vial : 12 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
LEONIA-TRENCH-LINE


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 02/20/2023
Supervised By : Ankita Jodhani 02/20/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 17 22:14:24 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012023.M
Quant Title : GC Extractables
QLast Update : Sun Jan 22 23:56:48 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

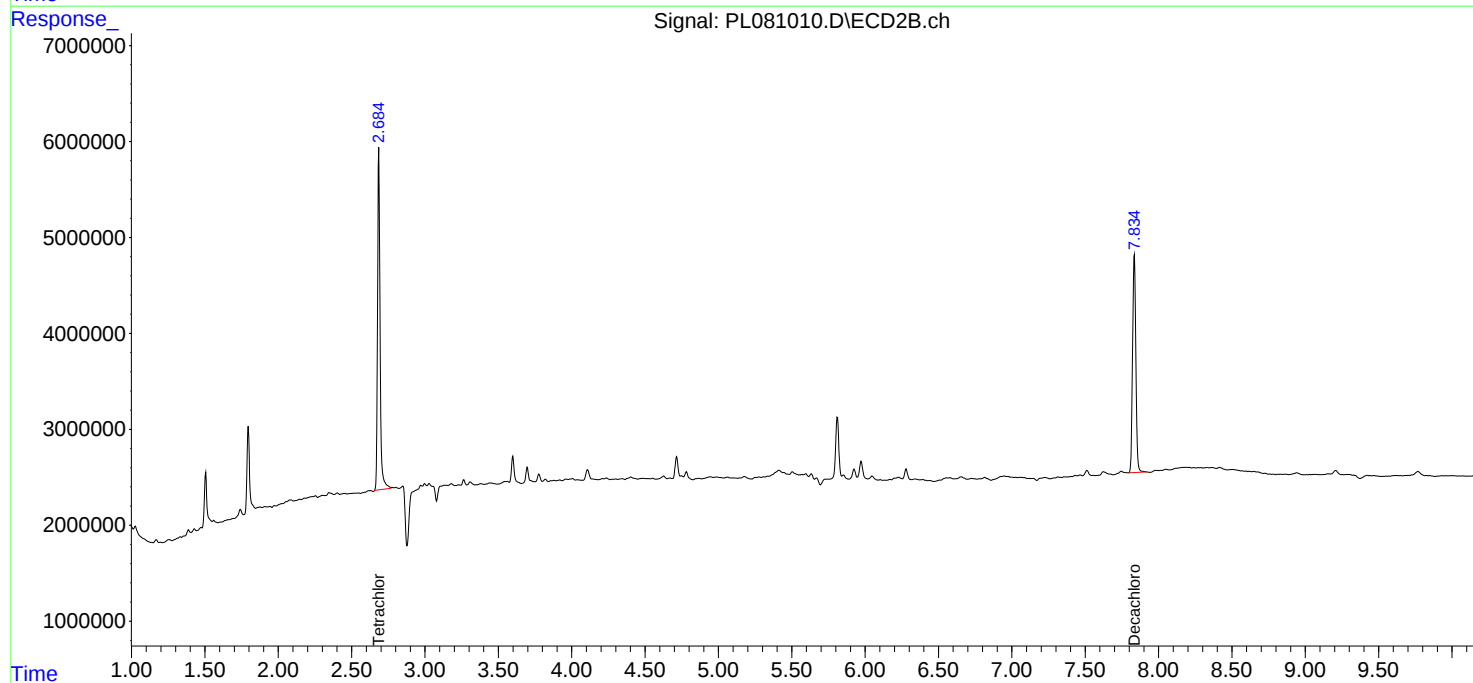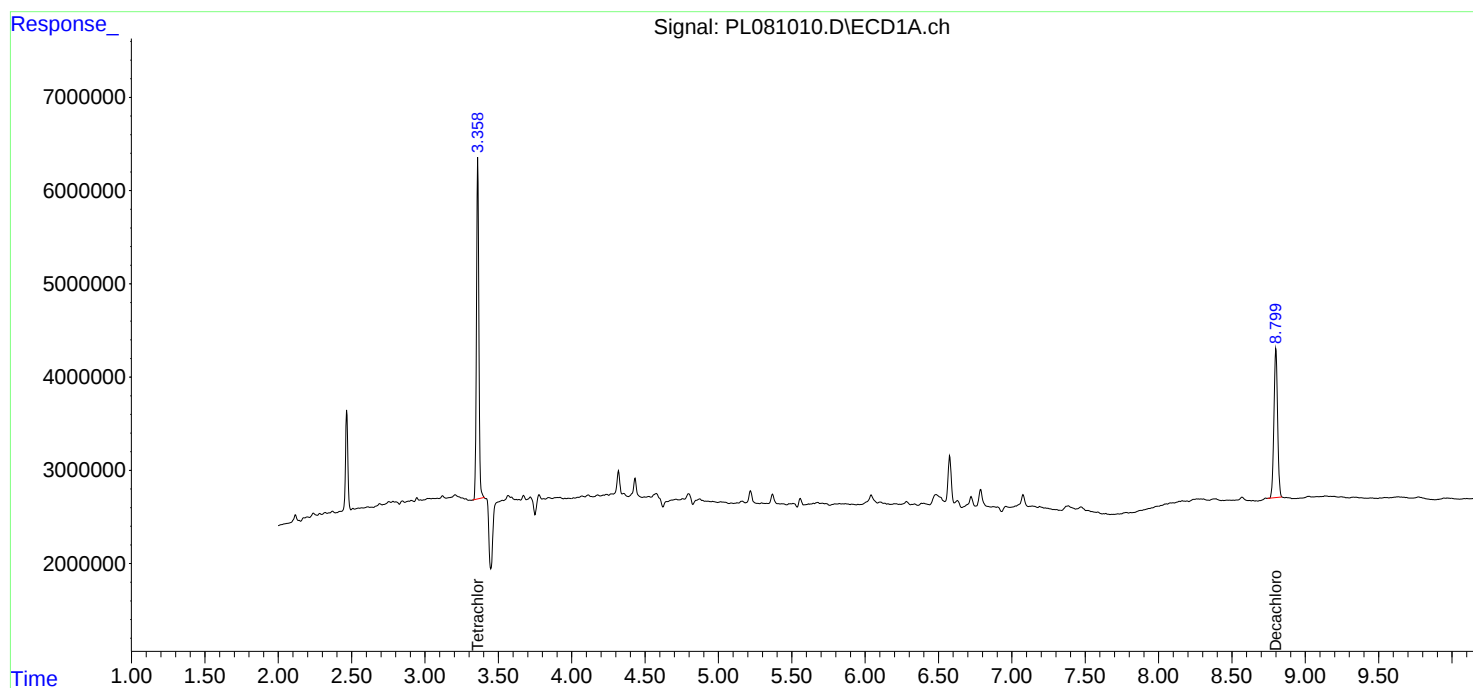

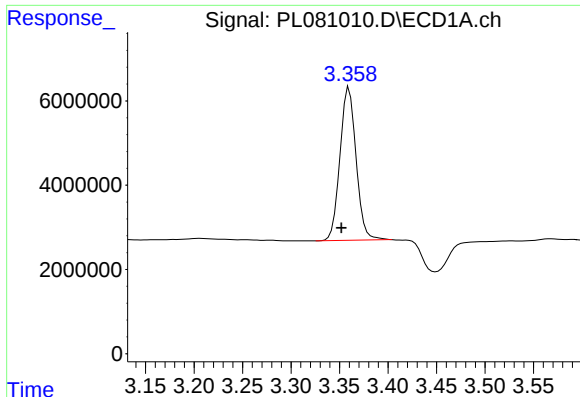


#1 Tetrachloro-m-xylene

R.T.: 3.358 min
Delta R.T.: 0.006 min
Response: 41882064
Conc: 19.53 ng/ml

Instrument :
ECD_L
ClientSampleId :
LEONIA-TRENCH-LINE


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 02/20/2023
Supervised By :Ankita Jodhani 02/20/2023

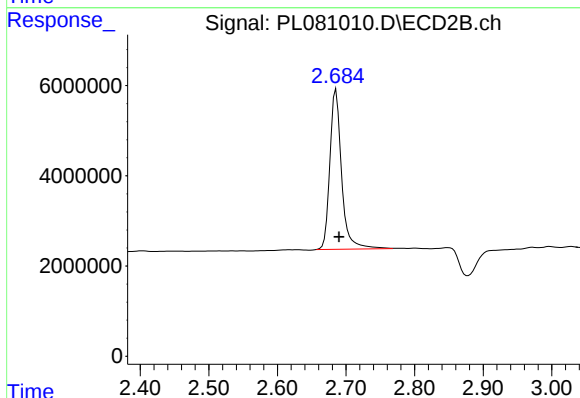


#1 Tetrachloro-m-xylene

R.T.: 2.685 min
Delta R.T.: -0.004 min
Response: 42170656
Conc: 19.20 ng/ml

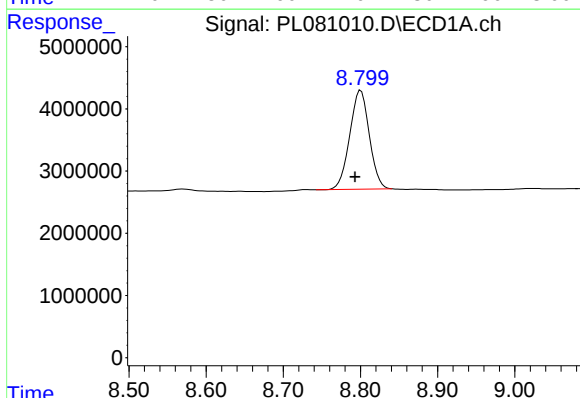

#28 Decachlorobiphenyl

R.T.: 8.800 min
Delta R.T.: 0.007 min
Response: 28030253
Conc: 16.01 ng/ml

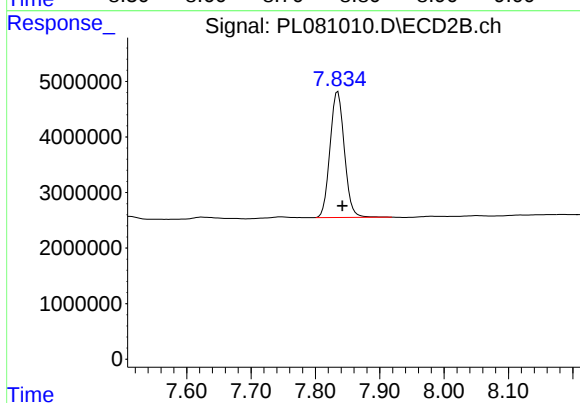

#28 Decachlorobiphenyl

R.T.: 7.835 min
Delta R.T.: -0.007 min
Response: 35138304
Conc: 14.75 ng/ml