

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL021920\
 Data File : PL056655.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Feb 2020 15:36
 Operator : AJ\MA
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 19 18:24:28 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL021920.M
 Quant Title : GC Extractables
 QLast Update : Wed Feb 19 18:03:26 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds

6) B	beta-BHC	0.000	4.878	0	8319276	N.D.	6.363	#
8) B	Heptachlo...	0.000	5.893	0	49458318	N.D.	16.916	#
9) A	Endosulfan I	5.555	0.000	183.4E6	0	13.720	N.D.	#
12) B	4,4'-DDE	5.686f	0.000	196.6E6	0	13.976	N.D.	#
13) MA	Dieldrin	5.785	0.000	213.6E6	0	14.333	N.D.	#
14) MA	Endrin	6.061	6.719	120.9E6	19077450	8.960	7.744	
15) B	Endosulfa...	6.303f	0.000	185.7E6	0	14.949	N.D.	#
18) B	Endrin al...	6.466f	0.000	81590865	0	7.538	N.D.	#
23)	Chlordane-1	4.351f	0.000	19116283	0	52.475	N.D.	#
27)	Chlordane-5	6.359f	0.000	321.2E6	0	981.024	N.D.	#



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL021920\
Data File : PL056655.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Feb 2020 15:36
Operator : AJ\MA
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 19 18:24:28 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL021920.M
Quant Title : GC Extractables
QLast Update : Wed Feb 19 18:03:26 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

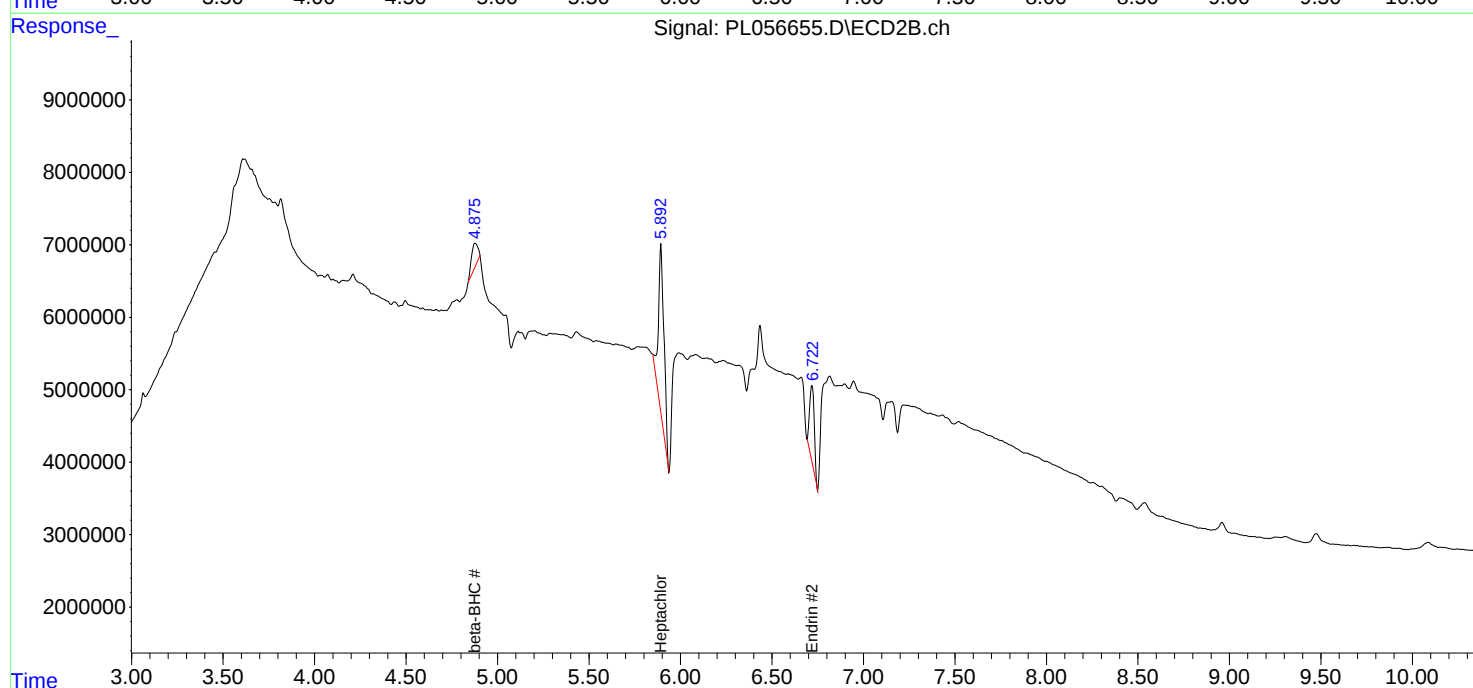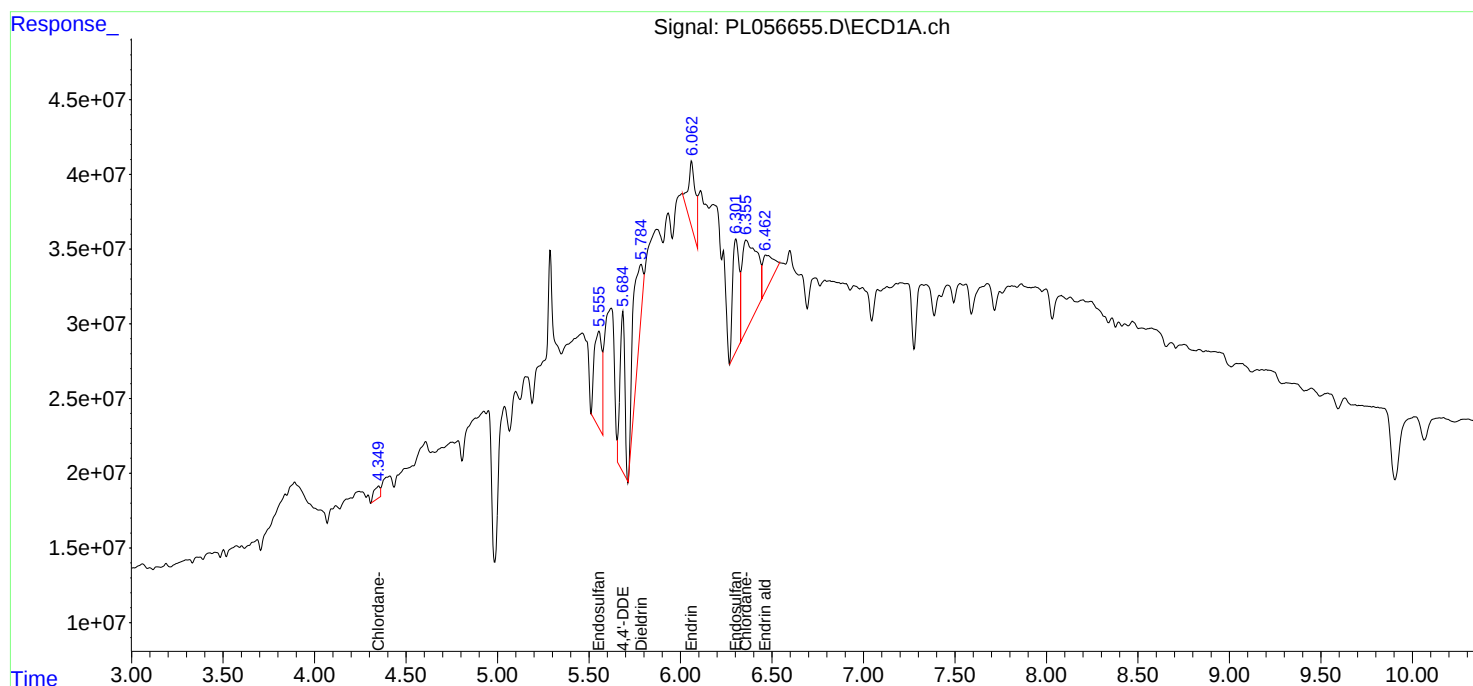


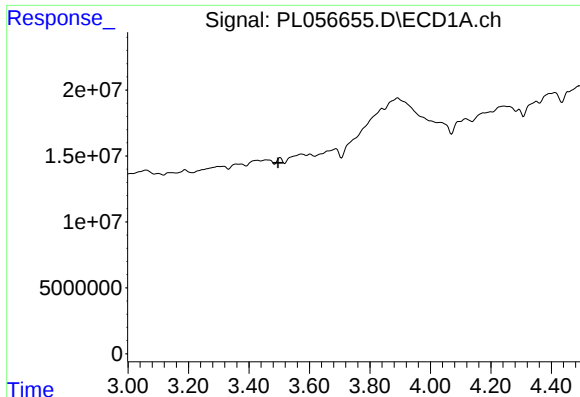

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 3.496 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

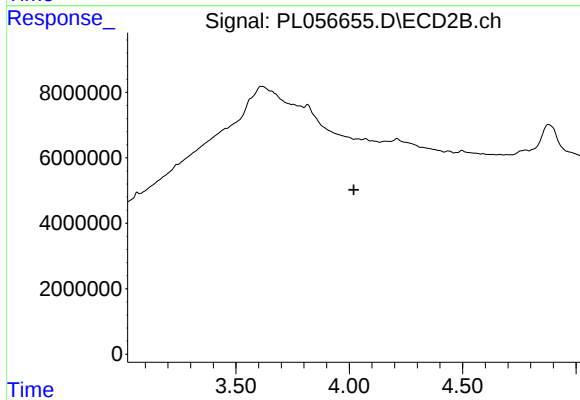


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 4.020 min
Response: 0
Conc: N.D.

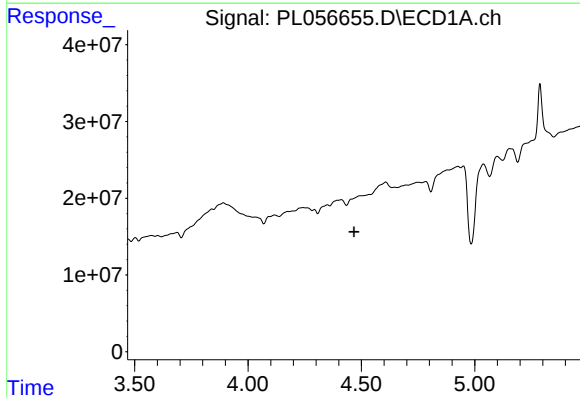


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.468 min
Response: 0
Conc: N.D.

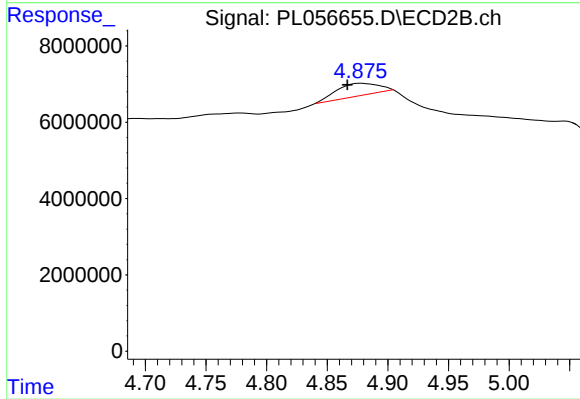

#6 beta-BHC


R.T.: 4.878 min
Delta R.T.: 0.011 min
Response: 8319276
Conc: 6.36 ng/ml

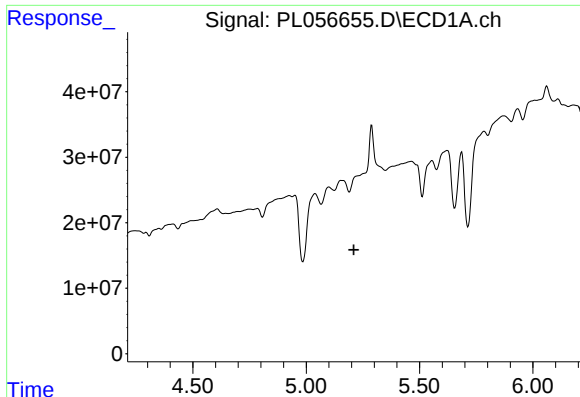

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.210 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

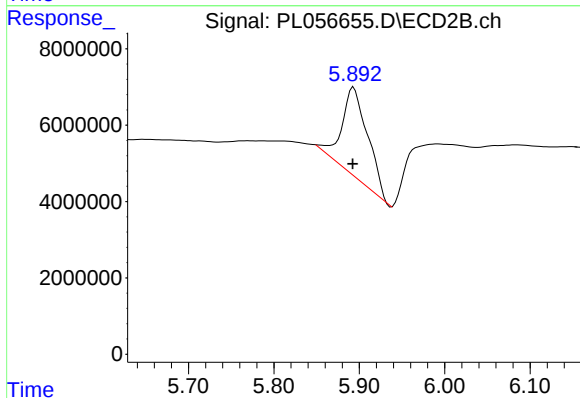


#8 Heptachlor epoxide

R.T.: 5.893 min
Delta R.T.: 0.001 min
Response: 49458318
Conc: 16.92 ng/ml

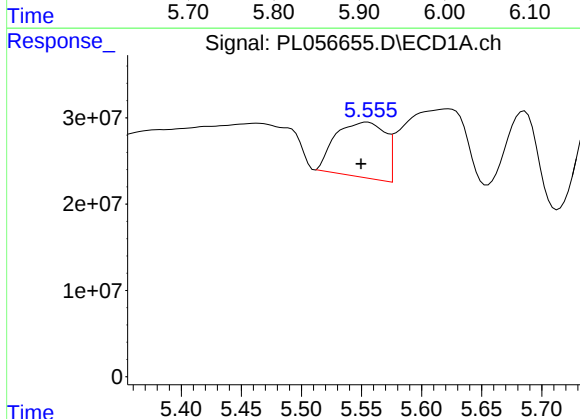


#9 Endosulfan I

R.T.: 5.555 min
Delta R.T.: 0.006 min
Response: 183407744
Conc: 13.72 ng/ml

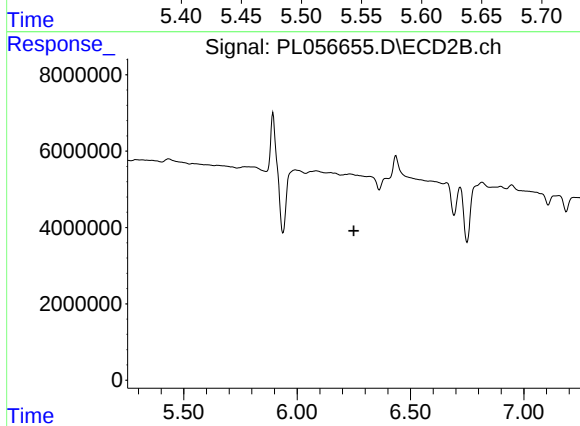

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 6.250 min
Response: 0
Conc: N.D.

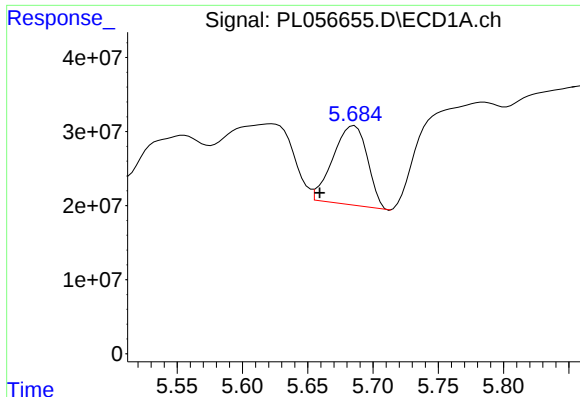

#12 4,4'-DDE


R.T.: 5.686 min
Delta R.T.: 0.027 min
Response: 196581758
Conc: 13.98 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

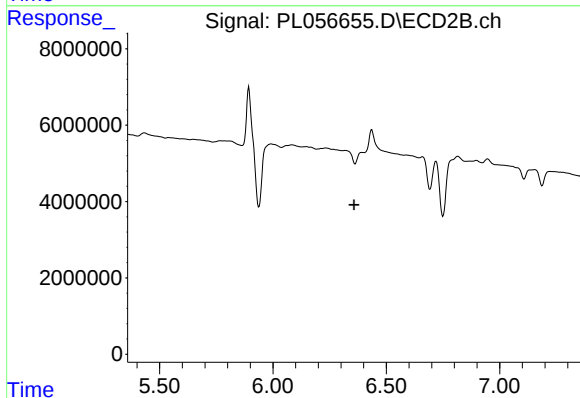


#12 4,4'-DDE

R.T.: 0.000 min
Exp R.T. : 6.358 min
Response: 0
Conc: N.D.

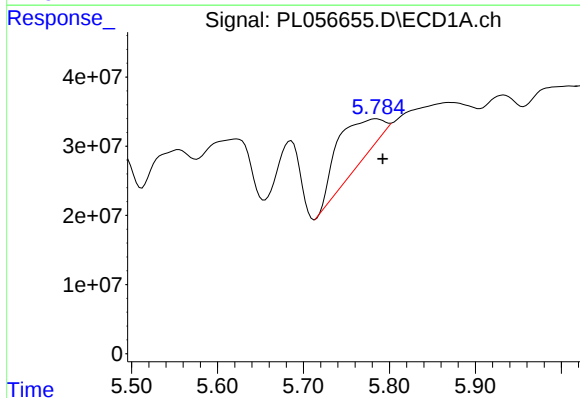


#13 Dieldrin

R.T.: 5.785 min
Delta R.T.: -0.007 min
Response: 213642591
Conc: 14.33 ng/ml

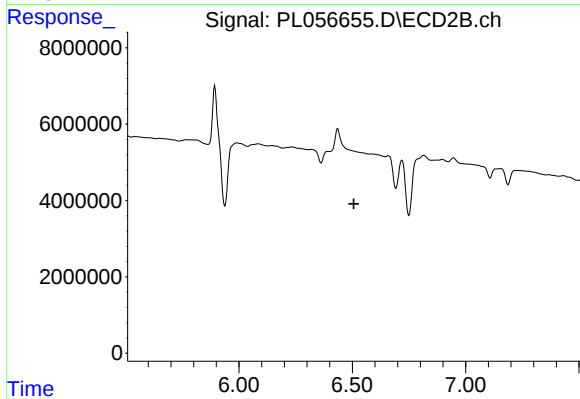

#13 Dieldrin


R.T.: 0.000 min
Exp R.T. : 6.506 min
Response: 0
Conc: N.D.

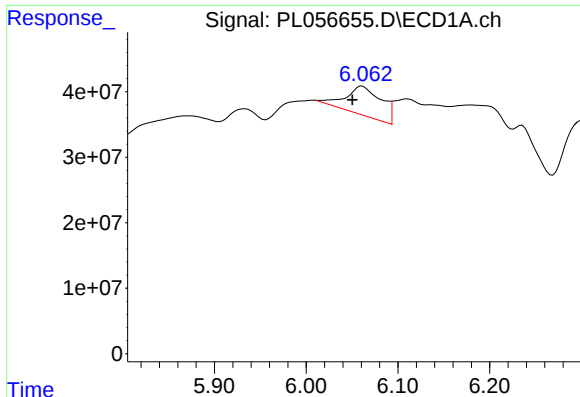

#14 Endrin


R.T.: 6.061 min
Delta R.T.: 0.011 min
Response: 120935518
Conc: 8.96 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

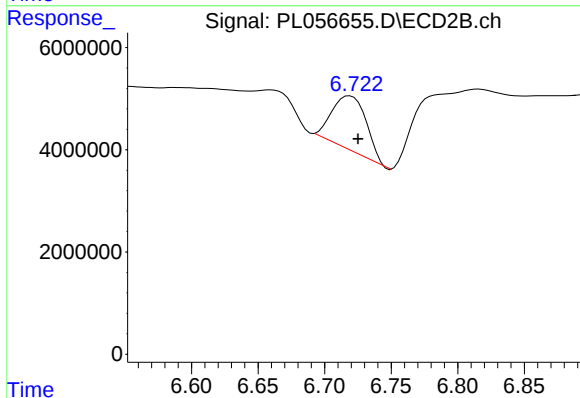


#14 Endrin

R.T.: 6.719 min
Delta R.T.: -0.006 min
Response: 19077450
Conc: 7.74 ng/ml

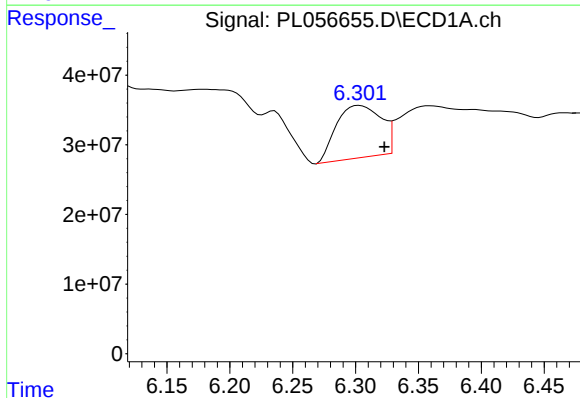


#15 Endosulfan II

R.T.: 6.303 min
Delta R.T.: -0.020 min
Response: 185654639
Conc: 14.95 ng/ml

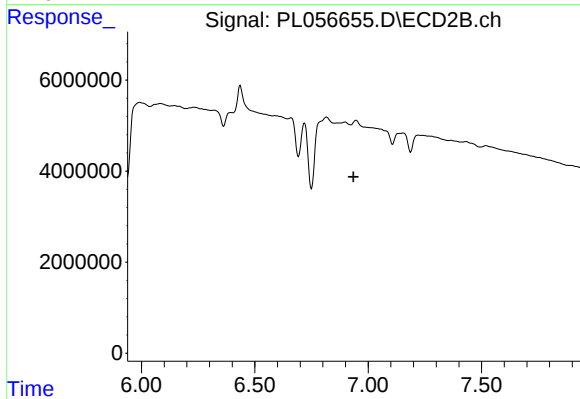

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.936 min
Response: 0
Conc: N.D.

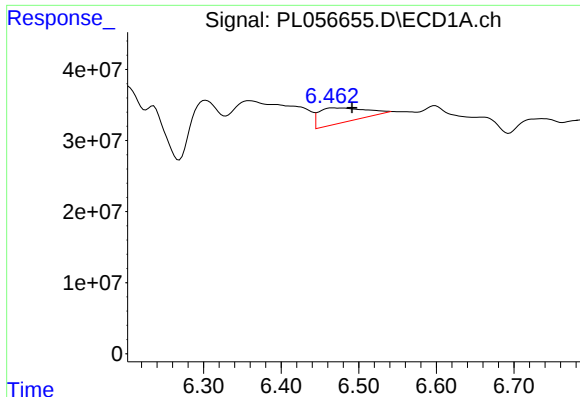

#18 Endrin aldehyde


R.T.: 6.466 min
Delta R.T.: -0.025 min
Response: 81590865
Conc: 7.54 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

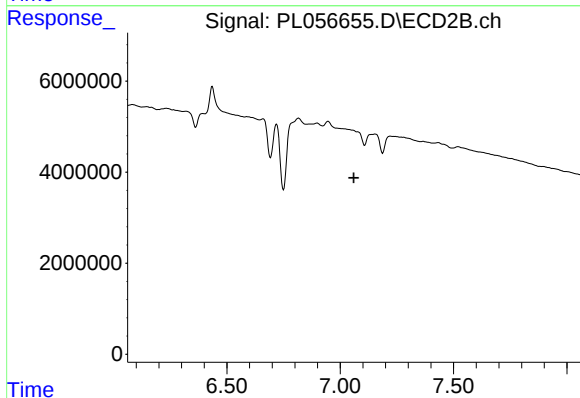


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T.: 7.060 min
Response: 0
Conc: N.D.

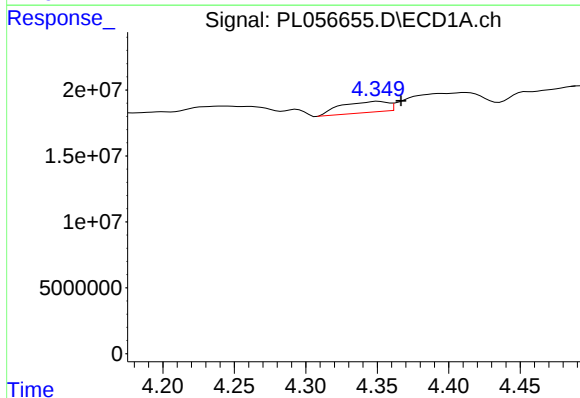


#23 Chlordane-1

R.T.: 4.351 min
Delta R.T.: -0.016 min
Response: 19116283
Conc: 52.47 ng/ml

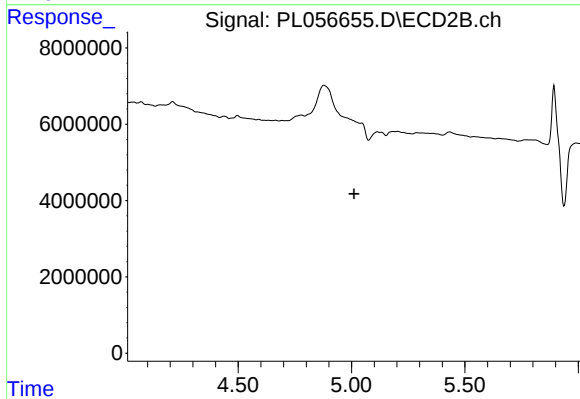

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 5.012 min
Response: 0
Conc: N.D.

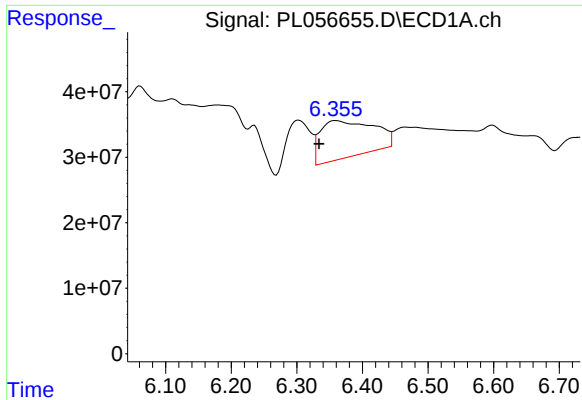

#27 Chlordane-5


R.T.: 6.359 min
Delta R.T.: 0.026 min
Response: 321223585
Conc: 981.02 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

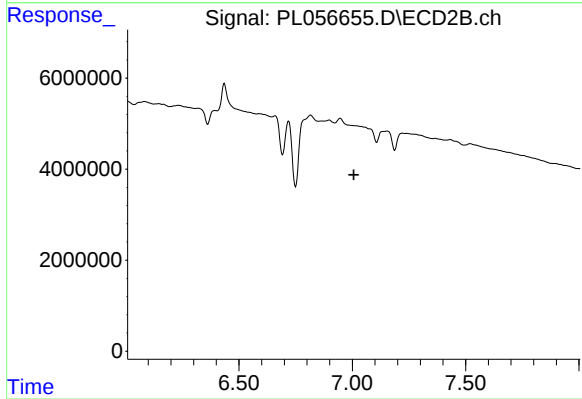


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 7.007 min
Response: 0
Conc: N.D.

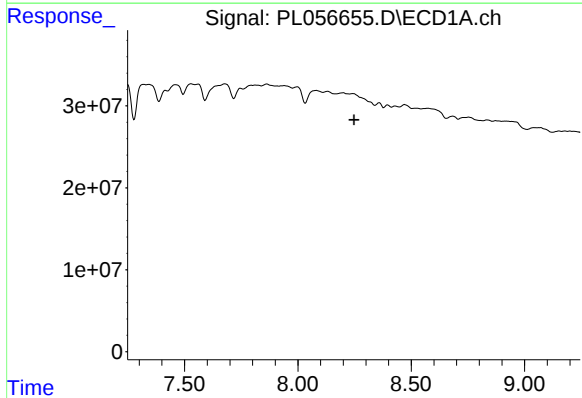

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 8.248 min
Response: 0
Conc: N.D.

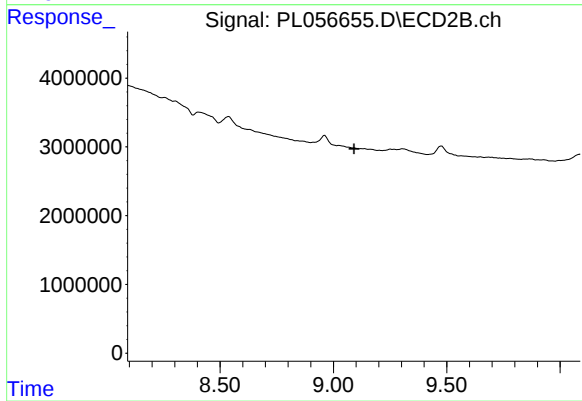

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 9.091 min
Response: 0
Conc: N.D.