

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL021920\
 Data File : PL056664.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Feb 2020 17:43
 Operator : AJ\MA
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 19 18:01:05 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL021920.M
 Quant Title : GC Extractables
 QLast Update : Wed Feb 19 18:00:50 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.496	4.020	498.8E6	130.0E6	50.000	50.000
28)	SA Decachlor...	8.249	9.091	610.1E6	106.8E6	50.000	50.000
Target Compounds							
23)	Chlordane-1	4.367	5.012	182.1E6	45211398	500.000	500.000
24)	Chlordane-2	4.868	5.480	195.0E6	49341140	500.000	500.000
25)	Chlordane-3	5.438	6.126	628.9E6	184.7E6	500.000	500.000
26)	Chlordane-4	5.495	6.200	537.1E6	214.6E6	500.000	500.000
27)	Chlordane-5	6.334	7.007	163.7E6	38505306	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL021920\
Data File : PL056664.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Feb 2020 17:43
Operator : AJ\MA
Sample : PCHLORICC500
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 19 18:01:05 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL021920.M
Quant Title : GC Extractables
QLast Update : Wed Feb 19 18:00:50 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

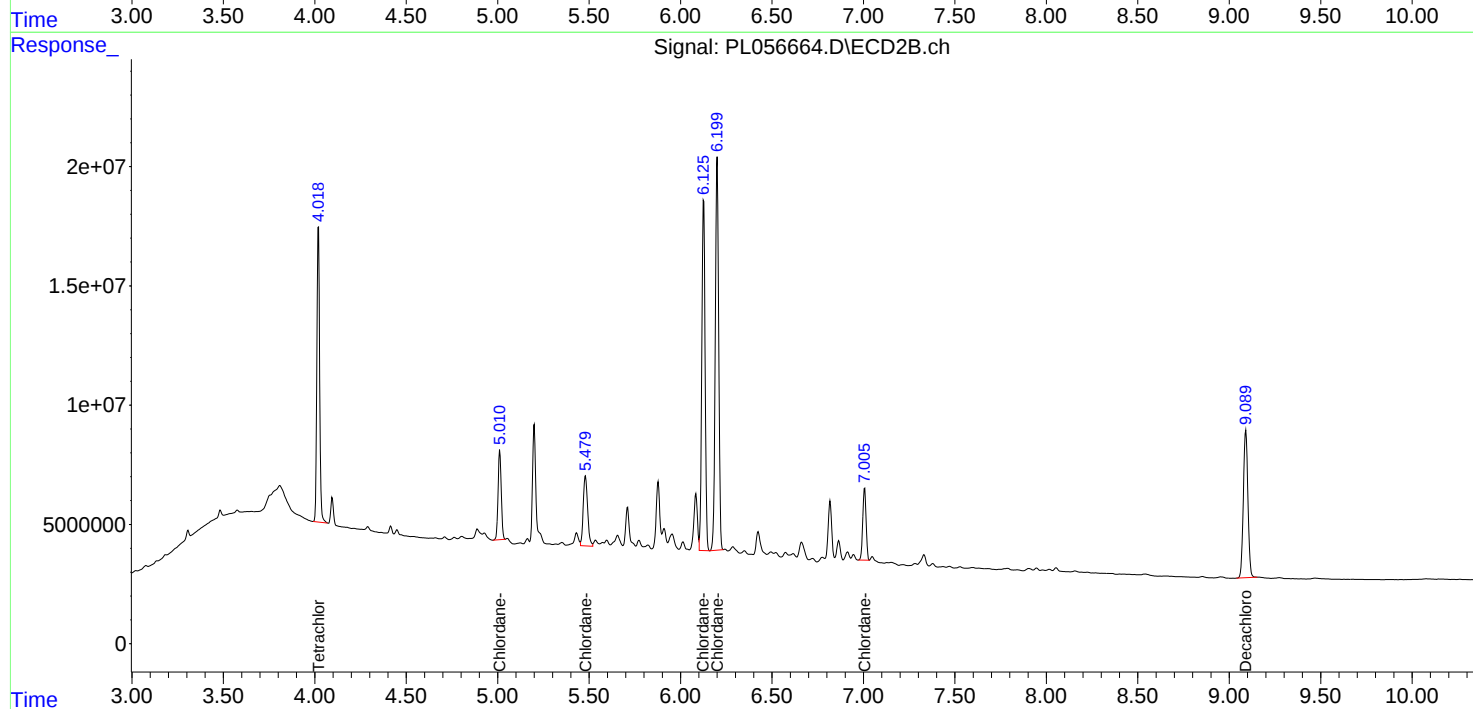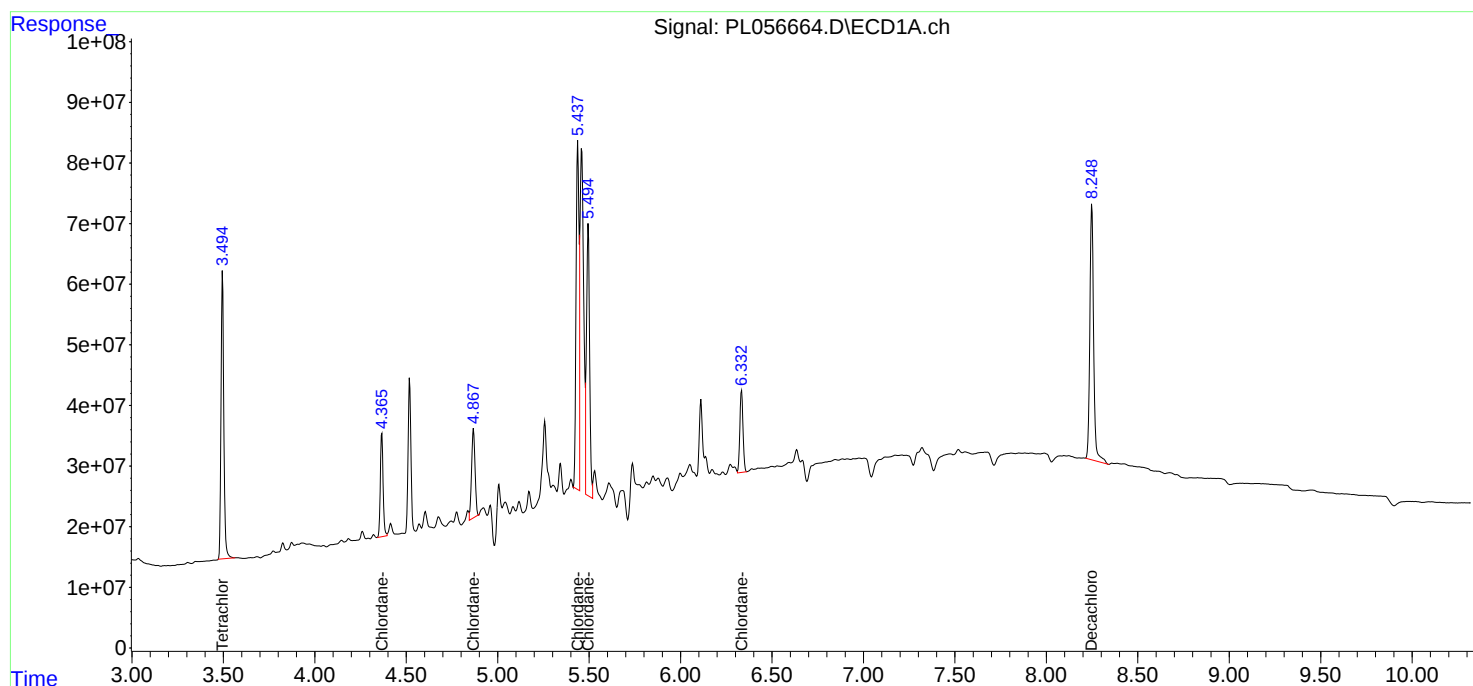


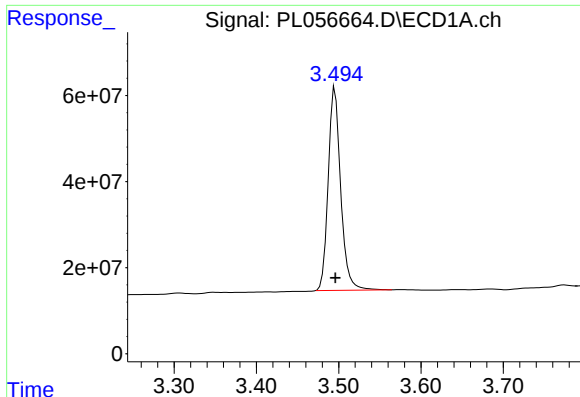

#1 Tetrachloro-m-xylene


R.T.: 3.496 min
Delta R.T.: 0.000 min
Response: 498750116
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

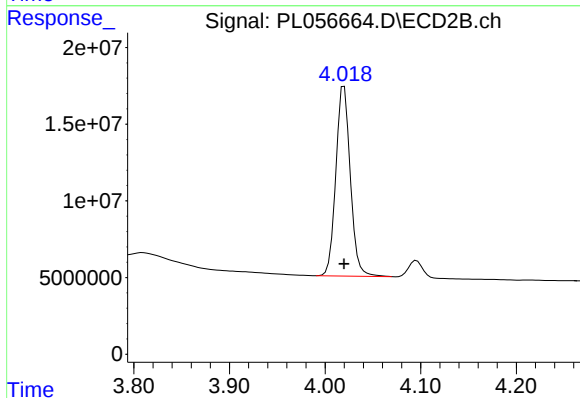


#1 Tetrachloro-m-xylene

R.T.: 4.020 min
Delta R.T.: 0.000 min
Response: 129951824
Conc: 50.00 ng/ml

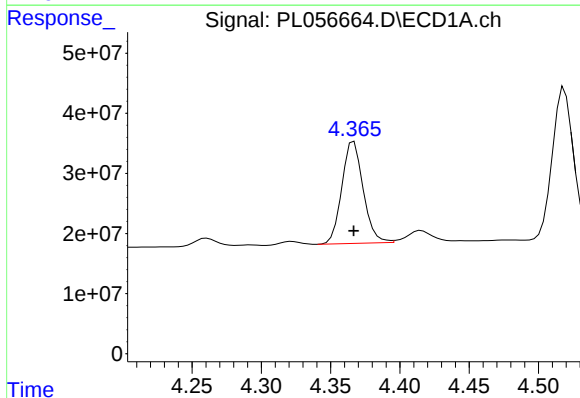


#23 Chlordane-1

R.T.: 4.367 min
Delta R.T.: 0.000 min
Response: 182147267
Conc: 500.00 ng/ml

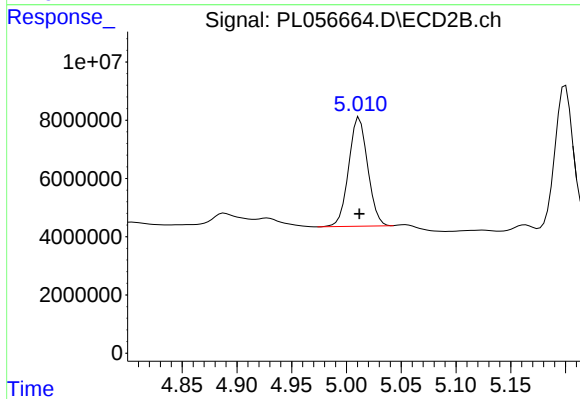

#23 Chlordane-1


R.T.: 5.012 min
Delta R.T.: 0.000 min
Response: 45211398
Conc: 500.00 ng/ml

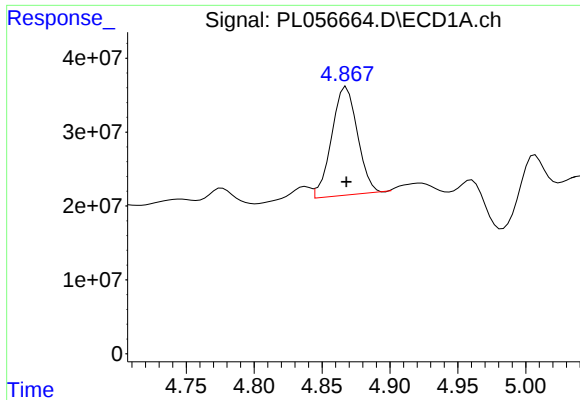

#24 Chlordane-2


R.T.: 4.868 min
Delta R.T.: 0.000 min
Response: 195040879
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

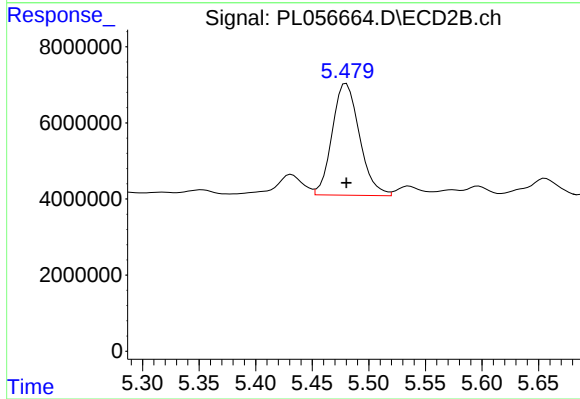


#24 Chlordane-2

R.T.: 5.480 min
Delta R.T.: 0.000 min
Response: 49341140
Conc: 500.00 ng/ml

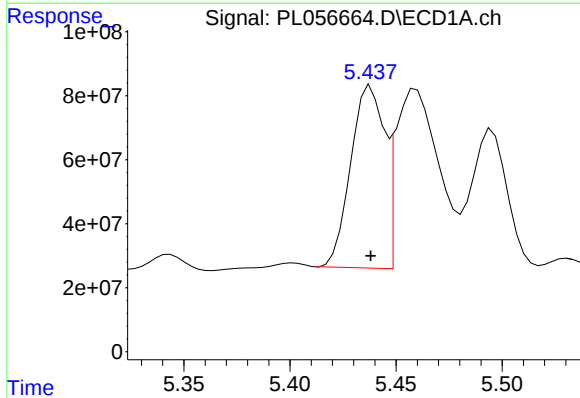


#25 Chlordane-3

R.T.: 5.438 min
Delta R.T.: 0.000 min
Response: 628931479
Conc: 500.00 ng/ml

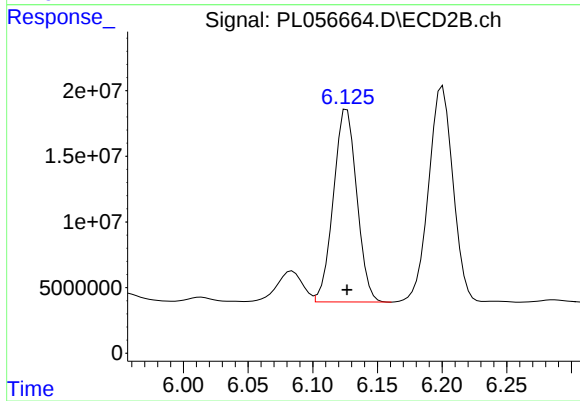

#25 Chlordane-3


R.T.: 6.126 min
Delta R.T.: 0.000 min
Response: 184654428
Conc: 500.00 ng/ml

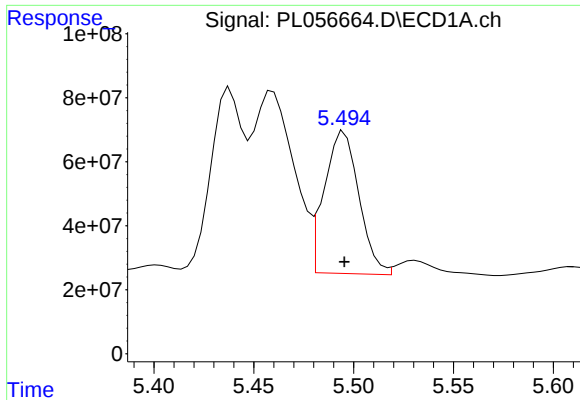

#26 Chlordane-4


R.T.: 5.495 min
Delta R.T.: 0.000 min
Response: 537107400
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

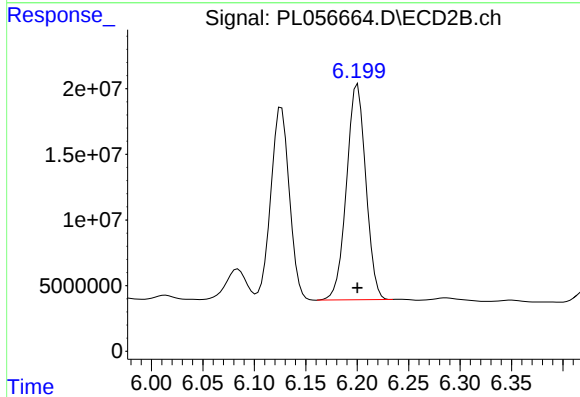


#26 Chlordane-4

R.T.: 6.200 min
Delta R.T.: 0.000 min
Response: 214623296
Conc: 500.00 ng/ml

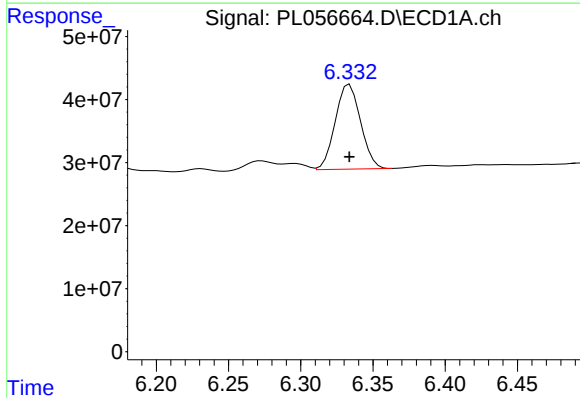


#27 Chlordane-5

R.T.: 6.334 min
Delta R.T.: 0.000 min
Response: 163718566
Conc: 500.00 ng/ml

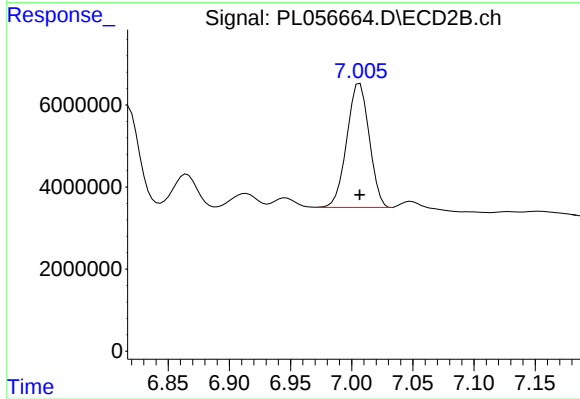

#27 Chlordane-5


R.T.: 7.007 min
Delta R.T.: 0.000 min
Response: 38505306
Conc: 500.00 ng/ml

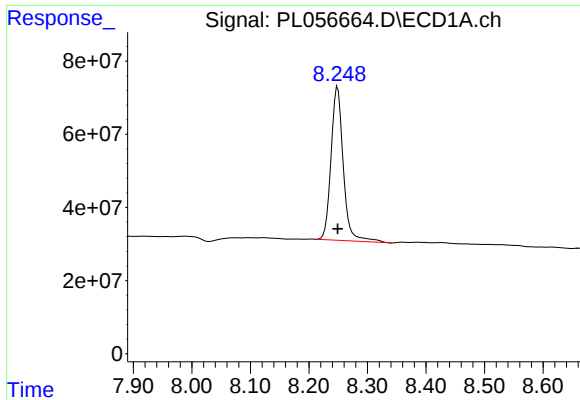

#28 Decachlorobiphenyl

R.T.: 8.249 min
Delta R.T.: 0.000 min
Response: 610120434
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

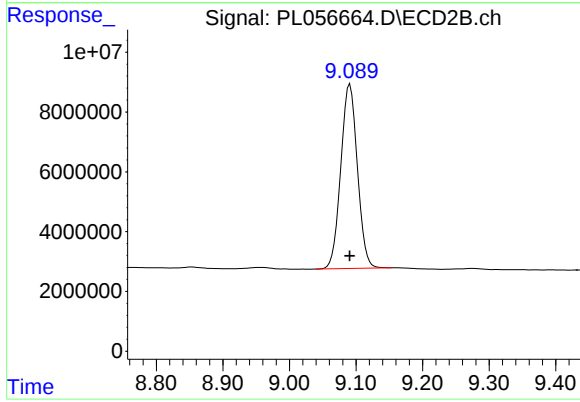

#28 Decachlorobiphenyl

R.T.: 9.091 min
Delta R.T.: 0.000 min
Response: 106768738
Conc: 50.00 ng/ml