

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL021920\
 Data File : PL056670.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Feb 2020 19:22
 Operator : AJ\MA
 Sample : PB126913BL
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 20 00:44:27 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL021920.M
 Quant Title : GC Extractables
 QLast Update : Wed Feb 19 18:03:26 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.496	4.020	179.5E6	50896034	20.756	20.432
28)	SA Decachlor...	8.248	9.090	234.1E6	45458971	19.682	21.634
Target Compounds							
12)	B 4,4'-DDE	5.636f	0.000	2068058	0	0.147	N.D. #
15)	B Endosulfa...	6.307f	0.000	24317673	0	1.958	N.D. #
16)	A 4,4'-DDD	6.195f	0.000	19238149	0	1.720	N.D. #
27)	Chlordane-5	6.307f	0.000	24317673	0	74.267	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL021920\
Data File : PL056670.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Feb 2020 19:22
Operator : AJ\MA
Sample : PB126913BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 20 00:44:27 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL021920.M
Quant Title : GC Extractables
QLast Update : Wed Feb 19 18:03:26 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

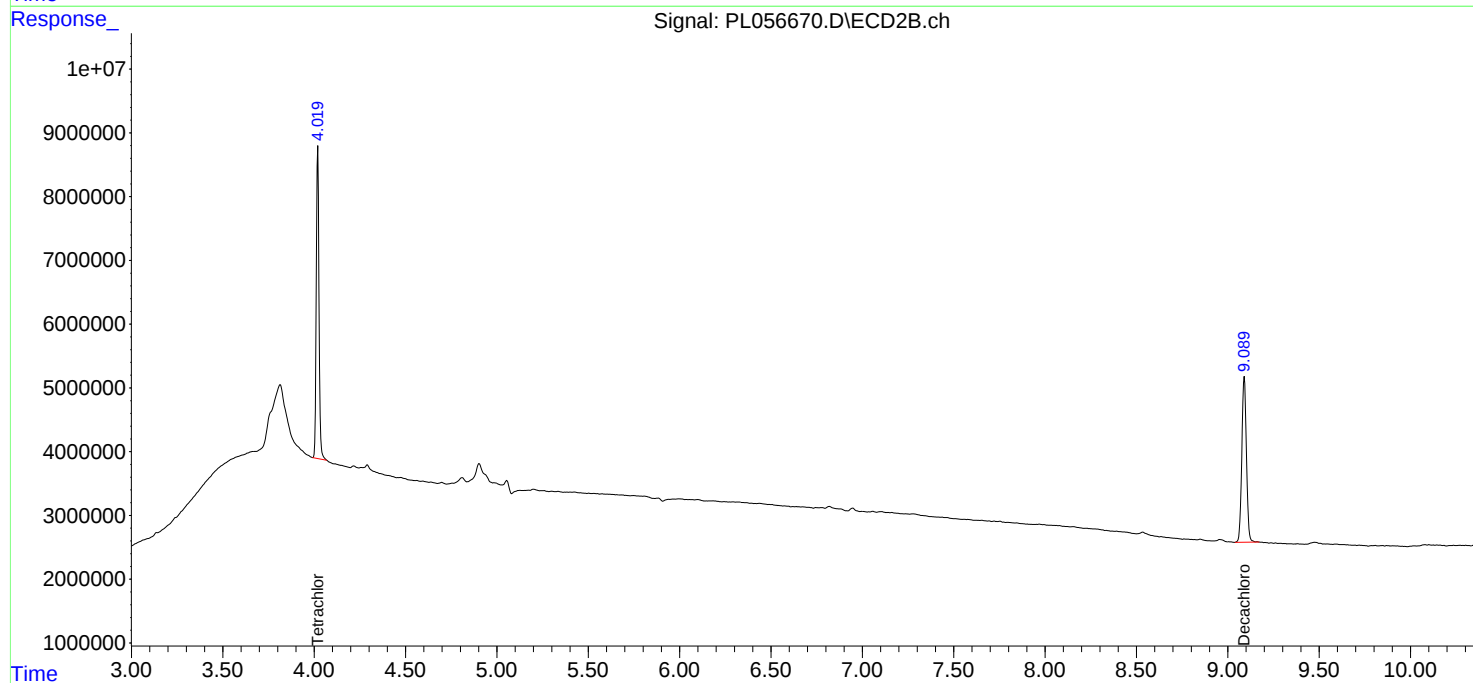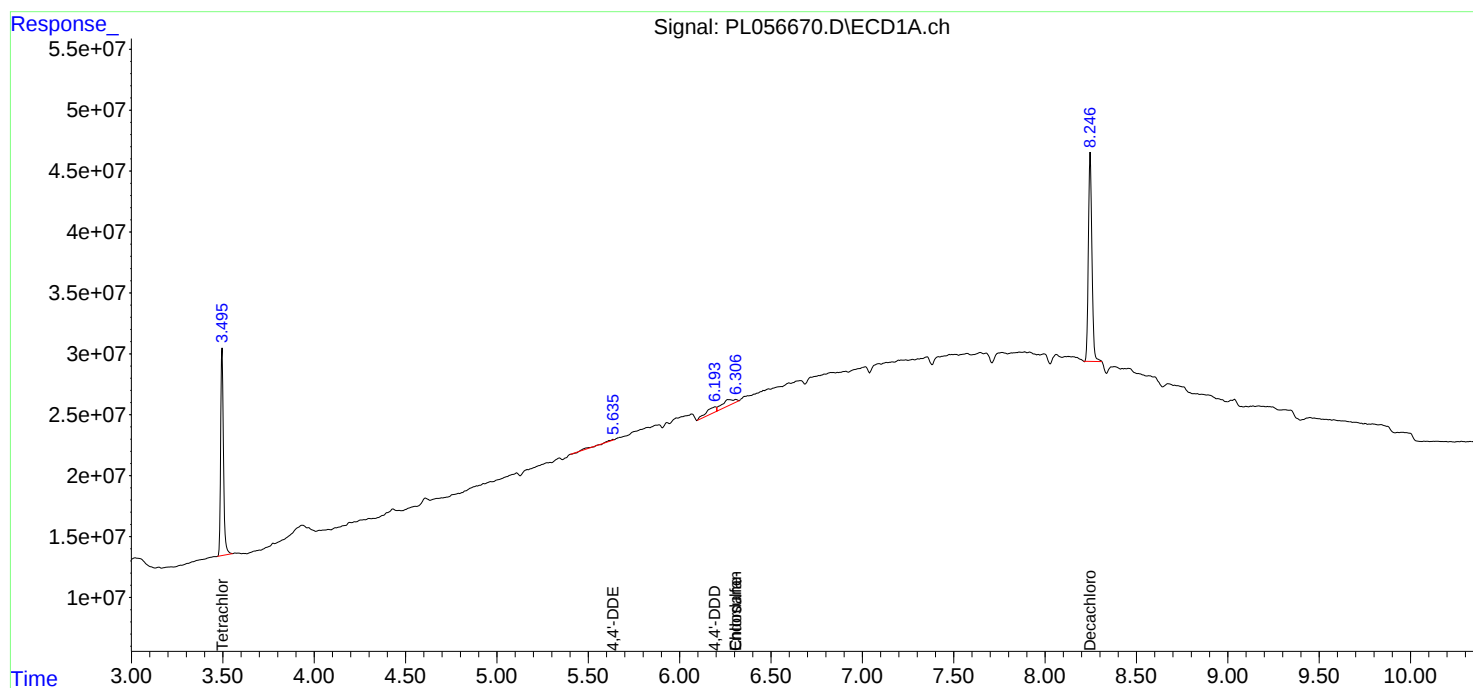


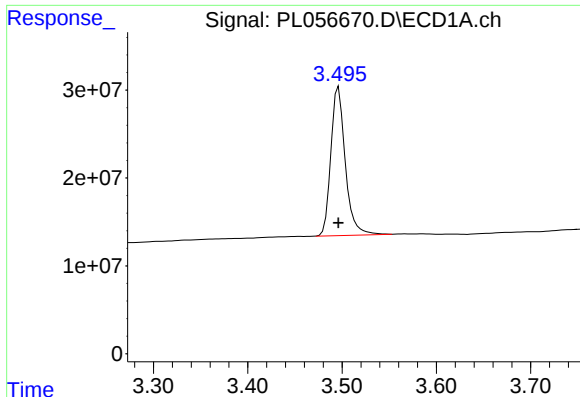

#1 Tetrachloro-m-xylene


R.T.: 3.496 min
Delta R.T.: 0.000 min
Response: 179489467
Conc: 20.76 ng/ml

Instrument :
ECD_L
ClientSampleId :

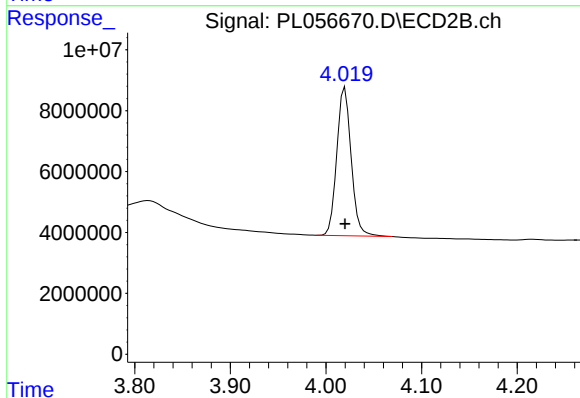


#1 Tetrachloro-m-xylene

R.T.: 4.020 min
Delta R.T.: 0.000 min
Response: 50896034
Conc: 20.43 ng/ml

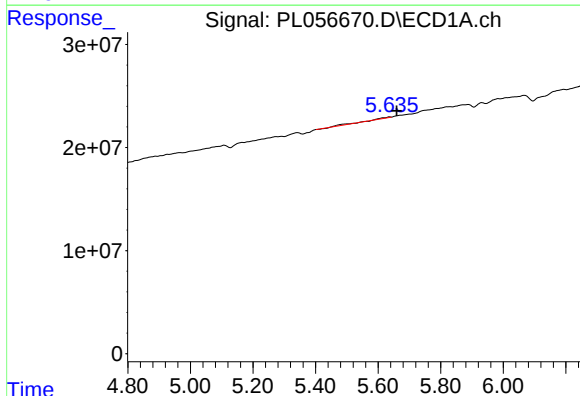


#12 4,4'-DDE

R.T.: 5.636 min
Delta R.T.: -0.023 min
Response: 2068058
Conc: 0.15 ng/ml

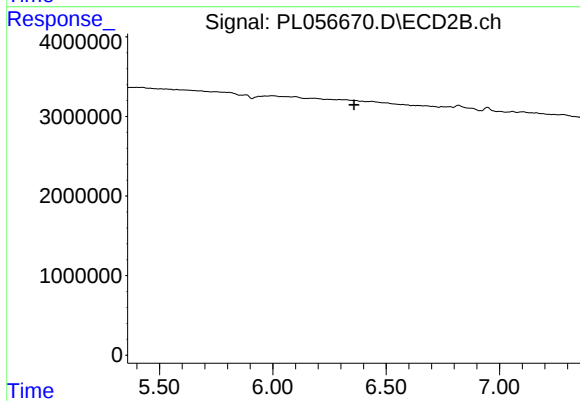

#12 4,4'-DDE


R.T.: 0.000 min
Exp R.T.: 6.358 min
Response: 0
Conc: N.D.

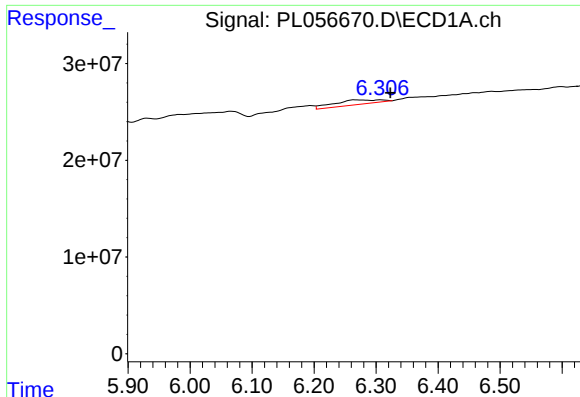

#15 Endosulfan II


R.T.: 6.307 min
Delta R.T.: -0.015 min
Response: 24317673
Conc: 1.96 ng/ml

Instrument :
ECD_L
ClientSampleId :

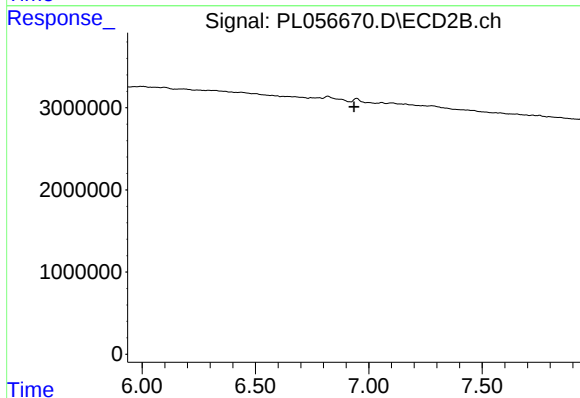


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.936 min
Response: 0
Conc: N.D.

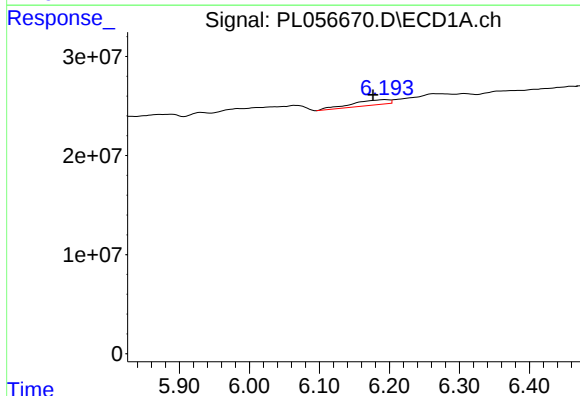


#16 4,4'-DDD

R.T.: 6.195 min
Delta R.T.: 0.018 min
Response: 19238149
Conc: 1.72 ng/ml

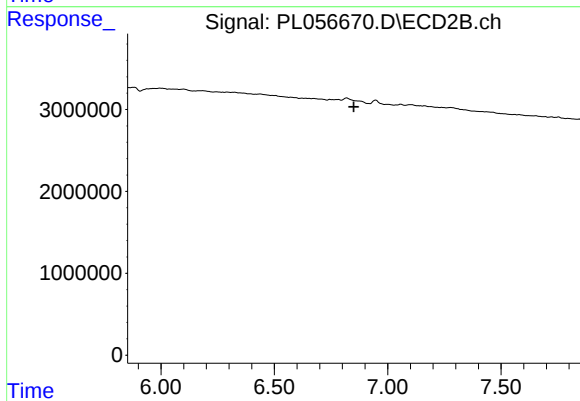

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T. : 6.850 min
Response: 0
Conc: N.D.

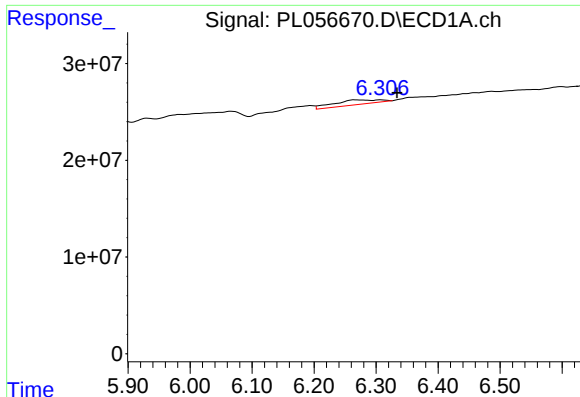

#27 Chlordane-5


R.T.: 6.307 min
Delta R.T.: -0.026 min
Response: 24317673
Conc: 74.27 ng/ml

Instrument :
ECD_L
ClientSampleId :

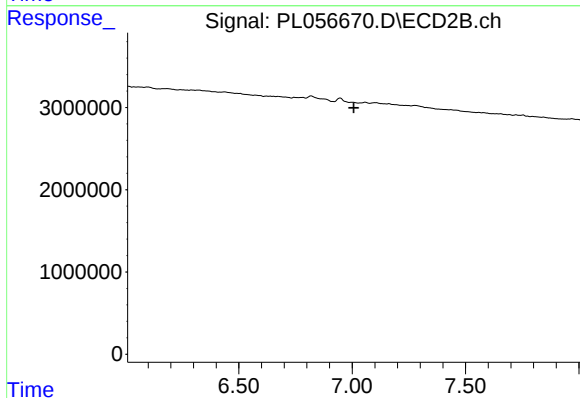


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 7.007 min
Response: 0
Conc: N.D.

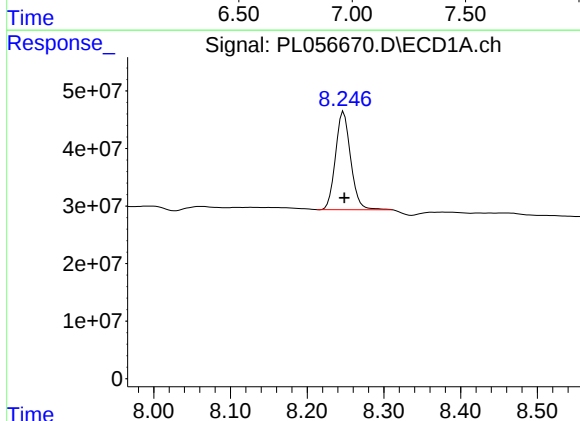

#28 Decachlorobiphenyl

R.T.: 8.248 min
Delta R.T.: 0.000 min
Response: 234118236
Conc: 19.68 ng/ml

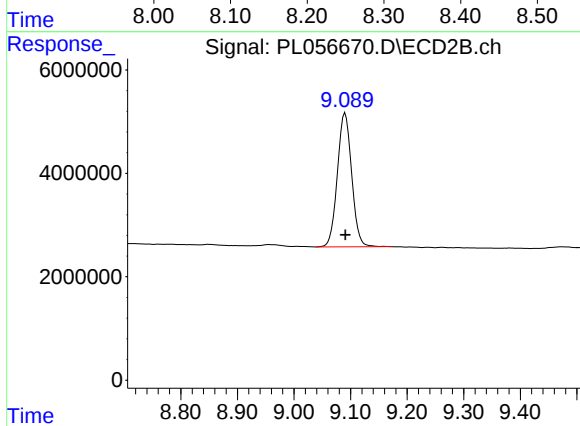

#28 Decachlorobiphenyl

R.T.: 9.090 min
Delta R.T.: 0.000 min
Response: 45458971
Conc: 21.63 ng/ml