

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL021920\
 Data File : PL056674.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Feb 2020 20:18
 Operator : AJ\MA
 Sample : L1575-07
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-A-D

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 20 00:45:13 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL021920.M
 Quant Title : GC Extractables
 QLast Update : Wed Feb 19 18:03:26 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.496	4.020	206.2E6	56352682	23.846	22.623
28)	SA Decachlor...	8.248	9.091	219.5E6	42619721	18.451	20.282
Target Compounds							
12)	B 4,4'-DDE	5.688f	0.000	39660417	0	2.820	N.D. #
13)	MA Dieldrin	5.816f	0.000	12021303	0	0.807	N.D. #
23)	Chlordane-1	4.389f	0.000	7063654	0	19.390	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL021920\
Data File : PL056674.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Feb 2020 20:18
Operator : AJ\MA
Sample : L1575-07
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
TP-A-D

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 20 00:45:13 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL021920.M
Quant Title : GC Extractables
QLast Update : Wed Feb 19 18:03:26 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

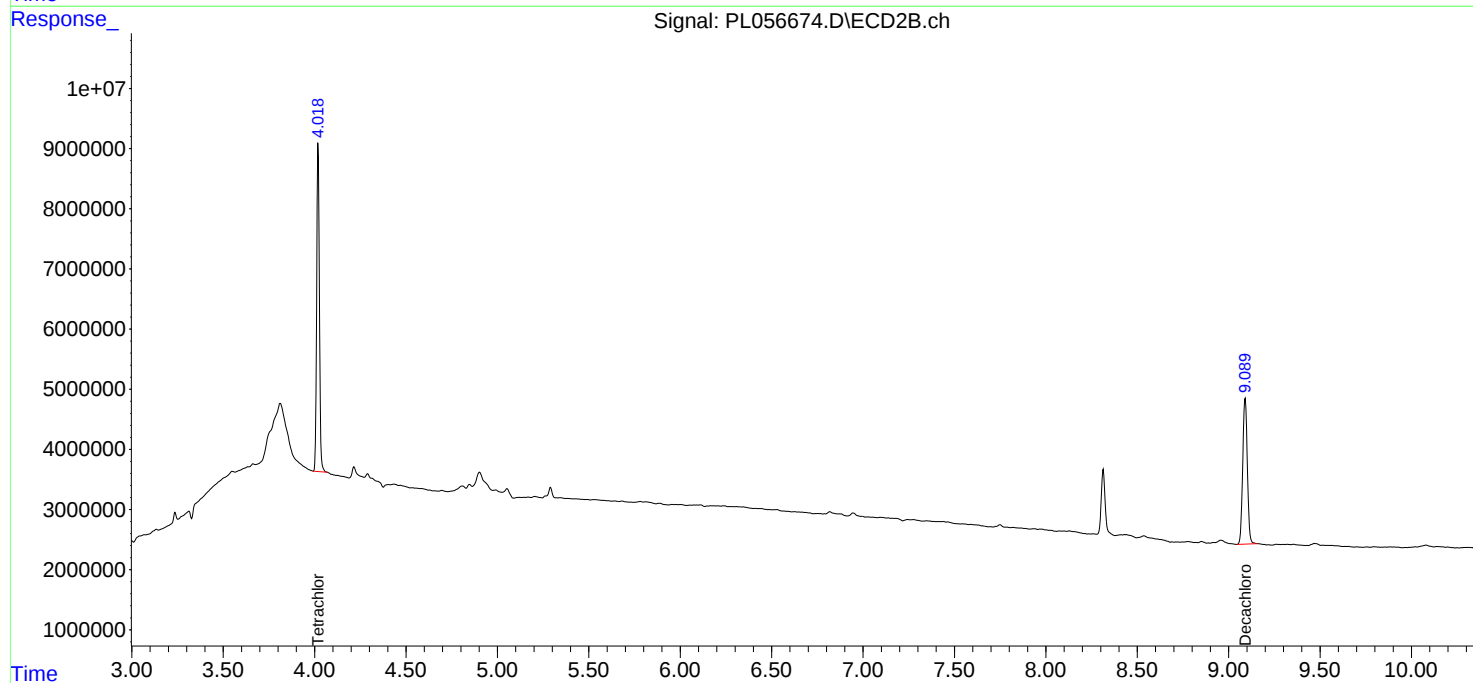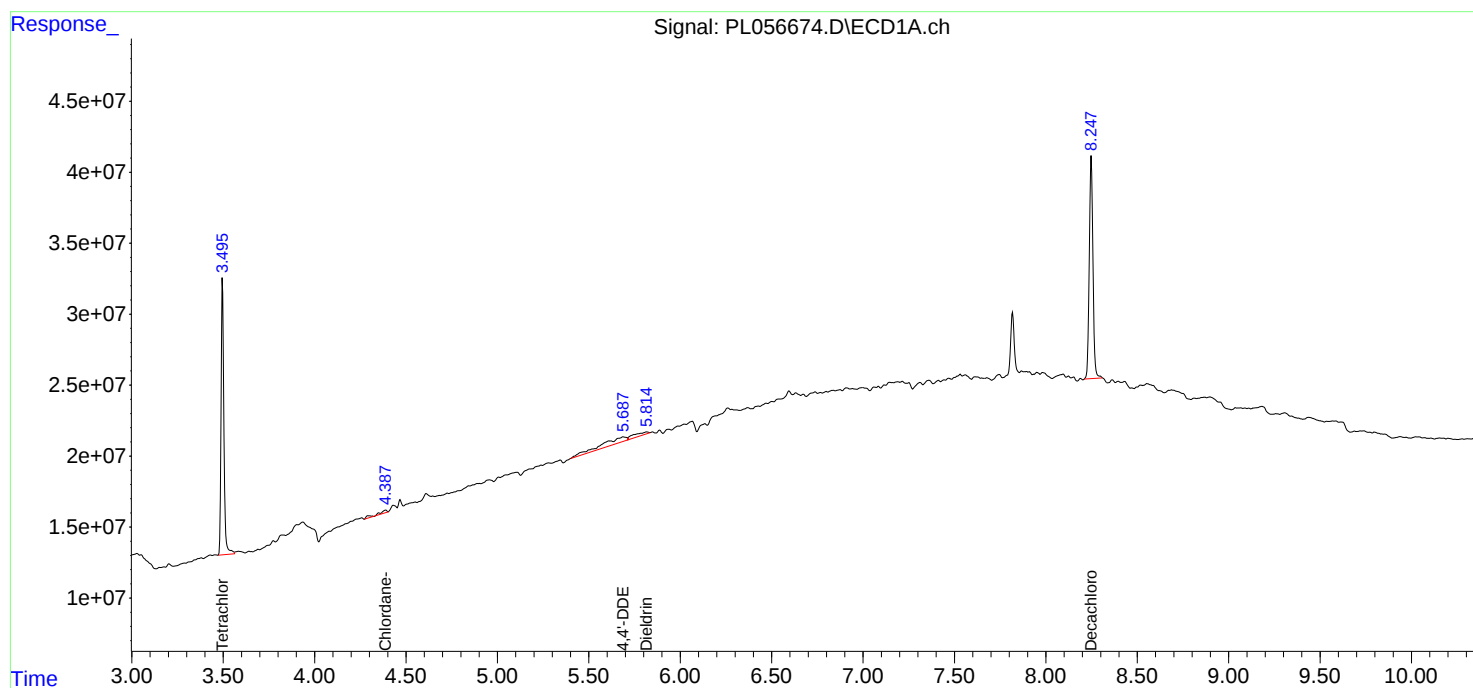


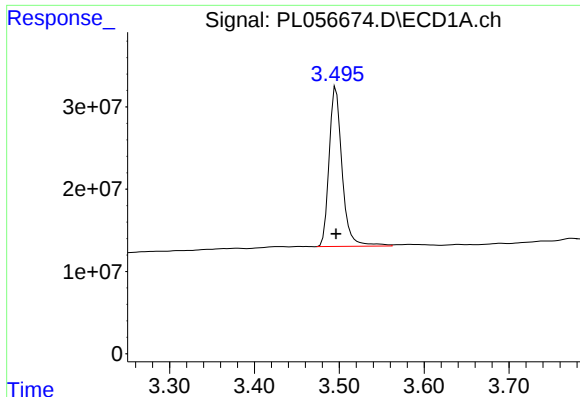

#1 Tetrachloro-m-xylene


R.T.: 3.496 min
Delta R.T.: 0.000 min
Response: 206210414
Conc: 23.85 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-A-D

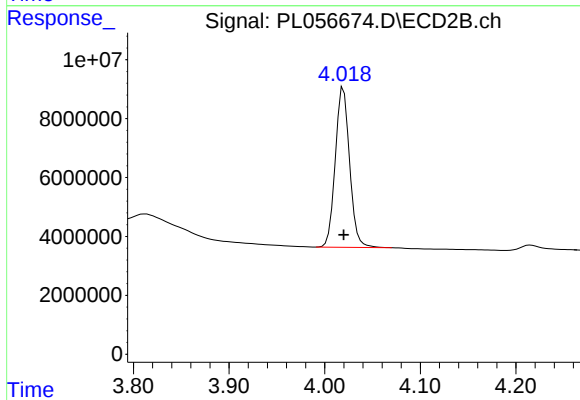


#1 Tetrachloro-m-xylene

R.T.: 4.020 min
Delta R.T.: 0.000 min
Response: 56352682
Conc: 22.62 ng/ml

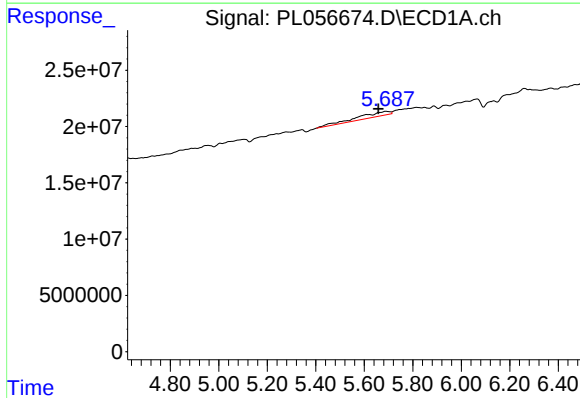


#12 4,4'-DDE

R.T.: 5.688 min
Delta R.T.: 0.029 min
Response: 39660417
Conc: 2.82 ng/ml

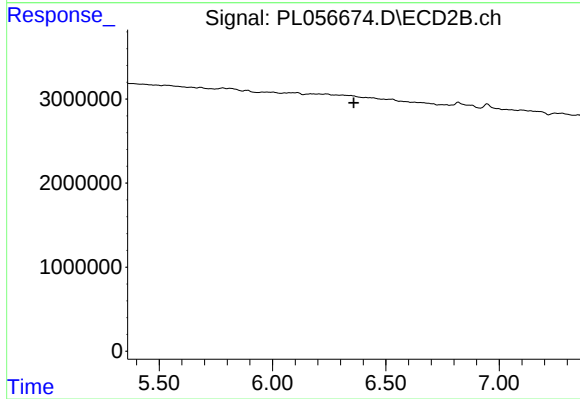

#12 4,4'-DDE


R.T.: 0.000 min
Exp R.T.: 6.358 min
Response: 0
Conc: N.D.

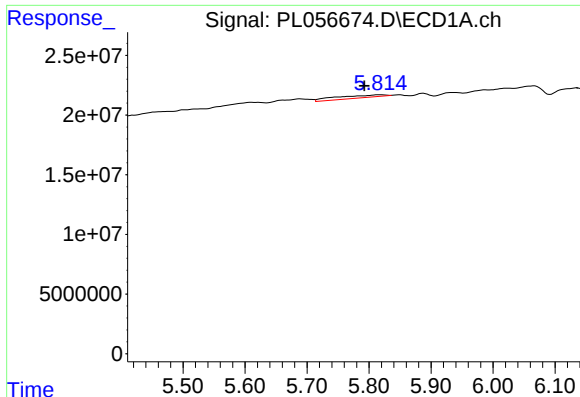

#13 Dieldrin


R.T.: 5.816 min
Delta R.T.: 0.024 min
Response: 12021303
Conc: 0.81 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-A-D

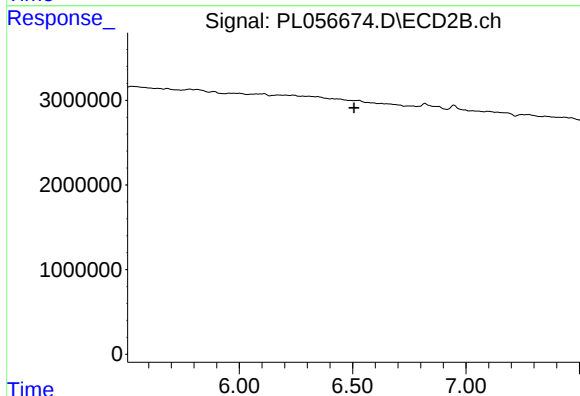


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 6.506 min
Response: 0
Conc: N.D.

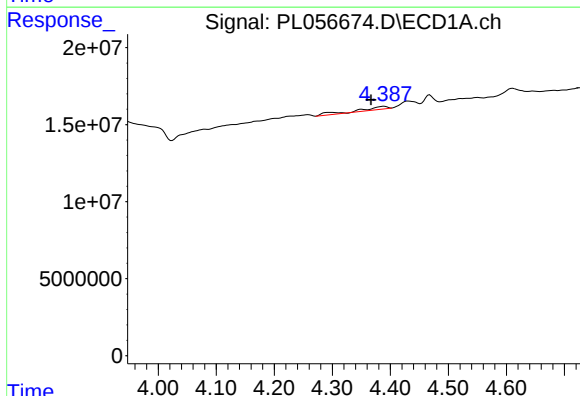


#23 Chlordane-1

R.T.: 4.389 min
Delta R.T.: 0.022 min
Response: 7063654
Conc: 19.39 ng/ml

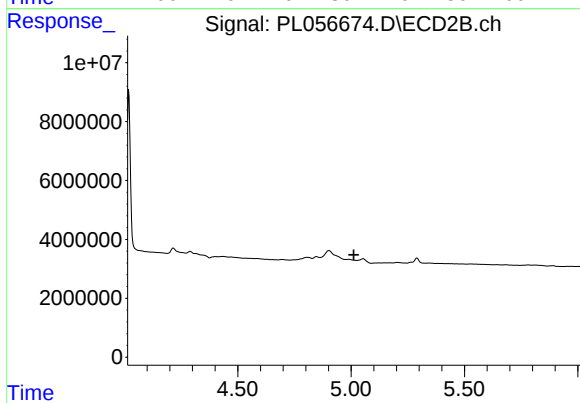

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 5.012 min
Response: 0
Conc: N.D.

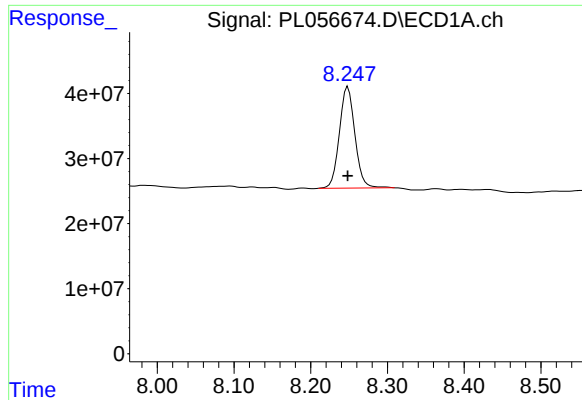

#28 Decachlorobiphenyl

R.T.: 8.248 min
Delta R.T.: 0.000 min
Response: 219480984
Conc: 18.45 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-A-D

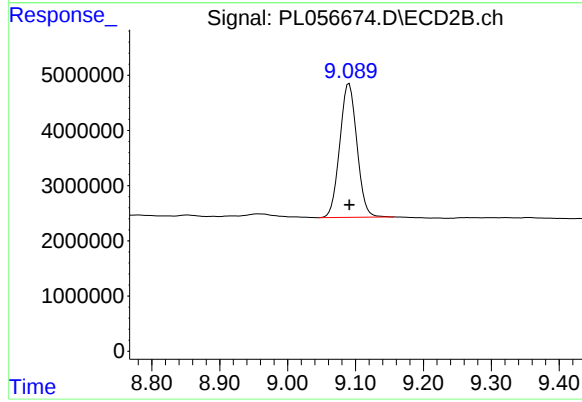

#28 Decachlorobiphenyl

R.T.: 9.091 min
Delta R.T.: 0.000 min
Response: 42619721
Conc: 20.28 ng/ml