

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022020\
 Data File : PL056681.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Feb 2020 10:33
 Operator : AJ\MA
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 21 00:26:14 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL021920.M
 Quant Title : GC Extractables
 QLast Update : Wed Feb 19 18:03:26 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds						
8) B	Heptachlo...	0.000	5.894	0	32467530	N.D. 11.105 #
9) A	Endosulfan I	5.553	0.000	106.3E6	0	7.955 N.D. #
12) B	4,4'-DDE	5.683f	0.000	102.4E6	0	7.277 N.D. #
13) MA	Dieldrin	5.780	0.000	112.8E6	0	7.568 N.D. #
14) MA	Endrin	6.060	6.718	84191564	7713541	6.238 3.131 #
15) B	Endosulfa...	6.302f	6.949	90087398	6958105	7.254 2.694 #
17) MA	4,4'-DDT	6.392f	0.000	123.5E6	0	11.337 N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022020\
Data File : PL056681.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Feb 2020 10:33
Operator : AJ\MA
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 21 00:26:14 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL021920.M
Quant Title : GC Extractables
QLast Update : Wed Feb 19 18:03:26 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

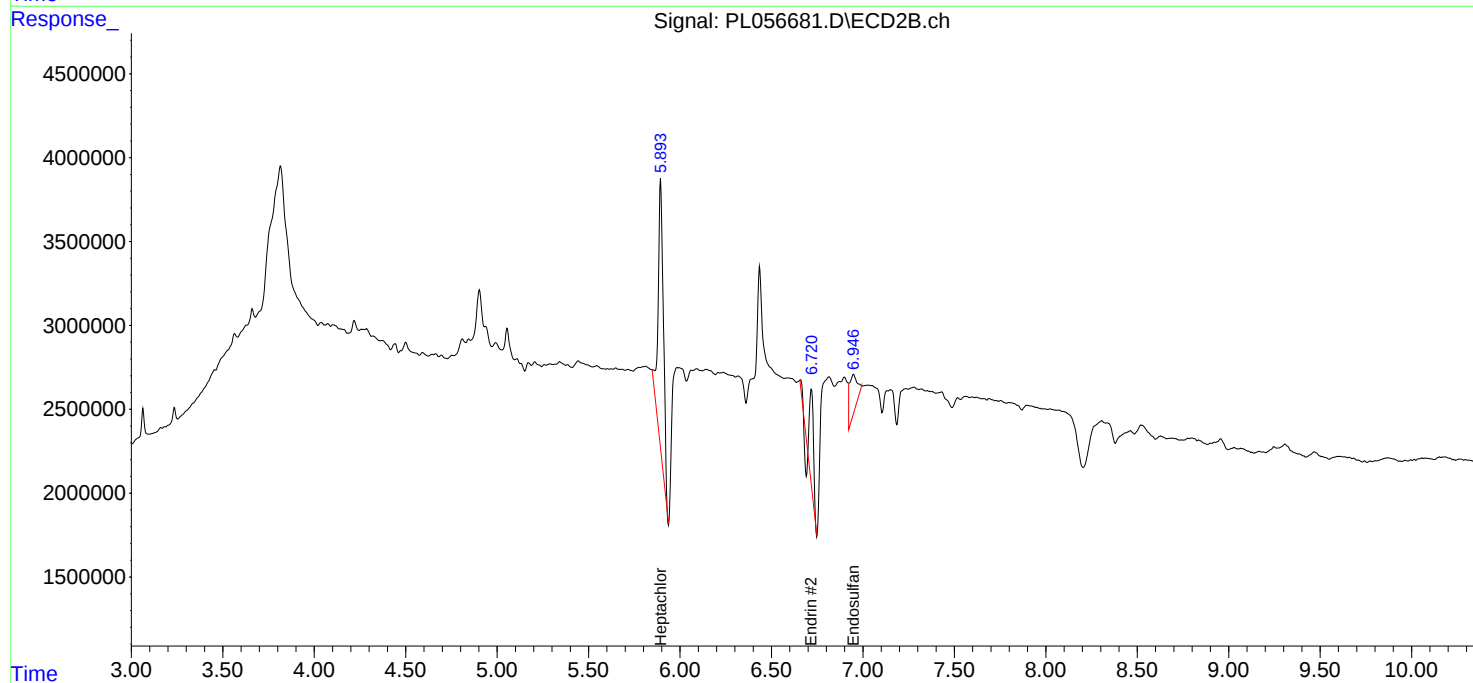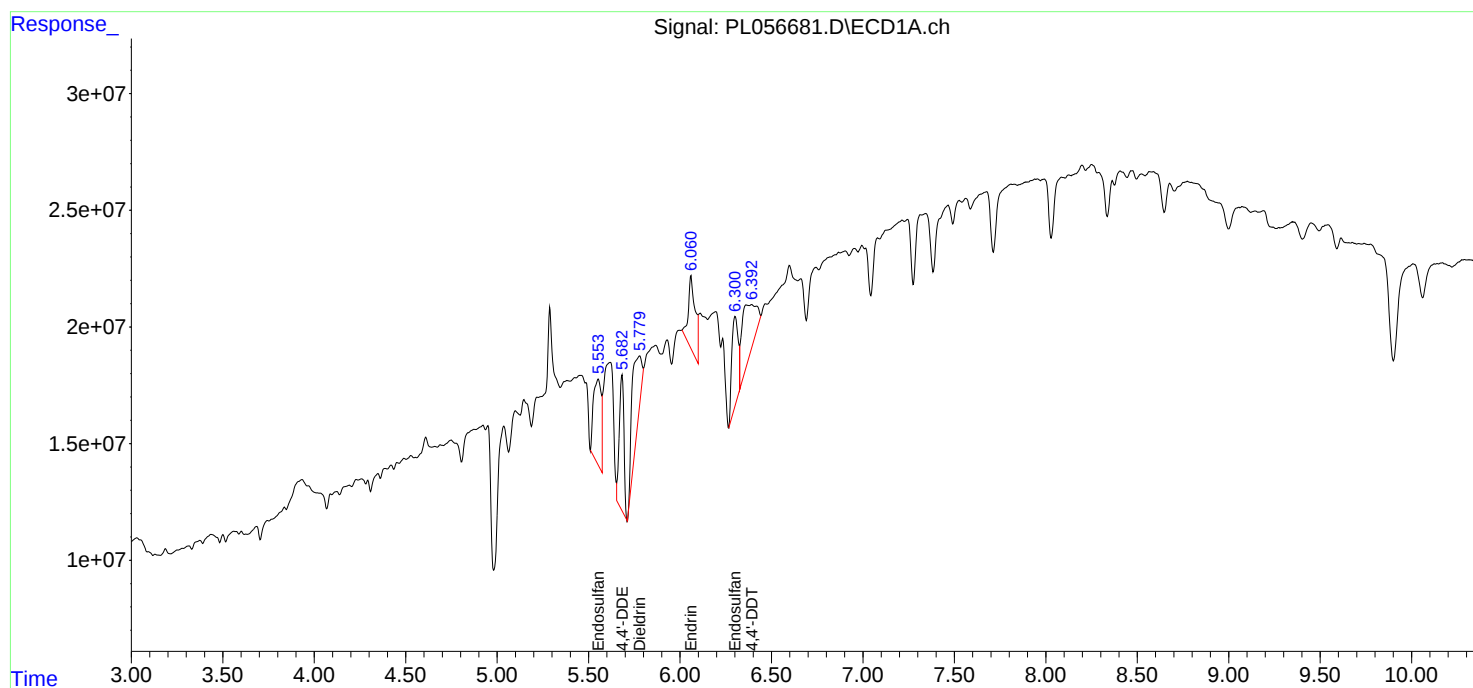


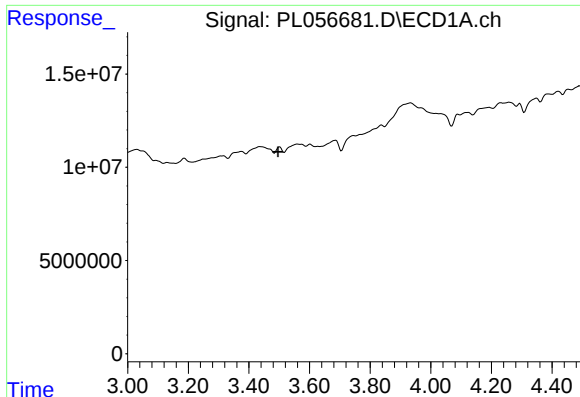

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 3.496 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

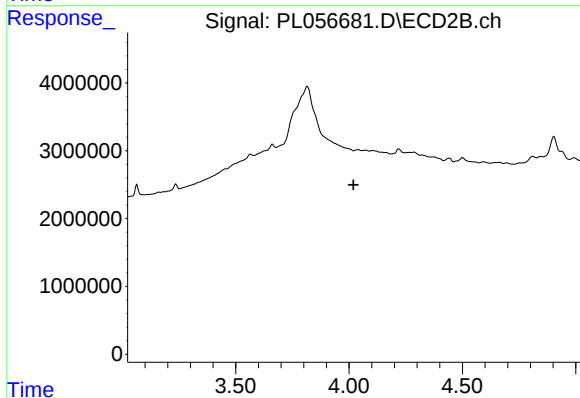


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 4.020 min
Response: 0
Conc: N.D.

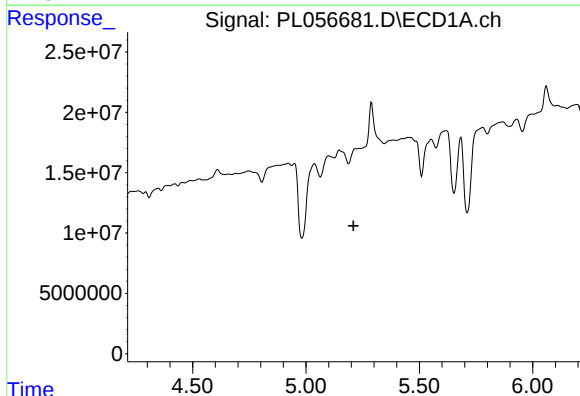


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.210 min
Response: 0
Conc: N.D.

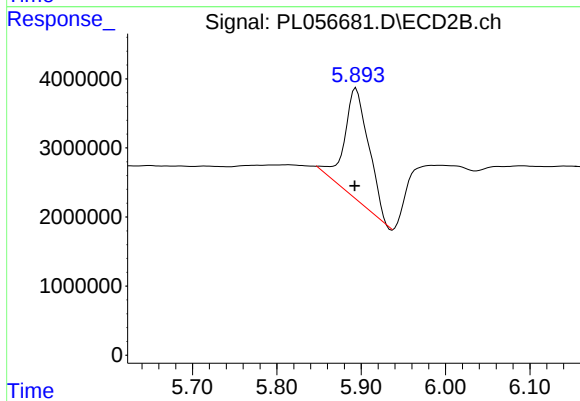

#8 Heptachlor epoxide


R.T.: 5.894 min
Delta R.T.: 0.002 min
Response: 32467530
Conc: 11.10 ng/ml

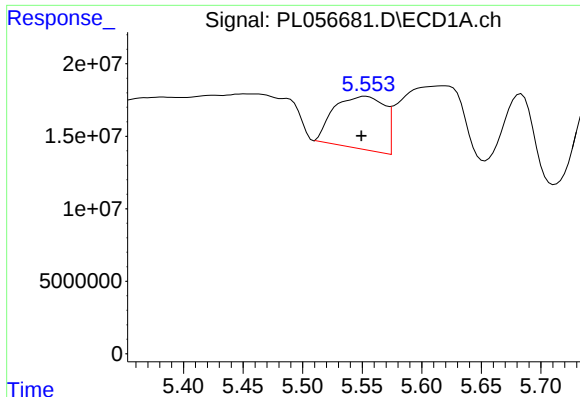

#9 Endosulfan I


R.T.: 5.553 min
Delta R.T.: 0.004 min
Response: 106343130
Conc: 7.95 ng/ml

Instrument :
ECD_L
ClientSampleId :

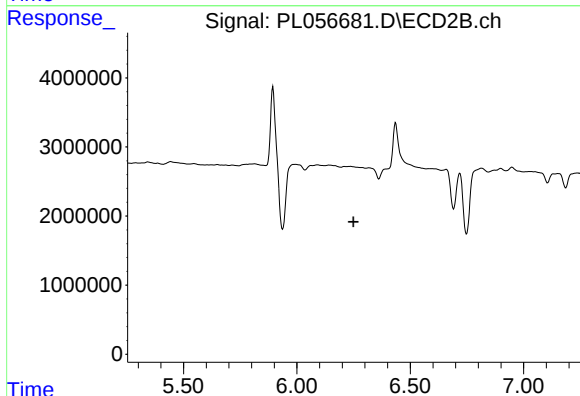


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 6.250 min
Response: 0
Conc: N.D.

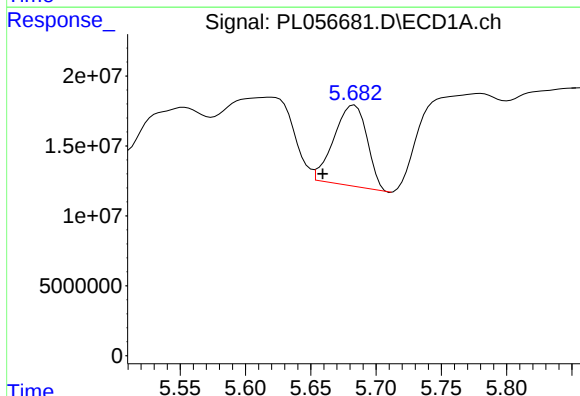


#12 4,4'-DDE

R.T.: 5.683 min
Delta R.T.: 0.024 min
Response: 102356631
Conc: 7.28 ng/ml

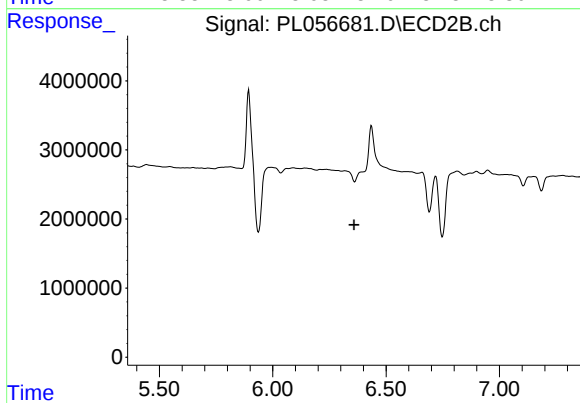

#12 4,4'-DDE


R.T.: 0.000 min
Exp R.T. : 6.358 min
Response: 0
Conc: N.D.

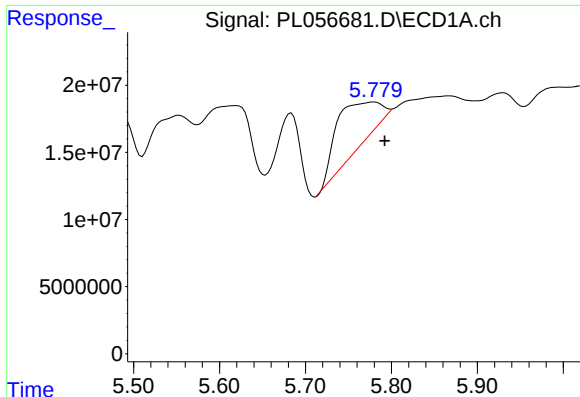

#13 Dieldrin


R.T.: 5.780 min
Delta R.T.: -0.012 min
Response: 112809109
Conc: 7.57 ng/ml

Instrument :
ECD_L
ClientSampleId :

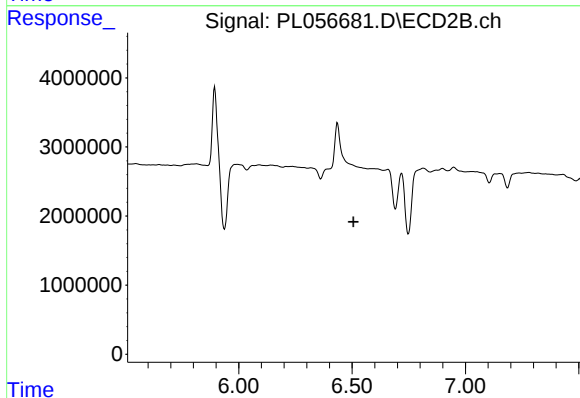


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 6.506 min
Response: 0
Conc: N.D.

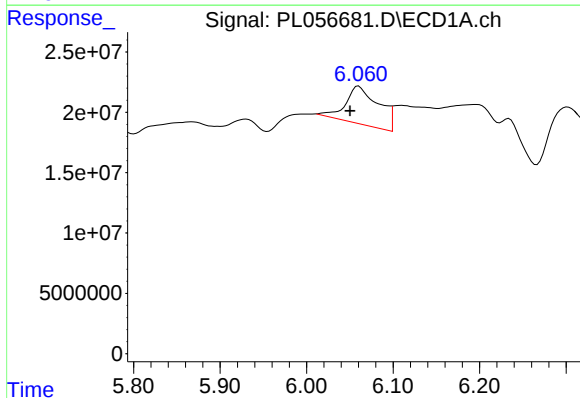


#14 Endrin

R.T.: 6.060 min
Delta R.T.: 0.010 min
Response: 84191564
Conc: 6.24 ng/ml

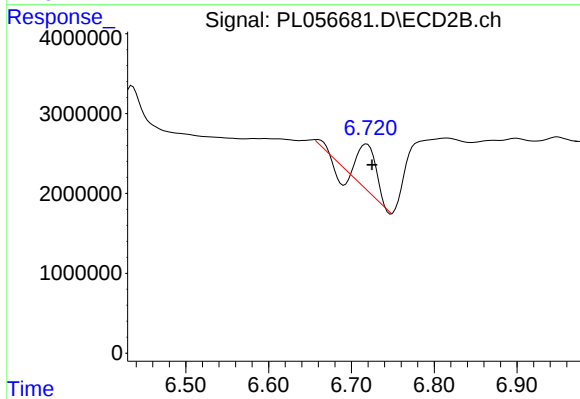

#14 Endrin


R.T.: 6.718 min
Delta R.T.: -0.007 min
Response: 7713541
Conc: 3.13 ng/ml

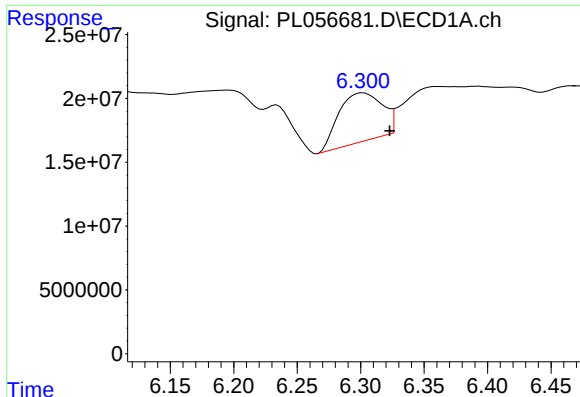

#15 Endosulfan II


R.T.: 6.302 min
Delta R.T.: -0.021 min
Response: 90087398
Conc: 7.25 ng/ml

Instrument :
ECD_L
ClientSampleId :

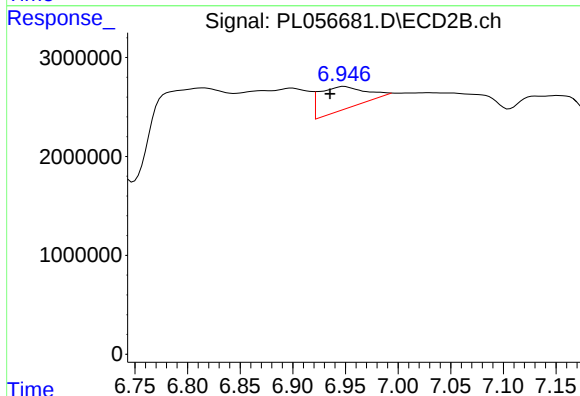


#15 Endosulfan II

R.T.: 6.949 min
Delta R.T.: 0.013 min
Response: 6958105
Conc: 2.69 ng/ml

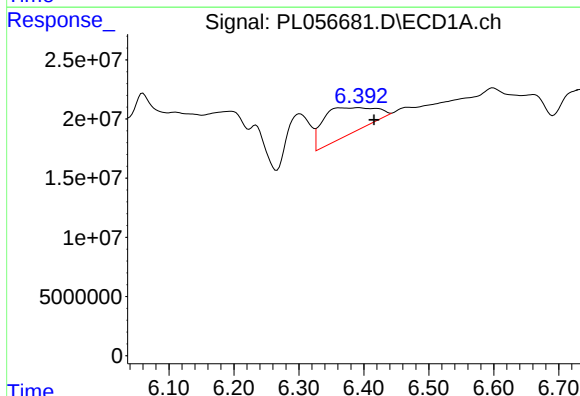


#17 4,4'-DDT

R.T.: 6.392 min
Delta R.T.: -0.024 min
Response: 123461310
Conc: 11.34 ng/ml

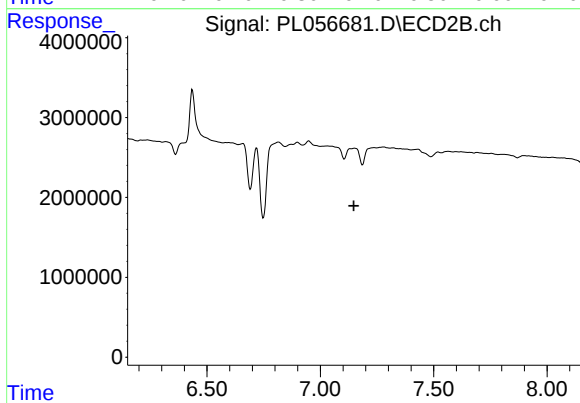

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 7.148 min
Response: 0
Conc: N.D.

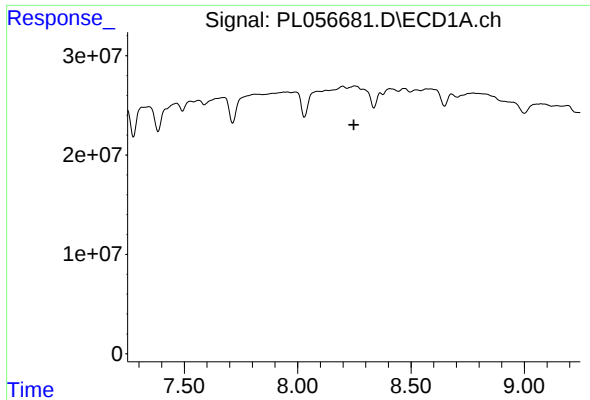

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 8.248 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

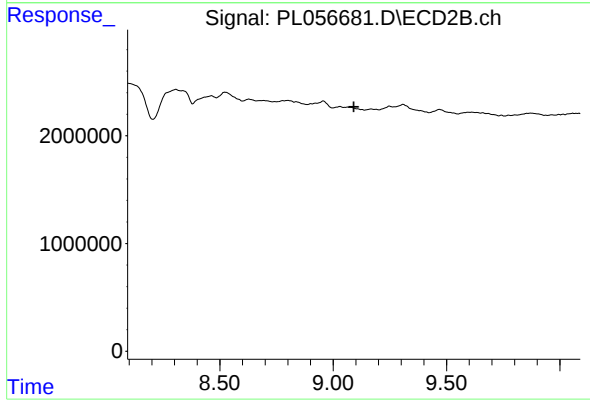

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 9.091 min
Response: 0
Conc: N.D.