

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022020\
 Data File : PL056692.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Feb 2020 14:06
 Operator : AJ\MA
 Sample : L1596-01
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 21 00:28:40 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL021920.M
 Quant Title : GC Extractables
 QLast Update : Thu Feb 20 02:32:45 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.498	4.019	105.7E6	31774818	12.223	12.756
28)	SA Decachlor...	8.249	9.090	141.4E6	26436944	11.886	12.581
Target Compounds							
10)	B gamma-Chl...	5.461f	0.000	18134137	0	1.248	N.D. #
11)	B alpha-Chl...	0.000	6.201	0	4425204	N.D.	1.555 #
12)	B 4,4'-DDE	5.661	0.000	8322647	0	0.592	N.D. #
13)	MA Dieldrin	5.789	0.000	3825573	0	0.257	N.D. #
17)	MA 4,4'-DDT	6.417	0.000	12248666	0	1.125	N.D. #
24)	Chlordane-2	4.877	0.000	8432764	0	21.618	N.D. #
25)	Chlordane-3	5.461f	0.000	18134137	0	14.417	N.D. #
26)	Chlordane-4	0.000	6.201	0	4425204	N.D.	10.309 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022020\
Data File : PL056692.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Feb 2020 14:06
Operator : AJ\MA
Sample : L1596-01
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 21 00:28:40 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL021920.M
Quant Title : GC Extractables
QLast Update : Thu Feb 20 02:32:45 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

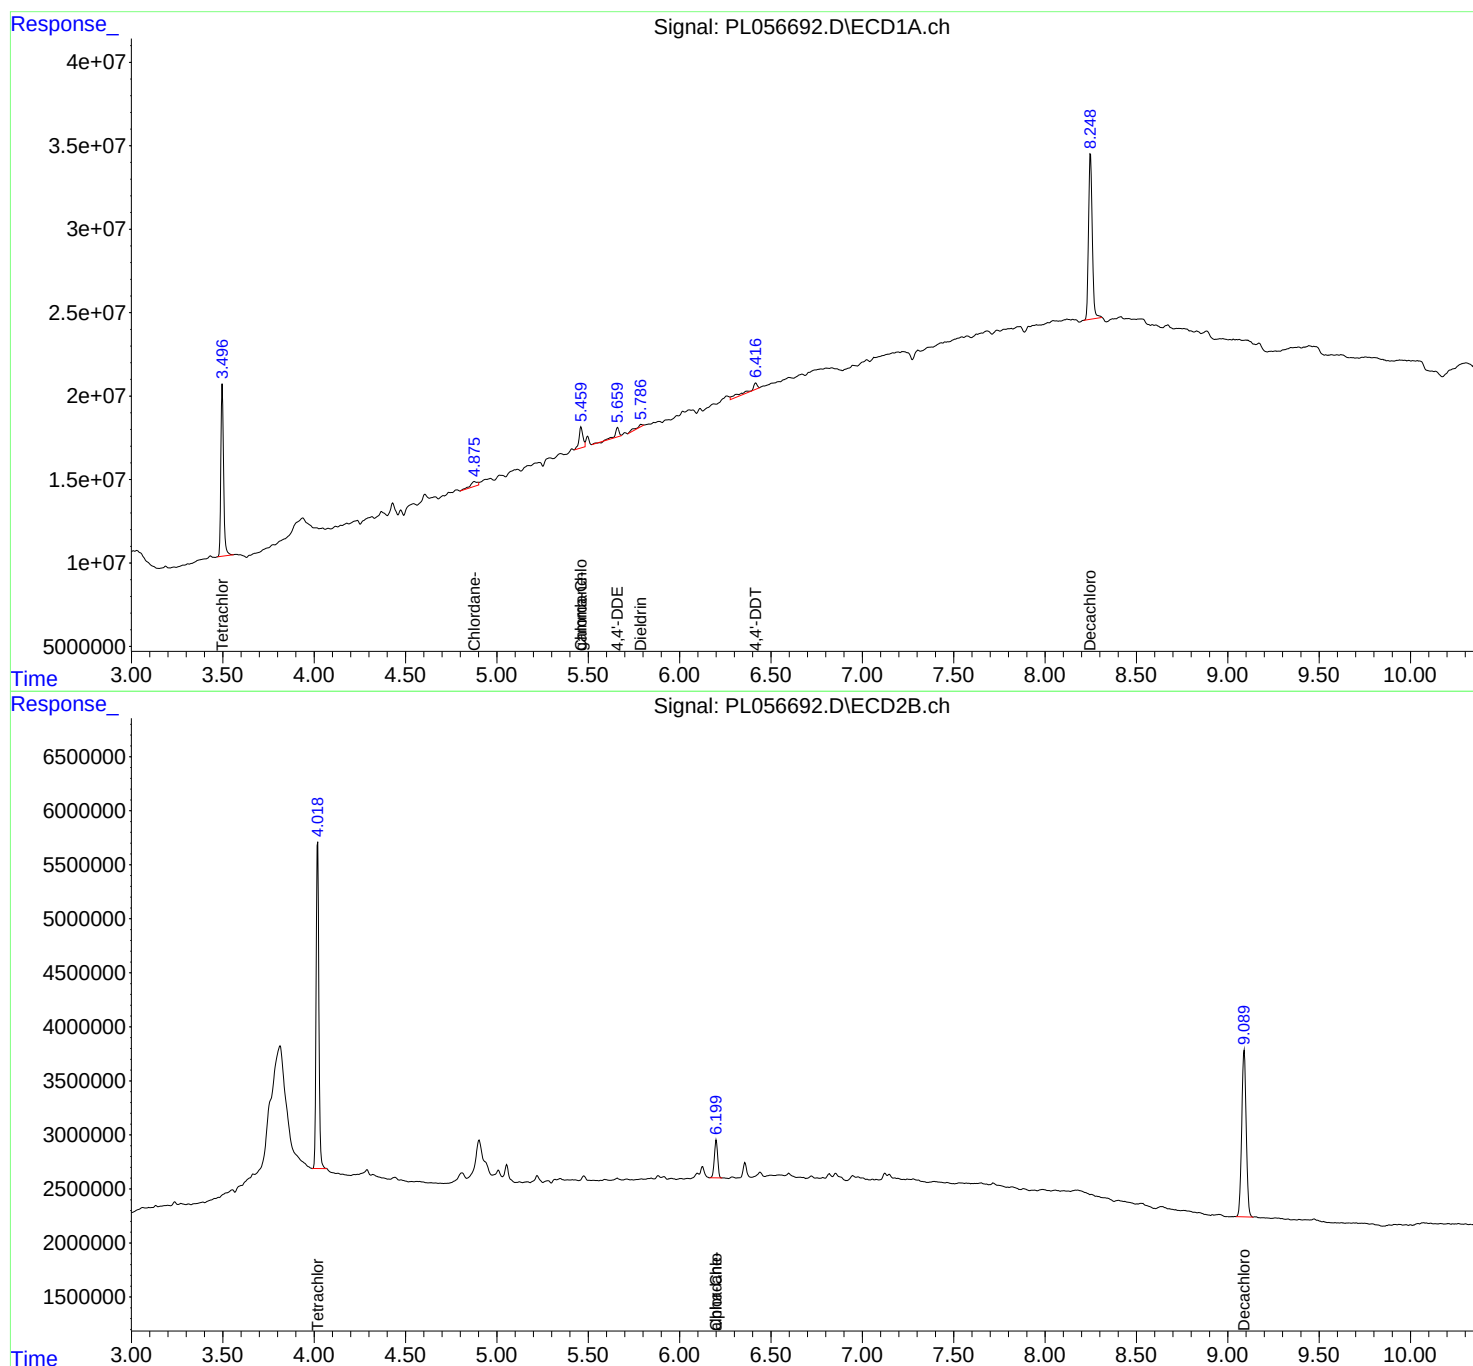


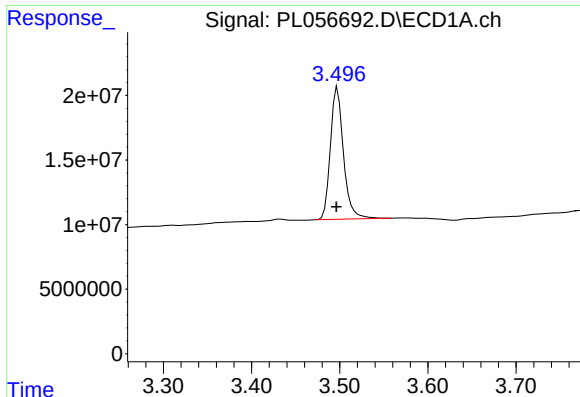

#1 Tetrachloro-m-xylene


R.T.: 3.498 min
Delta R.T.: 0.002 min
Response: 105700485
Conc: 12.22 ng/ml

Instrument :
ECD_L
ClientSampleId :

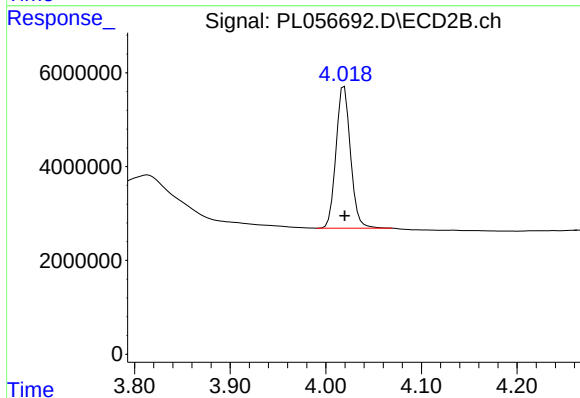


#1 Tetrachloro-m-xylene

R.T.: 4.019 min
Delta R.T.: 0.000 min
Response: 31774818
Conc: 12.76 ng/ml

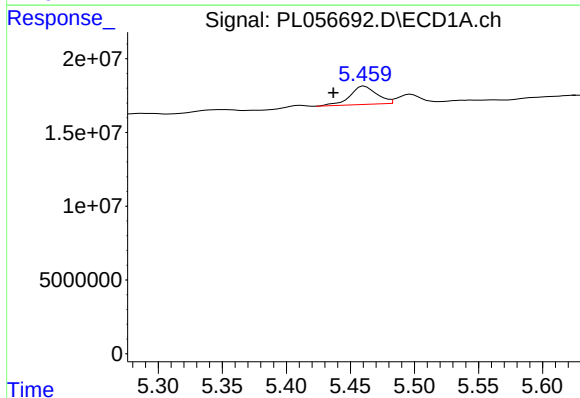


#10 gamma-Chlordane

R.T.: 5.461 min
Delta R.T.: 0.024 min
Response: 18134137
Conc: 1.25 ng/ml

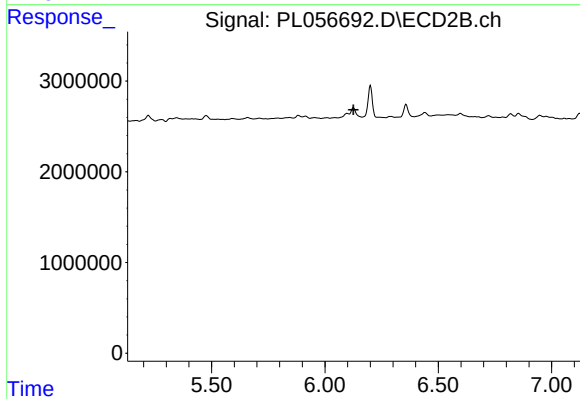

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 6.127 min
Response: 0
Conc: N.D.

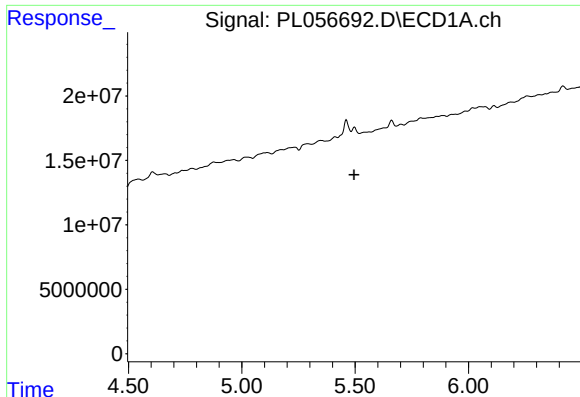

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.495 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

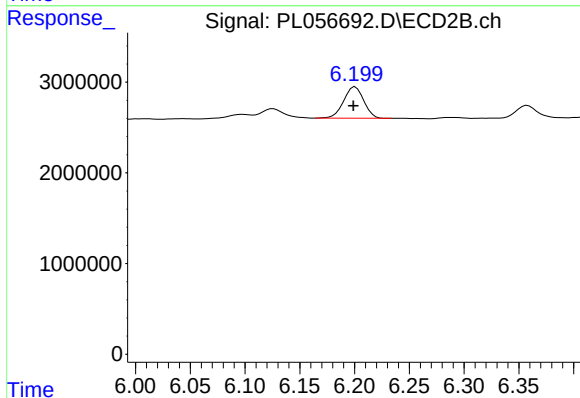


#11 alpha-Chlordane

R.T.: 6.201 min
Delta R.T.: 0.002 min
Response: 4425204
Conc: 1.56 ng/ml

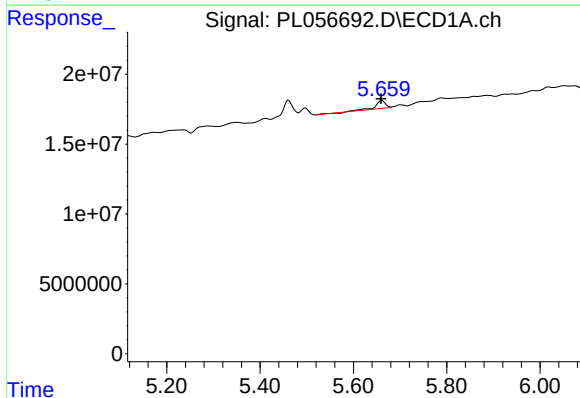


#12 4,4'-DDE

R.T.: 5.661 min
Delta R.T.: 0.002 min
Response: 8322647
Conc: 0.59 ng/ml

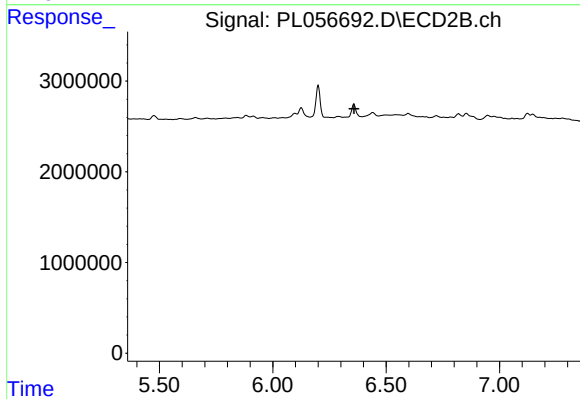

#12 4,4'-DDE


R.T.: 0.000 min
Exp R.T.: 6.358 min
Response: 0
Conc: N.D.

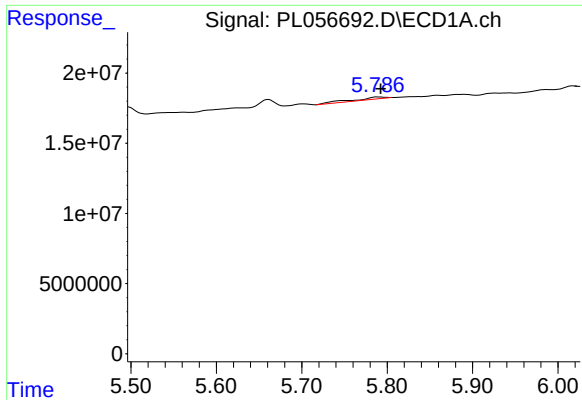

#13 Dieldrin


R.T.: 5.789 min
Delta R.T.: -0.003 min
Response: 3825573
Conc: 0.26 ng/ml

Instrument :
ECD_L
ClientSampleId :

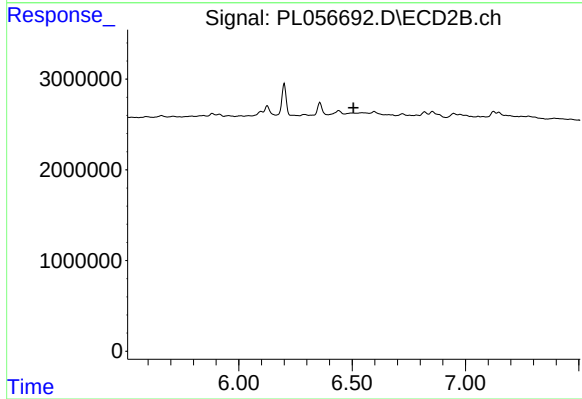


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 6.506 min
Response: 0
Conc: N.D.

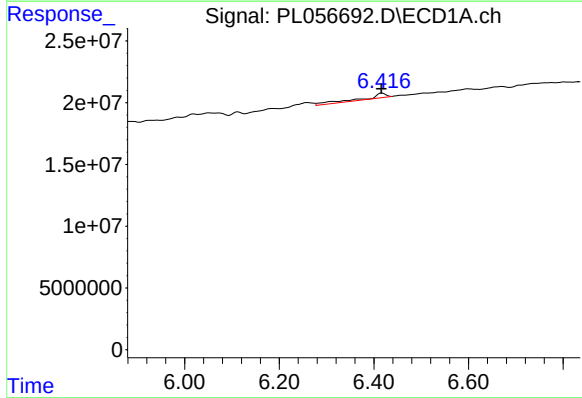


#17 4,4'-DDT

R.T.: 6.417 min
Delta R.T.: 0.001 min
Response: 12248666
Conc: 1.12 ng/ml

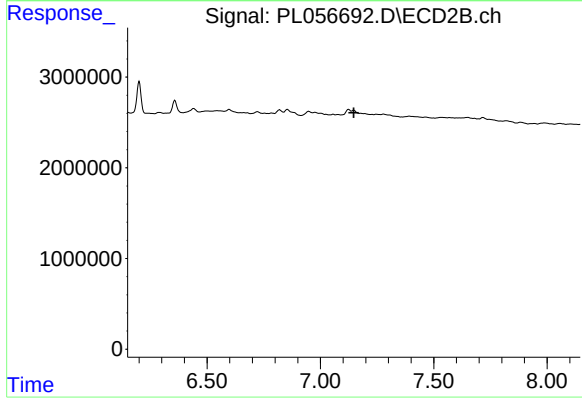

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T. : 7.148 min
Response: 0
Conc: N.D.

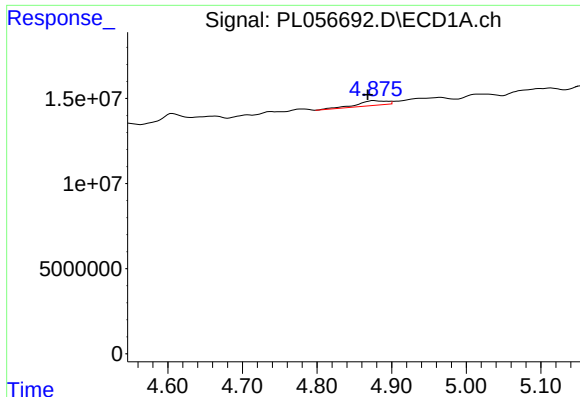

#24 Chlordane-2


R.T.: 4.877 min
Delta R.T.: 0.009 min
Response: 8432764
Conc: 21.62 ng/ml

Instrument :
ECD_L
ClientSampleId :

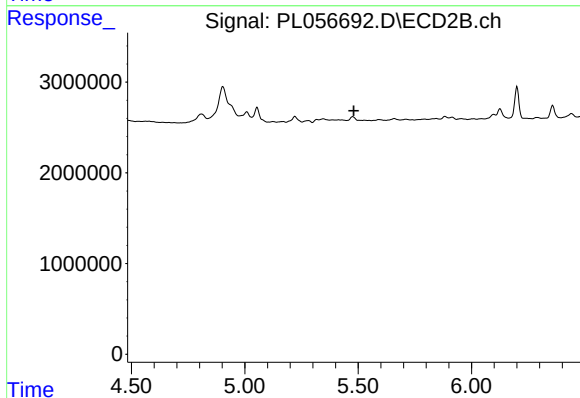


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 5.480 min
Response: 0
Conc: N.D.

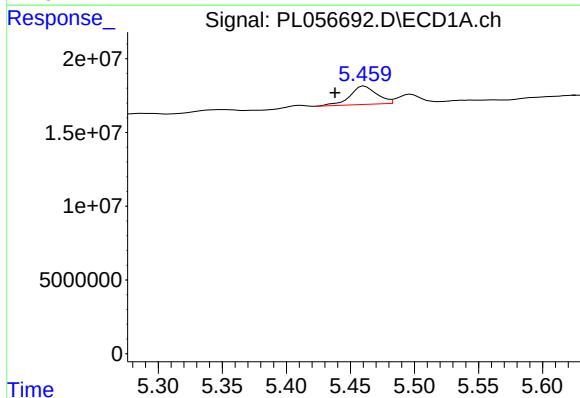


#25 Chlordane-3

R.T.: 5.461 min
Delta R.T.: 0.023 min
Response: 18134137
Conc: 14.42 ng/ml

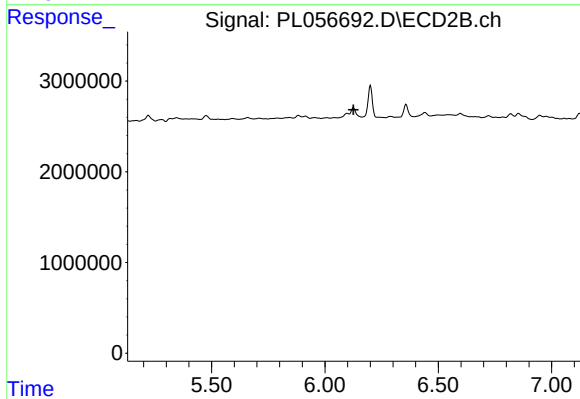

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T. : 6.126 min
Response: 0
Conc: N.D.

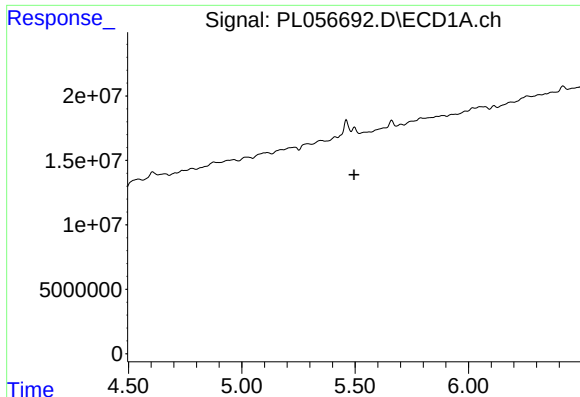

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 5.495 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

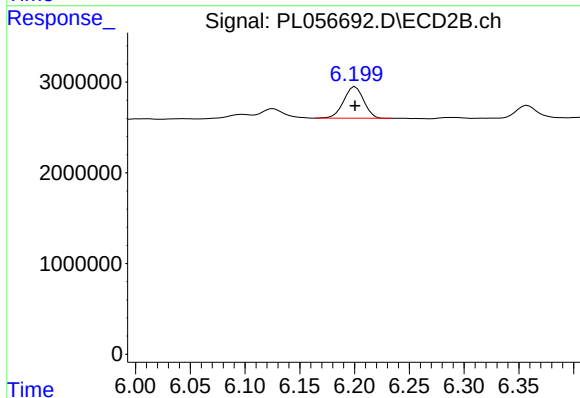


#26 Chlordane-4

R.T.: 6.201 min
Delta R.T.: 0.000 min
Response: 4425204
Conc: 10.31 ng/ml

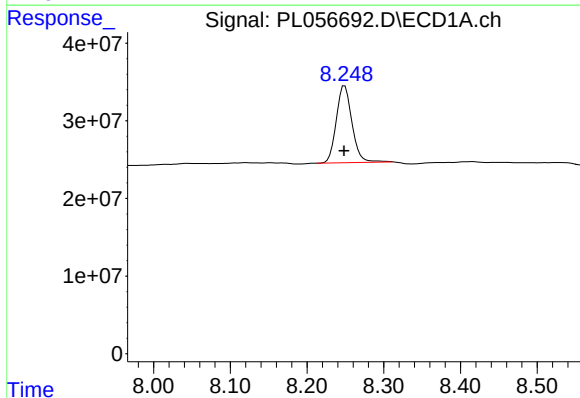

#28 Decachlorobiphenyl

R.T.: 8.249 min
Delta R.T.: 0.000 min
Response: 141385542
Conc: 11.89 ng/ml

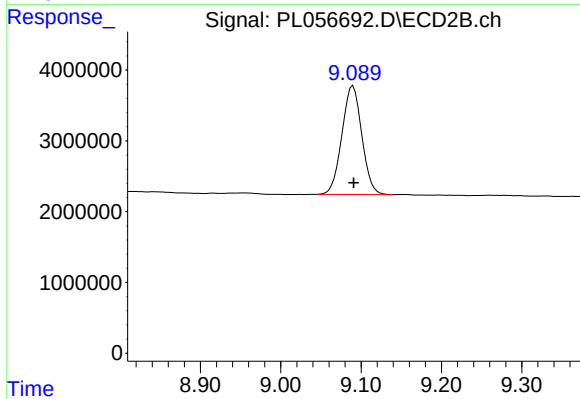

#28 Decachlorobiphenyl

R.T.: 9.090 min
Delta R.T.: -0.001 min
Response: 26436944
Conc: 12.58 ng/ml