

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022020\
 Data File : PL056697.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Feb 2020 15:17
 Operator : AJ\MA
 Sample : L1587-02
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 21 00:29:25 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL021920.M
 Quant Title : GC Extractables
 QLast Update : Thu Feb 20 02:32:45 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.498	4.019	186.4E6	55059081	21.550	22.103
28)	SA Decachlor...	8.250	9.090	197.0E6	37688319	16.560	17.936
Target Compounds							
12)	B 4,4'-DDE	5.661	0.000	21037038	0	1.496	N.D. #
13)	MA Dieldrin	5.812f	0.000	16095277	0	1.080	N.D. #
15)	B Endosulfa...	6.308f	0.000	13898971	0	1.119	N.D. #
17)	MA 4,4'-DDT	6.416	0.000	26471748	0	2.431	N.D. #
18)	B Endrin al...	6.493	0.000	10489855	0	0.969	N.D. #
27)	Chlordane-5	6.308f	0.000	13898971	0	42.448	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022020\
Data File : PL056697.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Feb 2020 15:17
Operator : AJ\MA
Sample : L1587-02
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 21 00:29:25 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL021920.M
Quant Title : GC Extractables
QLast Update : Thu Feb 20 02:32:45 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

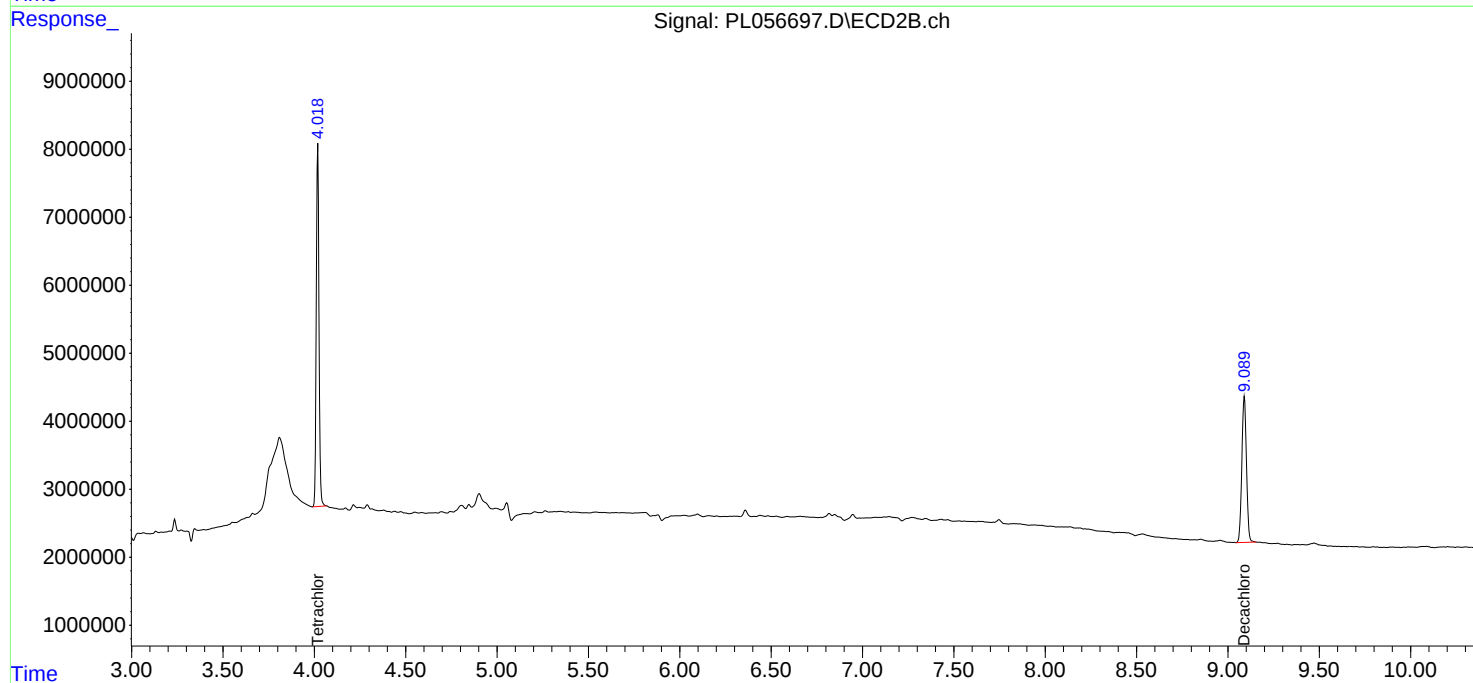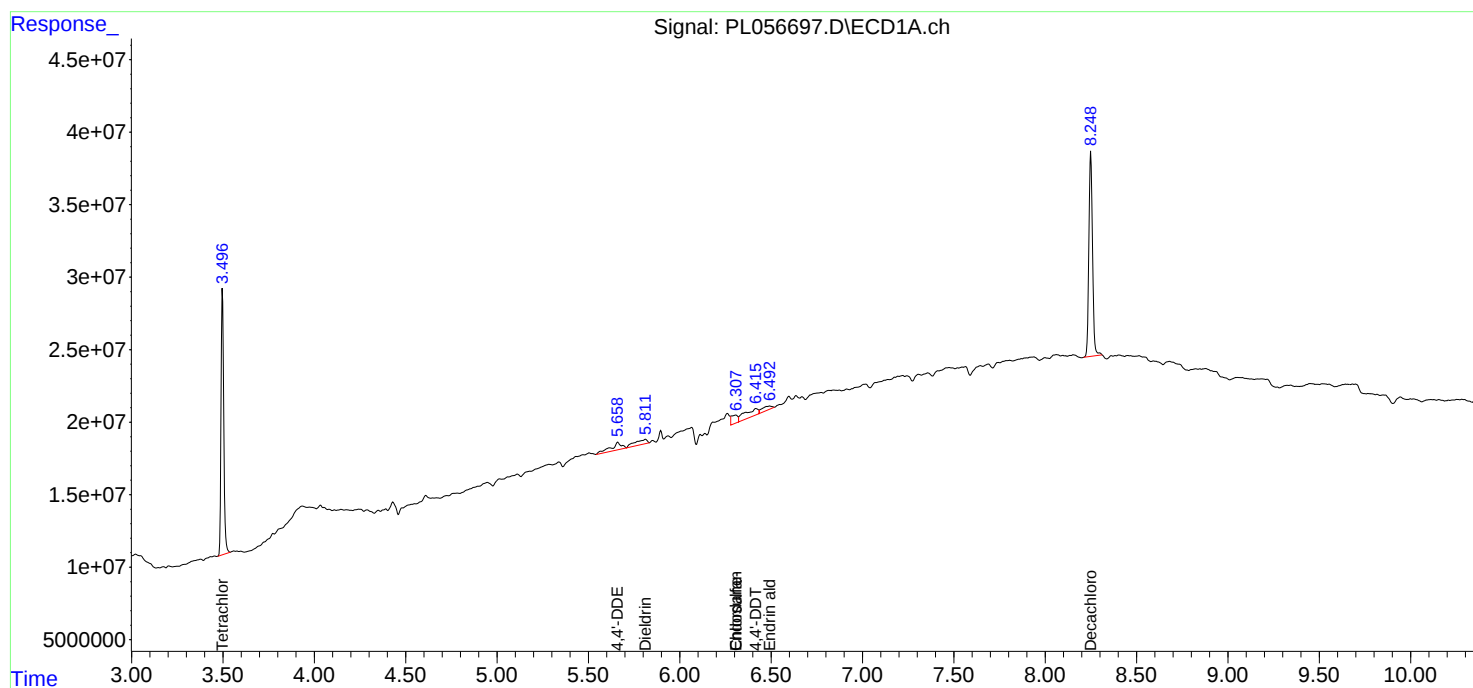


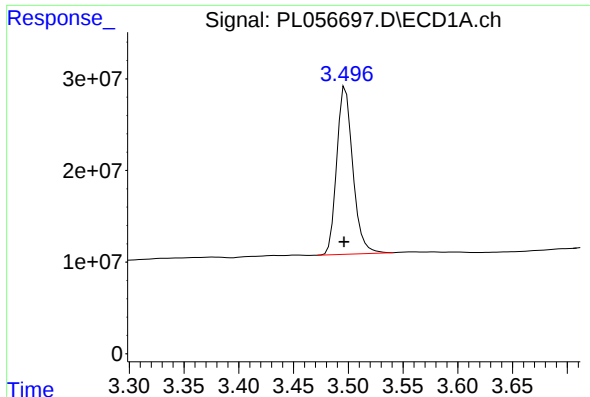

#1 Tetrachloro-m-xylene


R.T.: 3.498 min
Delta R.T.: 0.002 min
Response: 186352996
Conc: 21.55 ng/ml

Instrument :
ECD_L
ClientSampleId :

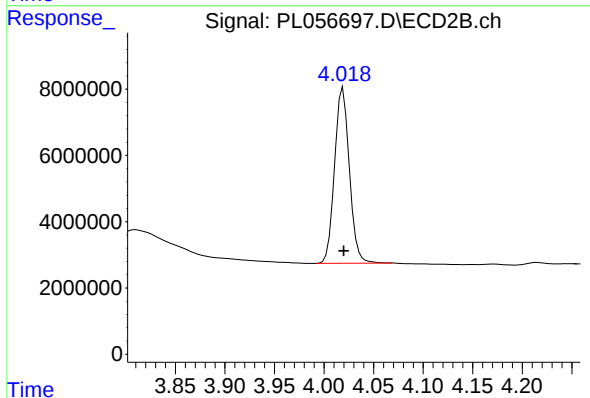


#1 Tetrachloro-m-xylene

R.T.: 4.019 min
Delta R.T.: 0.000 min
Response: 55059081
Conc: 22.10 ng/ml

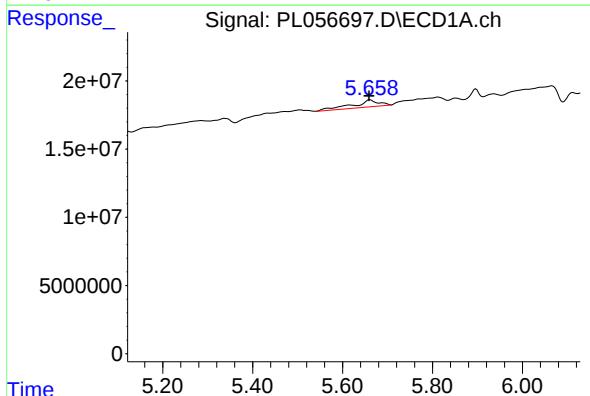


#12 4,4'-DDE

R.T.: 5.661 min
Delta R.T.: 0.002 min
Response: 21037038
Conc: 1.50 ng/ml

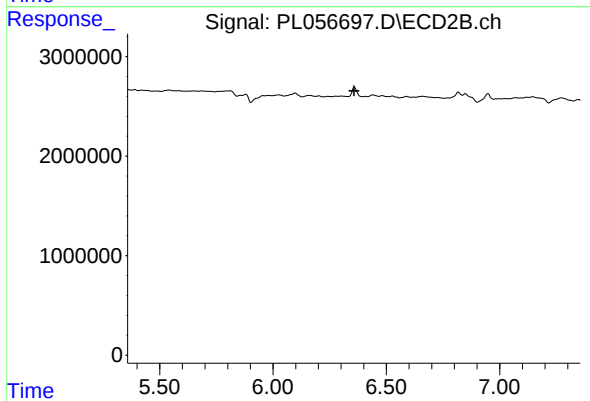

#12 4,4'-DDE


R.T.: 0.000 min
Exp R.T.: 6.358 min
Response: 0
Conc: N.D.

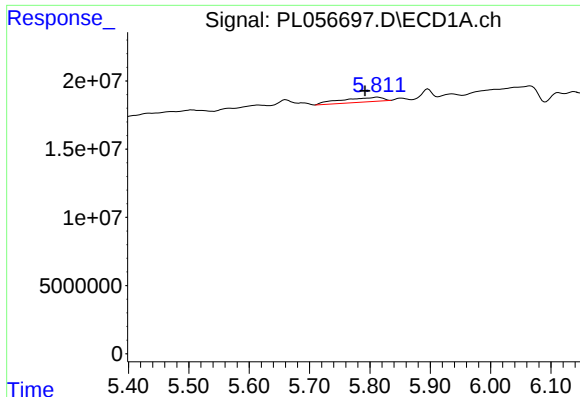

#13 Dieldrin


R.T.: 5.812 min
Delta R.T.: 0.020 min
Response: 16095277
Conc: 1.08 ng/ml

Instrument :
ECD_L
ClientSampleId :

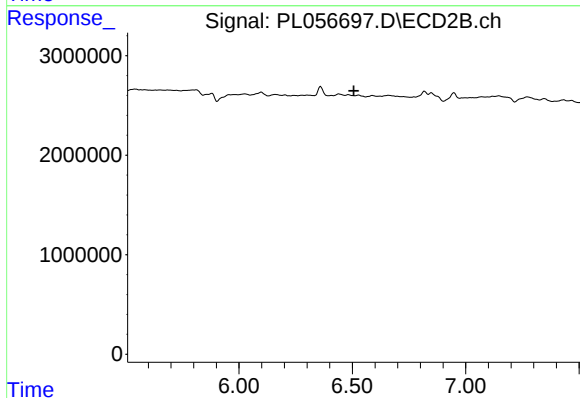


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 6.506 min
Response: 0
Conc: N.D.

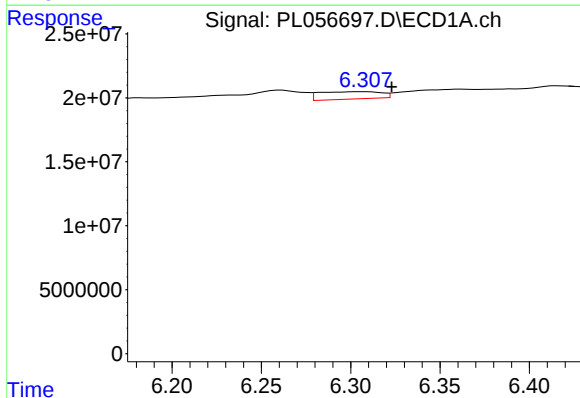


#15 Endosulfan II

R.T.: 6.308 min
Delta R.T.: -0.015 min
Response: 13898971
Conc: 1.12 ng/ml

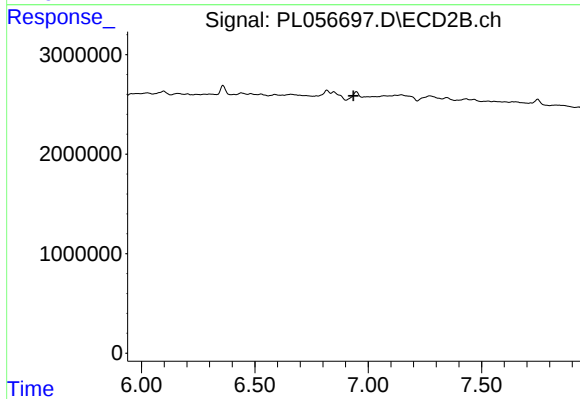

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T. : 6.936 min
Response: 0
Conc: N.D.

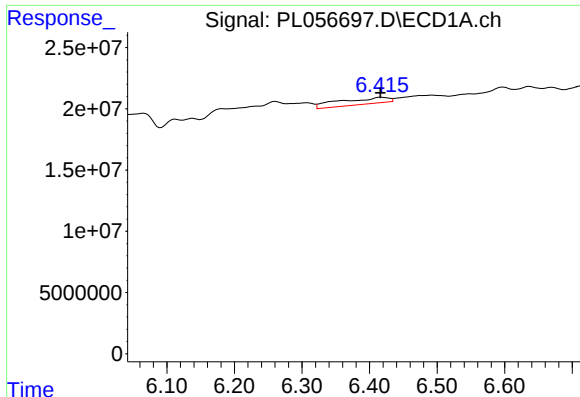

#17 4,4'-DDT


R.T.: 6.416 min
Delta R.T.: 0.000 min
Response: 26471748
Conc: 2.43 ng/ml

Instrument :
ECD_L
ClientSampleId :

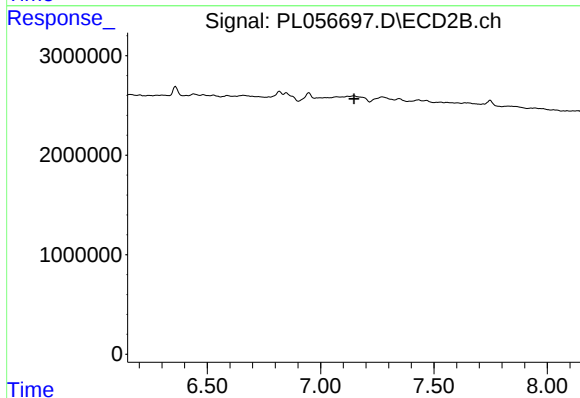


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 7.148 min
Response: 0
Conc: N.D.

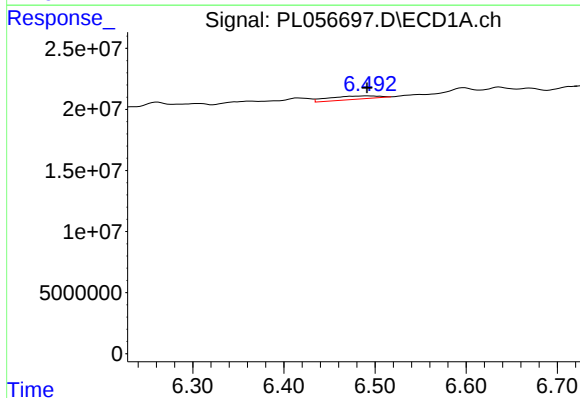


#18 Endrin aldehyde

R.T.: 6.493 min
Delta R.T.: 0.002 min
Response: 10489855
Conc: 0.97 ng/ml

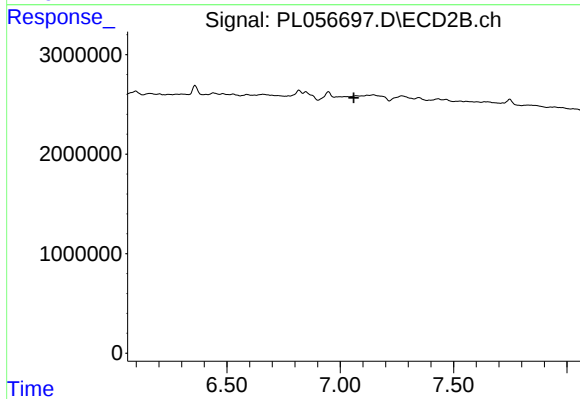

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T. : 7.060 min
Response: 0
Conc: N.D.

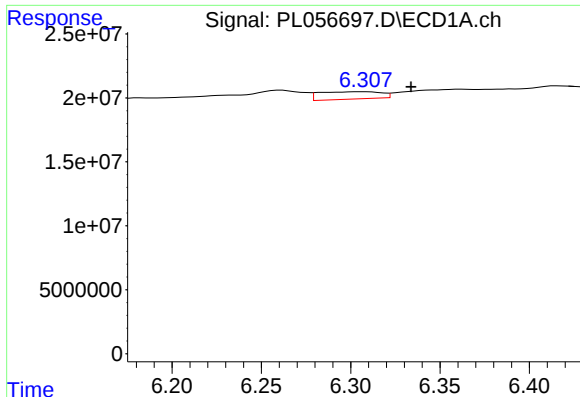

#27 Chlordane-5


R.T.: 6.308 min
Delta R.T.: -0.026 min
Response: 13898971
Conc: 42.45 ng/ml

Instrument :
ECD_L
ClientSampleId :

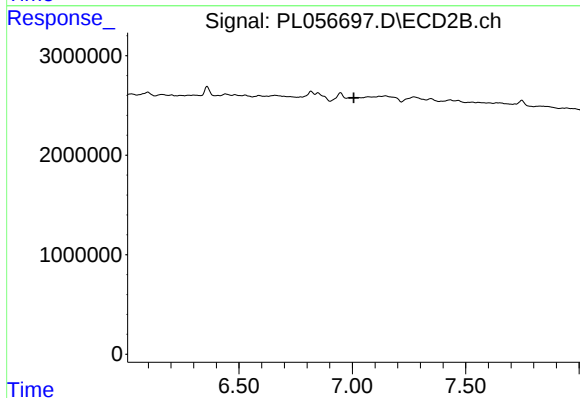


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 7.007 min
Response: 0
Conc: N.D.

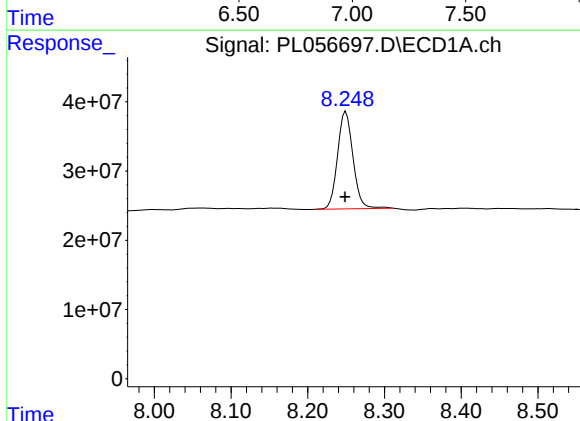

#28 Decachlorobiphenyl

R.T.: 8.250 min
Delta R.T.: 0.001 min
Response: 196984917
Conc: 16.56 ng/ml

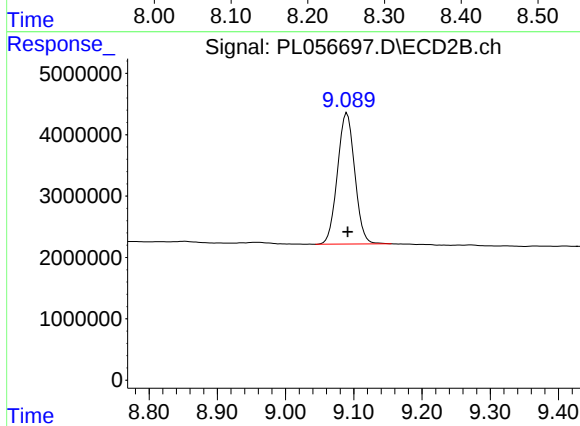

#28 Decachlorobiphenyl

R.T.: 9.090 min
Delta R.T.: 0.000 min
Response: 37688319
Conc: 17.94 ng/ml