

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022020\
 Data File : PL056704.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Feb 2020 16:55
 Operator : AJ\MA
 Sample : L1586-02
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 21 00:30:53 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL021920.M
 Quant Title : GC Extractables
 QLast Update : Thu Feb 20 02:32:45 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.498	4.019	186.6E6	55213773	21.584	22.165
28)	SA Decachlor...	8.250	9.090	167.3E6	33394198	14.063	15.892
Target Compounds							
4)	MA Heptachlor	4.548f	0.000	9847667	0	0.668	N.D. #
8)	B Heptachlo...	5.216	0.000	12007801	0	0.849	N.D. #
10)	B gamma-Chl...	0.000	6.108f	0	19613103	N.D.	6.838 #
13)	MA Dieldrin	5.795	0.000	7870905	0	0.528	N.D. #
15)	B Endosulfa...	6.294f	0.000	135.1E6	0	10.878	N.D. #
16)	A 4,4'-DDD	6.181	0.000	148.9E6	0	13.311	N.D. #
17)	MA 4,4'-DDT	6.418	0.000	67906297	0	6.235	N.D. #
24)	Chlordane-2	4.877	0.000	38323200	0	98.244	N.D. #
25)	Chlordane-3	0.000	6.108f	0	19613103	N.D.	53.108 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022020\
Data File : PL056704.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Feb 2020 16:55
Operator : AJ\MA
Sample : L1586-02
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 21 00:30:53 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL021920.M
Quant Title : GC Extractables
QLast Update : Thu Feb 20 02:32:45 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

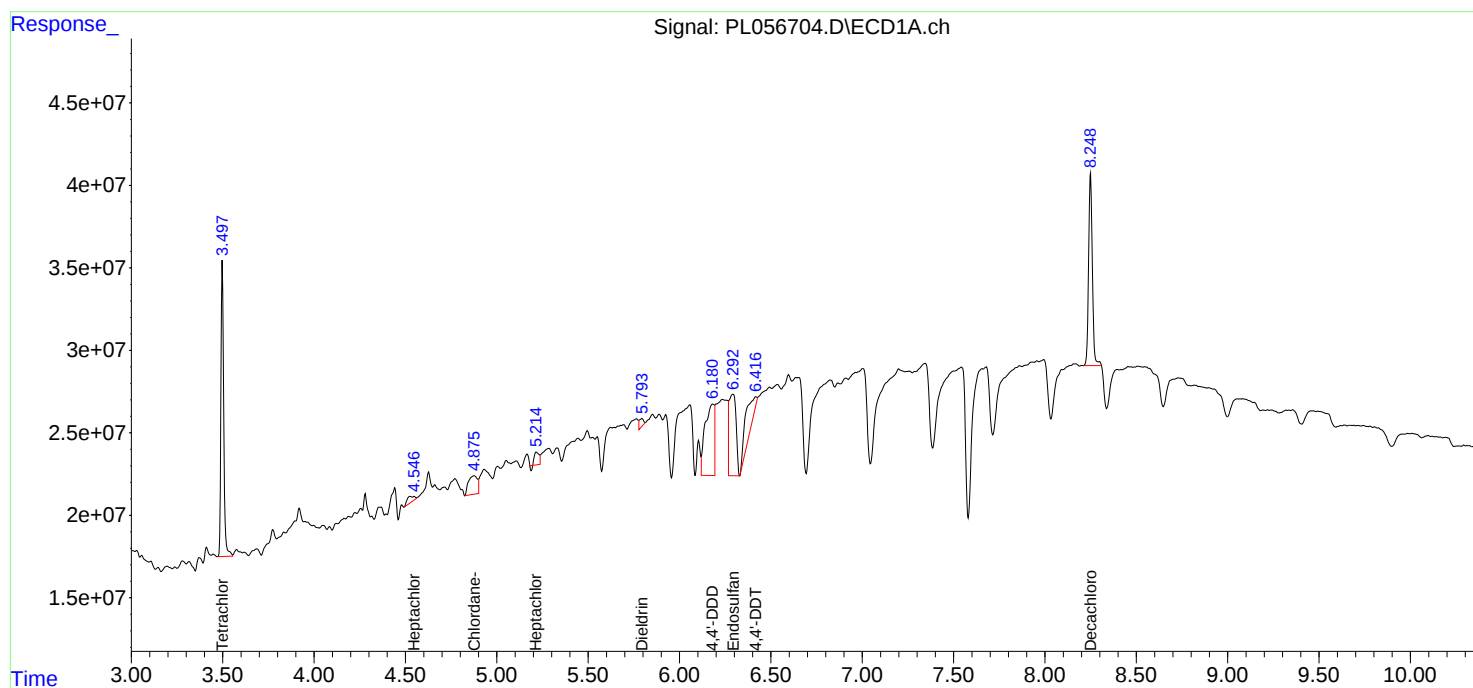


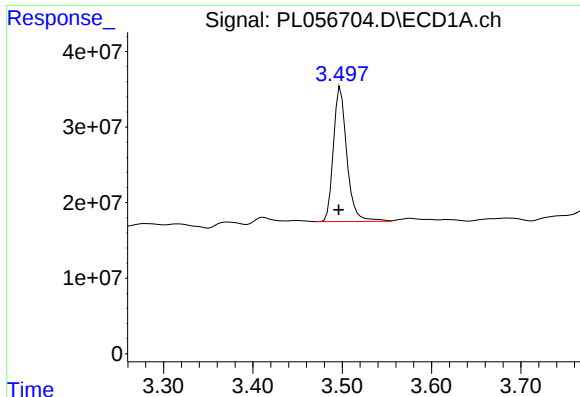

#1 Tetrachloro-m-xylene


R.T.: 3.498 min
Delta R.T.: 0.002 min
Response: 186647889
Conc: 21.58 ng/ml

Instrument :
ECD_L
ClientSampleId :

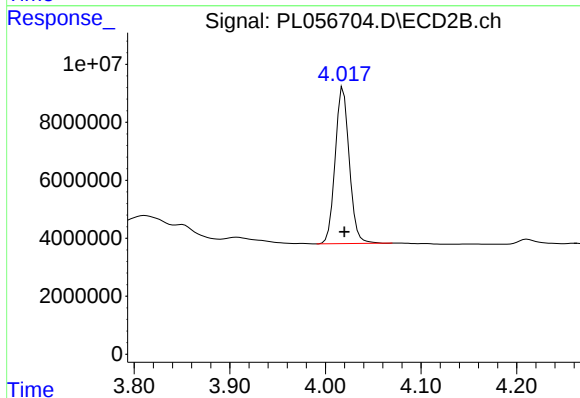


#1 Tetrachloro-m-xylene

R.T.: 4.019 min
Delta R.T.: -0.001 min
Response: 55213773
Conc: 22.17 ng/ml

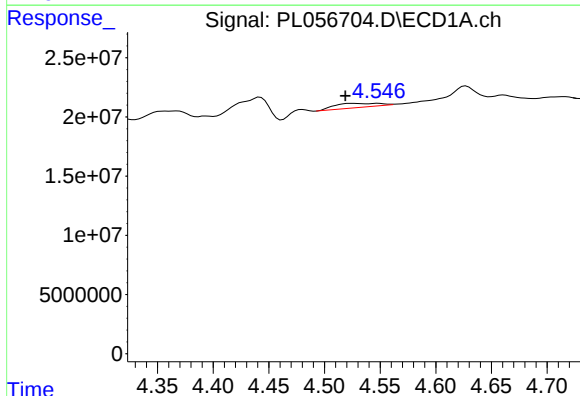


#4 Heptachlor

R.T.: 4.548 min
Delta R.T.: 0.030 min
Response: 9847667
Conc: 0.67 ng/ml

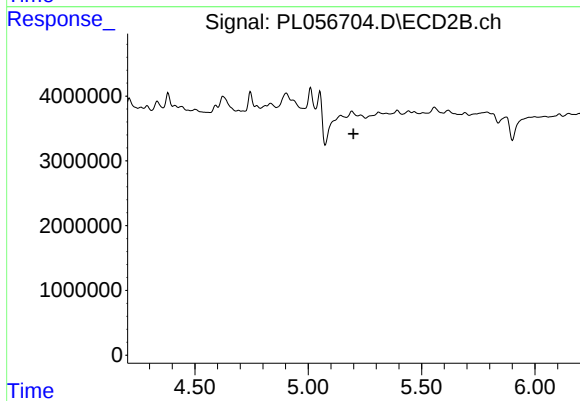

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 5.200 min
Response: 0
Conc: N.D.

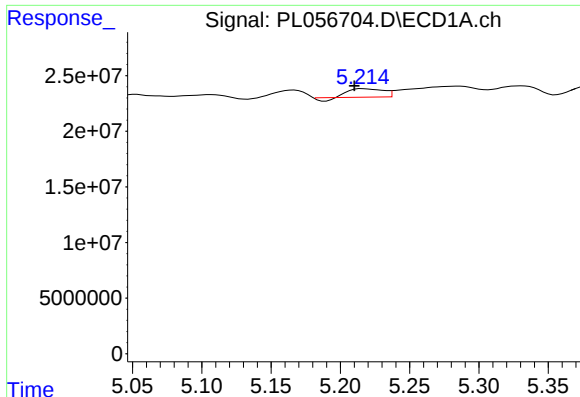

#8 Heptachlor epoxide


R.T.: 5.216 min
Delta R.T.: 0.006 min
Response: 12007801
Conc: 0.85 ng/ml

Instrument :
ECD_L
ClientSampleId :

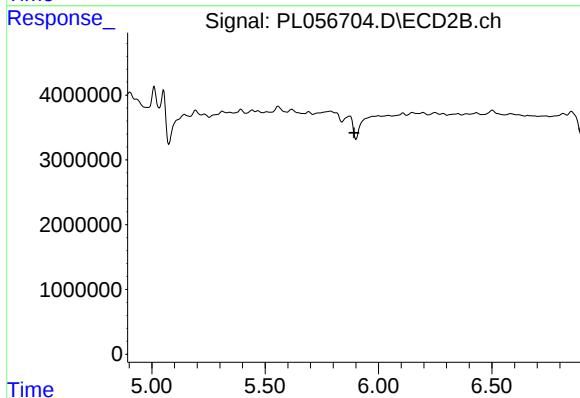


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.892 min
Response: 0
Conc: N.D.

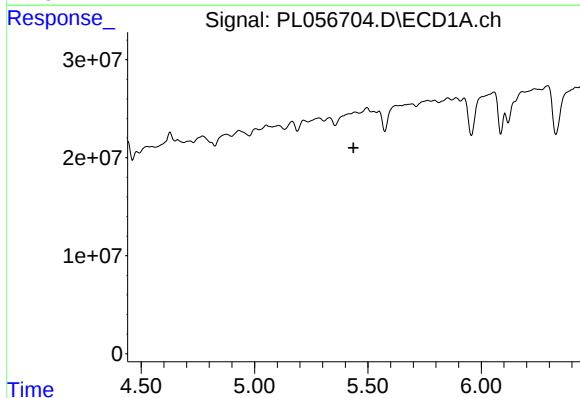


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.437 min
Response: 0
Conc: N.D.

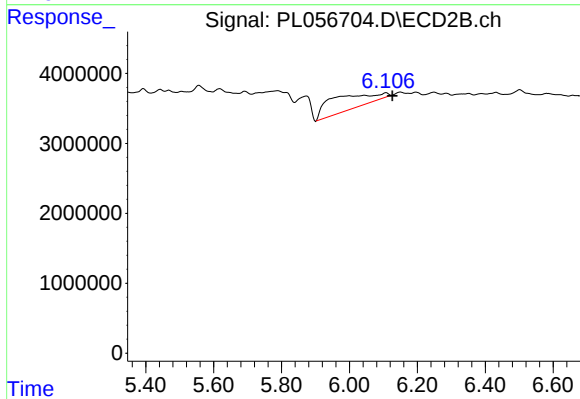

#10 gamma-Chlordane


R.T.: 6.108 min
Delta R.T.: -0.018 min
Response: 19613103
Conc: 6.84 ng/ml

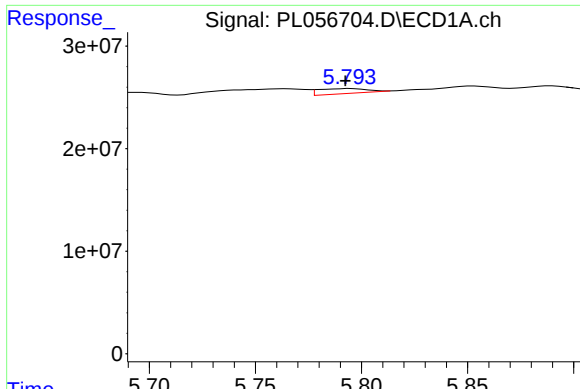

#13 Dieldrin


R.T.: 5.795 min
Delta R.T.: 0.003 min
Response: 7870905
Conc: 0.53 ng/ml

Instrument :
ECD_L
ClientSampleId :

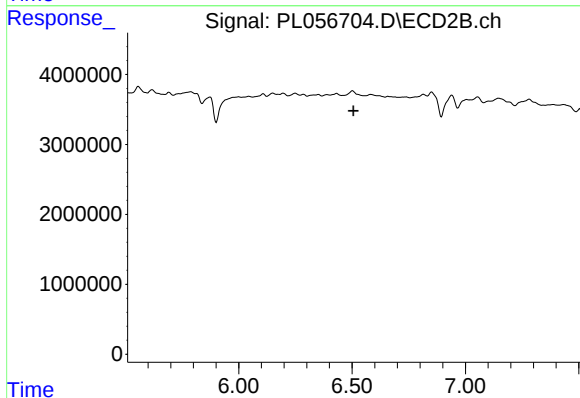


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 6.506 min
Response: 0
Conc: N.D.

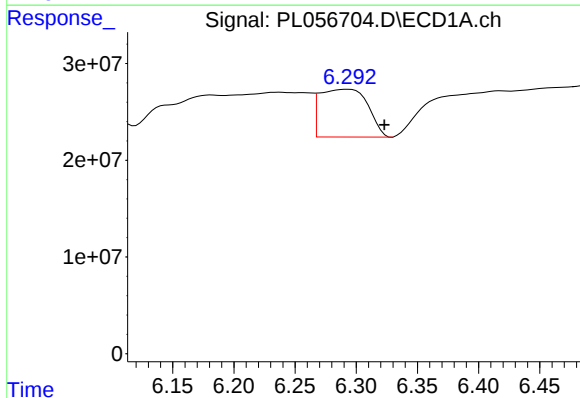


#15 Endosulfan II

R.T.: 6.294 min
Delta R.T.: -0.029 min
Response: 135093753
Conc: 10.88 ng/ml

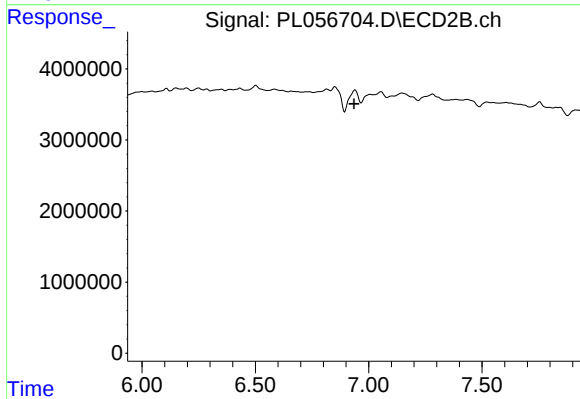

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T. : 6.936 min
Response: 0
Conc: N.D.

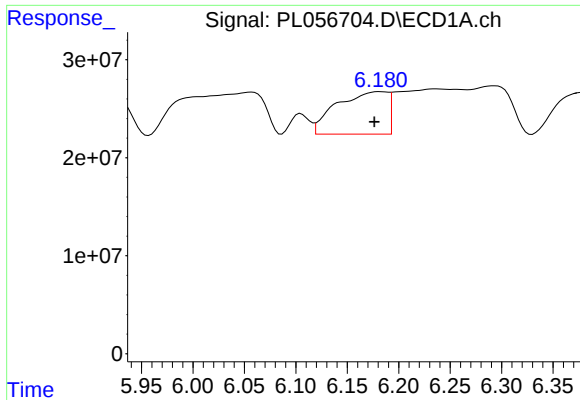

#16 4,4'-DDD


R.T.: 6.181 min
Delta R.T.: 0.005 min
Response: 148892000
Conc: 13.31 ng/ml

Instrument :
ECD_L
ClientSampleId :

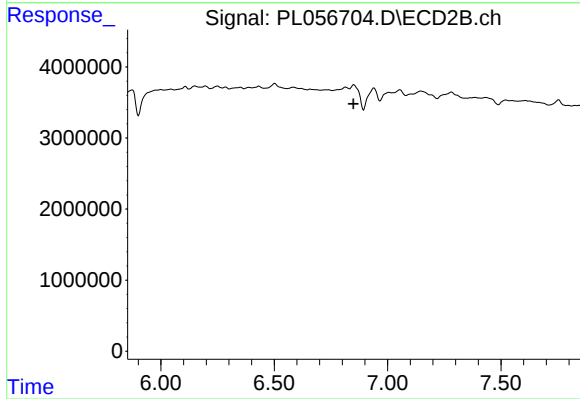


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 6.850 min
Response: 0
Conc: N.D.

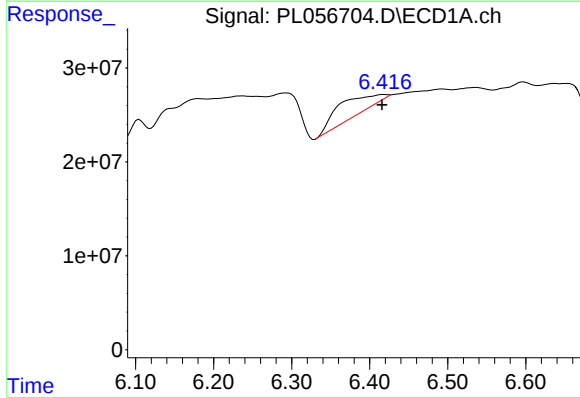


#17 4,4'-DDT

R.T.: 6.418 min
Delta R.T.: 0.002 min
Response: 67906297
Conc: 6.24 ng/ml

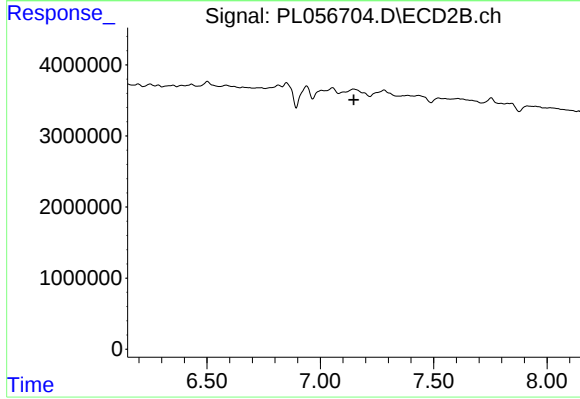

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T. : 7.148 min
Response: 0
Conc: N.D.

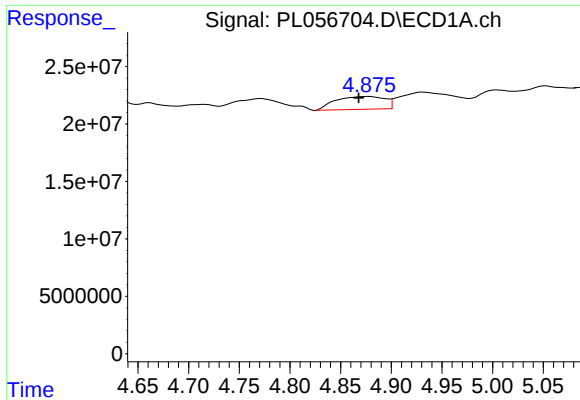

#24 Chlordane-2


R.T.: 4.877 min
Delta R.T.: 0.009 min
Response: 38323200
Conc: 98.24 ng/ml

Instrument :
ECD_L
ClientSampleId :

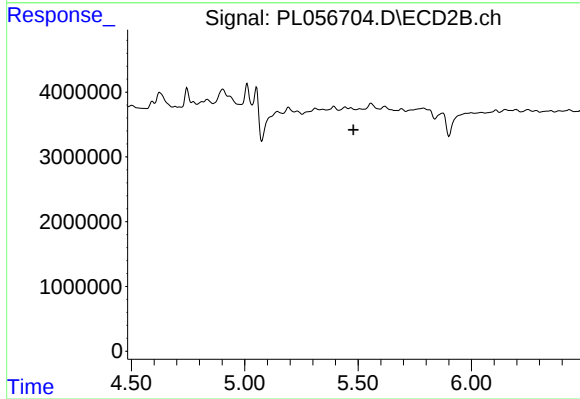


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 5.480 min
Response: 0
Conc: N.D.

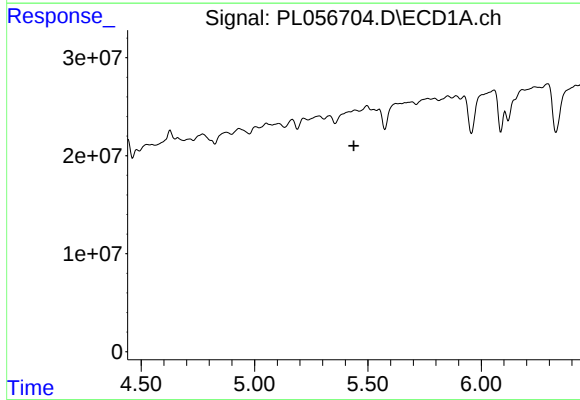


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 5.438 min
Response: 0
Conc: N.D.

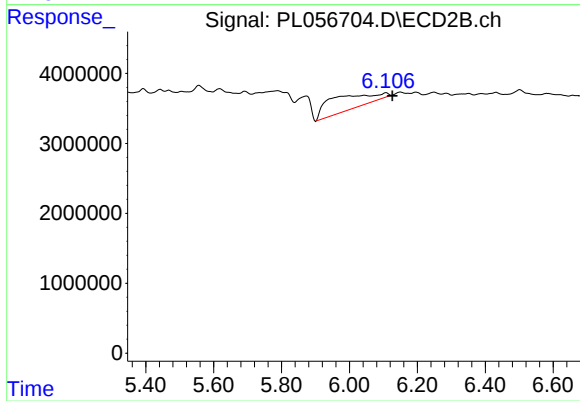

#25 Chlordane-3


R.T.: 6.108 min
Delta R.T.: -0.018 min
Response: 19613103
Conc: 53.11 ng/ml

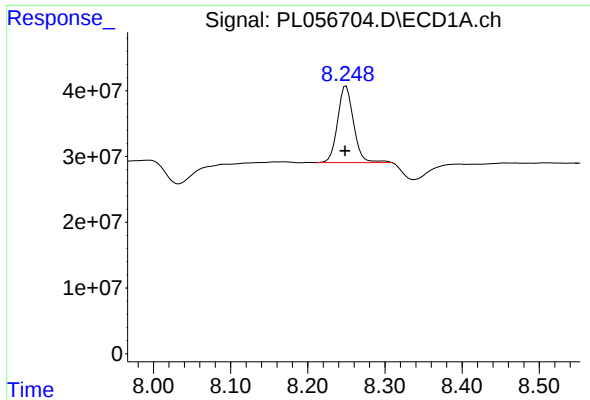

#28 Decachlorobiphenyl

R.T.: 8.250 min
Delta R.T.: 0.001 min
Response: 167281166
Conc: 14.06 ng/ml

Instrument :
ECD_L
ClientSampleId :

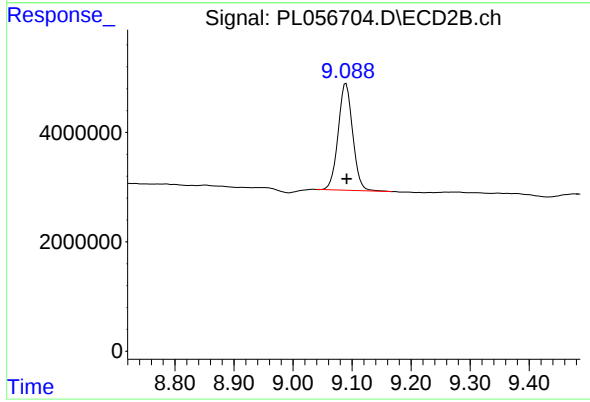

#28 Decachlorobiphenyl

R.T.: 9.090 min
Delta R.T.: -0.001 min
Response: 33394198
Conc: 15.89 ng/ml