

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022020\
 Data File : PL056707.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Feb 2020 17:38
 Operator : AJ\MA
 Sample : L1578-02
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 21 00:31:24 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL021920.M
 Quant Title : GC Extractables
 QLast Update : Thu Feb 20 02:32:45 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.498	4.019	162.1E6	48749695	18.742	19.570
28)	SA Decachlor...	8.250	9.089	174.2E6	34701043	14.644	16.514
Target Compounds							
4)	MA Heptachlor	4.526	0.000	11828893	0	0.802	N.D. #
11)	B alpha-Chl...	5.492	0.000	27989904	0	1.938	N.D. #
12)	B 4,4'-DDE	5.688f	0.000	12585907	0	0.895	N.D. #
15)	B Endosulfa...	6.335	0.000	11733444	0	0.945	N.D. #
16)	A 4,4'-DDD	6.191	0.000	29722572	0	2.657	N.D. #
18)	B Endrin al...	6.468f	0.000	24875035	0	2.298	N.D. #
24)	Chlordane-2	4.849f	0.000	7381435	0	18.923	N.D. #
26)	Chlordane-4	5.492	0.000	27989904	0	26.056	N.D. #
27)	Chlordane-5	6.335	0.000	11733444	0	35.834	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022020\
Data File : PL056707.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Feb 2020 17:38
Operator : AJ\MA
Sample : L1578-02
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 21 00:31:24 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL021920.M
Quant Title : GC Extractables
QLast Update : Thu Feb 20 02:32:45 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

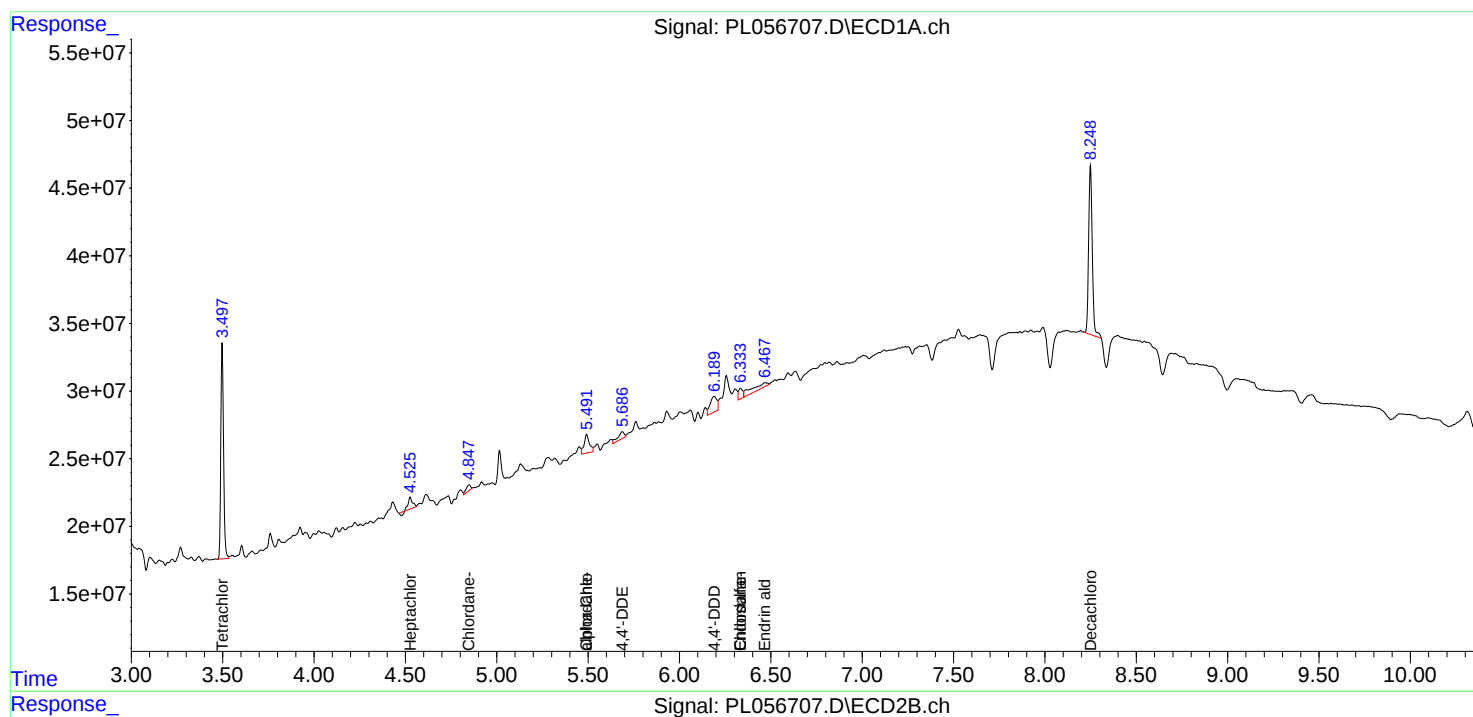


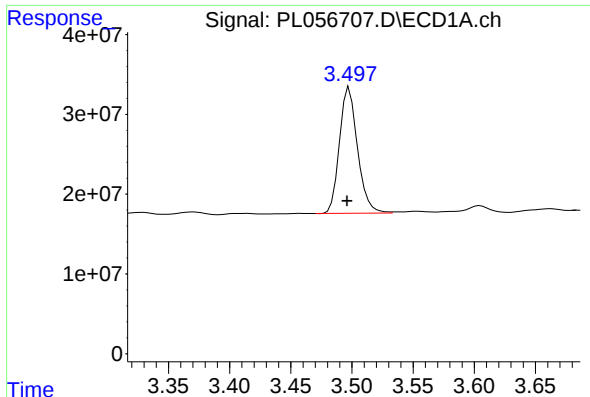

#1 Tetrachloro-m-xylene


R.T.: 3.498 min
Delta R.T.: 0.002 min
Response: 162076421
Conc: 18.74 ng/ml

Instrument :
ECD_L
ClientSampleId :

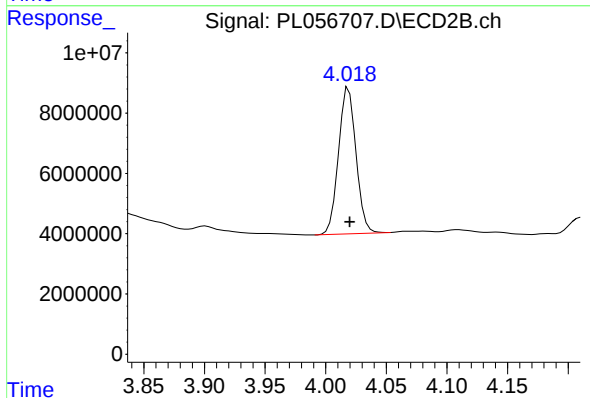


#1 Tetrachloro-m-xylene

R.T.: 4.019 min
Delta R.T.: 0.000 min
Response: 48749695
Conc: 19.57 ng/ml

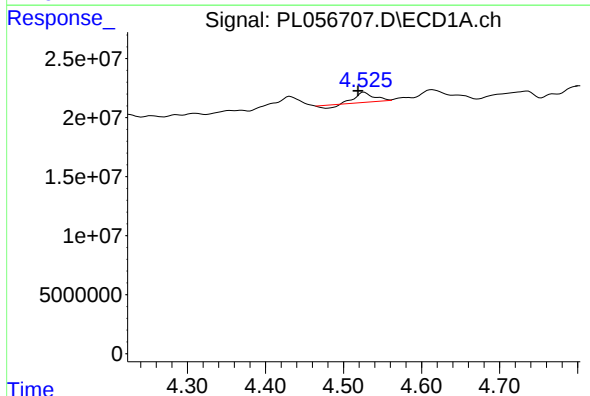


#4 Heptachlor

R.T.: 4.526 min
Delta R.T.: 0.008 min
Response: 11828893
Conc: 0.80 ng/ml

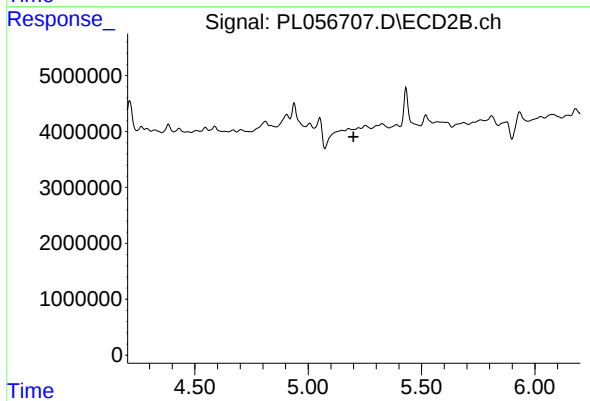

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 5.200 min
Response: 0
Conc: N.D.

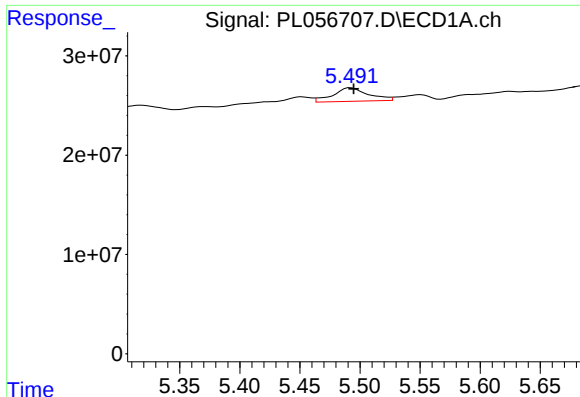

#11 alpha-Chlordane


R.T.: 5.492 min
Delta R.T.: -0.003 min
Response: 27989904
Conc: 1.94 ng/ml

Instrument :
ECD_L
ClientSampleId :

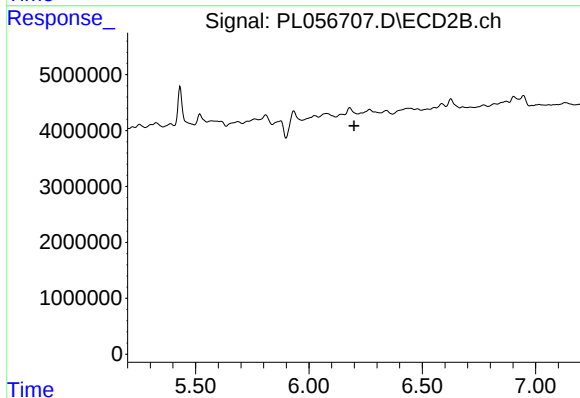


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.199 min
Response: 0
Conc: N.D.

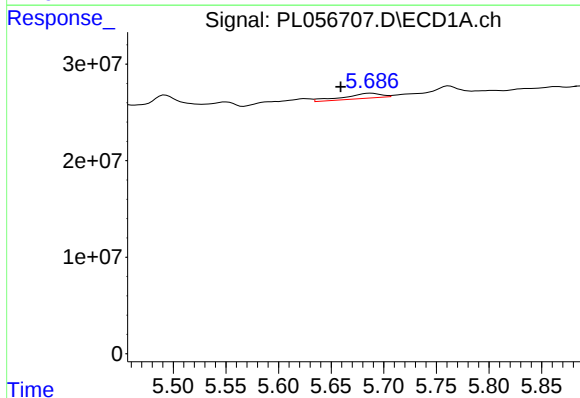


#12 4,4'-DDE

R.T.: 5.688 min
Delta R.T.: 0.029 min
Response: 12585907
Conc: 0.89 ng/ml

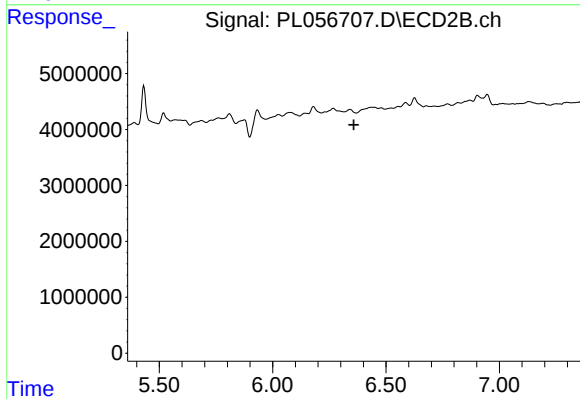

#12 4,4'-DDE


R.T.: 0.000 min
Exp R.T. : 6.358 min
Response: 0
Conc: N.D.

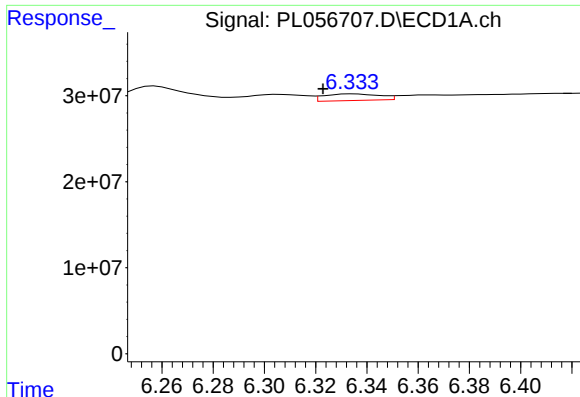

#15 Endosulfan II


R.T.: 6.335 min
Delta R.T.: 0.012 min
Response: 11733444
Conc: 0.94 ng/ml

Instrument :
ECD_L
ClientSampleId :

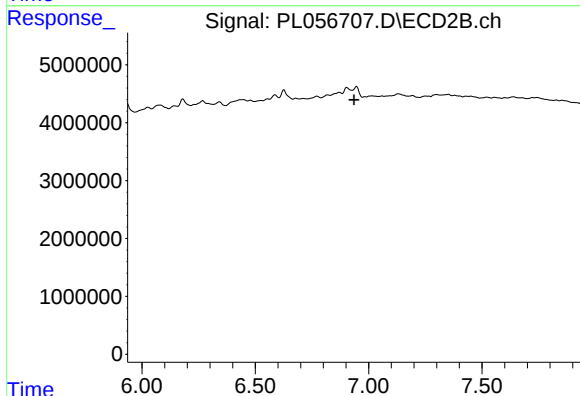


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.936 min
Response: 0
Conc: N.D.

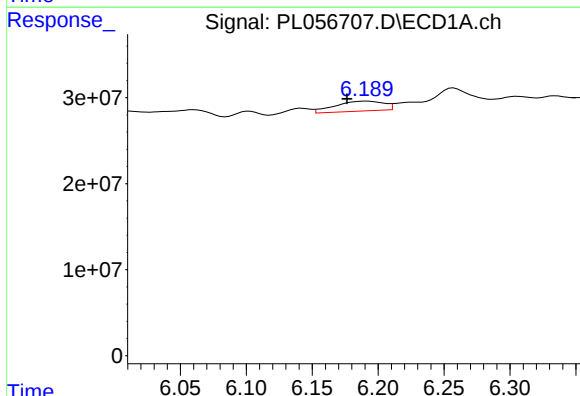


#16 4,4'-DDD

R.T.: 6.191 min
Delta R.T.: 0.014 min
Response: 29722572
Conc: 2.66 ng/ml

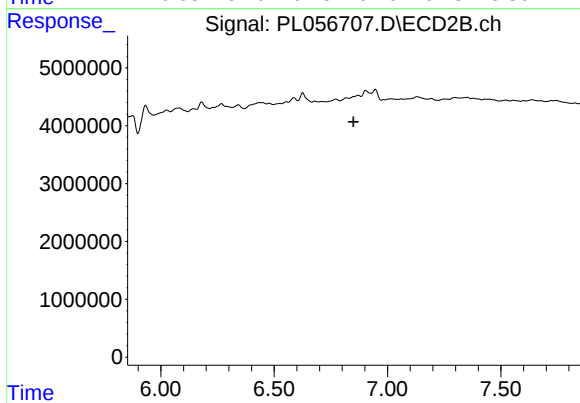

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T. : 6.850 min
Response: 0
Conc: N.D.

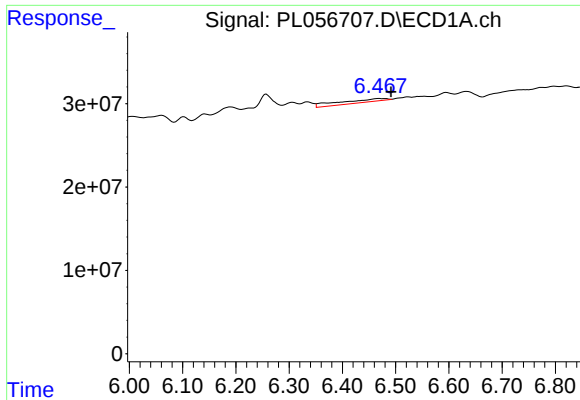

#18 Endrin aldehyde


R.T.: 6.468 min
Delta R.T.: -0.023 min
Response: 24875035
Conc: 2.30 ng/ml

Instrument :
ECD_L
ClientSampleId :

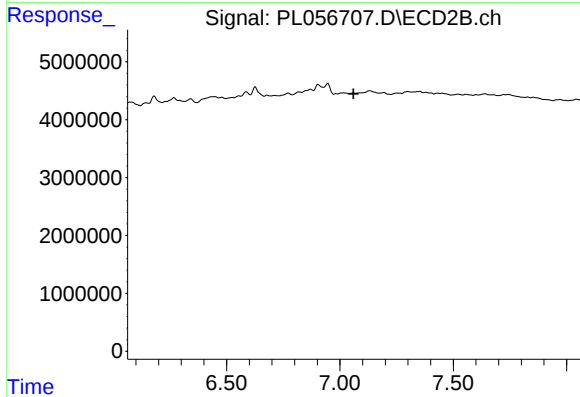


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T. : 7.060 min
Response: 0
Conc: N.D.

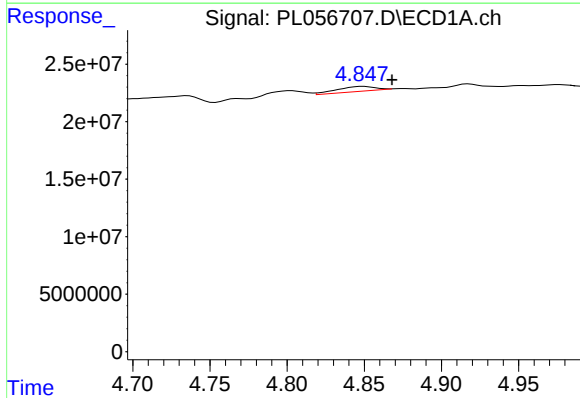


#24 Chlordane-2

R.T.: 4.849 min
Delta R.T.: -0.019 min
Response: 7381435
Conc: 18.92 ng/ml

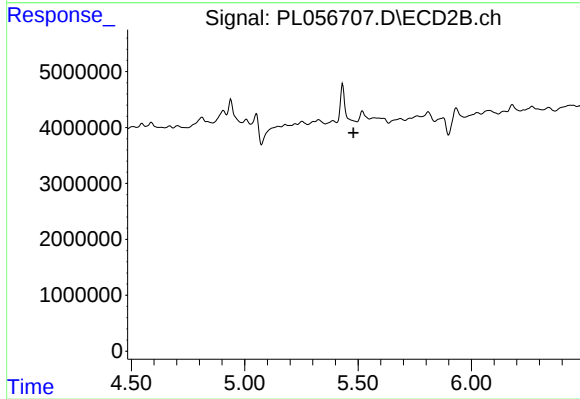

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T. : 5.480 min
Response: 0
Conc: N.D.

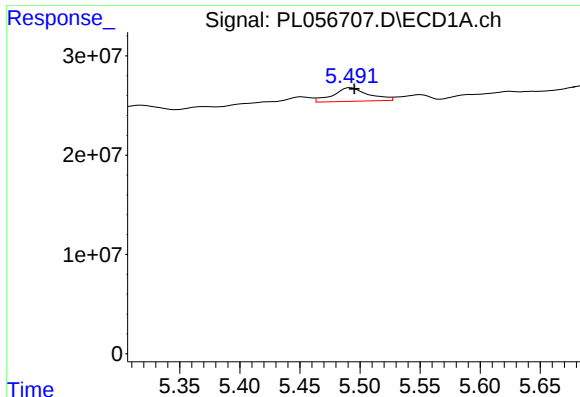

#26 Chlordane-4


R.T.: 5.492 min
Delta R.T.: -0.003 min
Response: 27989904
Conc: 26.06 ng/ml

Instrument :
ECD_L
ClientSampleId :

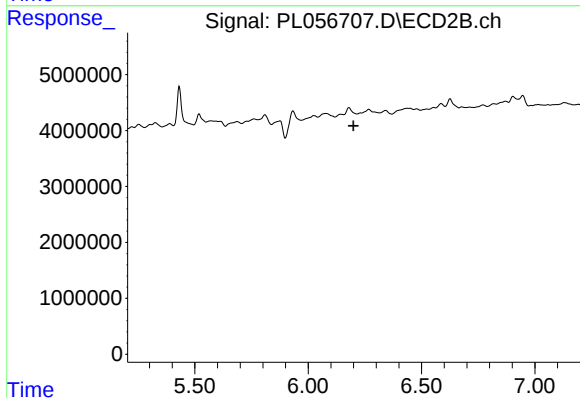


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 6.200 min
Response: 0
Conc: N.D.

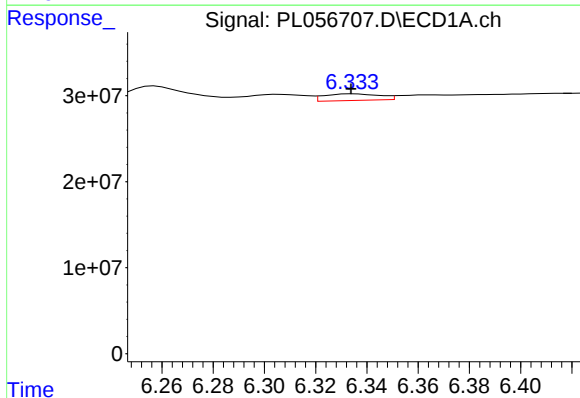


#27 Chlordane-5

R.T.: 6.335 min
Delta R.T.: 0.000 min
Response: 11733444
Conc: 35.83 ng/ml

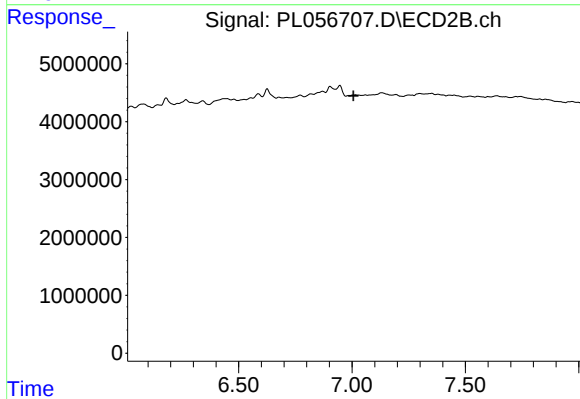

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T. : 7.007 min
Response: 0
Conc: N.D.

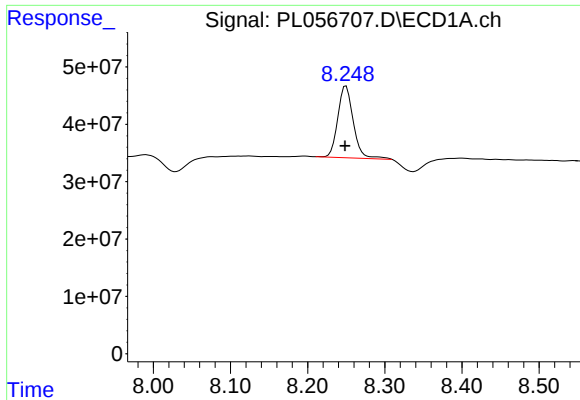

#28 Decachlorobiphenyl

R.T.: 8.250 min
Delta R.T.: 0.002 min
Response: 174193154
Conc: 14.64 ng/ml

Instrument :
ECD_L
ClientSampleId :

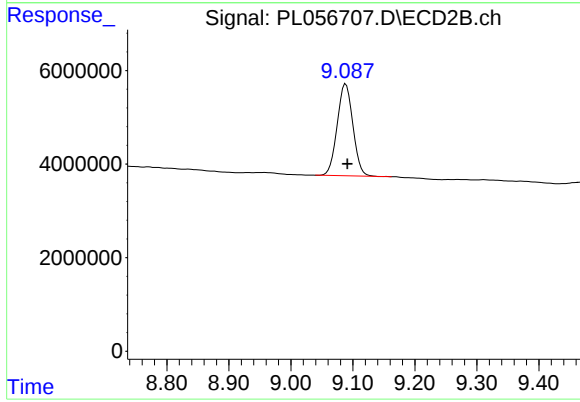

#28 Decachlorobiphenyl

R.T.: 9.089 min
Delta R.T.: -0.003 min
Response: 34701043
Conc: 16.51 ng/ml