

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022020\
 Data File : PL056708.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Feb 2020 17:52
 Operator : AJ\MA
 Sample : L1586-03
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 21 00:31:35 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL021920.M
 Quant Title : GC Extractables
 QLast Update : Thu Feb 20 02:32:45 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.497	4.019	150.0E6	45260816	17.349	18.170
28)	SA Decachlor...	8.250	9.090	133.5E6	25267632	11.220	12.025
Target Compounds							
10)	B gamma-Chl...	0.000	6.103f	0	26339499	N.D.	9.184 #
11)	B alpha-Chl...	0.000	6.171f	0	2656252	N.D.	0.934 #
13)	MA Dieldrin	5.789	0.000	7190049	0	0.482	N.D. #
15)	B Endosulfa...	6.307f	6.942	13017342	7907556	1.048	3.062 #
23)	Chlordane-1	4.352	0.000	45240352	0	124.186	N.D. #
24)	Chlordane-2	4.878	0.000	12139262	0	31.120	N.D. #
25)	Chlordane-3	0.000	6.103f	0	26339499	N.D.	71.321 #
26)	Chlordane-4	0.000	6.171f	0	2656252	N.D.	6.188 #
27)	Chlordane-5	6.340	0.000	19276058	0	58.869	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022020\
Data File : PL056708.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Feb 2020 17:52
Operator : AJ\MA
Sample : L1586-03
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 21 00:31:35 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL021920.M
Quant Title : GC Extractables
QLast Update : Thu Feb 20 02:32:45 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

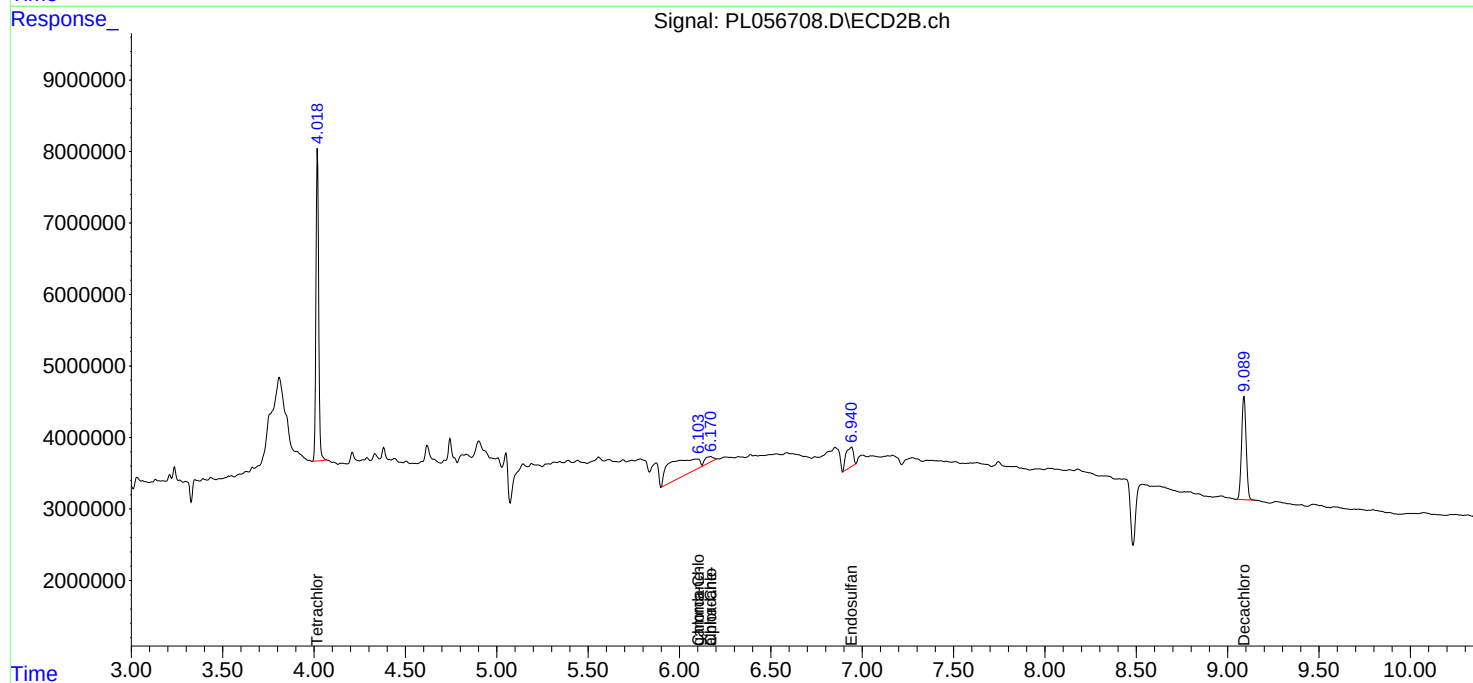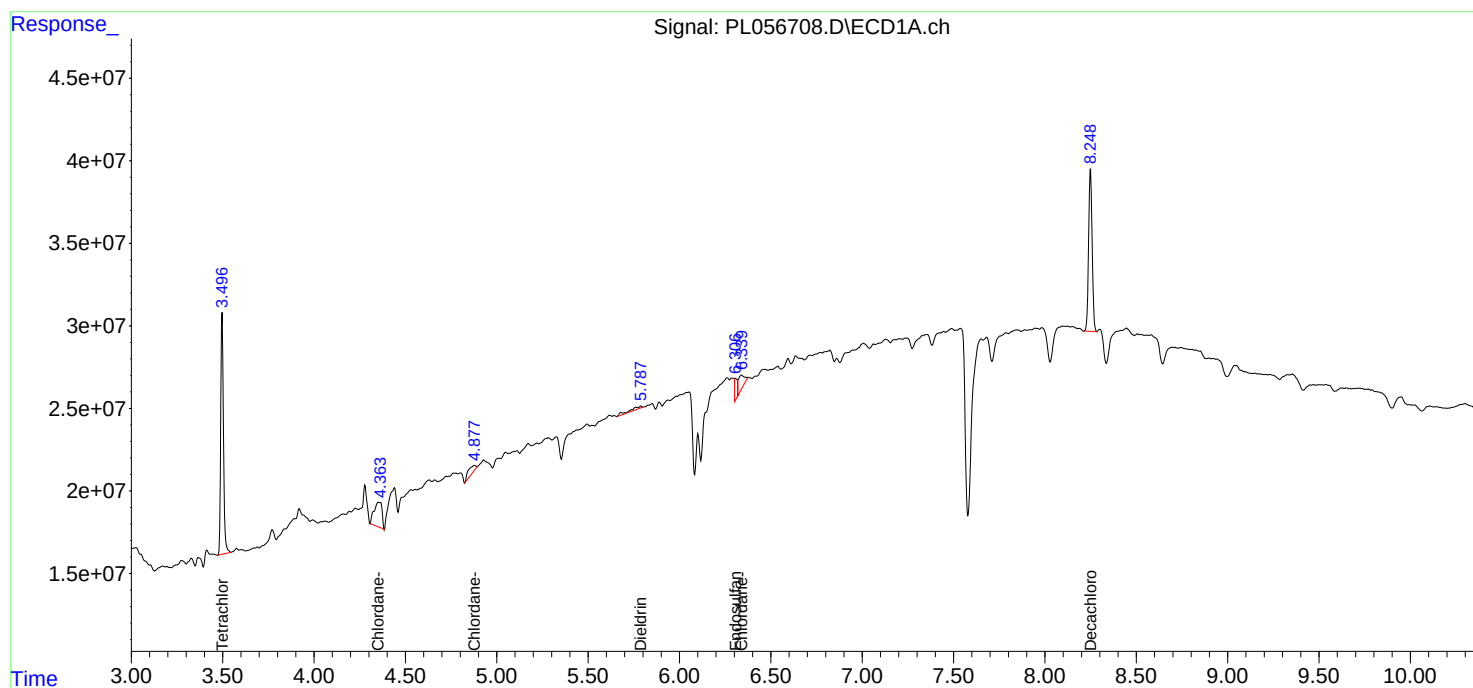


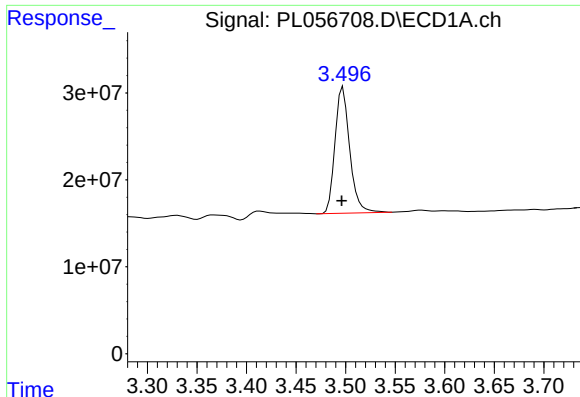

#1 Tetrachloro-m-xylene


R.T.: 3.497 min
Delta R.T.: 0.001 min
Response: 150028449
Conc: 17.35 ng/ml

Instrument :
ECD_L
ClientSampleId :

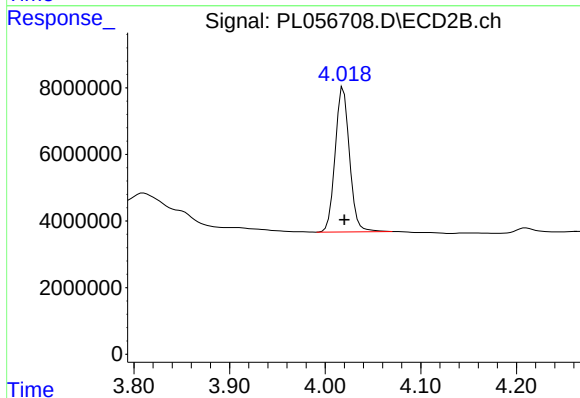


#1 Tetrachloro-m-xylene

R.T.: 4.019 min
Delta R.T.: 0.000 min
Response: 45260816
Conc: 18.17 ng/ml

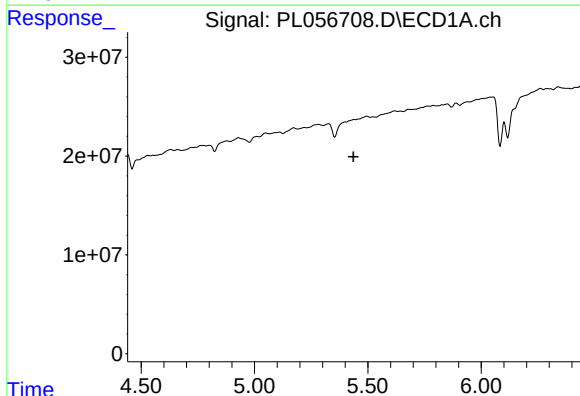


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.437 min
Response: 0
Conc: N.D.

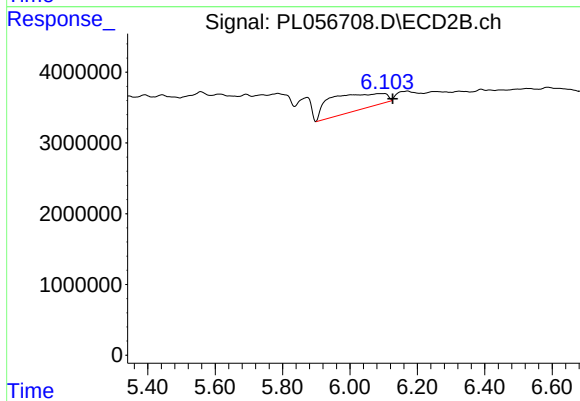

#10 gamma-Chlordane


R.T.: 6.103 min
Delta R.T.: -0.023 min
Response: 26339499
Conc: 9.18 ng/ml

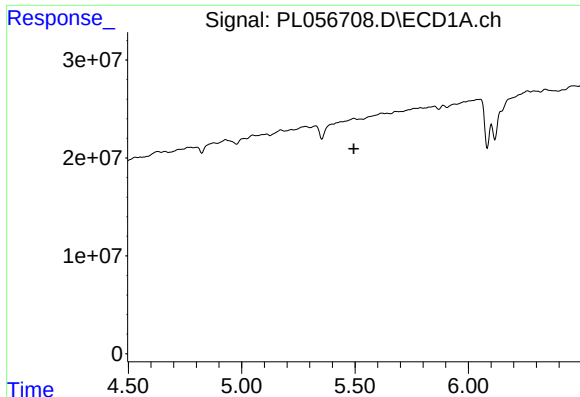

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.495 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

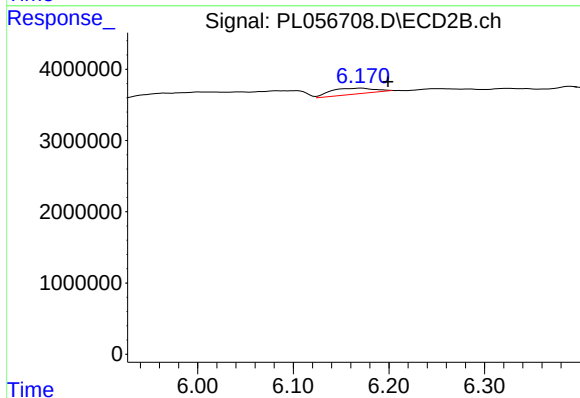


#11 alpha-Chlordane

R.T.: 6.171 min
Delta R.T.: -0.028 min
Response: 2656252
Conc: 0.93 ng/ml

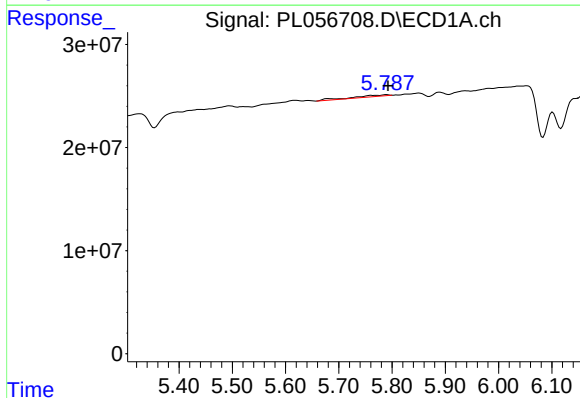


#13 Dieldrin

R.T.: 5.789 min
Delta R.T.: -0.003 min
Response: 7190049
Conc: 0.48 ng/ml

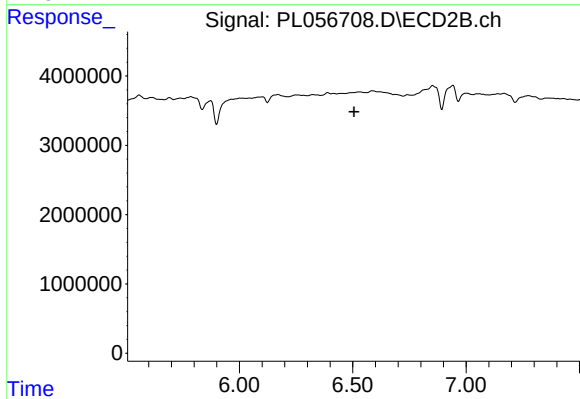

#13 Dieldrin


R.T.: 0.000 min
Exp R.T.: 6.506 min
Response: 0
Conc: N.D.

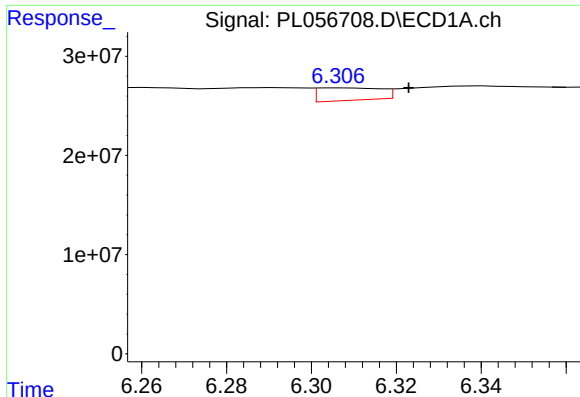

#15 Endosulfan II


R.T.: 6.307 min
Delta R.T.: -0.016 min
Response: 13017342
Conc: 1.05 ng/ml

Instrument :
ECD_L
ClientSampleId :

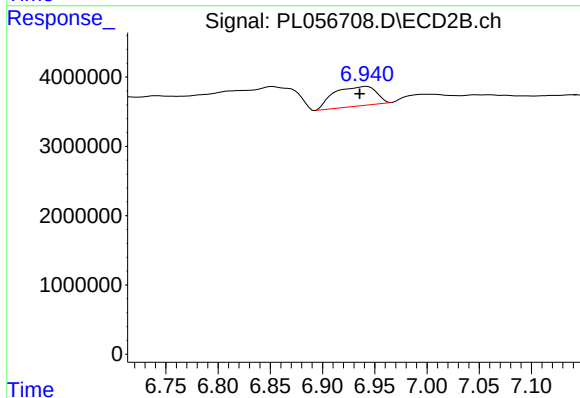


#15 Endosulfan II

R.T.: 6.942 min
Delta R.T.: 0.007 min
Response: 7907556
Conc: 3.06 ng/ml

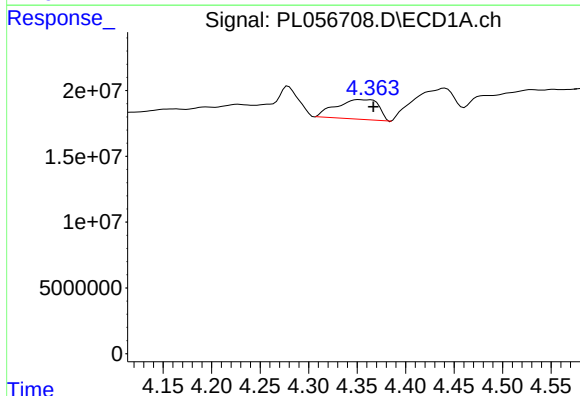


#23 Chlordane-1

R.T.: 4.352 min
Delta R.T.: -0.015 min
Response: 45240352
Conc: 124.19 ng/ml

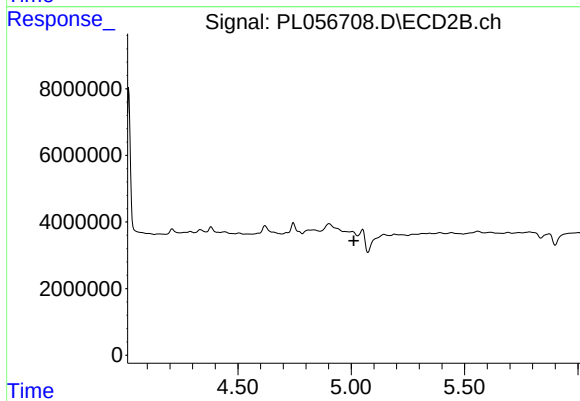

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 5.012 min
Response: 0
Conc: N.D.

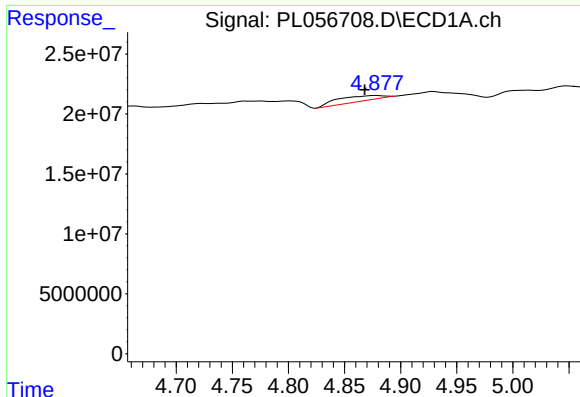

#24 Chlordane-2


R.T.: 4.878 min
Delta R.T.: 0.010 min
Response: 12139262
Conc: 31.12 ng/ml

Instrument :
ECD_L
ClientSampleId :

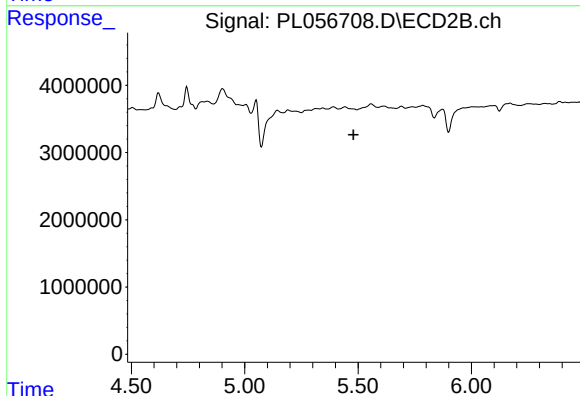


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 5.480 min
Response: 0
Conc: N.D.

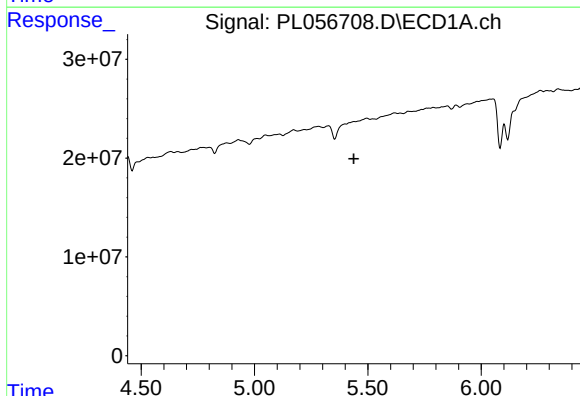


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 5.438 min
Response: 0
Conc: N.D.

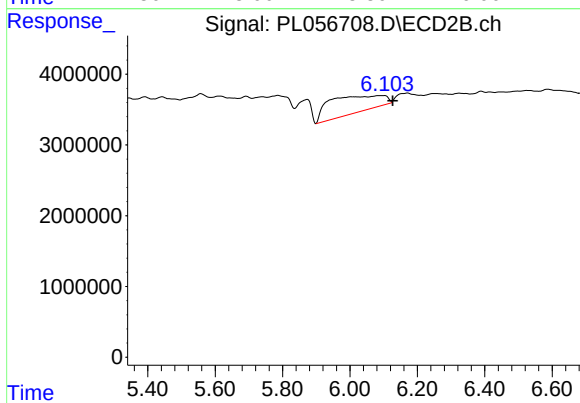

#25 Chlordane-3


R.T.: 6.103 min
Delta R.T.: -0.023 min
Response: 26339499
Conc: 71.32 ng/ml

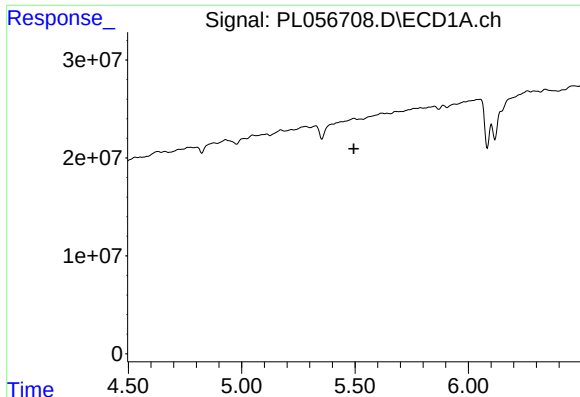

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 5.495 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

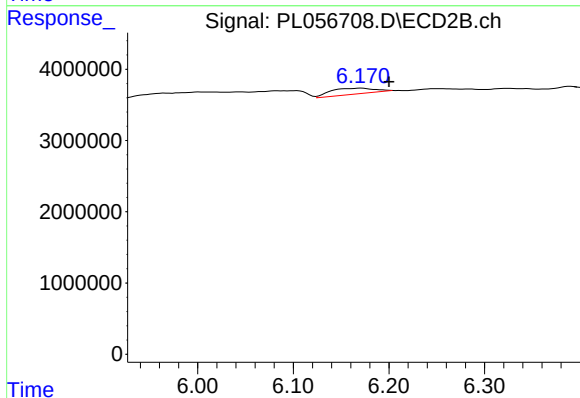


#26 Chlordane-4

R.T.: 6.171 min
Delta R.T.: -0.029 min
Response: 2656252
Conc: 6.19 ng/ml

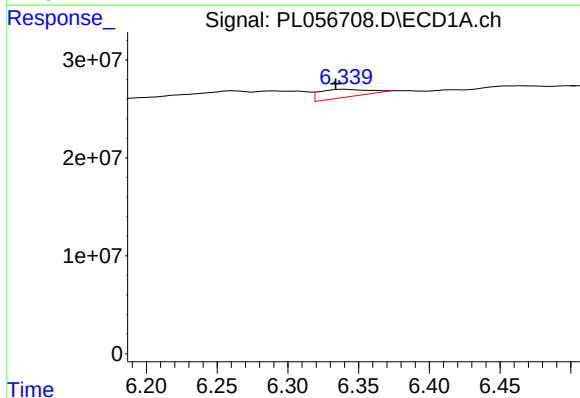


#27 Chlordane-5

R.T.: 6.340 min
Delta R.T.: 0.006 min
Response: 19276058
Conc: 58.87 ng/ml

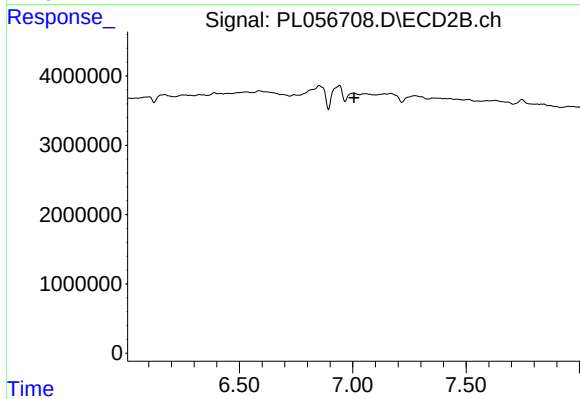

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T.: 7.007 min
Response: 0
Conc: N.D.

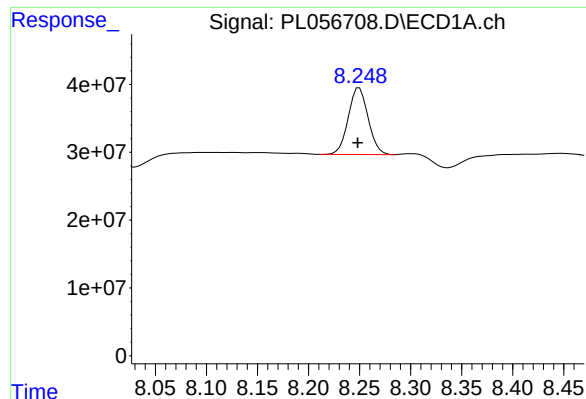

#28 Decachlorobiphenyl

R.T.: 8.250 min
Delta R.T.: 0.001 min
Response: 133464286
Conc: 11.22 ng/ml

Instrument :
ECD_L
ClientSampleId :

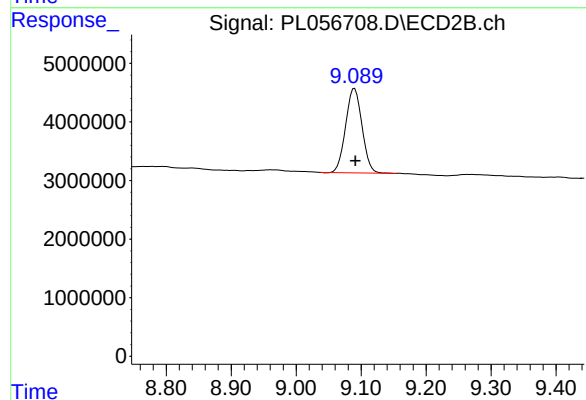

#28 Decachlorobiphenyl

R.T.: 9.090 min
Delta R.T.: -0.001 min
Response: 25267632
Conc: 12.02 ng/ml