

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022020\
 Data File : PL056709.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Feb 2020 18:06
 Operator : AJ\MA
 Sample : L1586-04
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 21 00:31:46 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL021920.M
 Quant Title : GC Extractables
 QLast Update : Thu Feb 20 02:32:45 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.498	4.019	177.0E6	52596735	20.471	21.115
28)	SA Decachlor...	8.250	9.090	156.6E6	30407261	13.165	14.471
Target Compounds							
10)	B gamma-Chl...	0.000	6.105f	0	27446409	N.D.	9.569 #
13)	MA Dieldrin	5.764f	0.000	13097095	0	0.879	N.D. #
15)	B Endosulfa...	6.338	6.941	49690810	12302261	4.001	4.763
23)	Chlordane-1	4.354	0.000	28645837	0	78.634	N.D. #
25)	Chlordane-3	0.000	6.105f	0	27446409	N.D.	74.318 #
27)	Chlordane-5	6.338	7.002	49690810	12770691	151.757	165.830



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022020\
Data File : PL056709.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Feb 2020 18:06
Operator : AJ\MA
Sample : L1586-04
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 21 00:31:46 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL021920.M
Quant Title : GC Extractables
QLast Update : Thu Feb 20 02:32:45 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

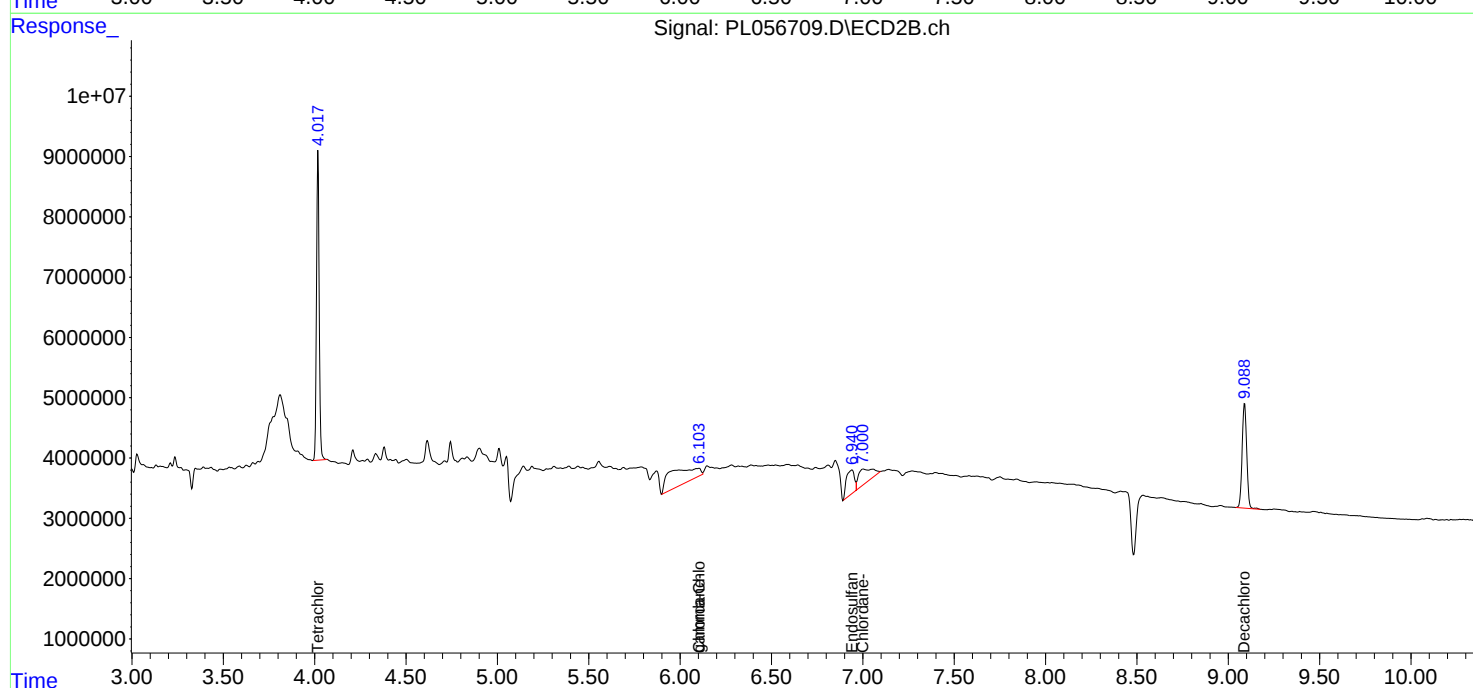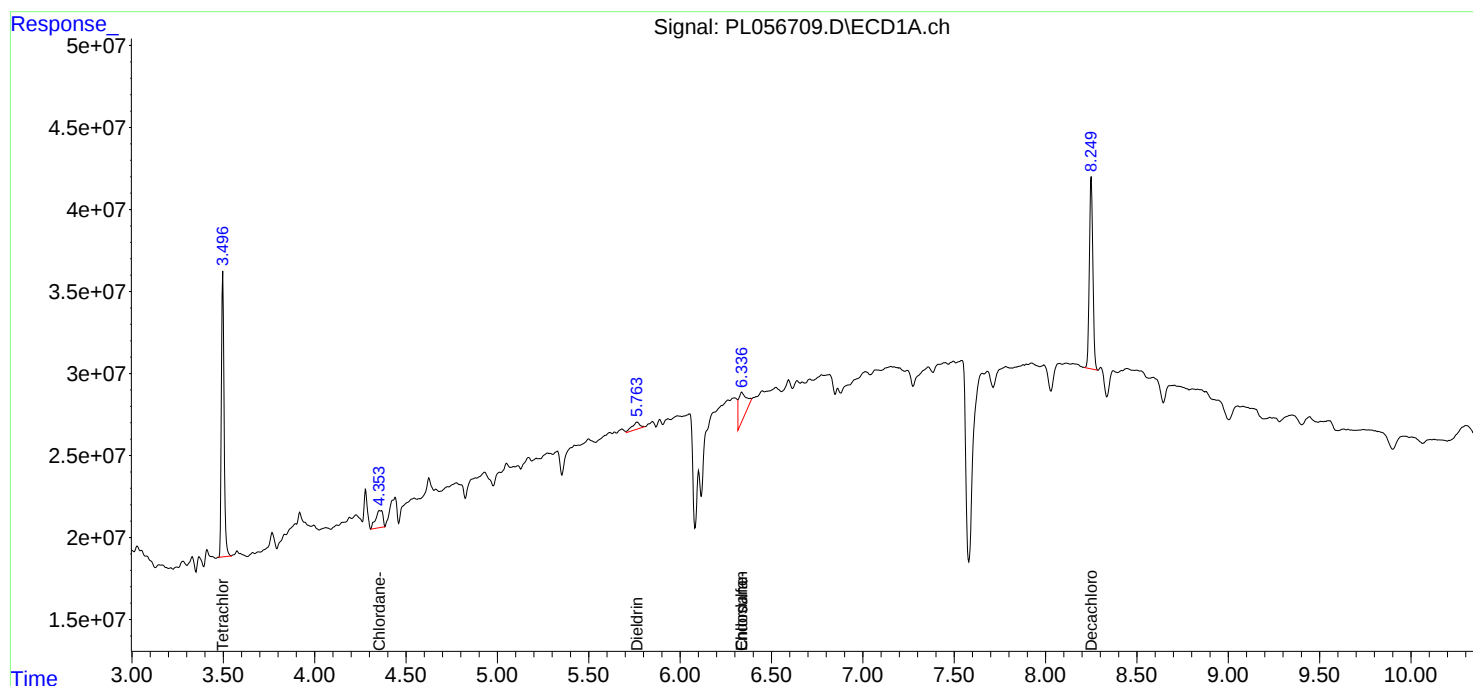


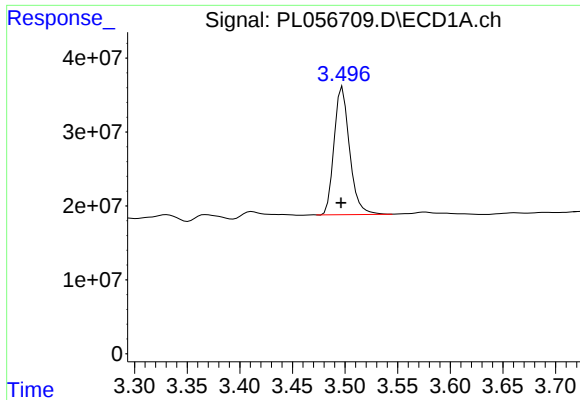

#1 Tetrachloro-m-xylene


R.T.: 3.498 min
Delta R.T.: 0.002 min
Response: 177023353
Conc: 20.47 ng/ml

Instrument :
ECD_L
ClientSampleId :

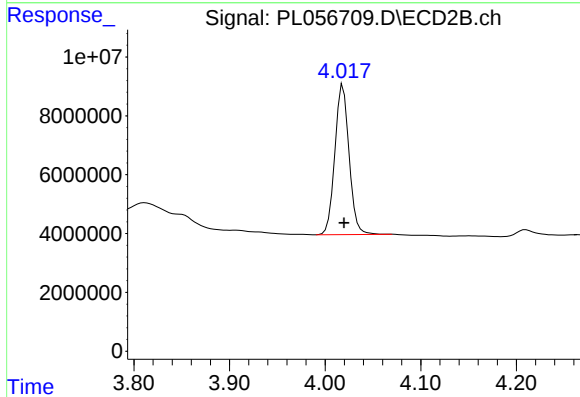


#1 Tetrachloro-m-xylene

R.T.: 4.019 min
Delta R.T.: -0.001 min
Response: 52596735
Conc: 21.11 ng/ml

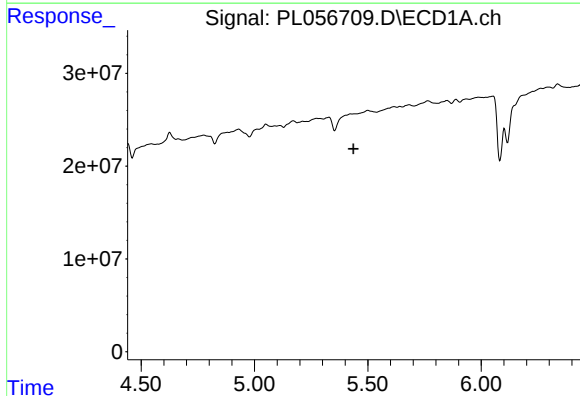


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.437 min
Response: 0
Conc: N.D.

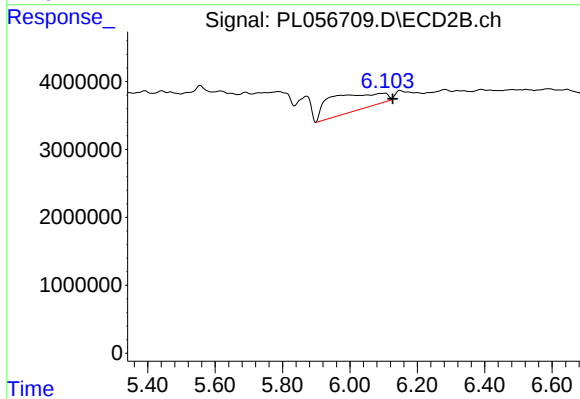

#10 gamma-Chlordane


R.T.: 6.105 min
Delta R.T.: -0.022 min
Response: 27446409
Conc: 9.57 ng/ml

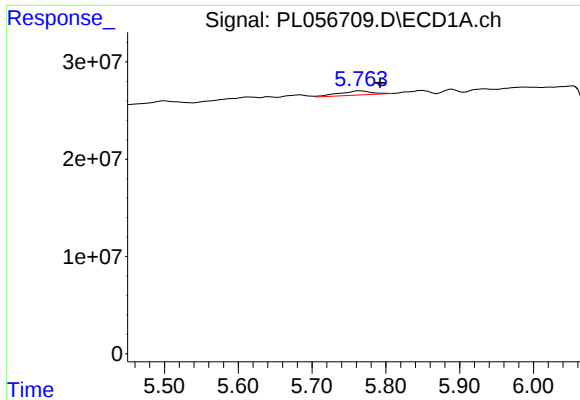

#13 Dieldrin


R.T.: 5.764 min
Delta R.T.: -0.028 min
Response: 13097095
Conc: 0.88 ng/ml

Instrument :
ECD_L
ClientSampleId :

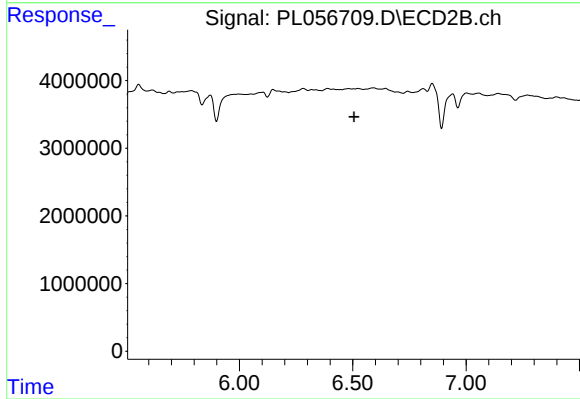


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 6.506 min
Response: 0
Conc: N.D.

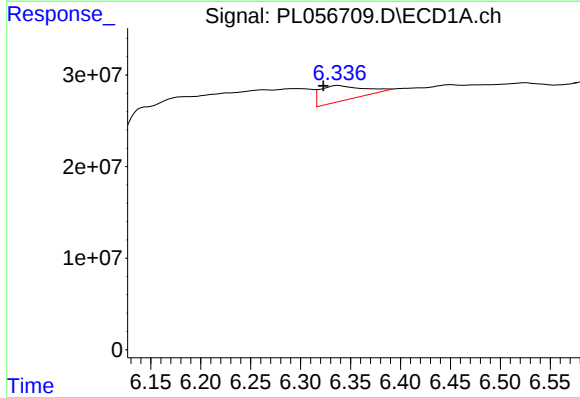


#15 Endosulfan II

R.T.: 6.338 min
Delta R.T.: 0.015 min
Response: 49690810
Conc: 4.00 ng/ml

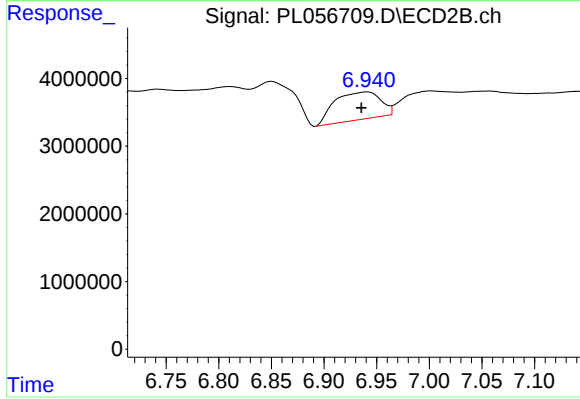

#15 Endosulfan II


R.T.: 6.941 min
Delta R.T.: 0.006 min
Response: 12302261
Conc: 4.76 ng/ml

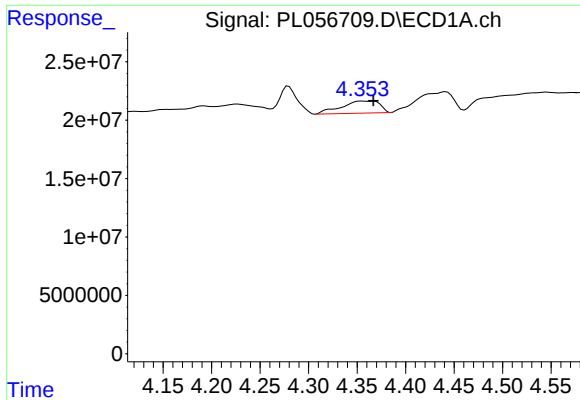

#23 Chlordane-1


R.T.: 4.354 min
Delta R.T.: -0.012 min
Response: 28645837
Conc: 78.63 ng/ml

Instrument :
ECD_L
ClientSampleId :

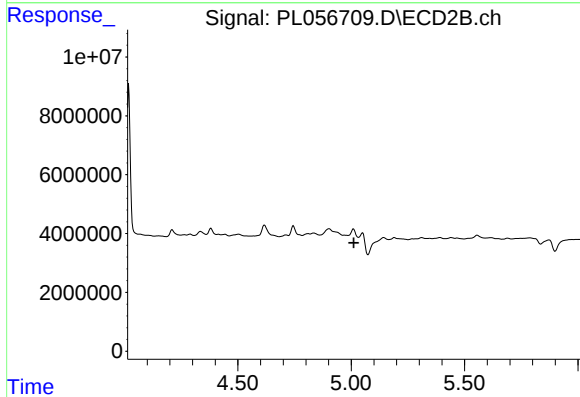


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.012 min
Response: 0
Conc: N.D.

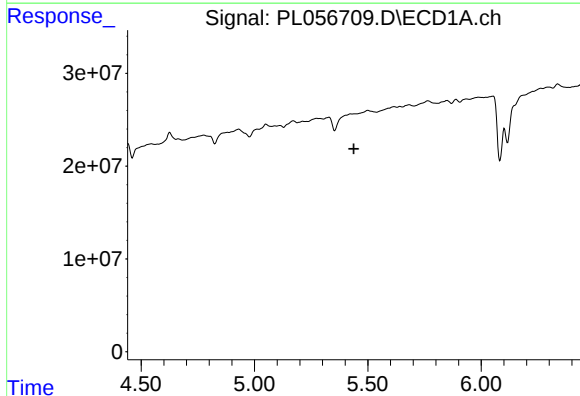


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 5.438 min
Response: 0
Conc: N.D.

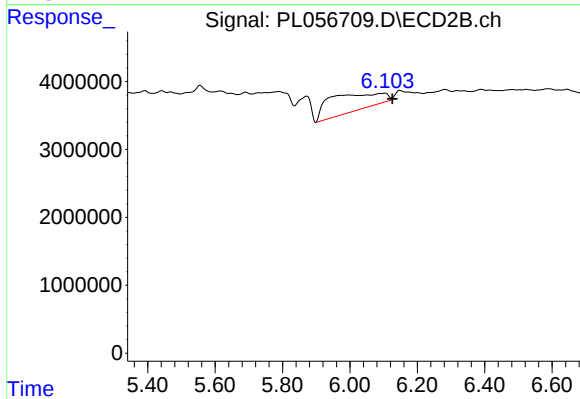

#25 Chlordane-3


R.T.: 6.105 min
Delta R.T.: -0.021 min
Response: 27446409
Conc: 74.32 ng/ml

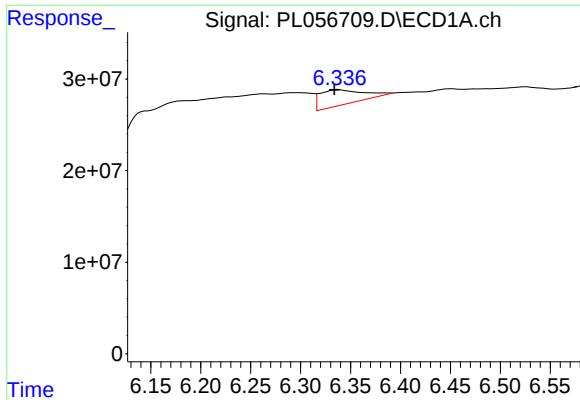

#27 Chlordane-5


R.T.: 6.338 min
Delta R.T.: 0.004 min
Response: 49690810
Conc: 151.76 ng/ml

Instrument :
ECD_L
ClientSampleId :

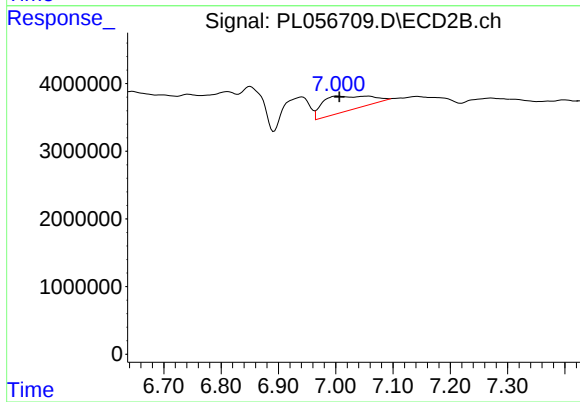


#27 Chlordane-5

R.T.: 7.002 min
Delta R.T.: -0.004 min
Response: 12770691
Conc: 165.83 ng/ml

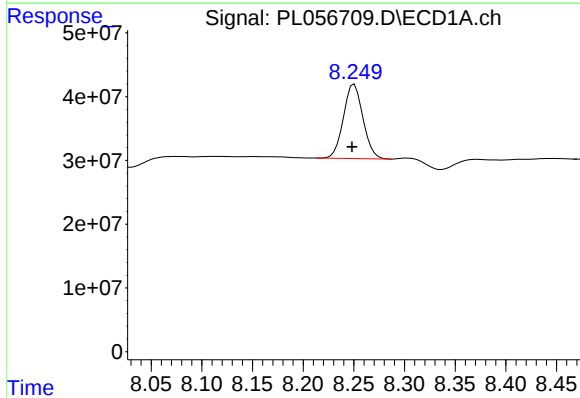

#28 Decachlorobiphenyl

R.T.: 8.250 min
Delta R.T.: 0.002 min
Response: 156594484
Conc: 13.16 ng/ml

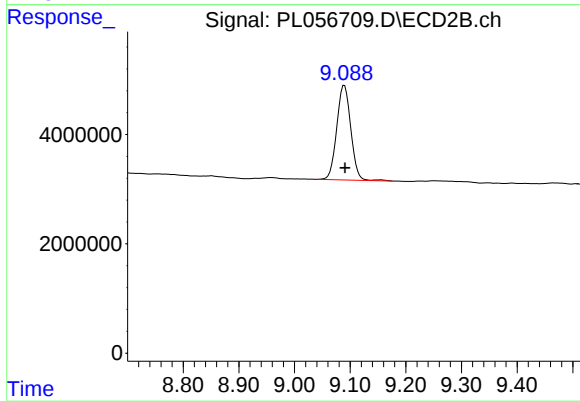

#28 Decachlorobiphenyl

R.T.: 9.090 min
Delta R.T.: -0.001 min
Response: 30407261
Conc: 14.47 ng/ml