

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022020\
 Data File : PL056714.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Feb 2020 19:16
 Operator : AJ\MA
 Sample : PB126947BL
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 21 00:32:49 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL021920.M
 Quant Title : GC Extractables
 QLast Update : Thu Feb 20 02:32:45 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.498	4.019	194.4E6	55293693	22.481	22.197
28)	SA Decachlor...	8.249	9.089	244.3E6	46341825	20.535	22.054
Target Compounds							
4)	MA Heptachlor	4.509	0.000	11470466	0	0.778	N.D. #
13)	MA Dieldrin	5.792	0.000	13305385	0	0.893	N.D. #
18)	B Endrin al...	6.486	0.000	76645291	0	7.081	N.D. #
23)	Chlordane-1	4.344f	0.000	35866052	0	98.453	N.D. #
24)	Chlordane-2	4.885f	0.000	10186170	0	26.113	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022020\
Data File : PL056714.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Feb 2020 19:16
Operator : AJ\MA
Sample : PB126947BL
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 21 00:32:49 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL021920.M
Quant Title : GC Extractables
QLast Update : Thu Feb 20 02:32:45 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

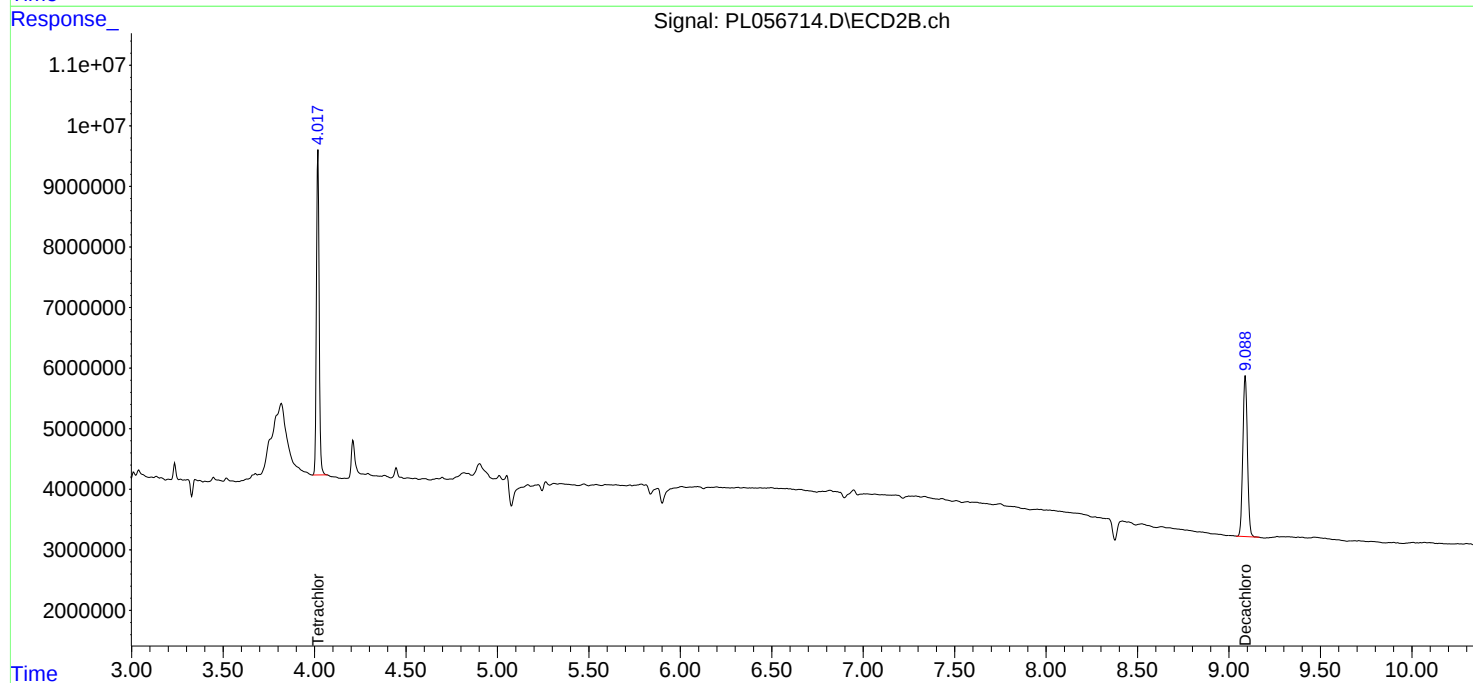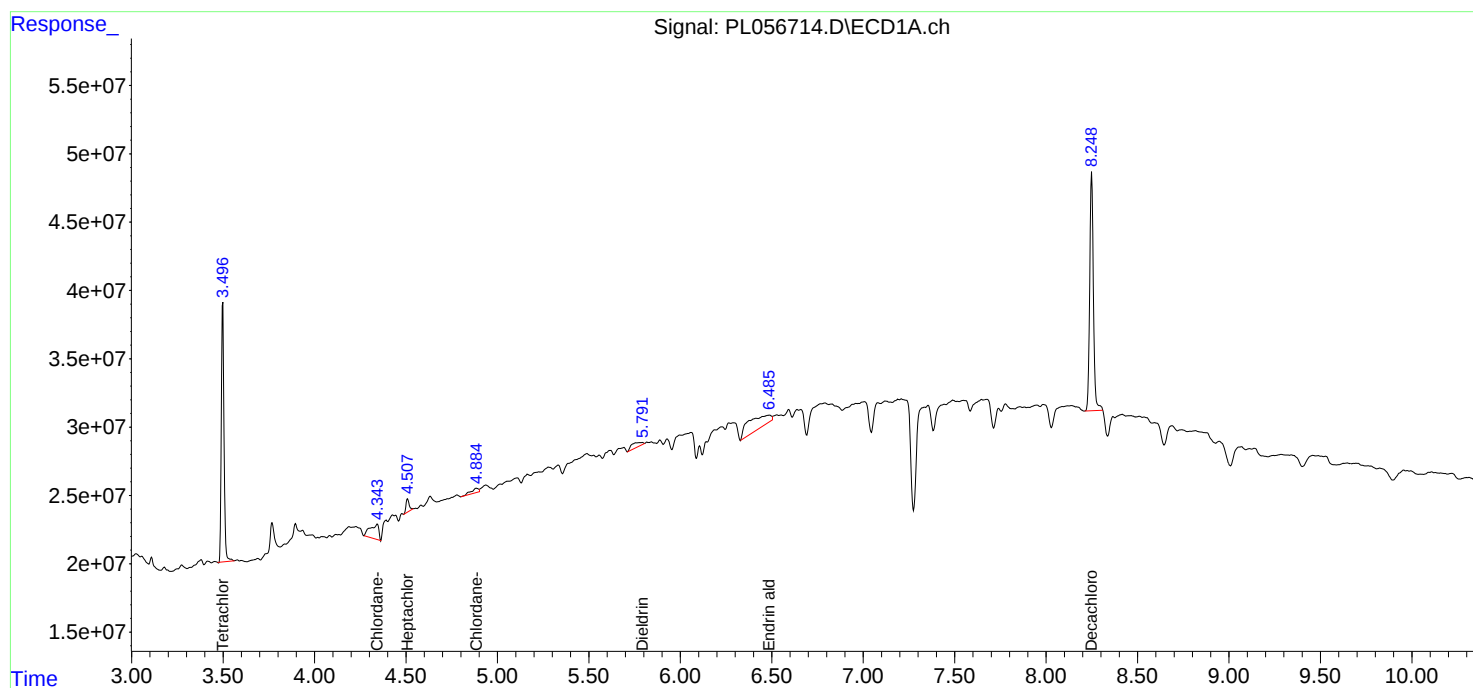


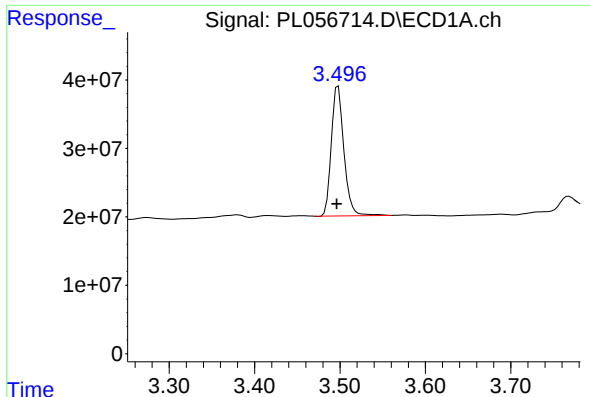

#1 Tetrachloro-m-xylene


R.T.: 3.498 min
Delta R.T.: 0.002 min
Response: 194403241
Conc: 22.48 ng/ml

Instrument :
ECD_L
ClientSampleId :

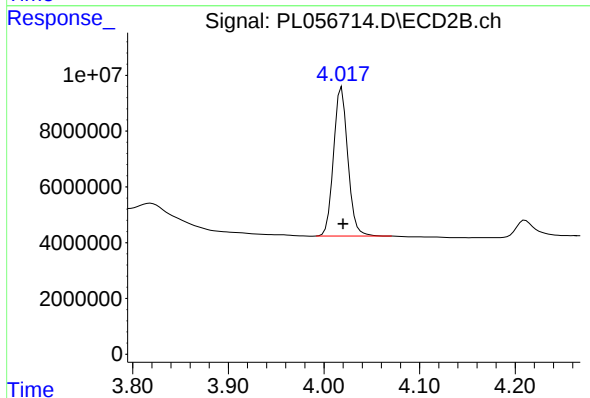


#1 Tetrachloro-m-xylene

R.T.: 4.019 min
Delta R.T.: -0.001 min
Response: 55293693
Conc: 22.20 ng/ml

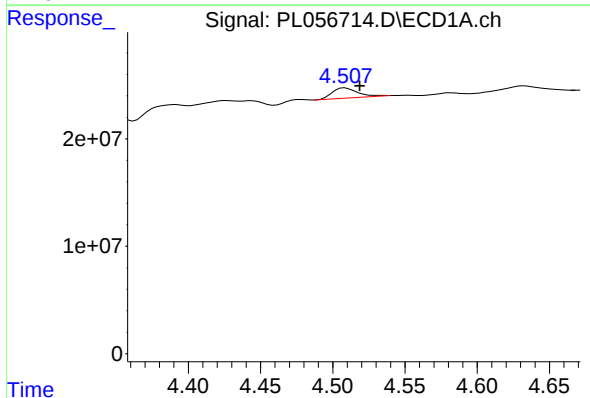


#4 Heptachlor

R.T.: 4.509 min
Delta R.T.: -0.010 min
Response: 11470466
Conc: 0.78 ng/ml

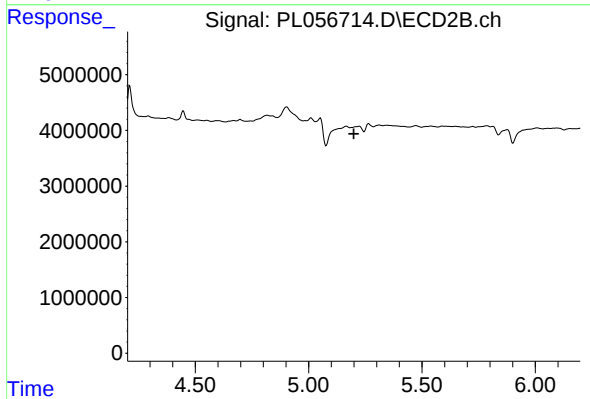

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 5.200 min
Response: 0
Conc: N.D.

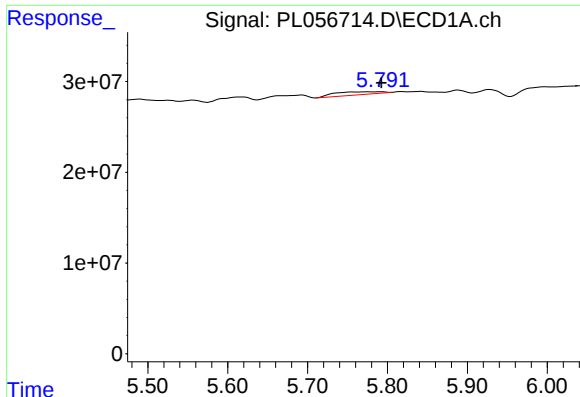

#13 Dieldrin


R.T.: 5.792 min
Delta R.T.: 0.000 min
Response: 13305385
Conc: 0.89 ng/ml

Instrument :
ECD_L
ClientSampleId :

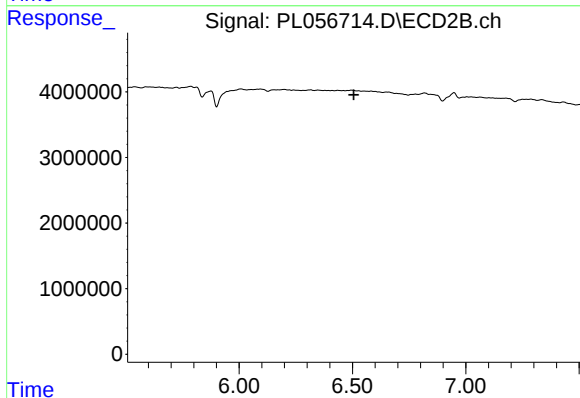


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 6.506 min
Response: 0
Conc: N.D.

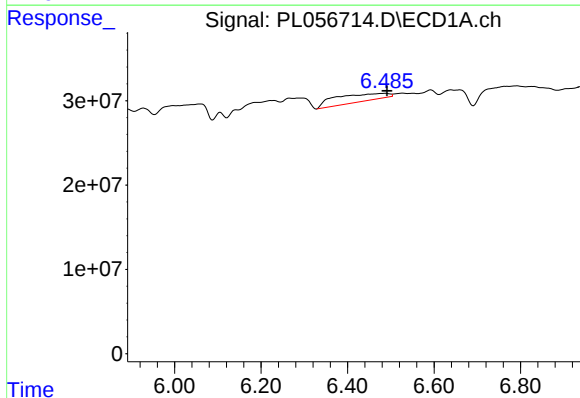


#18 Endrin aldehyde

R.T.: 6.486 min
Delta R.T.: -0.005 min
Response: 76645291
Conc: 7.08 ng/ml

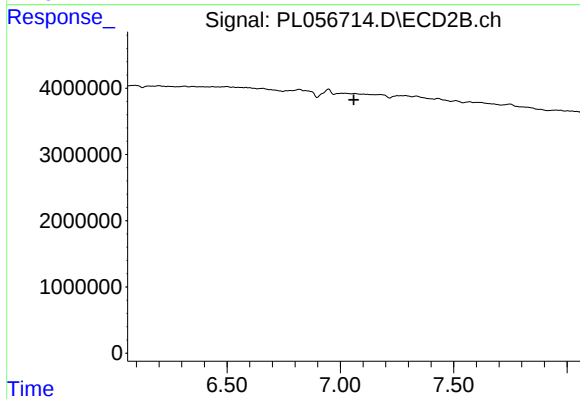

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T. : 7.060 min
Response: 0
Conc: N.D.

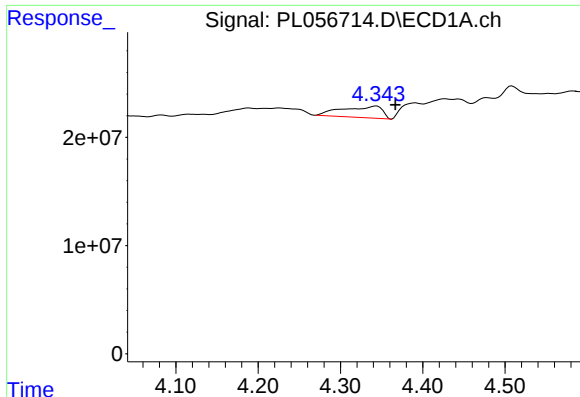

#23 Chlordane-1


R.T.: 4.344 min
Delta R.T.: -0.023 min
Response: 35866052
Conc: 98.45 ng/ml

Instrument :
ECD_L
ClientSampleId :

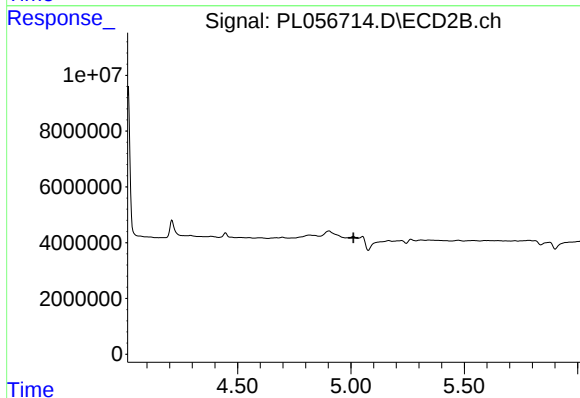


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.012 min
Response: 0
Conc: N.D.

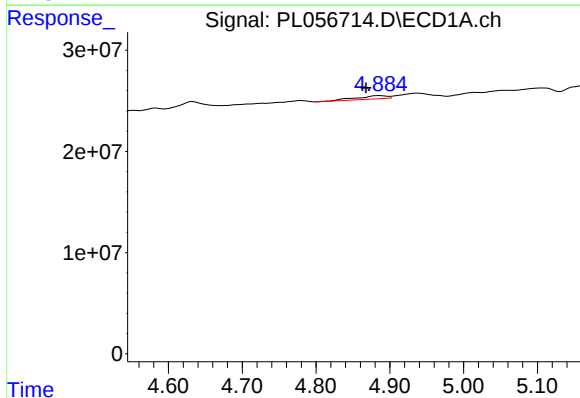


#24 Chlordane-2

R.T.: 4.885 min
Delta R.T.: 0.017 min
Response: 10186170
Conc: 26.11 ng/ml

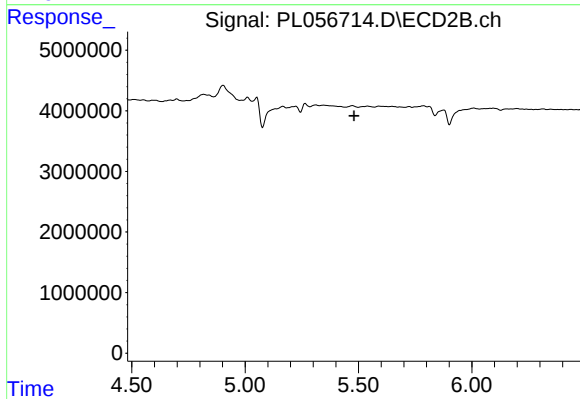

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T. : 5.480 min
Response: 0
Conc: N.D.

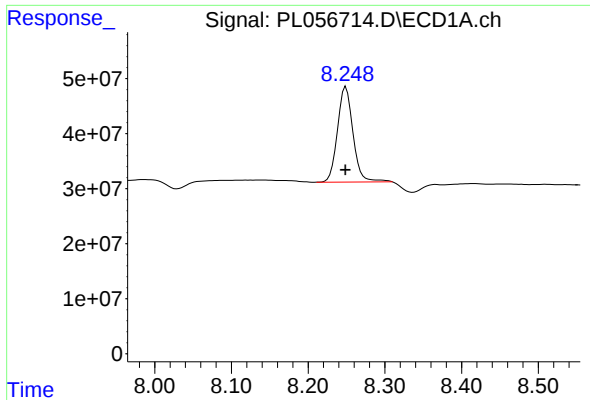

#28 Decachlorobiphenyl

R.T.: 8.249 min
Delta R.T.: 0.000 min
Response: 244268375
Conc: 20.54 ng/ml

Instrument :
ECD_L
ClientSampleId :

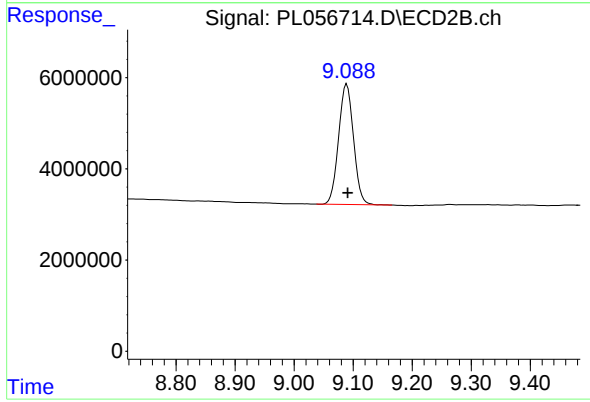

#28 Decachlorobiphenyl

R.T.: 9.089 min
Delta R.T.: -0.002 min
Response: 46341825
Conc: 22.05 ng/ml