

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022020\
 Data File : PL056718.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Feb 2020 20:13
 Operator : AJ\MA
 Sample : L1573-03
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 21 00:33:33 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL021920.M
 Quant Title : GC Extractables
 QLast Update : Thu Feb 20 02:32:45 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.498	4.019	193.3E6	56741765	22.350	22.779
28)	SA Decachlor...	8.250	9.089	232.2E6	43713369	19.522	20.803
Target Compounds							
13)	MA Dieldrin	5.763f	0.000	4211087	0	0.283	N.D. #
15)	B Endosulfa...	6.315	0.000	18872303	0	1.520	N.D. #
18)	B Endrin al...	6.479	0.000	43396710	0	4.009	N.D. #
19)	B Endosulfa...	6.708	0.000	2974963	0	0.251	N.D. #
23)	Chlordane-1	4.352	0.000	3406412	0	9.351	N.D. #
27)	Chlordane-5	6.315f	0.000	18872303	0	57.636	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022020\
Data File : PL056718.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Feb 2020 20:13
Operator : AJ\MA
Sample : L1573-03
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 21 00:33:33 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL021920.M
Quant Title : GC Extractables
QLast Update : Thu Feb 20 02:32:45 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

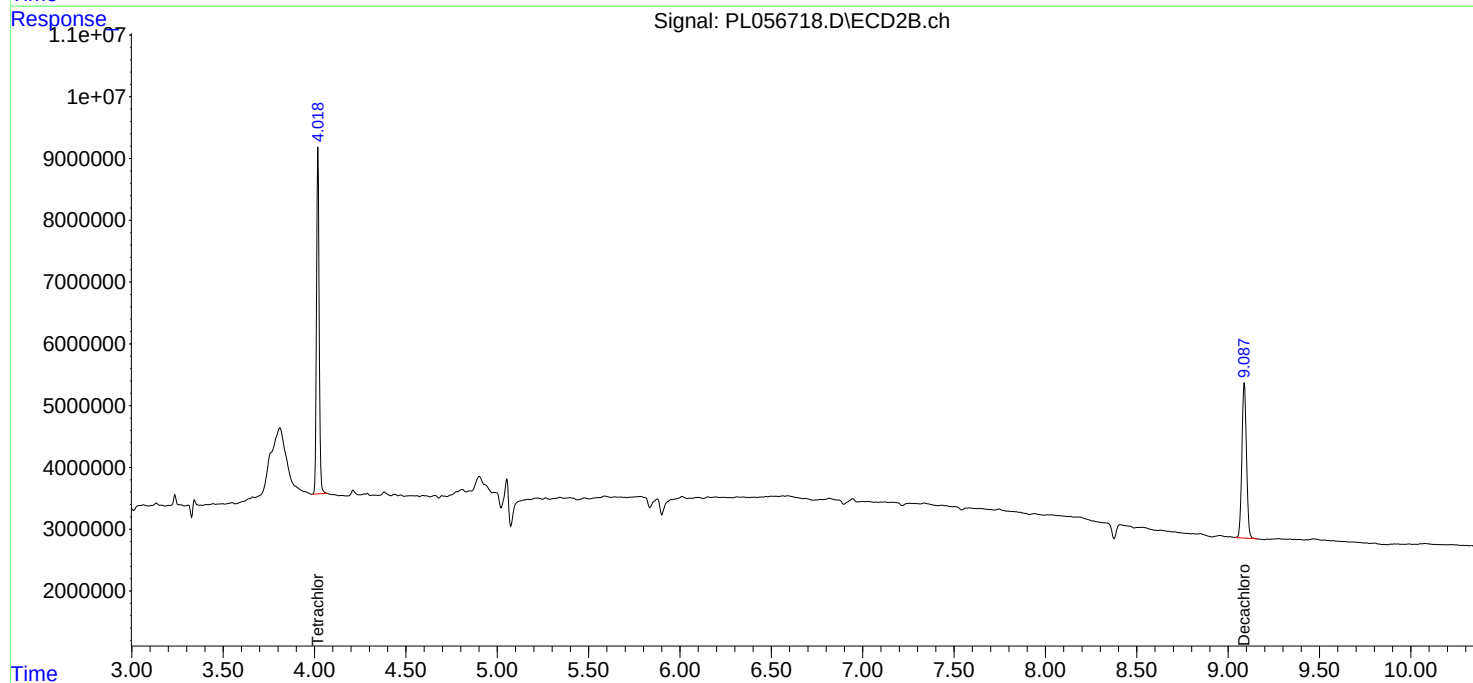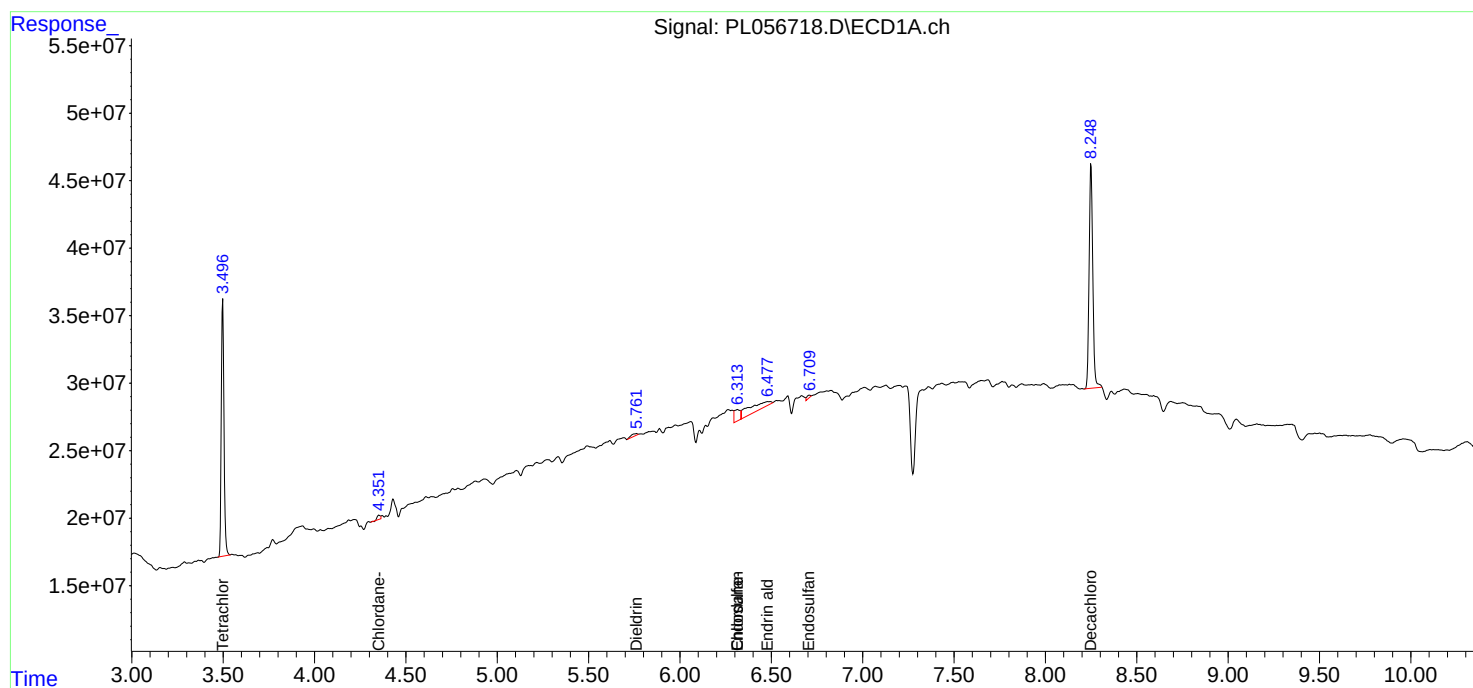


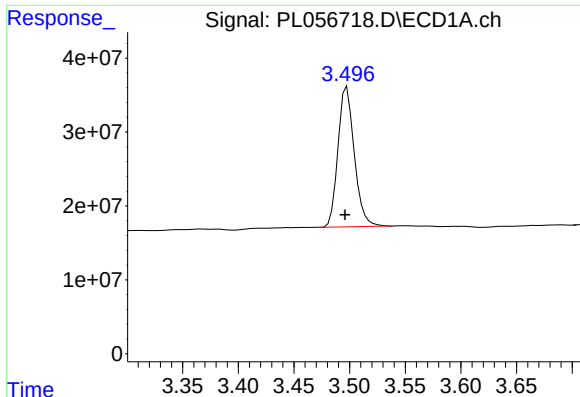

#1 Tetrachloro-m-xylene


R.T.: 3.498 min
Delta R.T.: 0.002 min
Response: 193277036
Conc: 22.35 ng/ml

Instrument :
ECD_L
ClientSampleId :

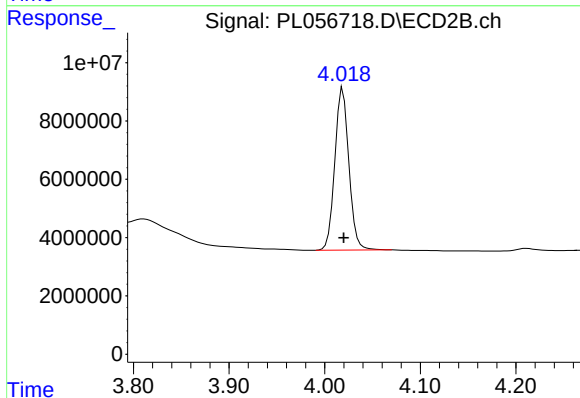


#1 Tetrachloro-m-xylene

R.T.: 4.019 min
Delta R.T.: 0.000 min
Response: 56741765
Conc: 22.78 ng/ml

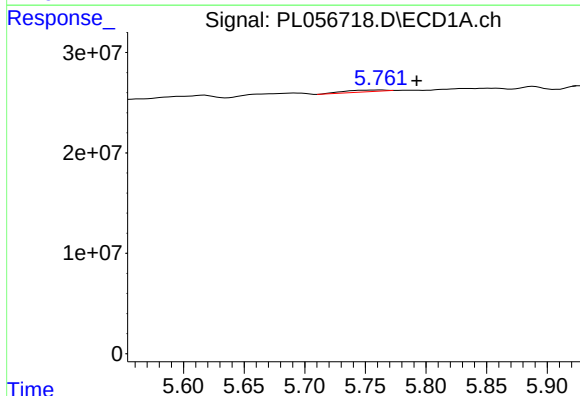


#13 Dieldrin

R.T.: 5.763 min
Delta R.T.: -0.030 min
Response: 4211087
Conc: 0.28 ng/ml

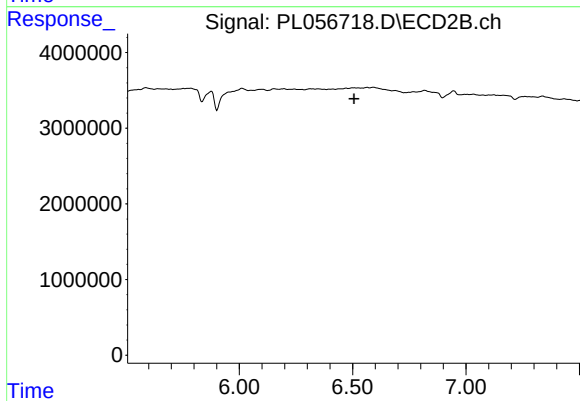

#13 Dieldrin


R.T.: 0.000 min
Exp R.T.: 6.506 min
Response: 0
Conc: N.D.

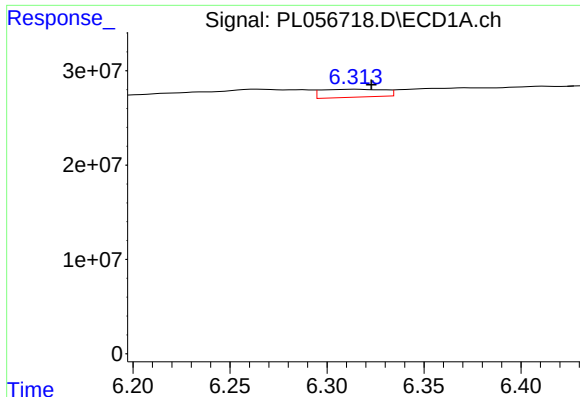

#15 Endosulfan II


R.T.: 6.315 min
Delta R.T.: -0.008 min
Response: 18872303
Conc: 1.52 ng/ml

Instrument :
ECD_L
ClientSampleId :

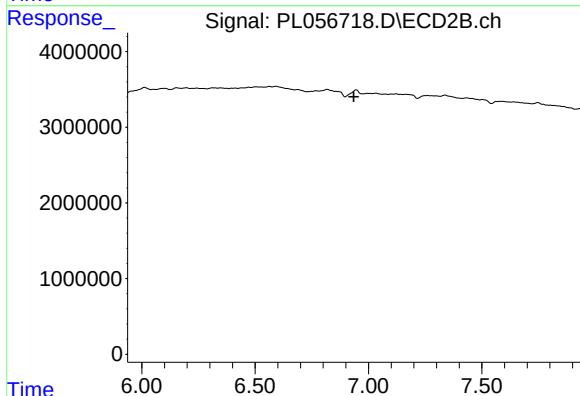


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.936 min
Response: 0
Conc: N.D.

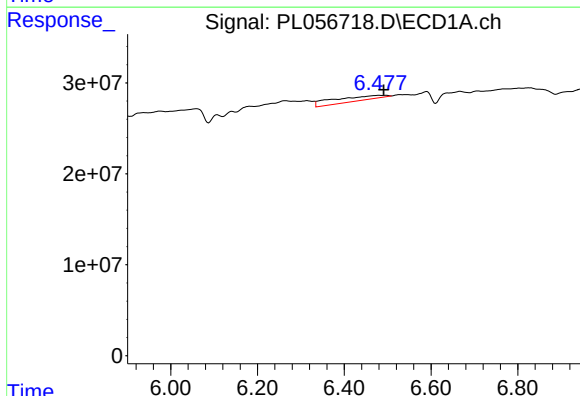


#18 Endrin aldehyde

R.T.: 6.479 min
Delta R.T.: -0.012 min
Response: 43396710
Conc: 4.01 ng/ml

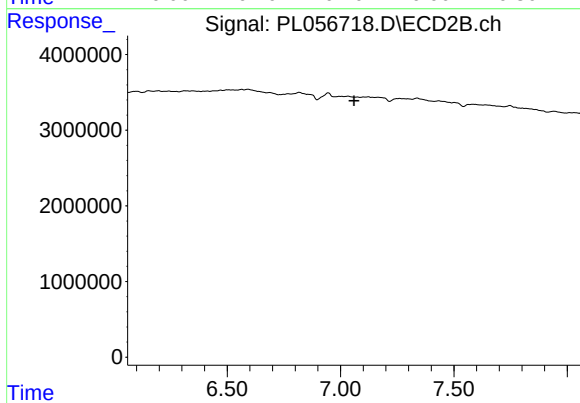

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T. : 7.060 min
Response: 0
Conc: N.D.

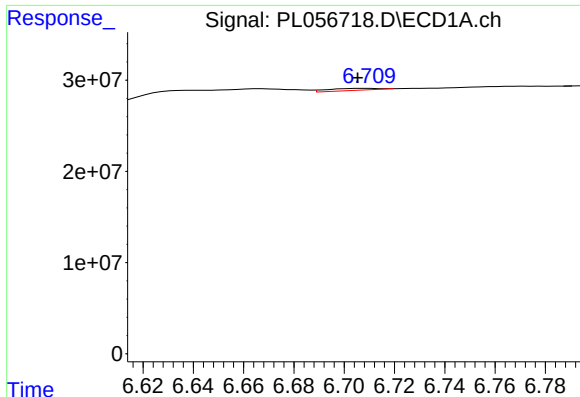

#19 Endosulfan Sulfate


R.T.: 6.708 min
Delta R.T.: 0.003 min
Response: 2974963
Conc: 0.25 ng/ml

Instrument :
ECD_L
ClientSampleId :

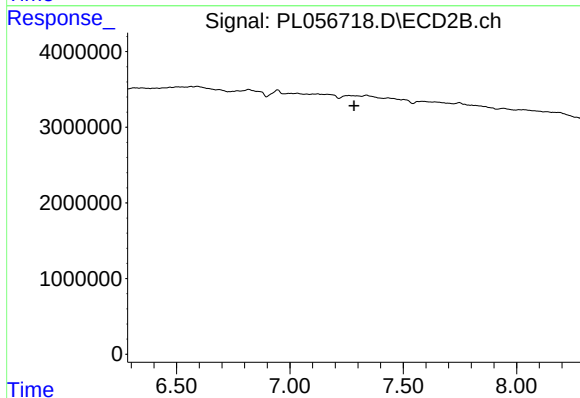


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T. : 7.283 min
Response: 0
Conc: N.D.

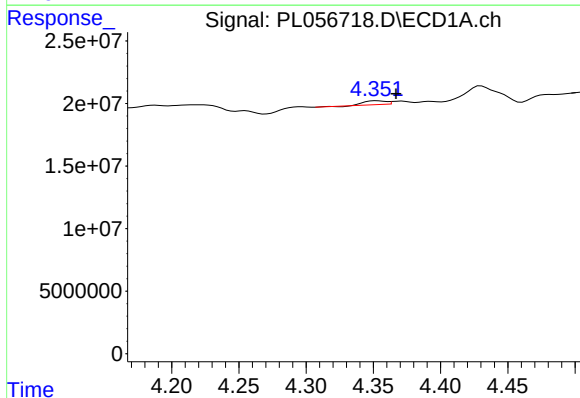


#23 Chlordane-1

R.T.: 4.352 min
Delta R.T.: -0.014 min
Response: 3406412
Conc: 9.35 ng/ml

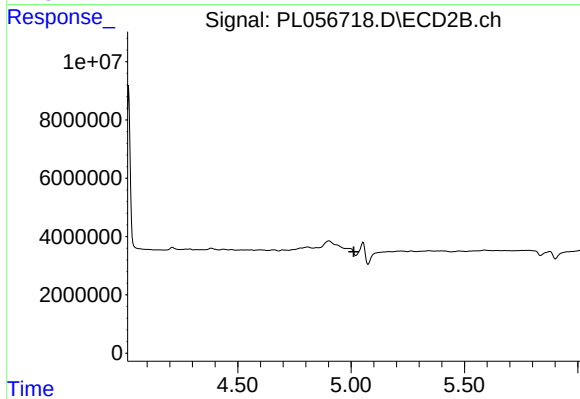

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 5.012 min
Response: 0
Conc: N.D.

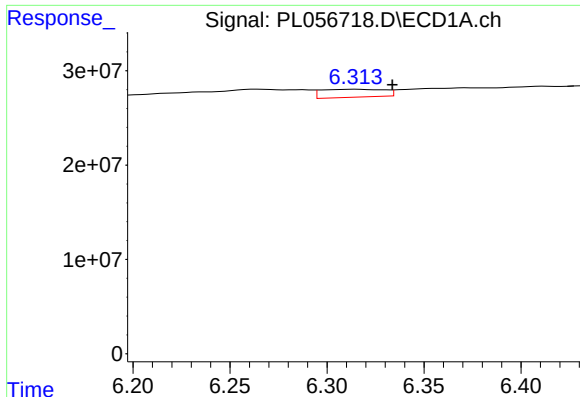

#27 Chlordane-5


R.T.: 6.315 min
Delta R.T.: -0.019 min
Response: 18872303
Conc: 57.64 ng/ml

Instrument :
ECD_L
ClientSampleId :

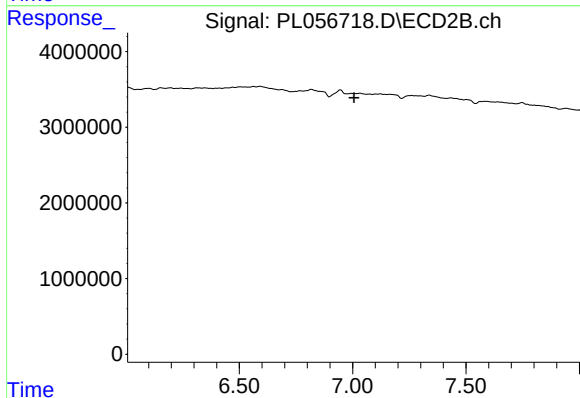


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T.: 7.007 min
Response: 0
Conc: N.D.

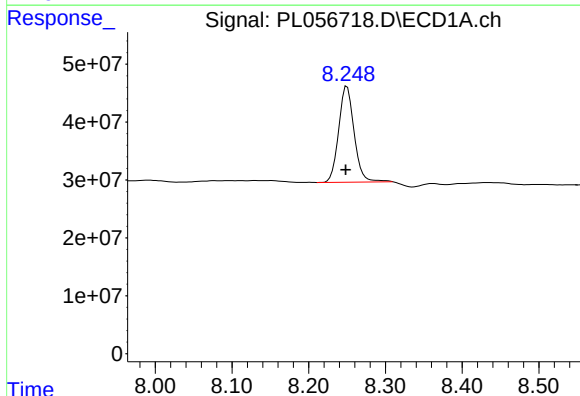

#28 Decachlorobiphenyl

R.T.: 8.250 min
Delta R.T.: 0.002 min
Response: 232222145
Conc: 19.52 ng/ml

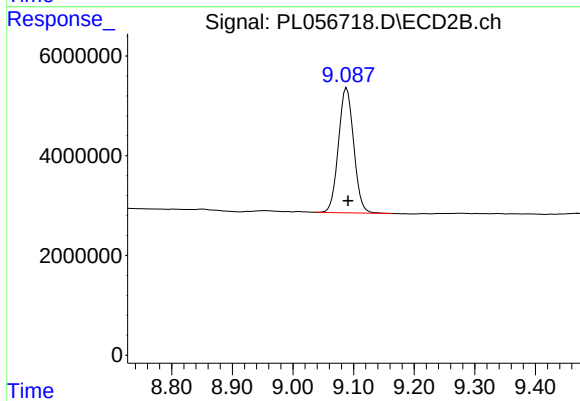

#28 Decachlorobiphenyl

R.T.: 9.089 min
Delta R.T.: -0.002 min
Response: 43713369
Conc: 20.80 ng/ml