

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022020\
 Data File : PL056719.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Feb 2020 20:27
 Operator : AJ\MA
 Sample : L1573-05
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 21 00:33:44 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL021920.M
 Quant Title : GC Extractables
 QLast Update : Thu Feb 20 02:32:45 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.498	4.019	193.1E6	56107335	22.332	22.524
28)	SA Decachlor...	8.250	9.089	225.8E6	44815676	18.983	21.327
Target Compounds							
12)	B 4,4'-DDE	5.680f	0.000	11027164	0	0.784	N.D. #
13)	MA Dieldrin	5.766f	0.000	4818366	0	0.323	N.D. #
15)	B Endosulfa...	6.309	0.000	42907849	0	3.455	N.D. #
16)	A 4,4'-DDD	6.188	0.000	20140364	0	1.801	N.D. #
17)	MA 4,4'-DDT	6.412	0.000	11496926	0	1.056	N.D. #
19)	B Endosulfa...	6.706	0.000	5468350	0	0.461	N.D. #
23)	Chlordane-1	4.352f	0.000	15146570	0	41.578	N.D. #
27)	Chlordane-5	6.309f	0.000	42907849	0	131.041	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022020\
Data File : PL056719.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Feb 2020 20:27
Operator : AJ\MA
Sample : L1573-05
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 21 00:33:44 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL021920.M
Quant Title : GC Extractables
QLast Update : Thu Feb 20 02:32:45 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

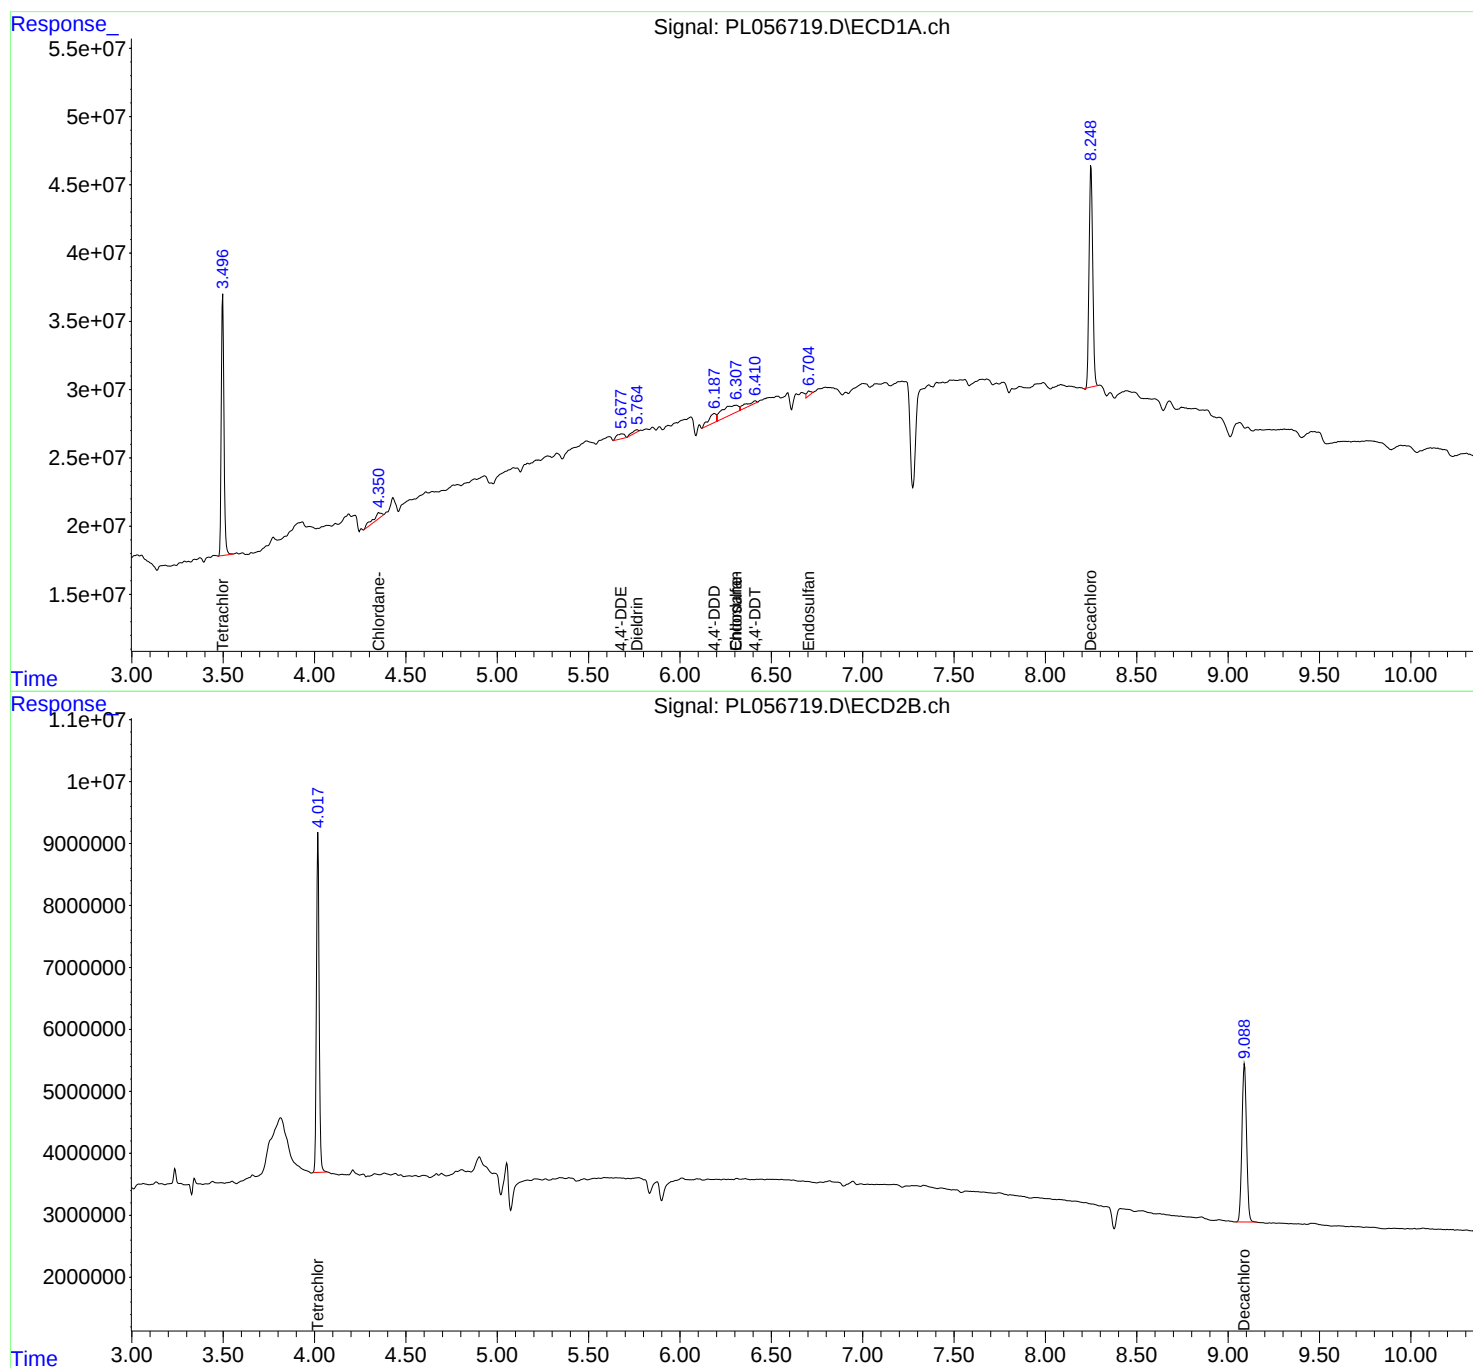


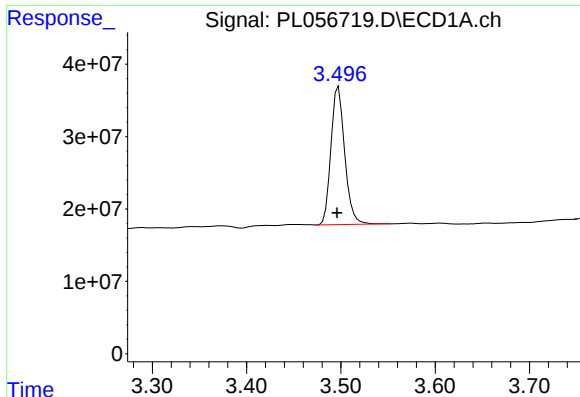

#1 Tetrachloro-m-xylene


R.T.: 3.498 min
Delta R.T.: 0.002 min
Response: 193116076
Conc: 22.33 ng/ml

Instrument :
ECD_L
ClientSampleId :

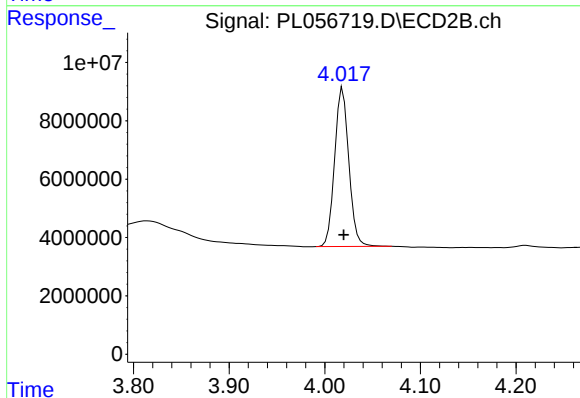


#1 Tetrachloro-m-xylene

R.T.: 4.019 min
Delta R.T.: -0.001 min
Response: 56107335
Conc: 22.52 ng/ml

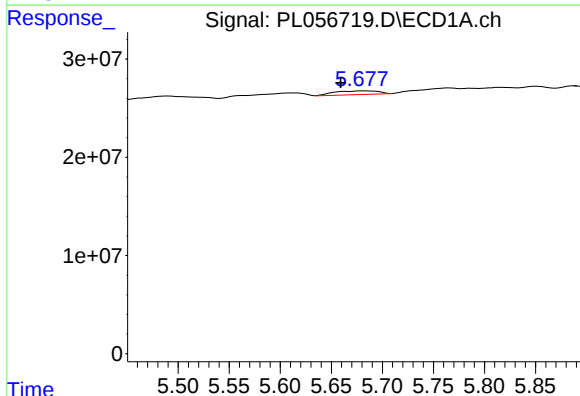


#12 4,4'-DDE

R.T.: 5.680 min
Delta R.T.: 0.020 min
Response: 11027164
Conc: 0.78 ng/ml

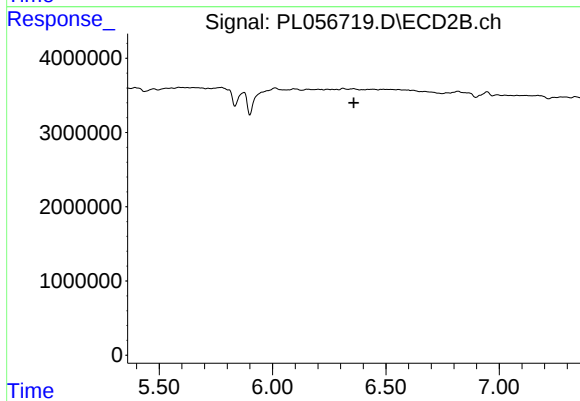

#12 4,4'-DDE


R.T.: 0.000 min
Exp R.T.: 6.358 min
Response: 0
Conc: N.D.

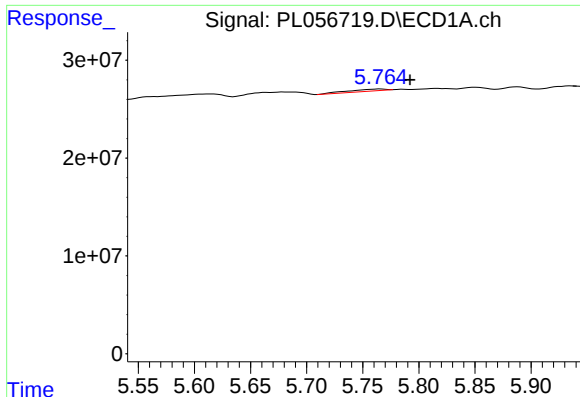

#13 Dieldrin


R.T.: 5.766 min
Delta R.T.: -0.027 min
Response: 4818366
Conc: 0.32 ng/ml

Instrument :
ECD_L
ClientSampleId :

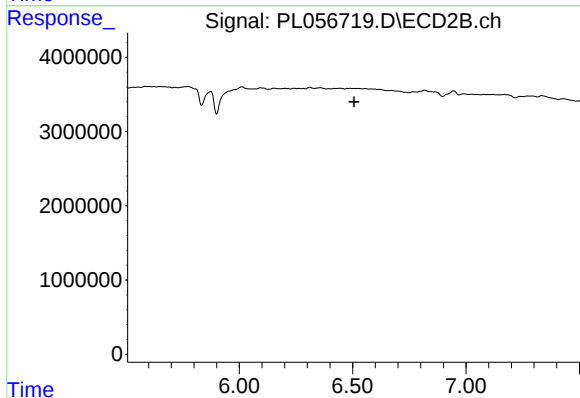


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 6.506 min
Response: 0
Conc: N.D.

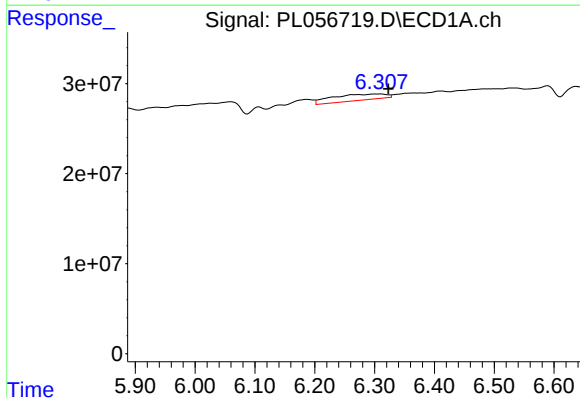


#15 Endosulfan II

R.T.: 6.309 min
Delta R.T.: -0.014 min
Response: 42907849
Conc: 3.45 ng/ml

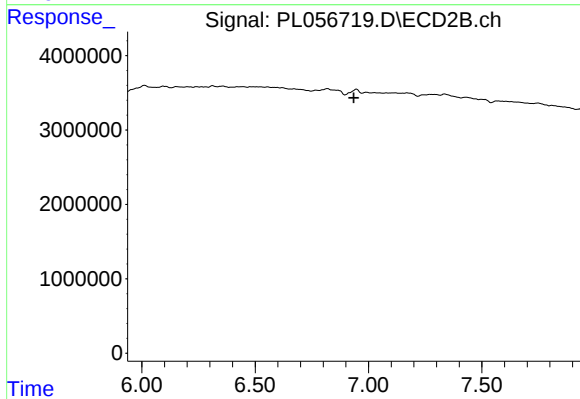

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T. : 6.936 min
Response: 0
Conc: N.D.

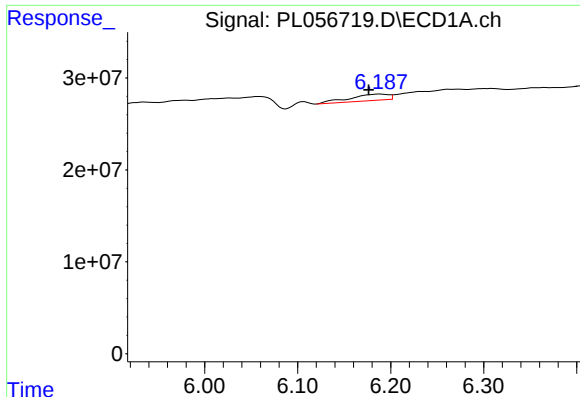

#16 4,4'-DDD


R.T.: 6.188 min
Delta R.T.: 0.012 min
Response: 20140364
Conc: 1.80 ng/ml

Instrument :
ECD_L
ClientSampleId :

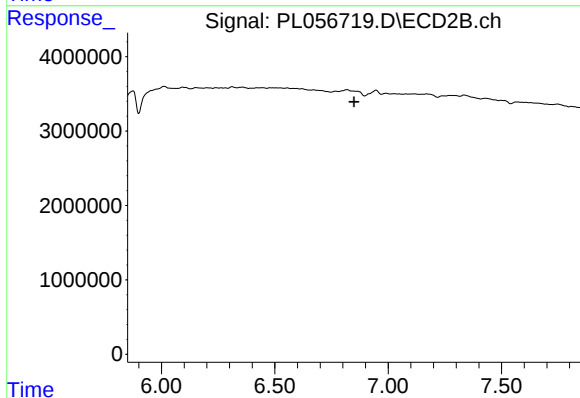


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 6.850 min
Response: 0
Conc: N.D.

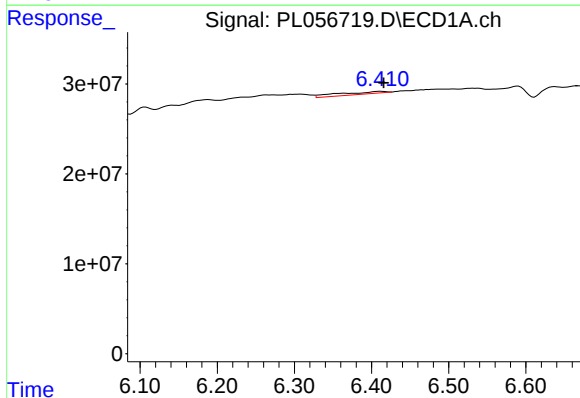


#17 4,4'-DDT

R.T.: 6.412 min
Delta R.T.: -0.003 min
Response: 11496926
Conc: 1.06 ng/ml

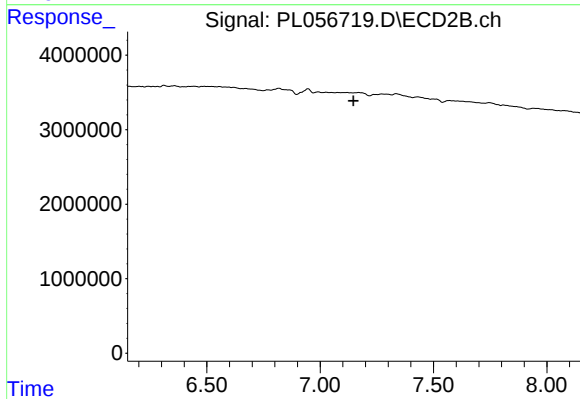

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T. : 7.148 min
Response: 0
Conc: N.D.

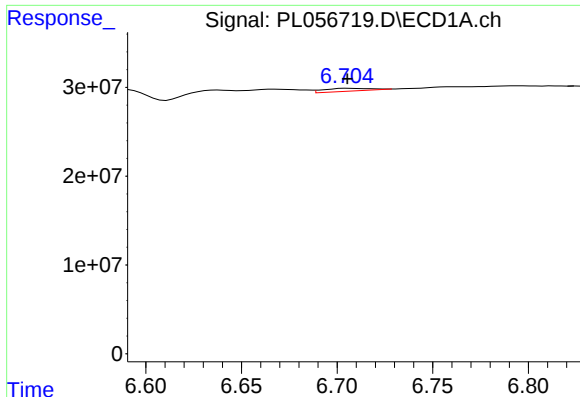

#19 Endosulfan Sulfate


R.T.: 6.706 min
Delta R.T.: 0.000 min
Response: 5468350
Conc: 0.46 ng/ml

Instrument :
ECD_L
ClientSampleId :

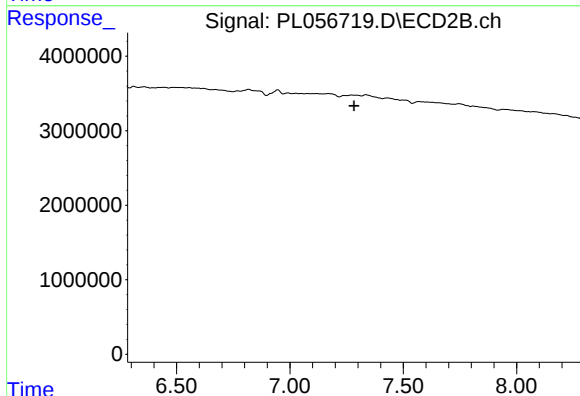


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T. : 7.283 min
Response: 0
Conc: N.D.

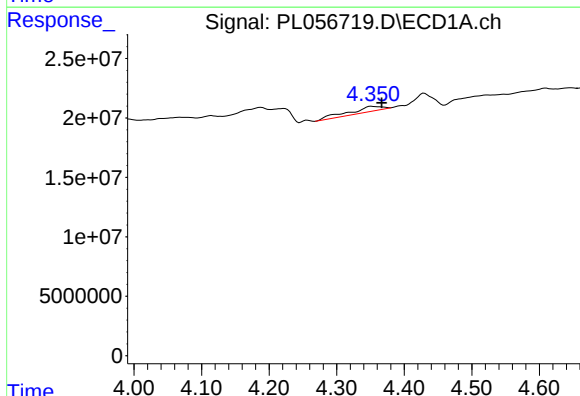


#23 Chlordane-1

R.T.: 4.352 min
Delta R.T.: -0.015 min
Response: 15146570
Conc: 41.58 ng/ml

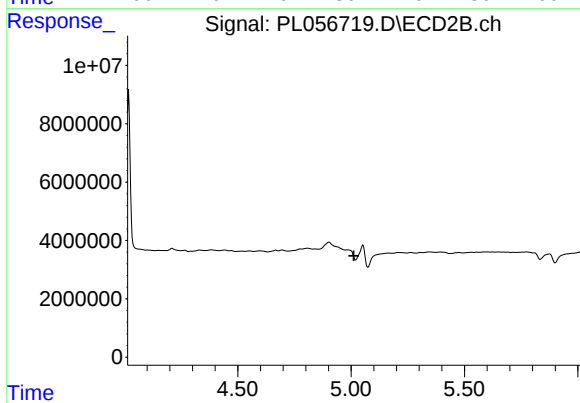

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 5.012 min
Response: 0
Conc: N.D.

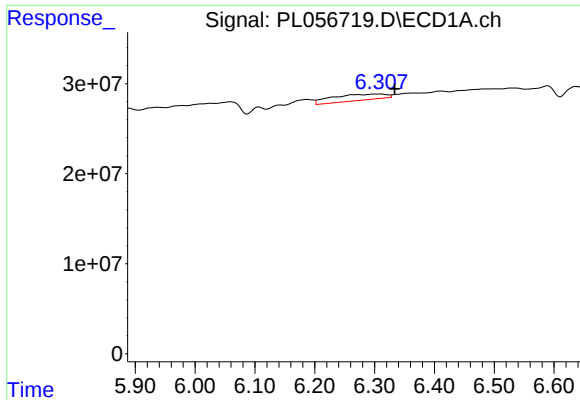

#27 Chlordane-5


R.T.: 6.309 min
Delta R.T.: -0.025 min
Response: 42907849
Conc: 131.04 ng/ml

Instrument :
ECD_L
ClientSampleId :

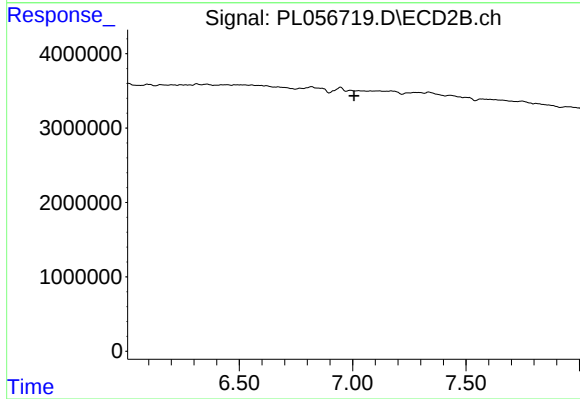


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T.: 7.007 min
Response: 0
Conc: N.D.

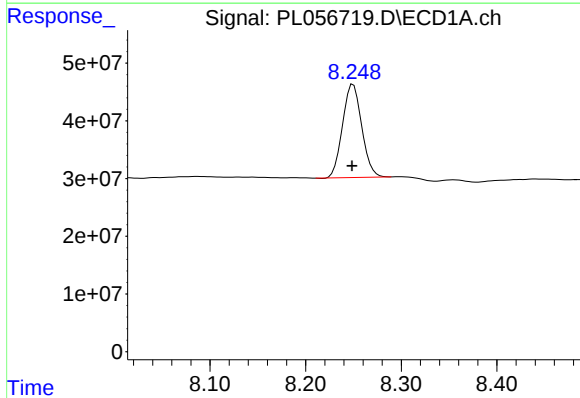

#28 Decachlorobiphenyl

R.T.: 8.250 min
Delta R.T.: 0.001 min
Response: 225807022
Conc: 18.98 ng/ml

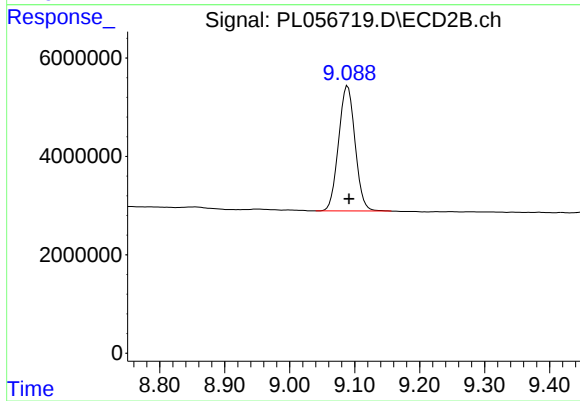

#28 Decachlorobiphenyl

R.T.: 9.089 min
Delta R.T.: -0.002 min
Response: 44815676
Conc: 21.33 ng/ml