

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022020\
 Data File : PL056720.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Feb 2020 20:41
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 21 00:33:54 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL021920.M
 Quant Title : GC Extractables
 QLast Update : Thu Feb 20 02:32:45 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.497	4.019	185.1E6	52052794	21.402	20.896
28)	SA Decachlor...	8.249	9.089	229.7E6	43449963	19.312	20.678
Target Compounds							
12)	B 4,4'-DDE	5.684f	0.000	85696515	0	6.092	N.D. #
18)	B Endrin al...	6.499	0.000	18556323	0	1.714	N.D. #
24)	Chlordane-2	4.883	0.000	7307399	0	18.733	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022020\
Data File : PL056720.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Feb 2020 20:41
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 21 00:33:54 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL021920.M
Quant Title : GC Extractables
QLast Update : Thu Feb 20 02:32:45 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

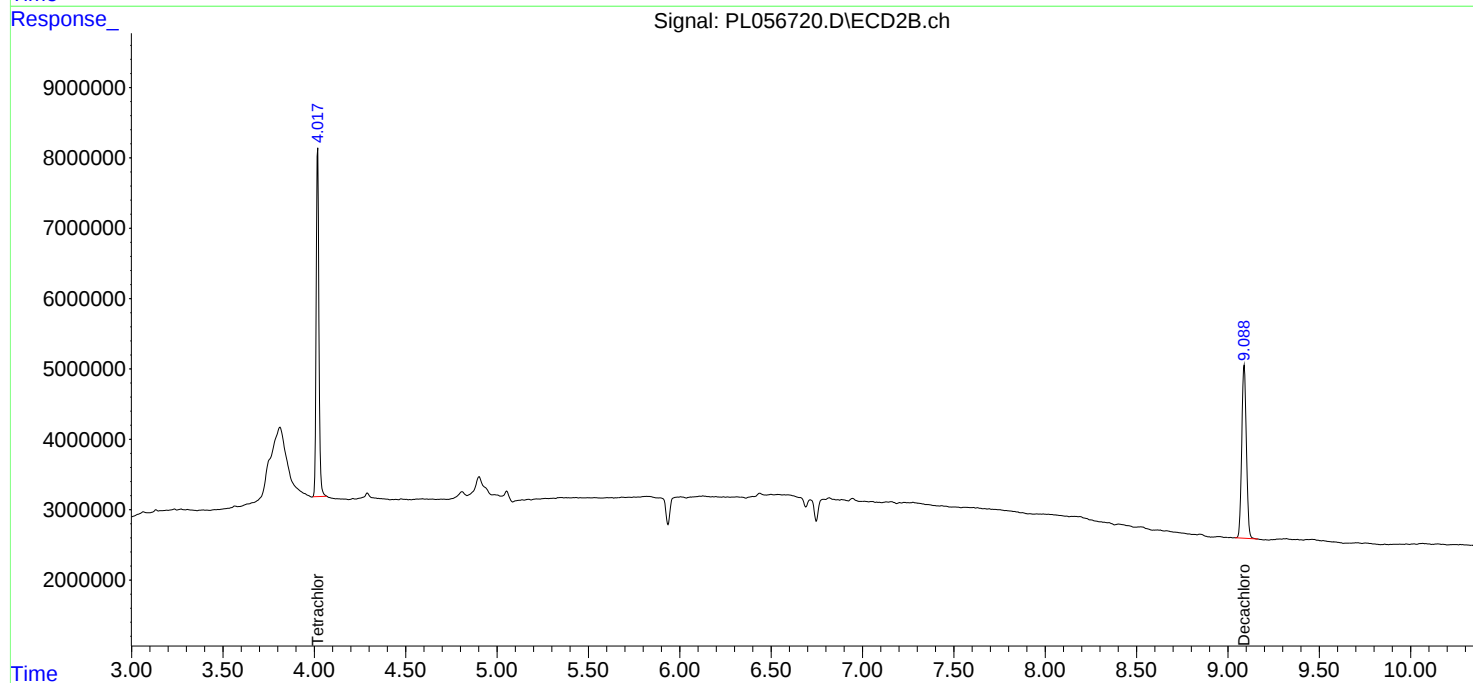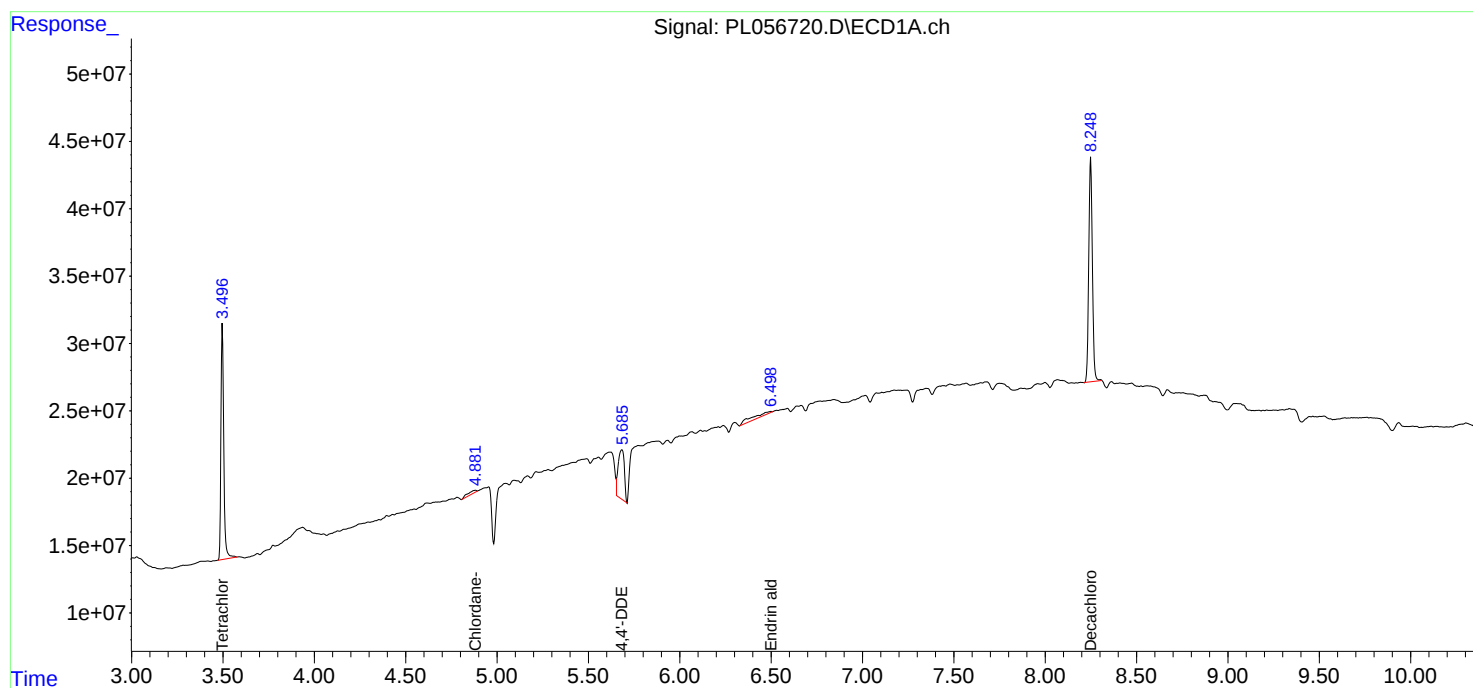


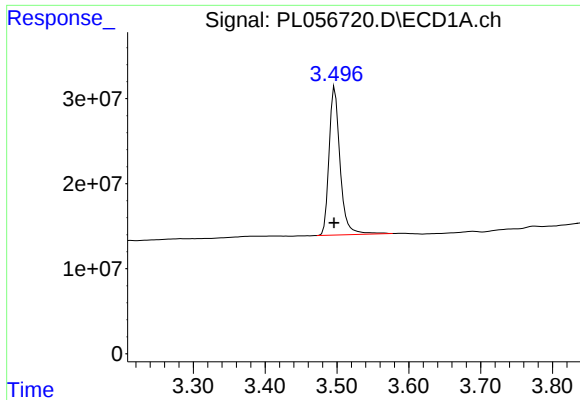

#1 Tetrachloro-m-xylene


R.T.: 3.497 min
Delta R.T.: 0.001 min
Response: 185079955
Conc: 21.40 ng/ml

Instrument :
ECD_L
ClientSampleId :

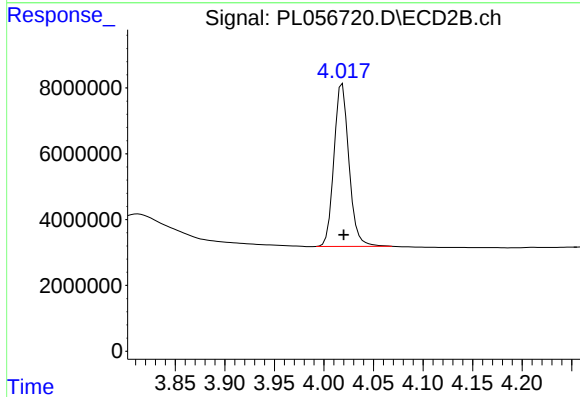


#1 Tetrachloro-m-xylene

R.T.: 4.019 min
Delta R.T.: -0.001 min
Response: 52052794
Conc: 20.90 ng/ml

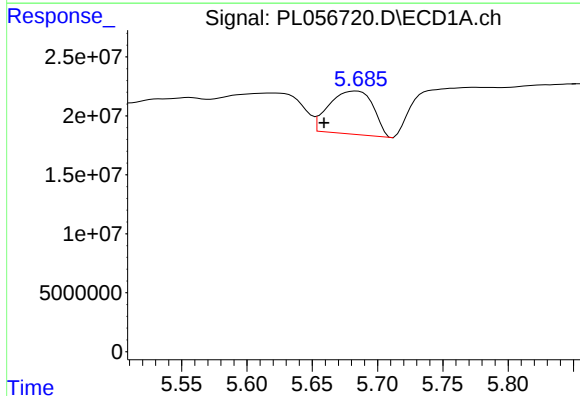


#12 4,4'-DDE

R.T.: 5.684 min
Delta R.T.: 0.025 min
Response: 85696515
Conc: 6.09 ng/ml

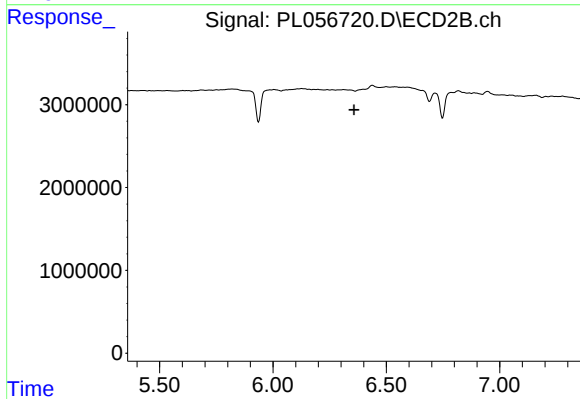

#12 4,4'-DDE


R.T.: 0.000 min
Exp R.T.: 6.358 min
Response: 0
Conc: N.D.

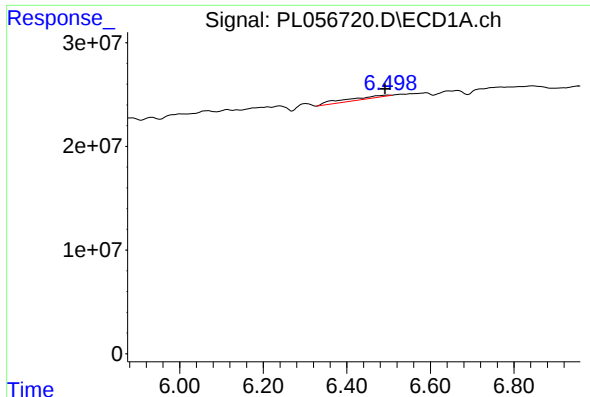

#18 Endrin aldehyde


R.T.: 6.499 min
Delta R.T.: 0.008 min
Response: 18556323
Conc: 1.71 ng/ml

Instrument :
ECD_L
ClientSampleId :

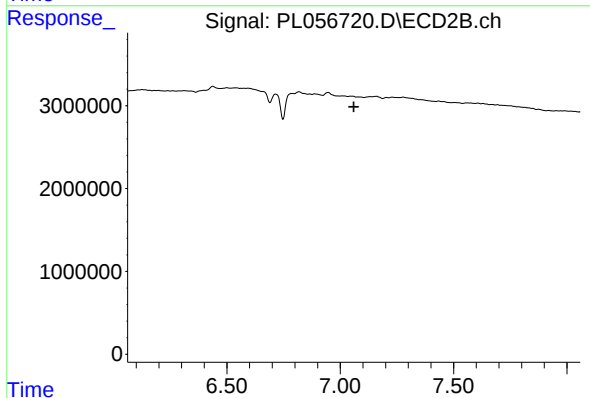


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T. : 7.060 min
Response: 0
Conc: N.D.

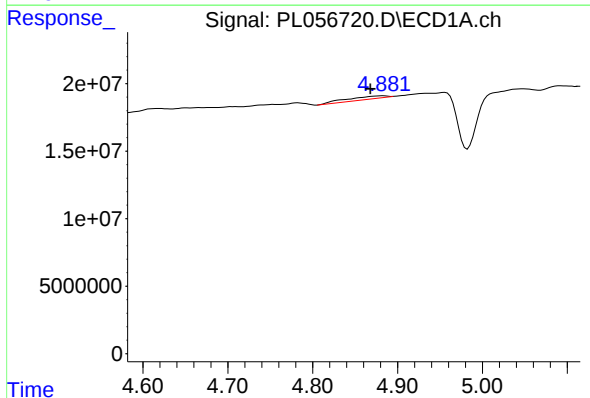


#24 Chlordane-2

R.T.: 4.883 min
Delta R.T.: 0.015 min
Response: 7307399
Conc: 18.73 ng/ml

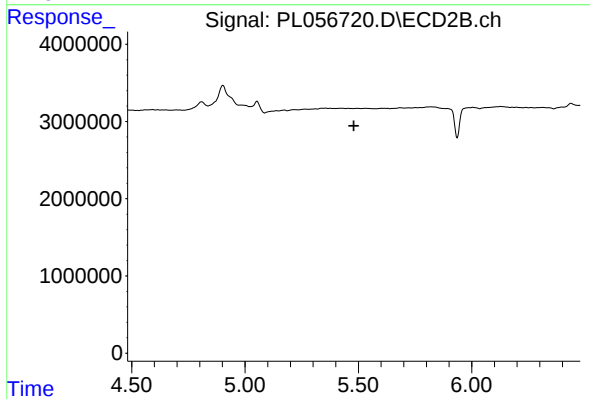

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T. : 5.480 min
Response: 0
Conc: N.D.

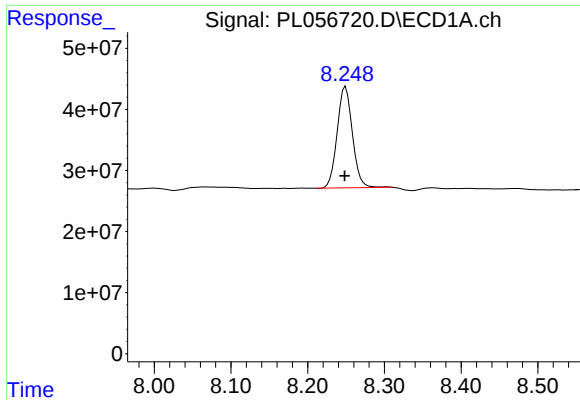

#28 Decachlorobiphenyl

R.T.: 8.249 min
Delta R.T.: 0.001 min
Response: 229716813
Conc: 19.31 ng/ml

Instrument :
ECD_L
ClientSampleId :

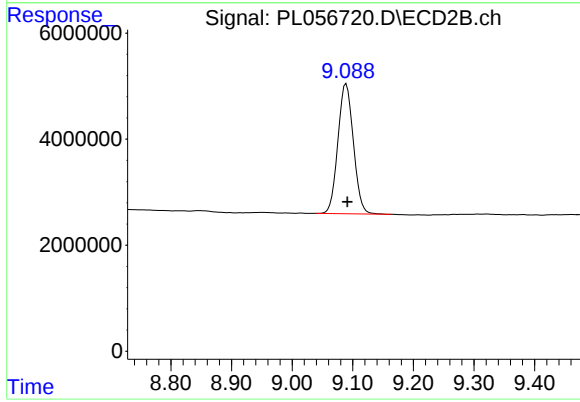

#28 Decachlorobiphenyl

R.T.: 9.089 min
Delta R.T.: -0.002 min
Response: 43449963
Conc: 20.68 ng/ml