

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022020\
 Data File : PL056693.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Feb 2020 14:20
 Operator : AJ\MA
 Sample : L1599-01
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 FK-BPM-03-011-ABCD

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 21 00:28:50 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL021920.M
 Quant Title : GC Extractables
 QLast Update : Thu Feb 20 02:32:45 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.498	4.019	188.9E6	54424983	21.843	21.849
28)	SA Decachlor...	8.249	9.090	221.9E6	42234772	18.656	20.099

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022020\
Data File : PL056693.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Feb 2020 14:20
Operator : AJ\MA
Sample : L1599-01
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
FK-BPM-03-011-ABCD

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 21 00:28:50 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL021920.M
Quant Title : GC Extractables
QLast Update : Thu Feb 20 02:32:45 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

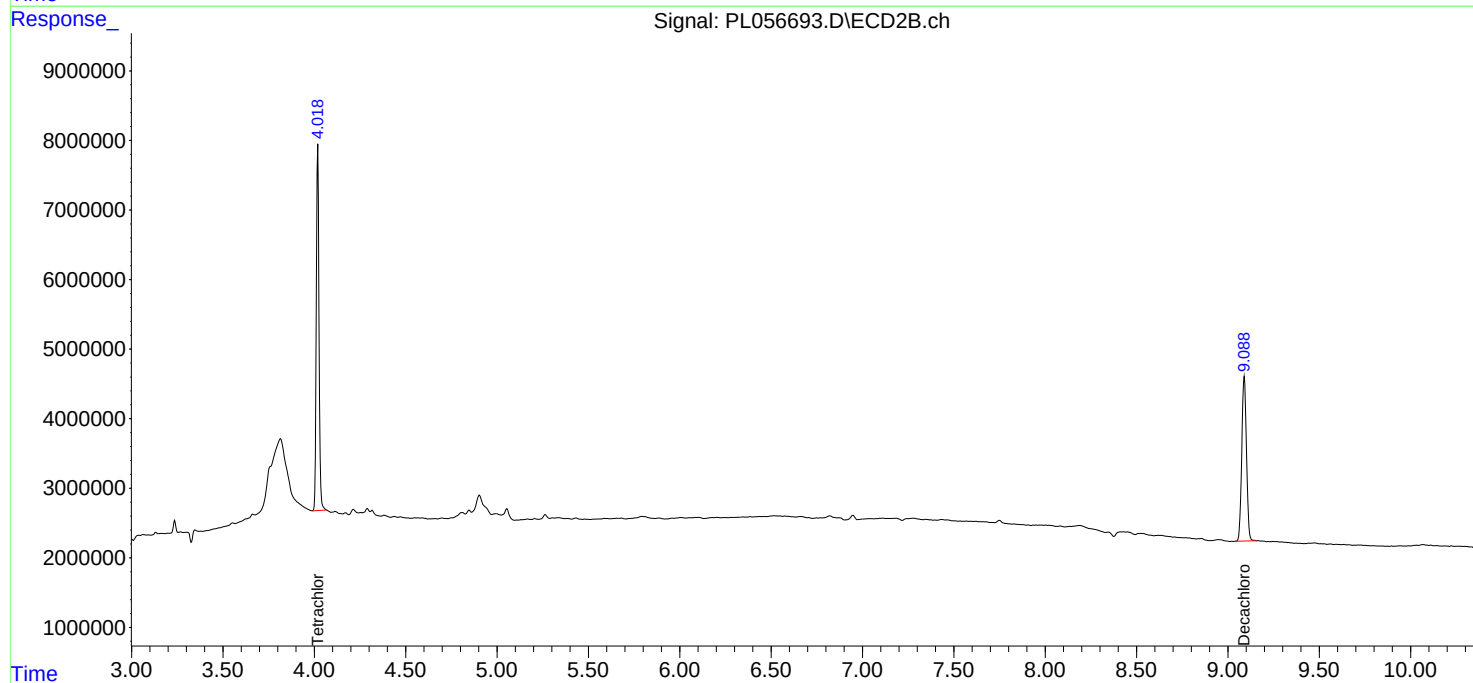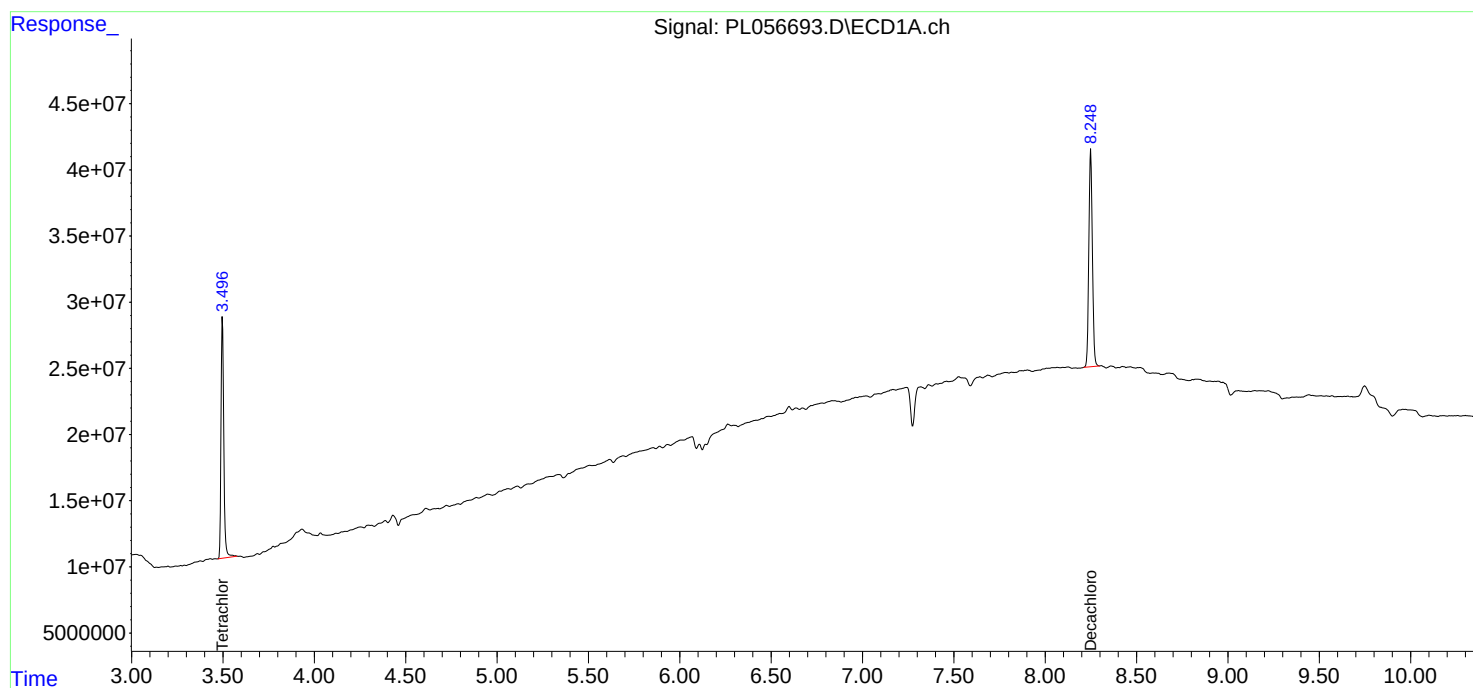


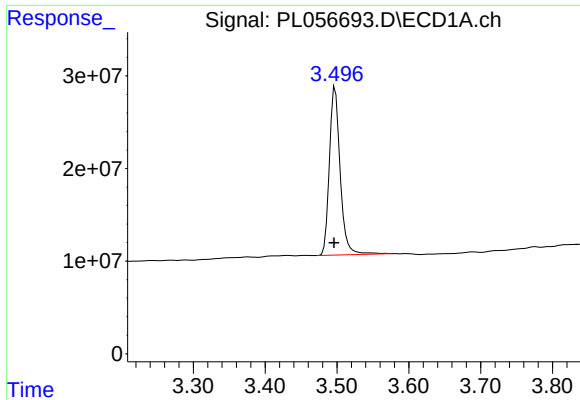

#1 Tetrachloro-m-xylene


R.T.: 3.498 min
Delta R.T.: 0.002 min
Response: 188893987
Conc: 21.84 ng/ml

Instrument :
ECD_L
ClientSampleId :
FK-BPM-03-011-ABCD

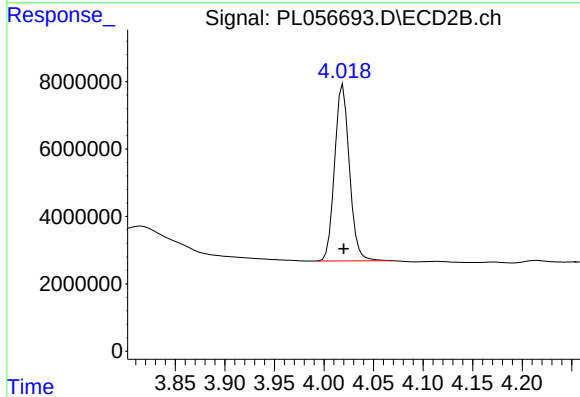


#1 Tetrachloro-m-xylene

R.T.: 4.019 min
Delta R.T.: 0.000 min
Response: 54424983
Conc: 21.85 ng/ml

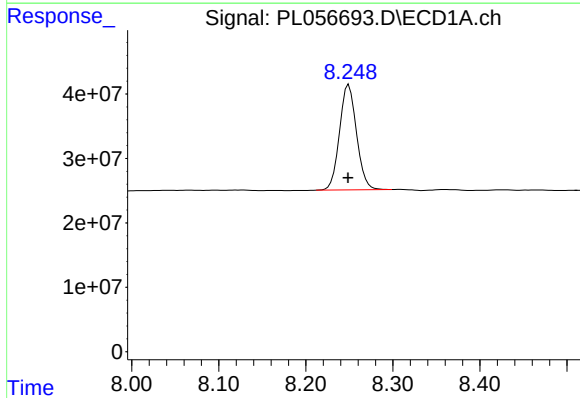

#28 Decachlorobiphenyl

R.T.: 8.249 min
Delta R.T.: 0.001 min
Response: 221912311
Conc: 18.66 ng/ml

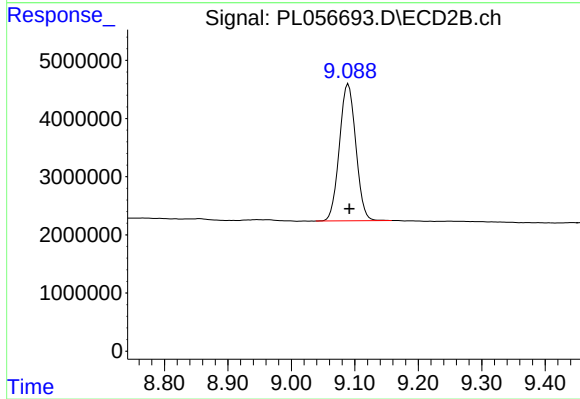

#28 Decachlorobiphenyl

R.T.: 9.090 min
Delta R.T.: -0.001 min
Response: 42234772
Conc: 20.10 ng/ml