

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022023\
 Data File : PL081030.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Feb 2023 14:51
 Operator : AR\AJ
 Sample : PCHLORICC750 (Sig #1); CHLORICC750 (Sig #2)
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 20 15:36:56 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022023.M
 Quant Title : GC Extractables
 QLast Update : Mon Feb 20 15:36:19 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.351	2.687	169.0E6	214.0E6	74.840	75.119
28)	SA Decachlor...	8.790	7.832	136.7E6	167.5E6	72.921	73.428
Target Compounds							
23)	Chlordane-1	4.498	3.683	70173997	62362096	742.000	751.521
24)	Chlordane-2	5.025	4.259	76183626	66921144	734.547	730.476
25)	Chlordane-3	5.731	4.889	294.9E6	206.9E6	759.086	766.984
26)	Chlordane-4	5.813	4.951	356.2E6	208.7E6	753.123	764.338
27)	Chlordane-5	6.655	5.619	60399955	56742700	752.023	747.932



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022023\
Data File : PL081030.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Feb 2023 14:51
Operator : AR\AJ
Sample : PCHLORICC750 (Sig #1); CHLORICC750 (Sig #2)
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 20 15:36:56 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022023.M
Quant Title : GC Extractables
QLast Update : Mon Feb 20 15:36:19 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

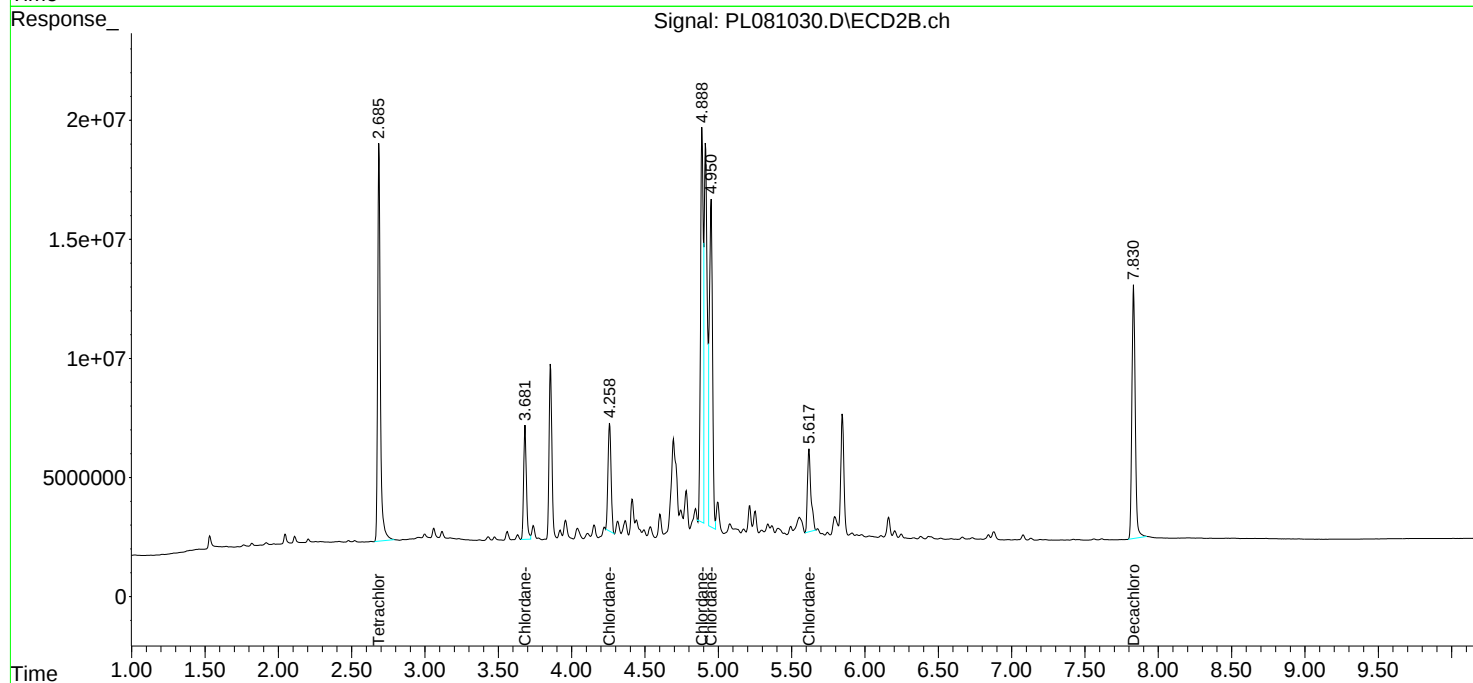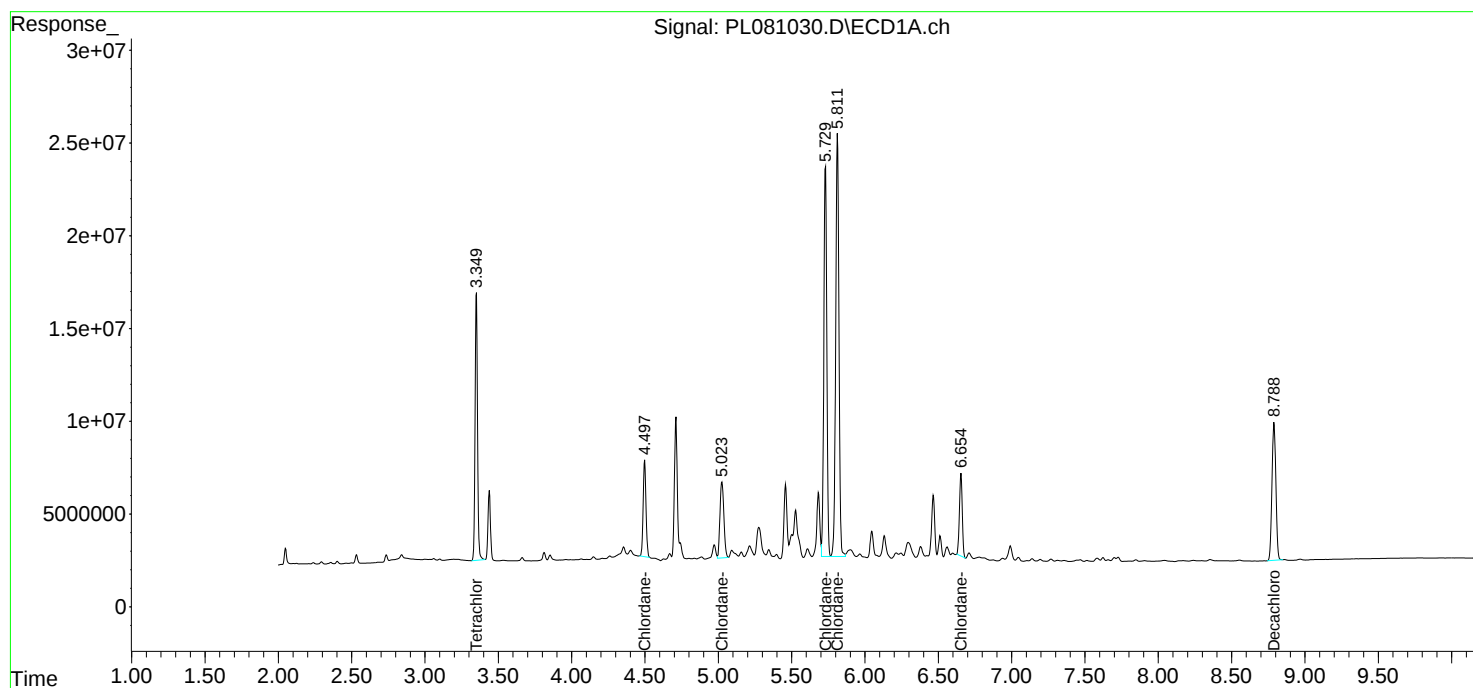


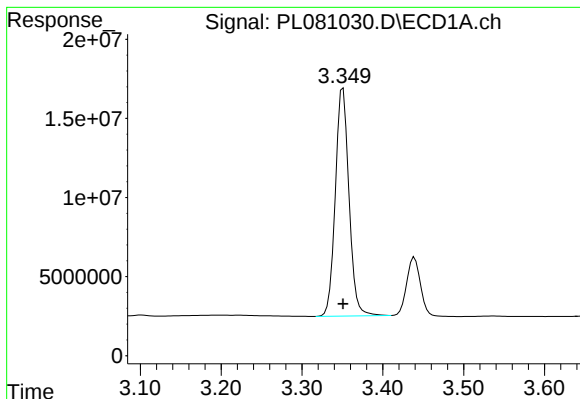

#1 Tetrachloro-m-xylene


R.T.: 3.351 min
Delta R.T.: 0.000 min
Response: 169002078
Conc: 74.84 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

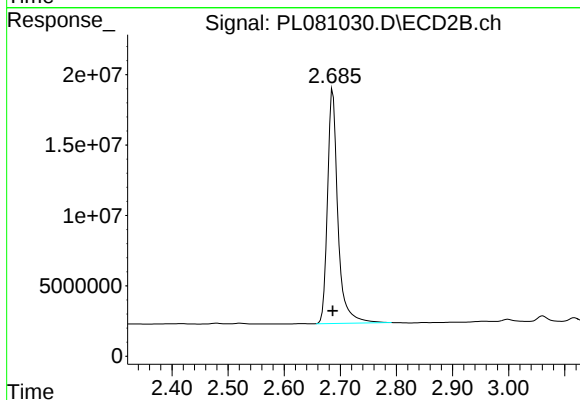


#1 Tetrachloro-m-xylene

R.T.: 2.687 min
Delta R.T.: 0.000 min
Response: 213957759
Conc: 75.12 ng/ml

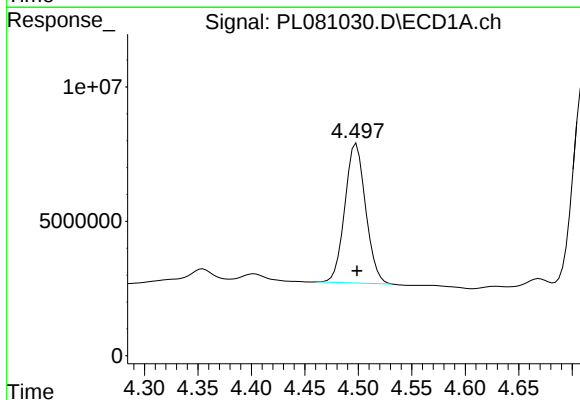


#23 Chlordane-1

R.T.: 4.498 min
Delta R.T.: 0.000 min
Response: 70173997
Conc: 742.00 ng/ml

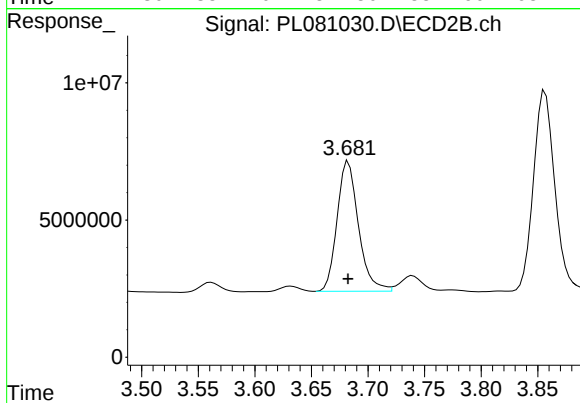

#23 Chlordane-1


R.T.: 3.683 min
Delta R.T.: 0.000 min
Response: 62362096
Conc: 751.52 ng/ml

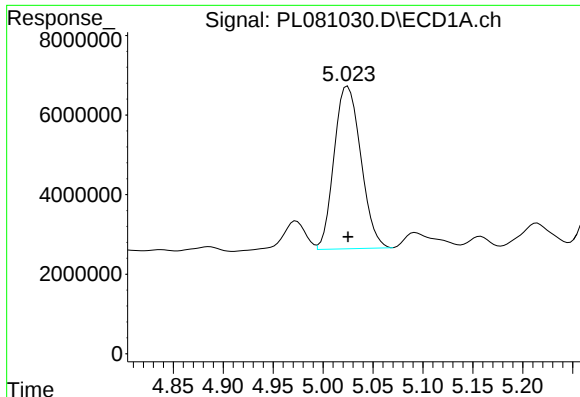

#24 Chlordane-2


R.T.: 5.025 min
Delta R.T.: 0.000 min
Response: 76183626
Conc: 734.55 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

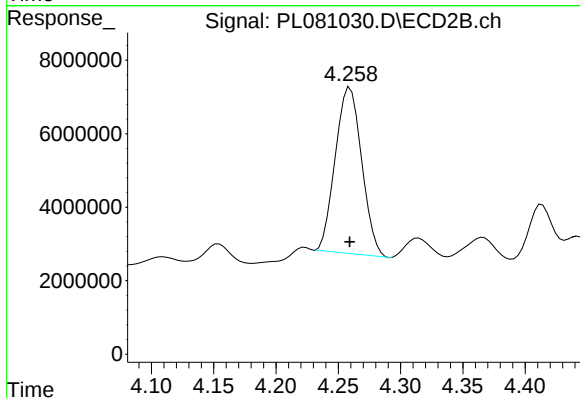


#24 Chlordane-2

R.T.: 4.259 min
Delta R.T.: 0.000 min
Response: 66921144
Conc: 730.48 ng/ml

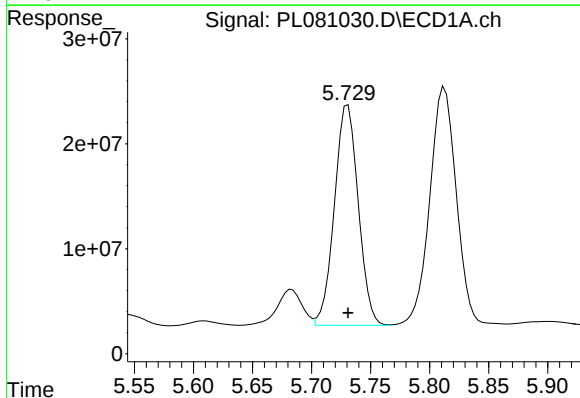


#25 Chlordane-3

R.T.: 5.731 min
Delta R.T.: 0.000 min
Response: 294939648
Conc: 759.09 ng/ml

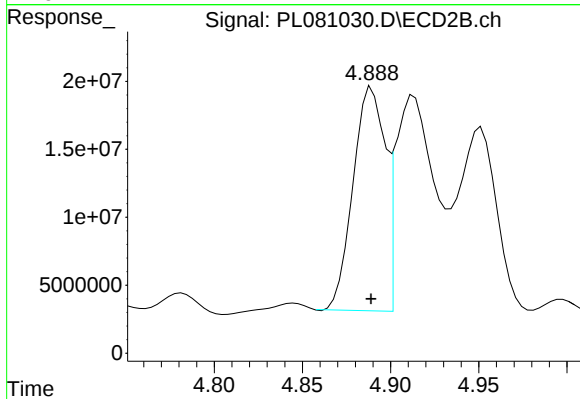

#25 Chlordane-3


R.T.: 4.889 min
Delta R.T.: 0.000 min
Response: 206935008
Conc: 766.98 ng/ml

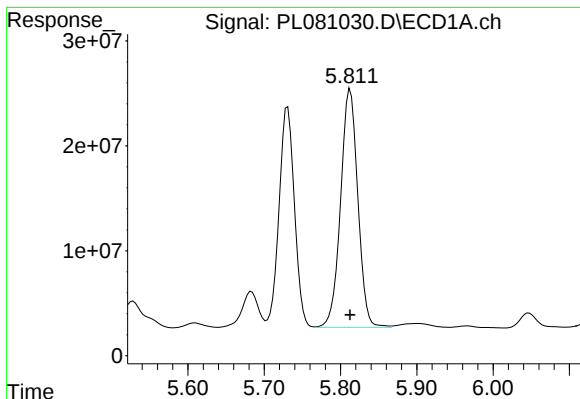

#26 Chlordane-4


R.T.: 5.813 min
Delta R.T.: 0.000 min
Response: 356178272
Conc: 753.12 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

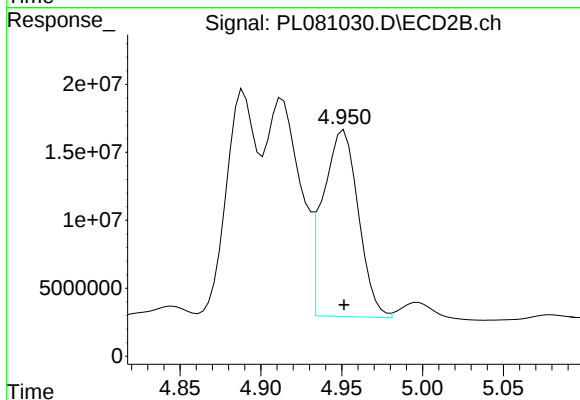


#26 Chlordane-4

R.T.: 4.951 min
Delta R.T.: 0.000 min
Response: 208682640
Conc: 764.34 ng/ml

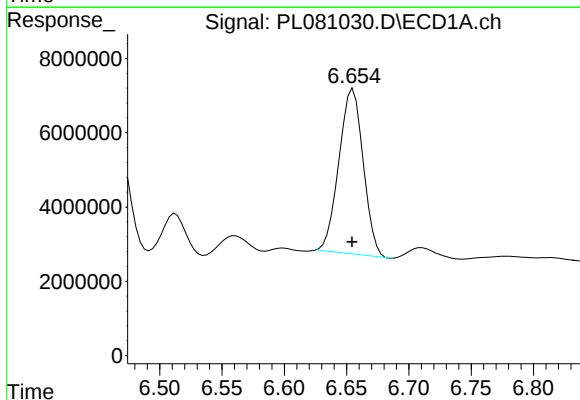


#27 Chlordane-5

R.T.: 6.655 min
Delta R.T.: 0.000 min
Response: 60399955
Conc: 752.02 ng/ml

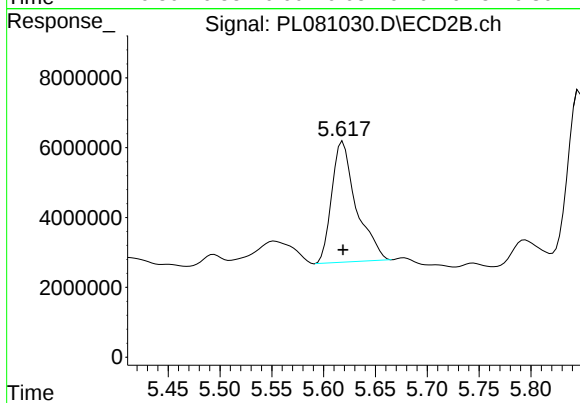

#27 Chlordane-5


R.T.: 5.619 min
Delta R.T.: 0.000 min
Response: 56742700
Conc: 747.93 ng/ml

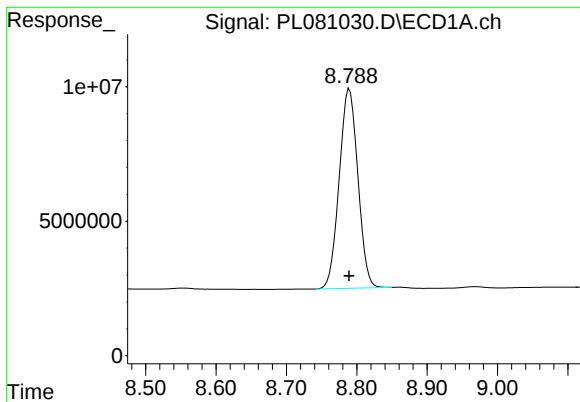

#28 Decachlorobiphenyl

R.T.: 8.790 min
Delta R.T.: 0.000 min
Response: 136719499
Conc: 72.92 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

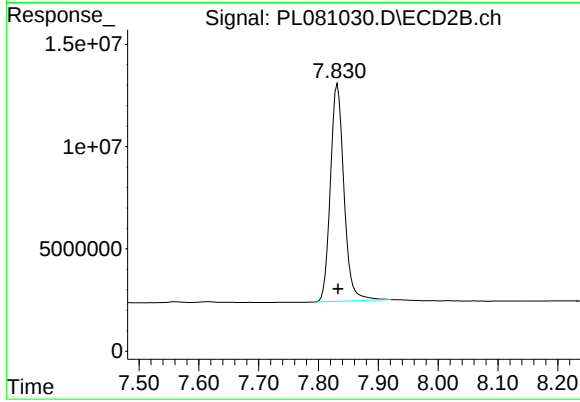

#28 Decachlorobiphenyl

R.T.: 7.832 min
Delta R.T.: 0.000 min
Response: 167498588
Conc: 73.43 ng/ml