

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022023\
 Data File : PL081031.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Feb 2023 15:05
 Operator : AR\AJ
 Sample : PCHLORICC500 (Sig #1); CHLORICC500 (Sig #2)
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 20 15:37:06 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022023.M
 Quant Title : GC Extractables
 QLast Update : Mon Feb 20 15:36:19 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.351	2.686	112.9E6	142.4E6	50.000	50.000
28)	SA Decachlor...	8.789	7.833	93745003	114.1E6	50.000	50.000
Target Compounds							
23)	Chlordane-1	4.499	3.682	47287068	41490584	500.000	500.000
24)	Chlordane-2	5.025	4.259	51857564	45806522	500.000	500.000
25)	Chlordane-3	5.731	4.889	194.3E6	134.9E6	500.000	500.000
26)	Chlordane-4	5.813	4.951	236.5E6	136.5E6	500.000	500.000
27)	Chlordane-5	6.654	5.619	40158322	37933070	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022023\
Data File : PL081031.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Feb 2023 15:05
Operator : AR\AJ
Sample : PCHLORICC500 (Sig #1); CHLORICC500 (Sig #2)
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 20 15:37:06 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022023.M
Quant Title : GC Extractables
QLast Update : Mon Feb 20 15:36:19 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

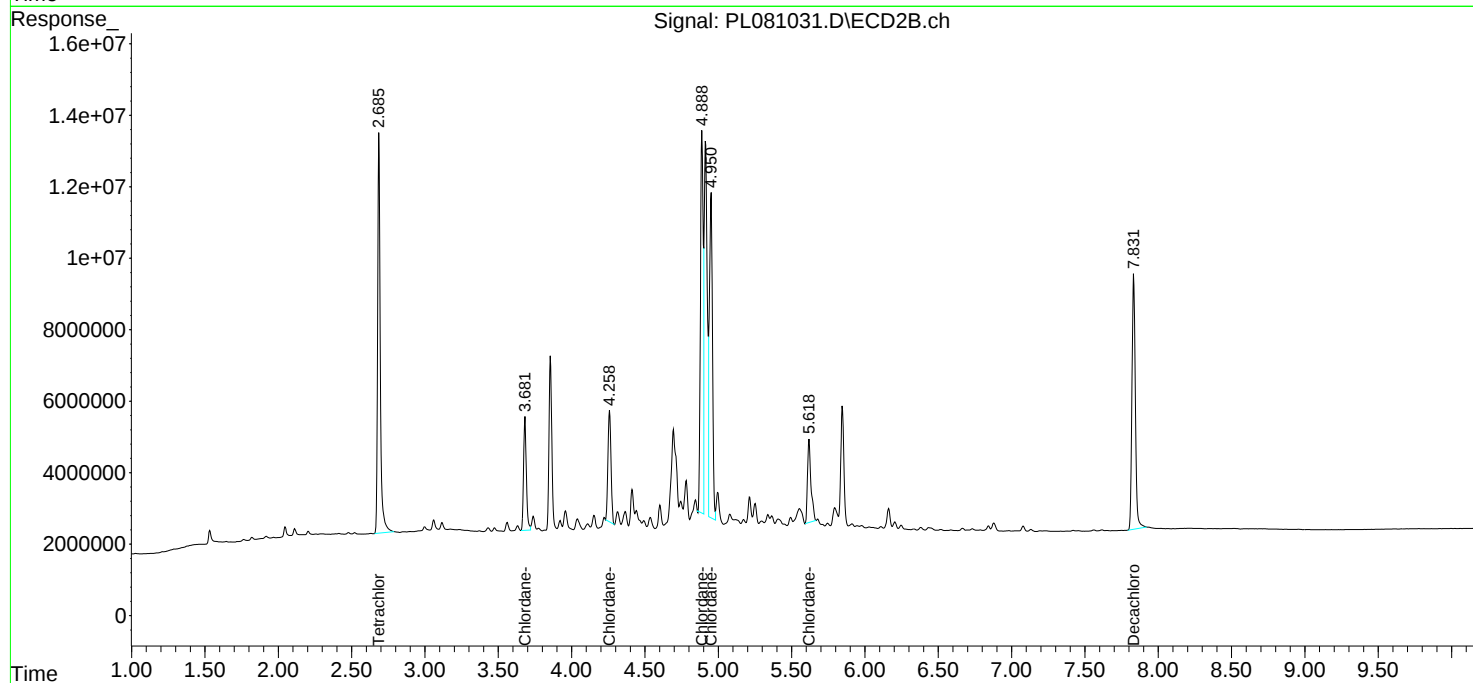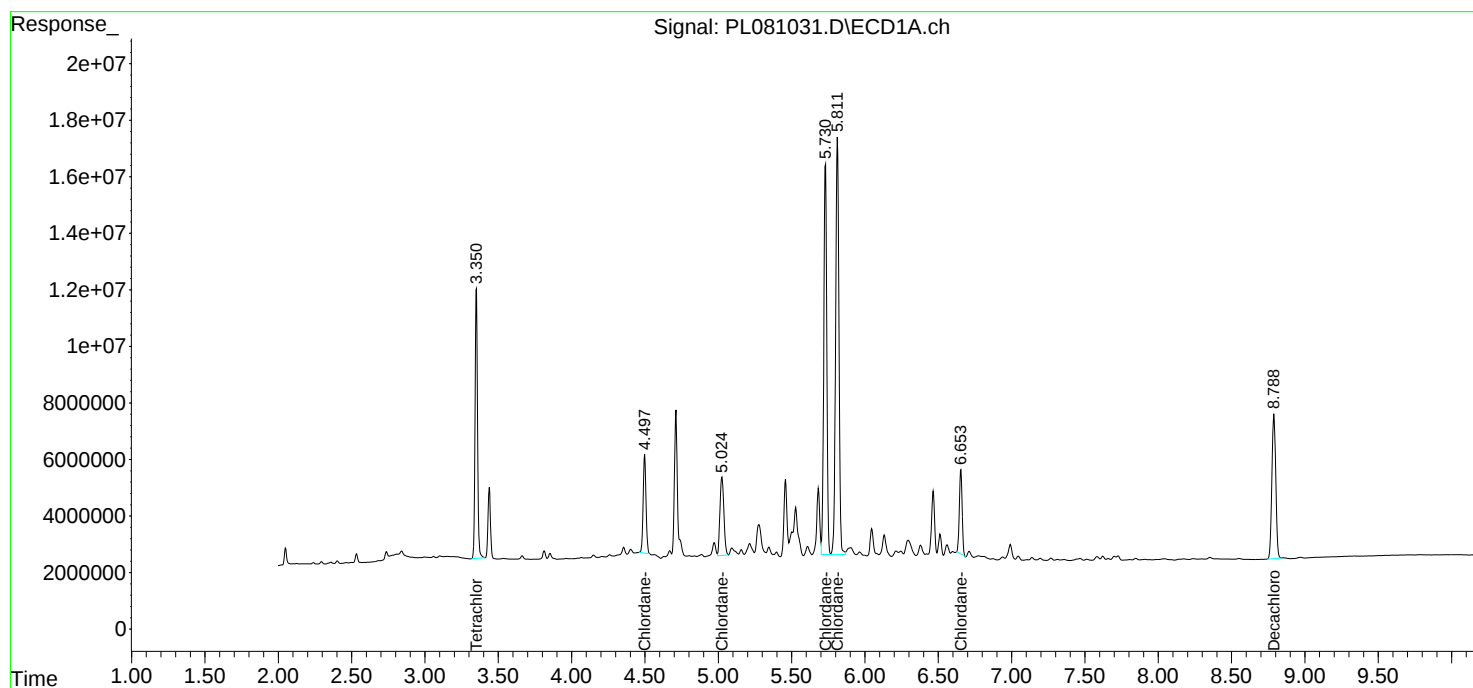


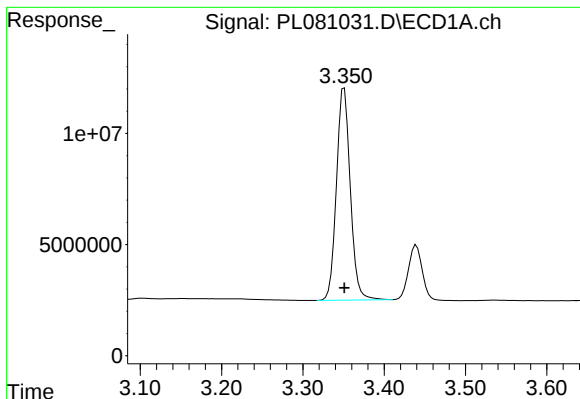

#1 Tetrachloro-m-xylene


R.T.: 3.351 min
Delta R.T.: 0.000 min
Response: 112908932
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

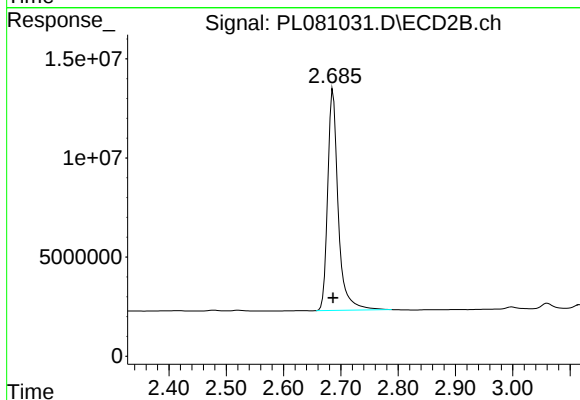


#1 Tetrachloro-m-xylene

R.T.: 2.686 min
Delta R.T.: 0.000 min
Response: 142412690
Conc: 50.00 ng/ml

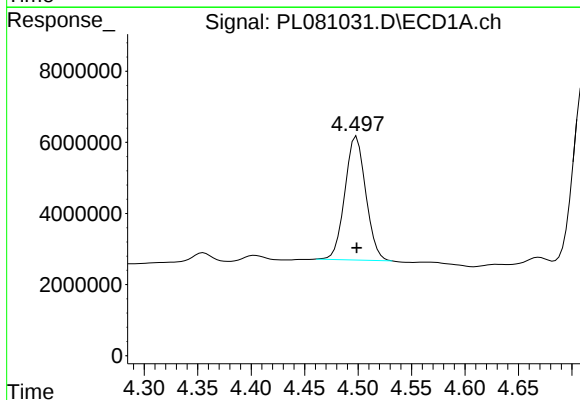


#23 Chlordane-1

R.T.: 4.499 min
Delta R.T.: 0.000 min
Response: 47287068
Conc: 500.00 ng/ml

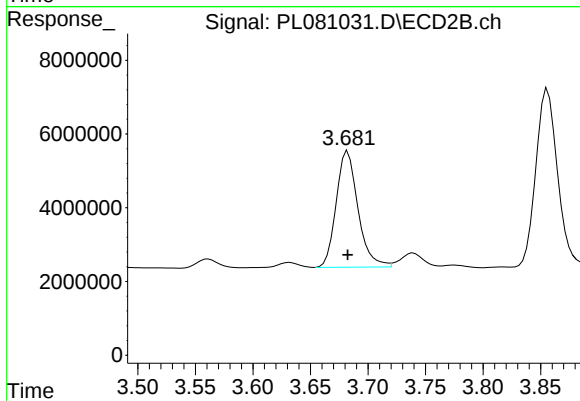

#23 Chlordane-1


R.T.: 3.682 min
Delta R.T.: 0.000 min
Response: 41490584
Conc: 500.00 ng/ml

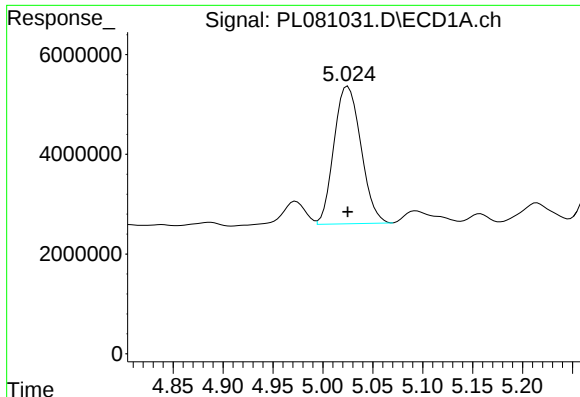

#24 Chlordane-2


R.T.: 5.025 min
Delta R.T.: 0.000 min
Response: 51857564
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

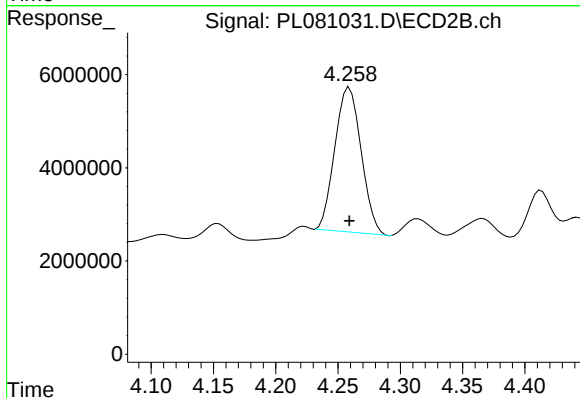


#24 Chlordane-2

R.T.: 4.259 min
Delta R.T.: 0.000 min
Response: 45806522
Conc: 500.00 ng/ml

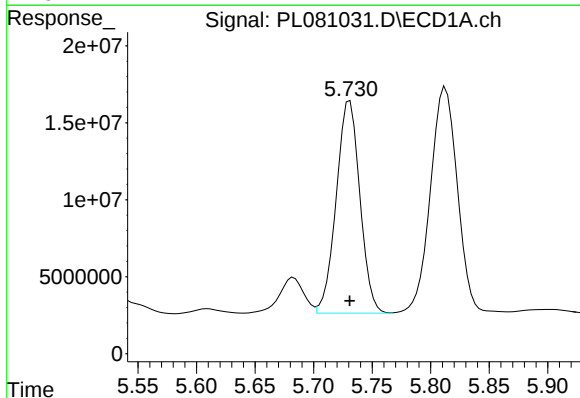


#25 Chlordane-3

R.T.: 5.731 min
Delta R.T.: 0.000 min
Response: 194273005
Conc: 500.00 ng/ml

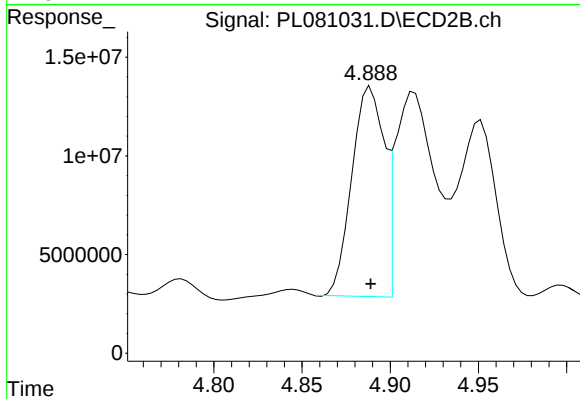

#25 Chlordane-3


R.T.: 4.889 min
Delta R.T.: 0.000 min
Response: 134901815
Conc: 500.00 ng/ml

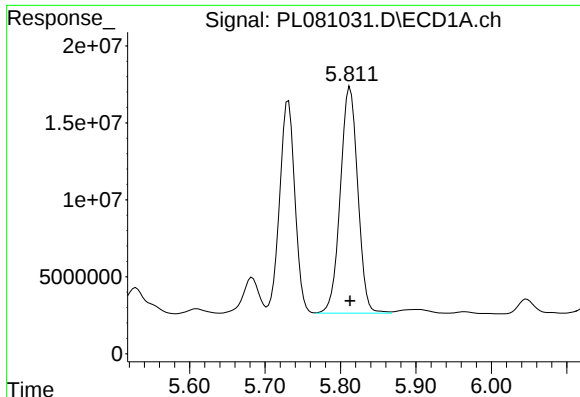

#26 Chlordane-4


R.T.: 5.813 min
Delta R.T.: 0.000 min
Response: 236467680
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

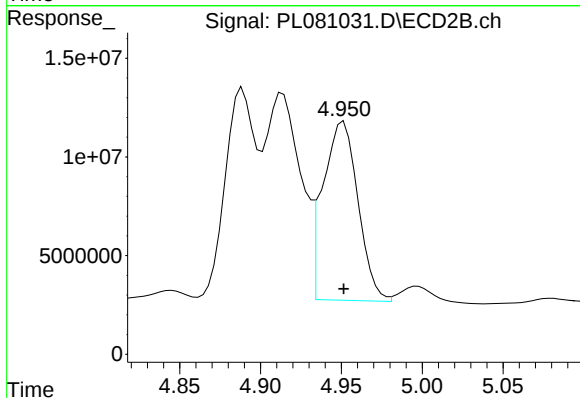


#26 Chlordane-4

R.T.: 4.951 min
Delta R.T.: 0.000 min
Response: 136511927
Conc: 500.00 ng/ml

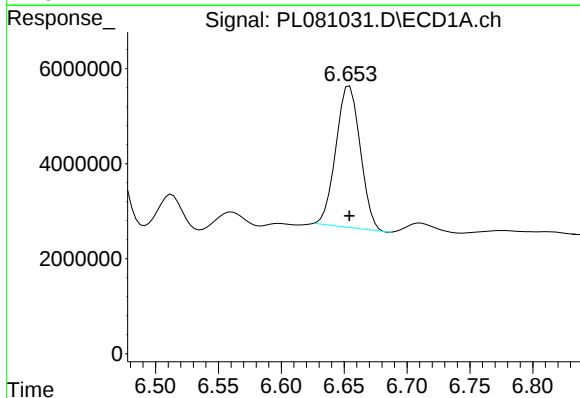


#27 Chlordane-5

R.T.: 6.654 min
Delta R.T.: 0.000 min
Response: 40158322
Conc: 500.00 ng/ml

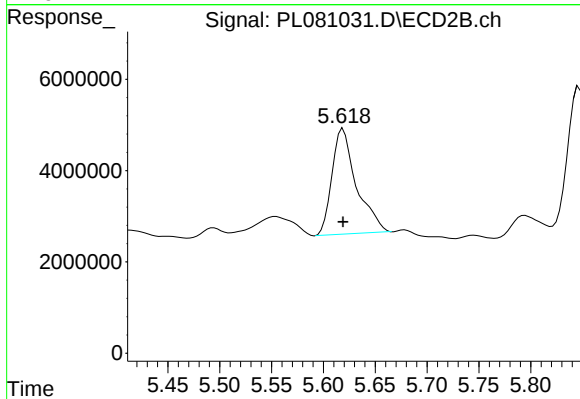

#27 Chlordane-5


R.T.: 5.619 min
Delta R.T.: 0.000 min
Response: 37933070
Conc: 500.00 ng/ml

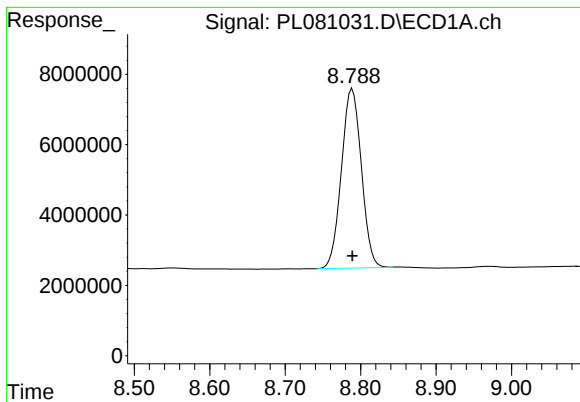

#28 Decachlorobiphenyl

R.T.: 8.789 min
Delta R.T.: 0.000 min
Response: 93745003
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

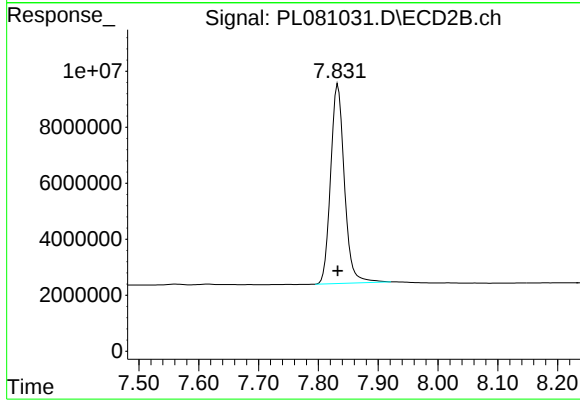

#28 Decachlorobiphenyl

R.T.: 7.833 min
Delta R.T.: 0.000 min
Response: 114055946
Conc: 50.00 ng/ml