

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022023\
 Data File : PL081032.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Feb 2023 15:19
 Operator : AR\AJ
 Sample : PCHLORICC250 (Sig #1); CHLORICC250 (Sig #2)
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 20 15:37:13 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022023.M
 Quant Title : GC Extractables
 QLast Update : Mon Feb 20 15:36:19 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.351	2.686	54684153	68554455	24.216	24.069
28)	SA Decachlor...	8.789	7.832	48095227	58706630	25.652	25.736
Target Compounds							
23)	Chlordane-1	4.499	3.682	22459319	20124514	237.478	242.519
24)	Chlordane-2	5.025	4.259	25620398	23100248	247.027	252.150
25)	Chlordane-3	5.731	4.889	91624073	62923154	235.813	233.218
26)	Chlordane-4	5.813	4.951	113.4E6	65213064	239.816	238.855
27)	Chlordane-5	6.655	5.619	19410941	18835866	241.680	248.278



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022023\
Data File : PL081032.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Feb 2023 15:19
Operator : AR\AJ
Sample : PCHLORICC250 (Sig #1); CHLORICC250 (Sig #2)
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 20 15:37:13 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022023.M
Quant Title : GC Extractables
QLast Update : Mon Feb 20 15:36:19 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

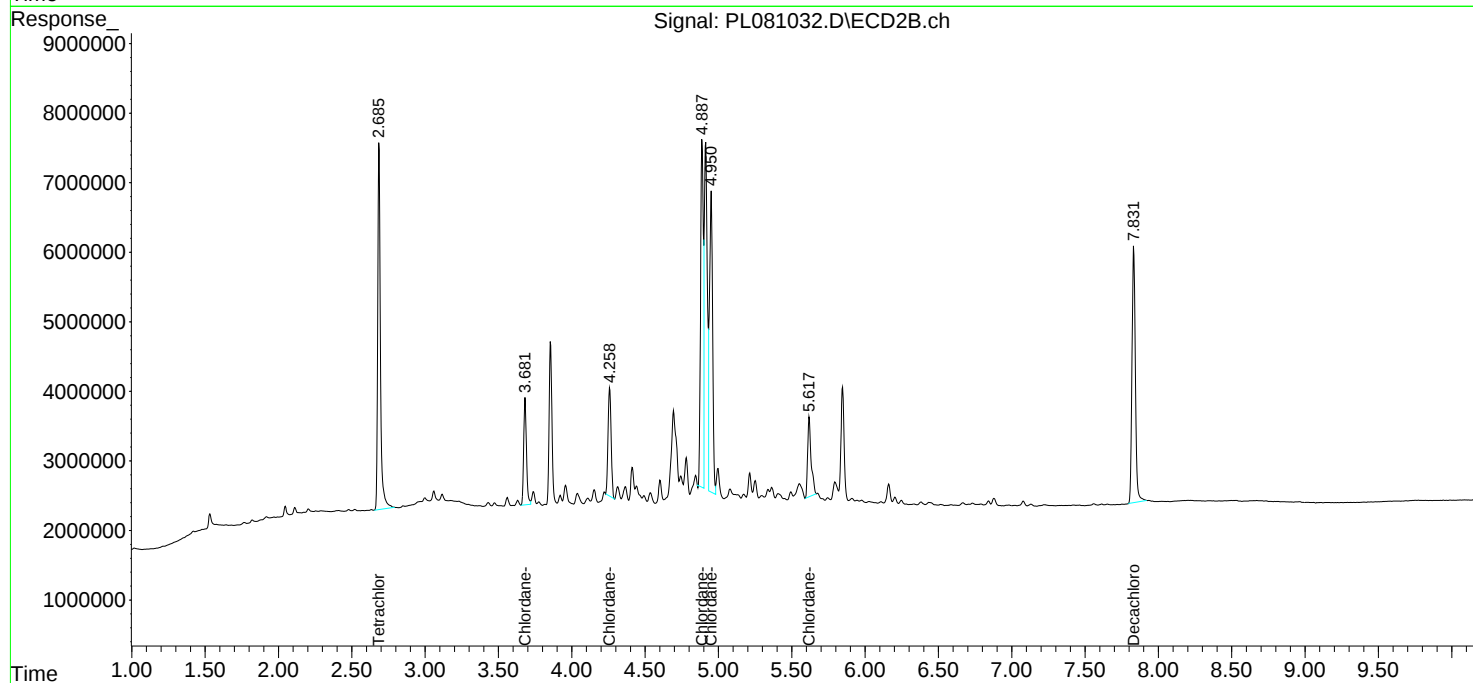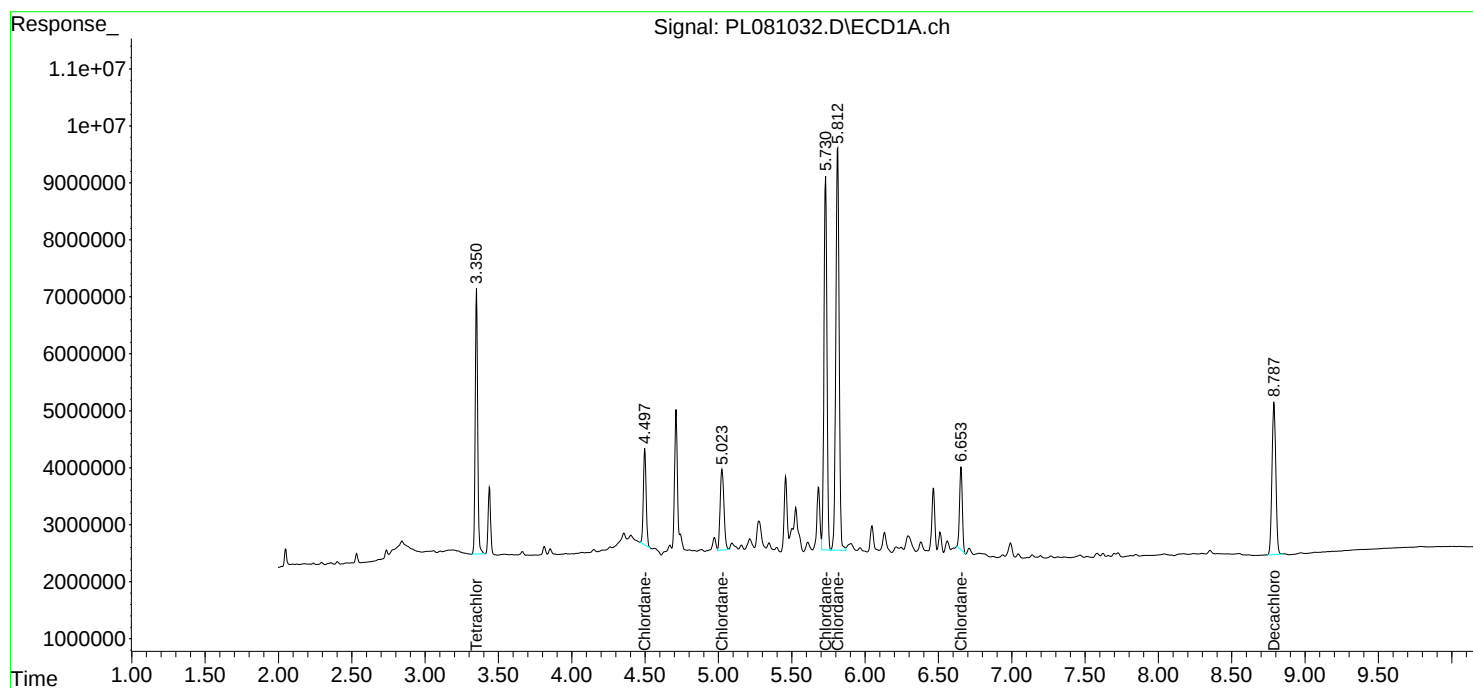


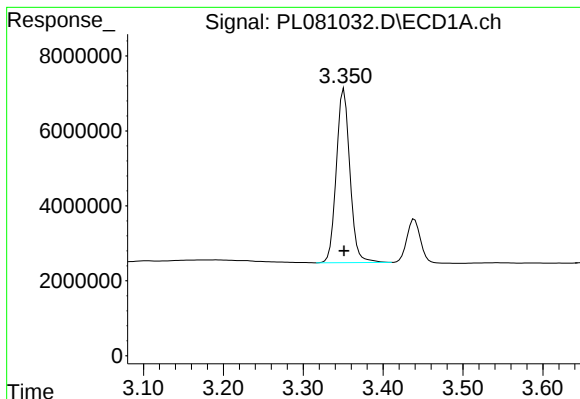

#1 Tetrachloro-m-xylene


R.T.: 3.351 min
Delta R.T.: 0.000 min
Response: 54684153
Conc: 24.22 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

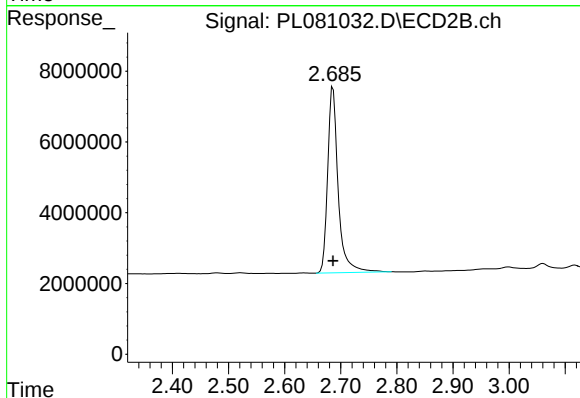


#1 Tetrachloro-m-xylene

R.T.: 2.686 min
Delta R.T.: 0.000 min
Response: 68554455
Conc: 24.07 ng/ml

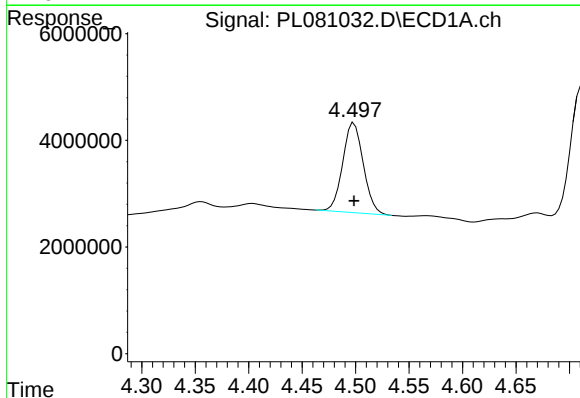


#23 Chlordane-1

R.T.: 4.499 min
Delta R.T.: 0.000 min
Response: 22459319
Conc: 237.48 ng/ml

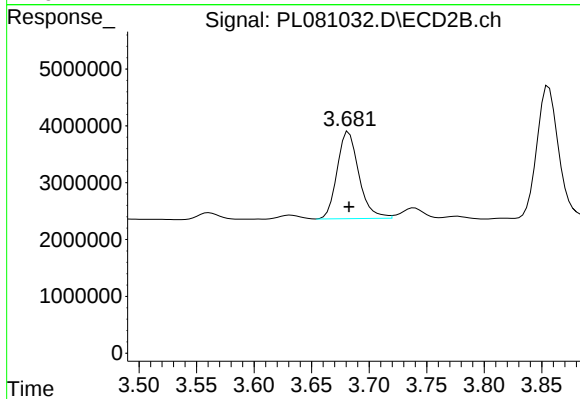

#23 Chlordane-1


R.T.: 3.682 min
Delta R.T.: 0.000 min
Response: 20124514
Conc: 242.52 ng/ml

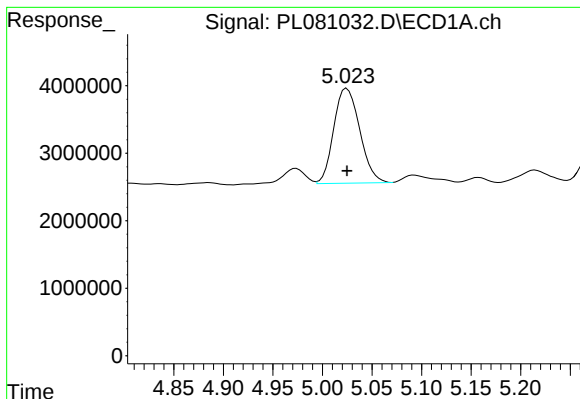

#24 Chlordane-2


R.T.: 5.025 min
Delta R.T.: 0.000 min
Response: 25620398
Conc: 247.03 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

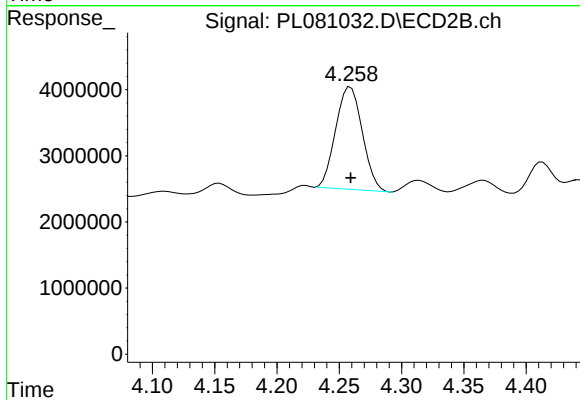


#24 Chlordane-2

R.T.: 4.259 min
Delta R.T.: 0.000 min
Response: 23100248
Conc: 252.15 ng/ml

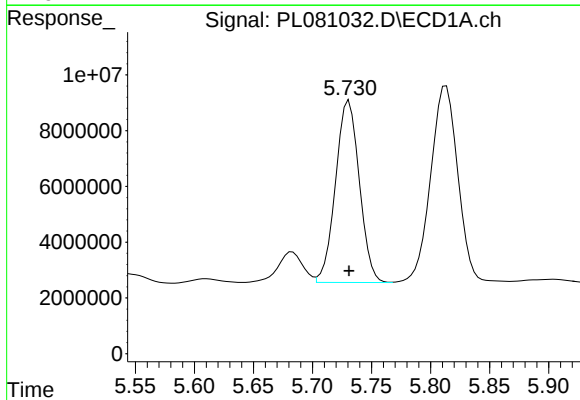


#25 Chlordane-3

R.T.: 5.731 min
Delta R.T.: 0.000 min
Response: 91624073
Conc: 235.81 ng/ml

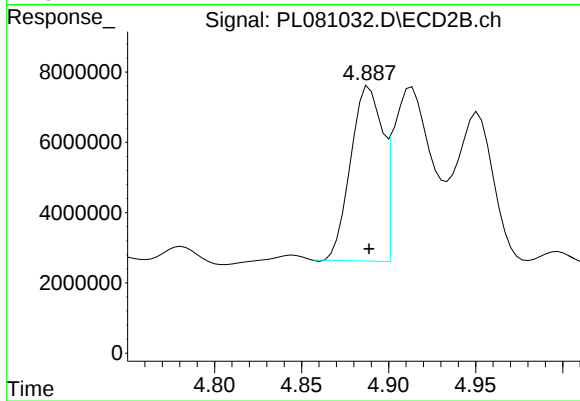

#25 Chlordane-3


R.T.: 4.889 min
Delta R.T.: 0.000 min
Response: 62923154
Conc: 233.22 ng/ml

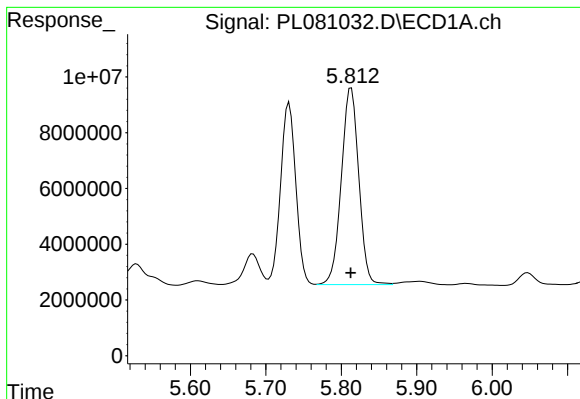

#26 Chlordane-4


R.T.: 5.813 min
Delta R.T.: 0.000 min
Response: 113417632
Conc: 239.82 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

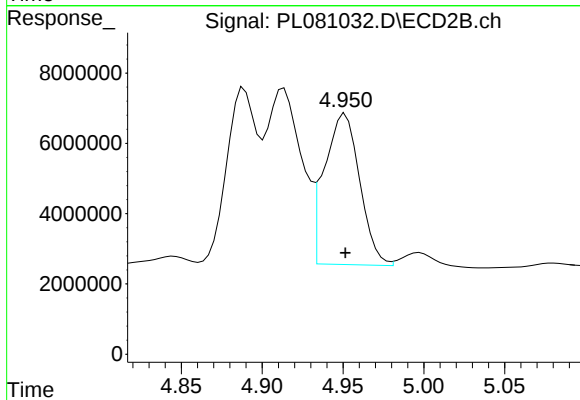


#26 Chlordane-4

R.T.: 4.951 min
Delta R.T.: 0.000 min
Response: 65213064
Conc: 238.85 ng/ml

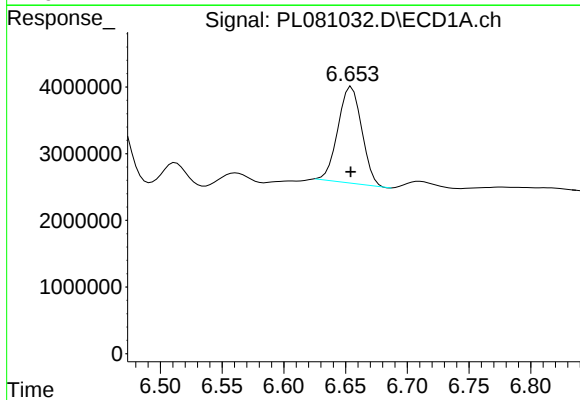


#27 Chlordane-5

R.T.: 6.655 min
Delta R.T.: 0.000 min
Response: 19410941
Conc: 241.68 ng/ml

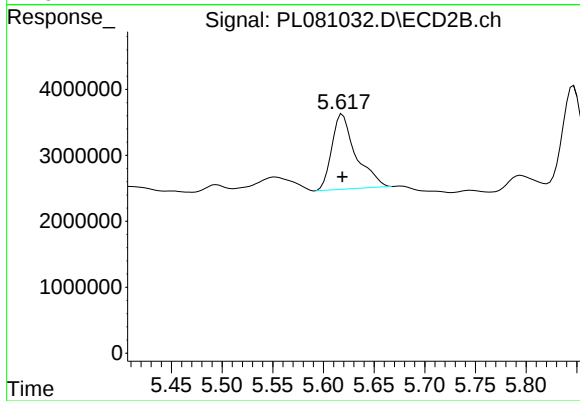

#27 Chlordane-5


R.T.: 5.619 min
Delta R.T.: 0.000 min
Response: 18835866
Conc: 248.28 ng/ml

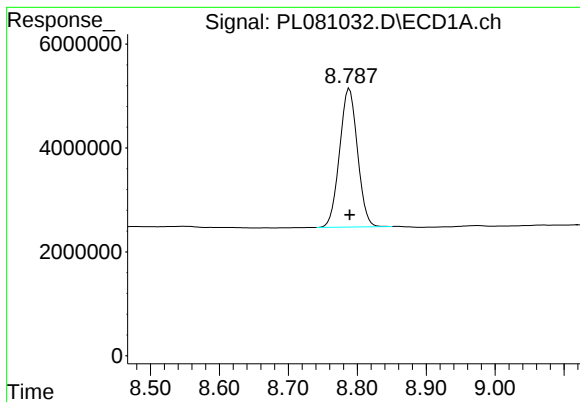

#28 Decachlorobiphenyl

R.T.: 8.789 min
Delta R.T.: 0.000 min
Response: 48095227
Conc: 25.65 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

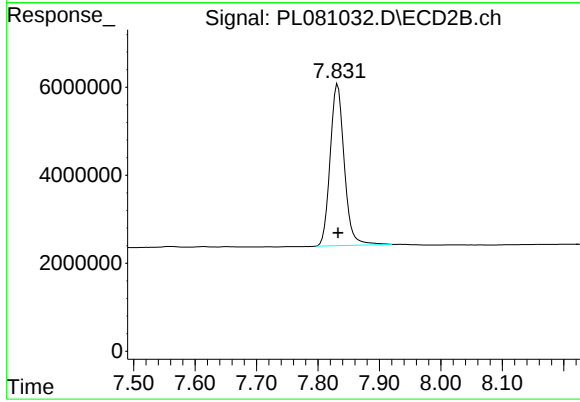

#28 Decachlorobiphenyl

R.T.: 7.832 min
Delta R.T.: 0.000 min
Response: 58706630
Conc: 25.74 ng/ml