

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022023\
 Data File : PL081033.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Feb 2023 15:33
 Operator : AR\AJ
 Sample : PCHLORICC050 (Sig #1); CHLORICC050 (Sig #2)
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC050

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 20 15:45:13 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022023.M
 Quant Title : GC Extractables
 QLast Update : Mon Feb 20 15:36:19 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.351	2.686	10572628	12815997	4.682	4.500
28)	SA Decachlor...	8.790	7.833	9849721	12409359	5.253	5.440
Target Compounds							
23)	Chlordane-1	4.498	3.683	4076081	3897971	43.099	46.974
24)	Chlordane-2	5.025	4.259	5018870	4670279	48.391	50.978
25)	Chlordane-3	5.731	4.889	17644375	11975177	45.411	44.385
26)	Chlordane-4	5.813	4.952	21851233	12350152	46.203	45.235
27)	Chlordane-5	6.653	5.619	3350300	4091217	41.714m	53.927 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022023\
Data File : PL081033.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Feb 2023 15:33
Operator : AR\AJ
Sample : PCHLORICC050 (Sig #1); CHLORICC050 (Sig #2)
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC050

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 20 15:45:13 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022023.M
Quant Title : GC Extractables
QLast Update : Mon Feb 20 15:36:19 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

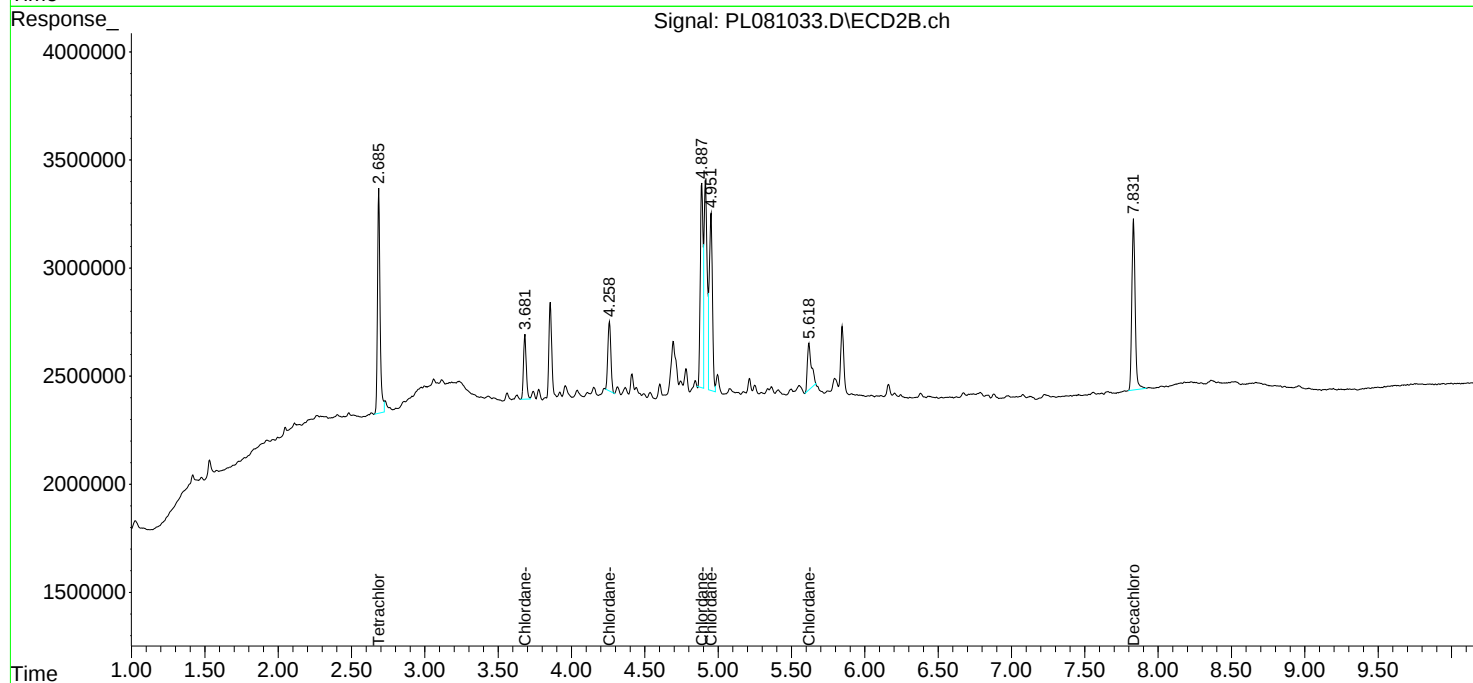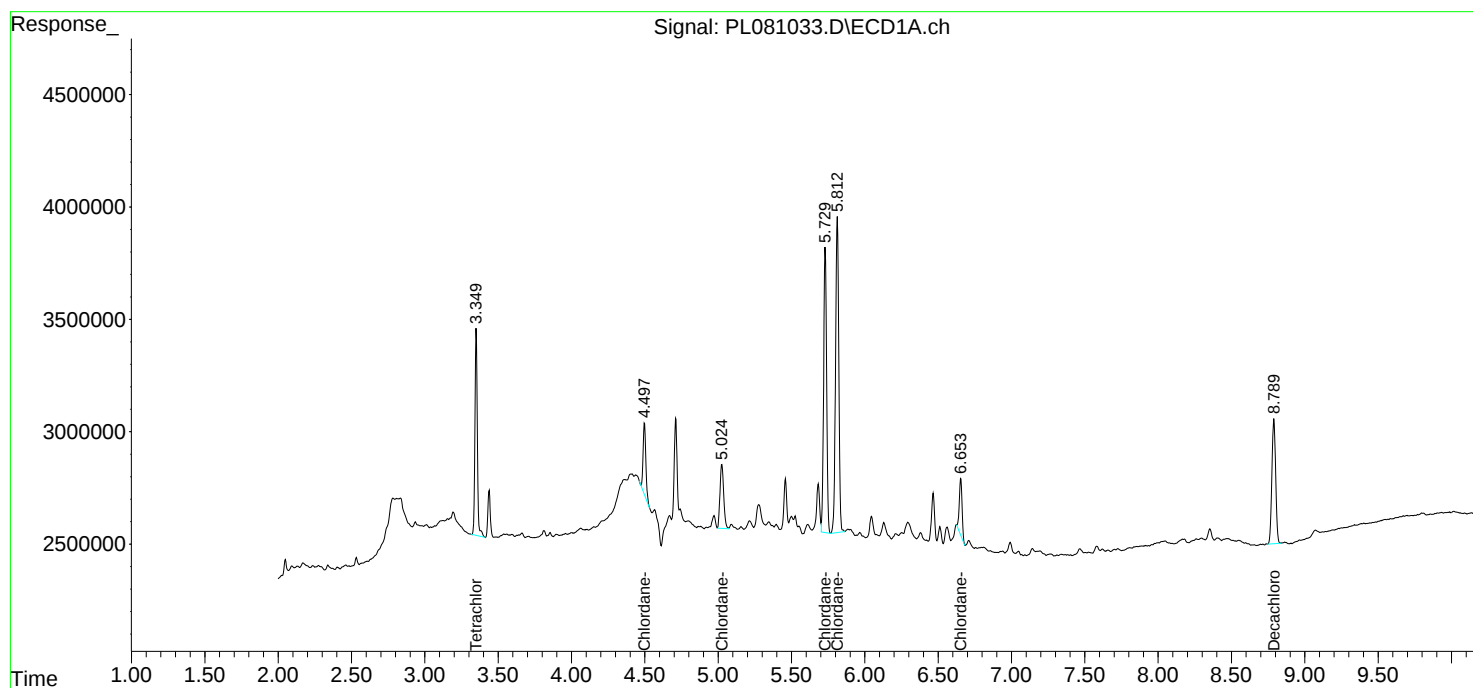


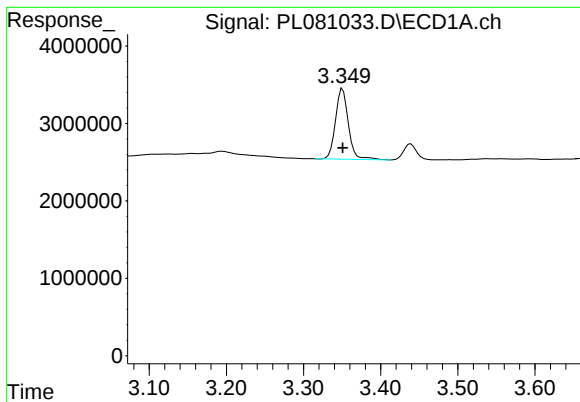

#1 Tetrachloro-m-xylene


R.T.: 3.351 min
Delta R.T.: 0.000 min
Response: 10572628
Conc: 4.68 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC050

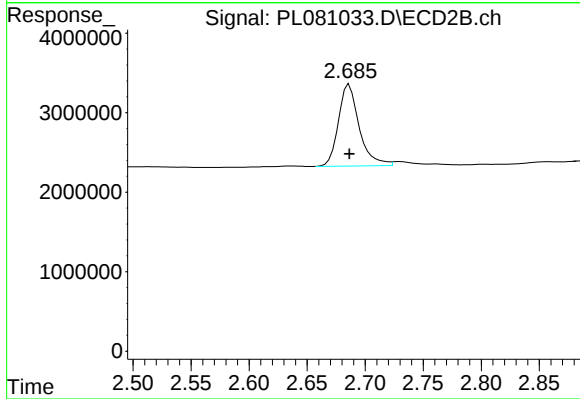


#1 Tetrachloro-m-xylene

R.T.: 2.686 min
Delta R.T.: 0.000 min
Response: 12815997
Conc: 4.50 ng/ml

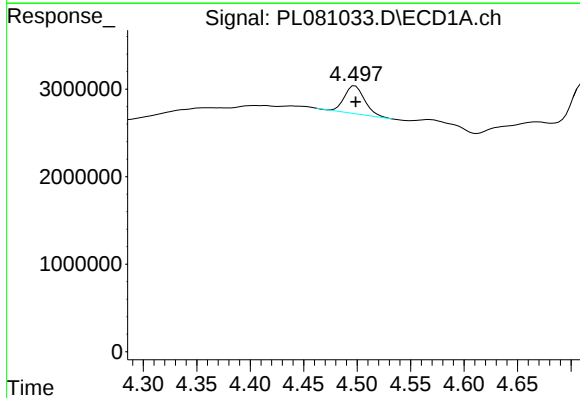


#23 Chlordane-1

R.T.: 4.498 min
Delta R.T.: 0.000 min
Response: 4076081
Conc: 43.10 ng/ml

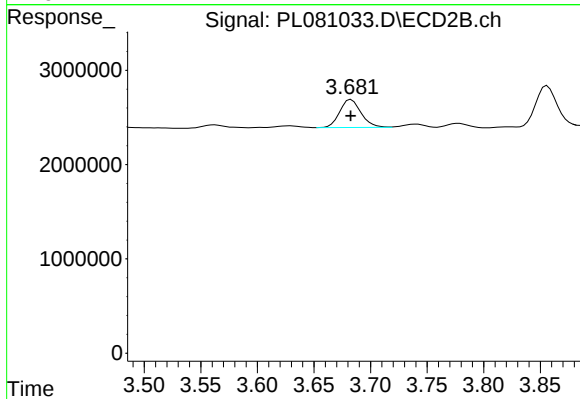

#23 Chlordane-1


R.T.: 3.683 min
Delta R.T.: 0.000 min
Response: 3897971
Conc: 46.97 ng/ml

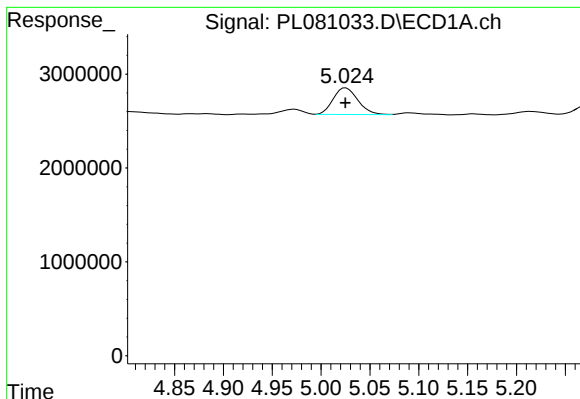

#24 Chlordane-2


R.T.: 5.025 min
Delta R.T.: 0.000 min
Response: 5018870
Conc: 48.39 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC050

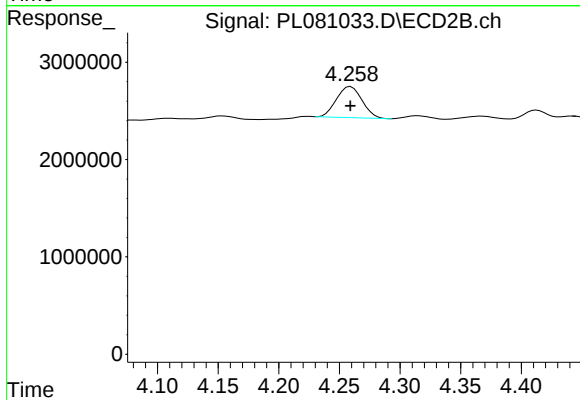


#24 Chlordane-2

R.T.: 4.259 min
Delta R.T.: 0.000 min
Response: 4670279
Conc: 50.98 ng/ml

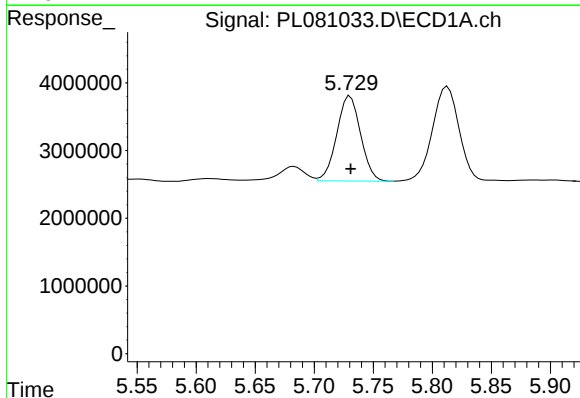


#25 Chlordane-3

R.T.: 5.731 min
Delta R.T.: 0.000 min
Response: 17644375
Conc: 45.41 ng/ml

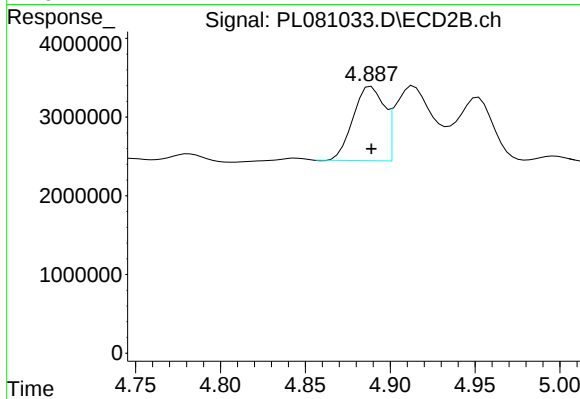

#25 Chlordane-3


R.T.: 4.889 min
Delta R.T.: 0.000 min
Response: 11975177
Conc: 44.38 ng/ml

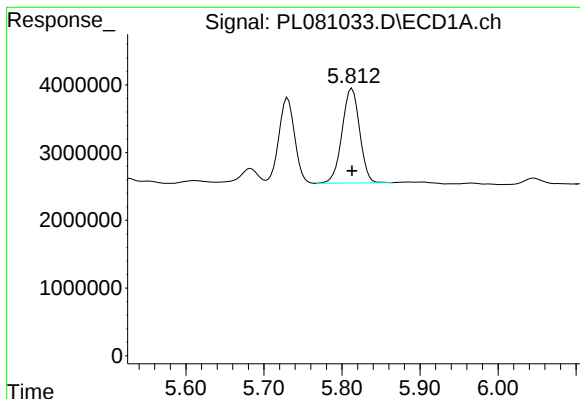

#26 Chlordane-4


R.T.: 5.813 min
Delta R.T.: 0.000 min
Response: 21851233
Conc: 46.20 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC050

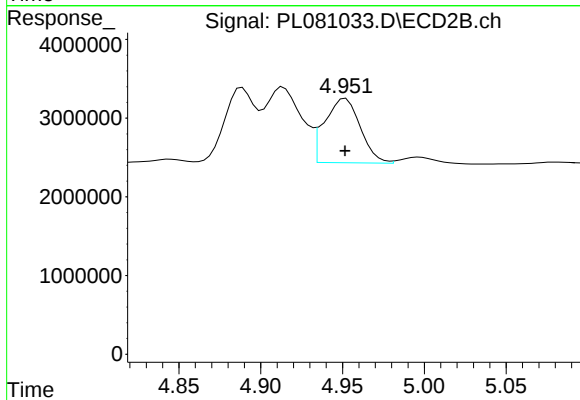


#26 Chlordane-4

R.T.: 4.952 min
Delta R.T.: 0.000 min
Response: 12350152
Conc: 45.23 ng/ml

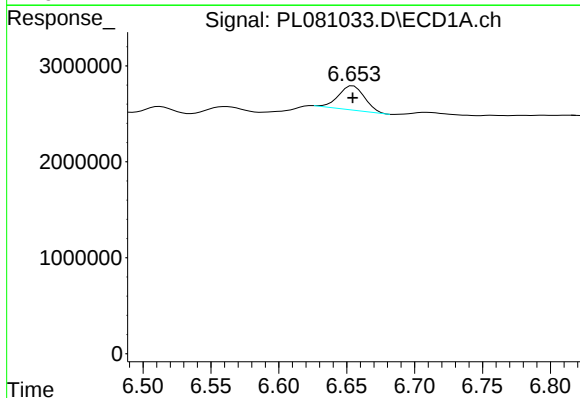


#27 Chlordane-5

R.T.: 6.653 min
Delta R.T.: 0.000 min
Response: 3350300
Conc: 41.71 ng/ml m

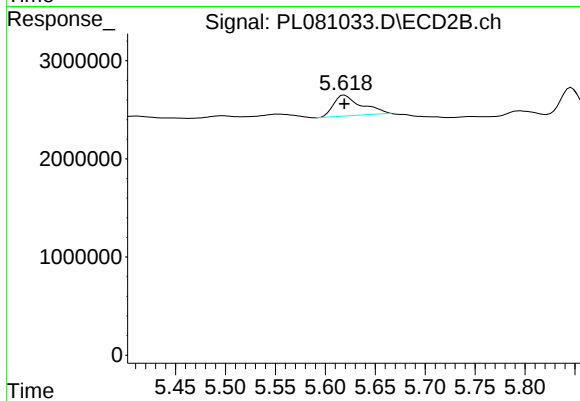

#27 Chlordane-5


R.T.: 5.619 min
Delta R.T.: 0.000 min
Response: 4091217
Conc: 53.93 ng/ml

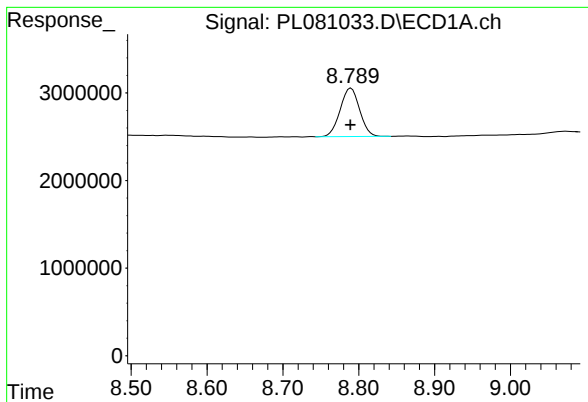

#28 Decachlorobiphenyl

R.T.: 8.790 min
Delta R.T.: 0.000 min
Response: 9849721
Conc: 5.25 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC050

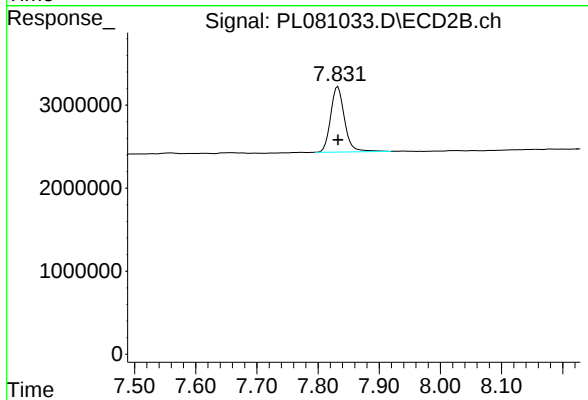

#28 Decachlorobiphenyl

R.T.: 7.833 min
Delta R.T.: 0.000 min
Response: 12409359
Conc: 5.44 ng/ml