

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022023\
 Data File : PL081040.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Feb 2023 17:09
 Operator : AR\AJ
 Sample : PCHLORICV500
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 ICVPL022023CHLOR

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 20 17:27:57 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022023.M
 Quant Title : GC Extractables
 QLast Update : Mon Feb 20 17:26:43 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.351	2.686	114.6E6	144.1E6	51.648	51.947
28)	SA Decachlor...	8.789	7.832	94684795	115.8E6	50.452	50.127
Target Compounds							
23)	Chlordane-1	4.499	3.682	47740494	41739831	525.876	511.974
24)	Chlordane-2	5.025	4.259	52584829	46180581	517.076	508.055
25)	Chlordane-3	5.731	4.889	196.0E6	135.9E6	515.805	517.088
26)	Chlordane-4	5.813	4.951	238.2E6	138.7E6	514.009	516.870
27)	Chlordane-5	6.655	5.618	40406777	38443060	522.625	499.245



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022023\
Data File : PL081040.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Feb 2023 17:09
Operator : AR\AJ
Sample : PCHLORICV500
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
ICVPL022023CHLOR

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 20 17:27:57 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022023.M
Quant Title : GC Extractables
QLast Update : Mon Feb 20 17:26:43 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

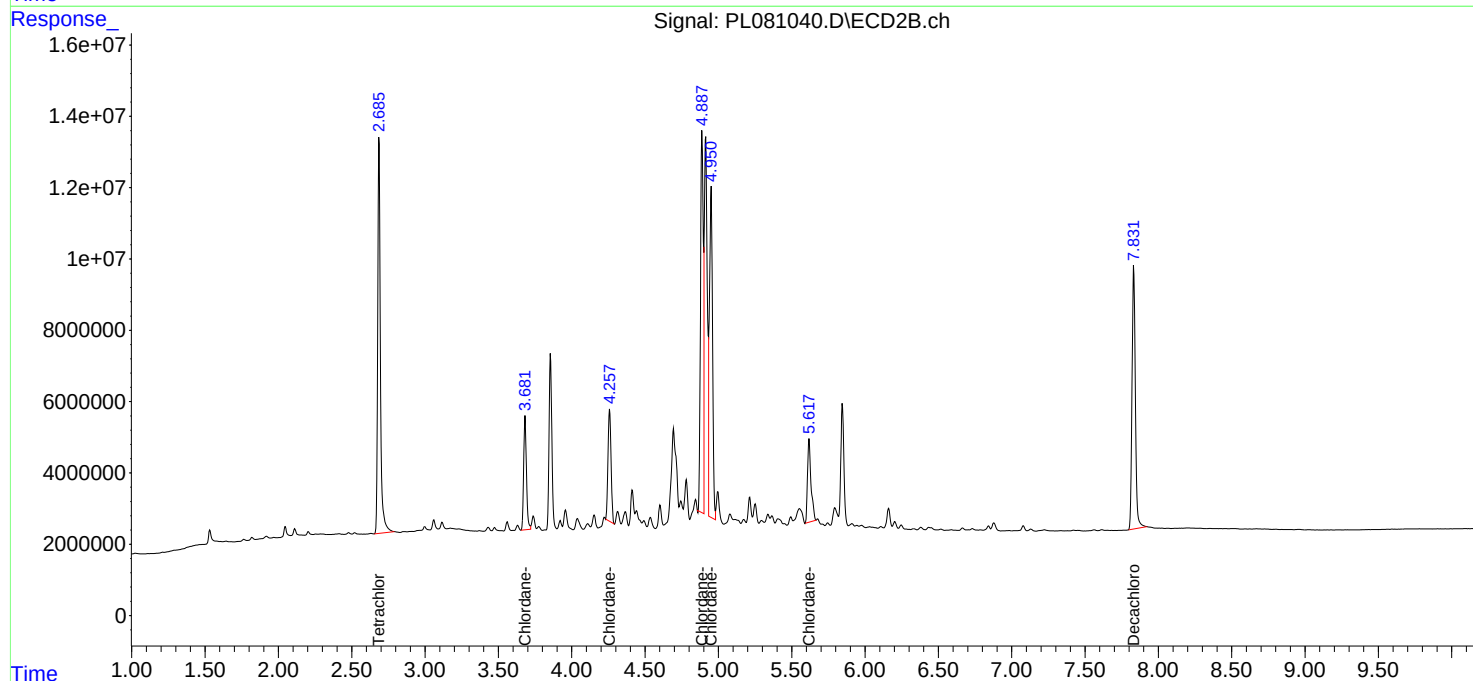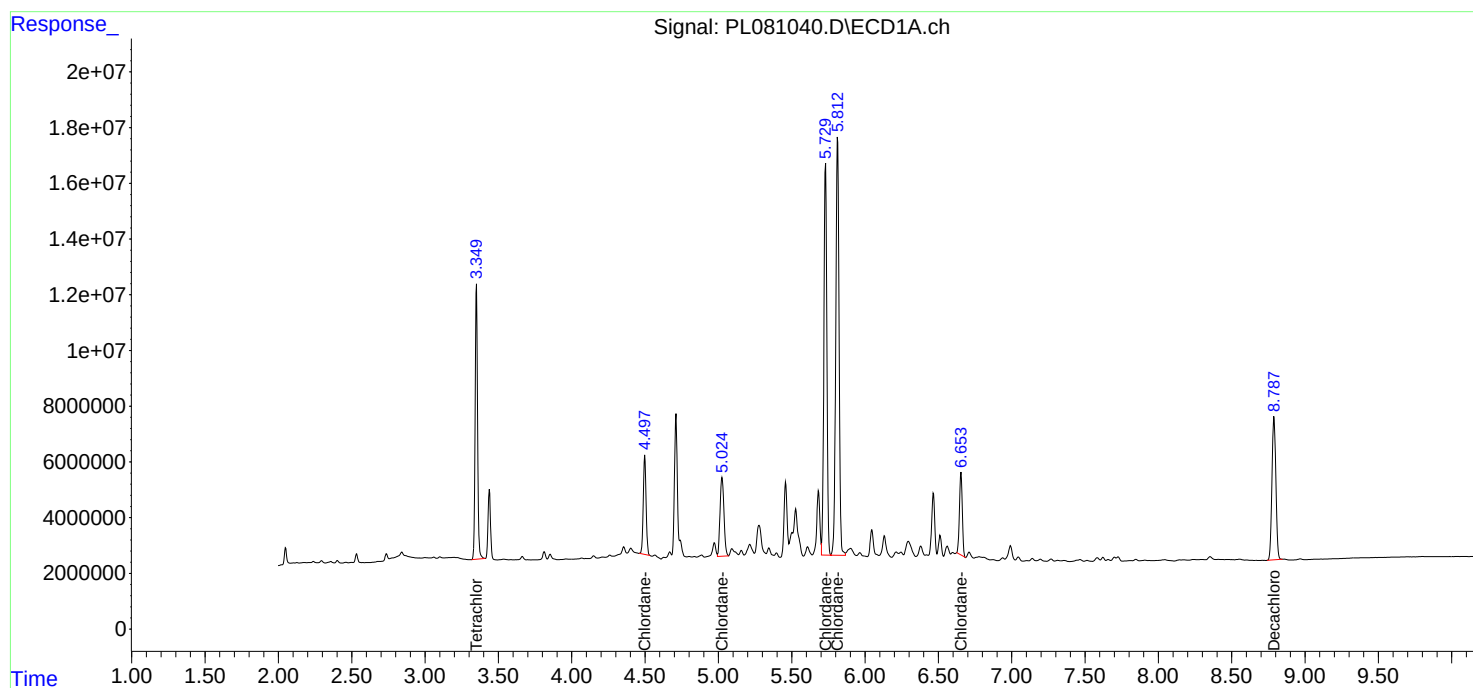


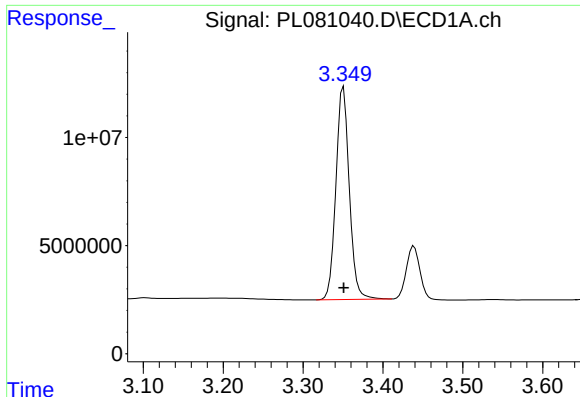

#1 Tetrachloro-m-xylene


R.T.: 3.351 min
Delta R.T.: 0.000 min
Response: 114560254
Conc: 51.65 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL022023CHLOR

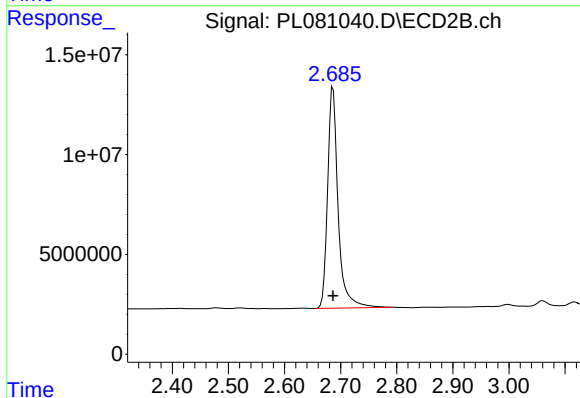


#1 Tetrachloro-m-xylene

R.T.: 2.686 min
Delta R.T.: 0.000 min
Response: 144086752
Conc: 51.95 ng/ml

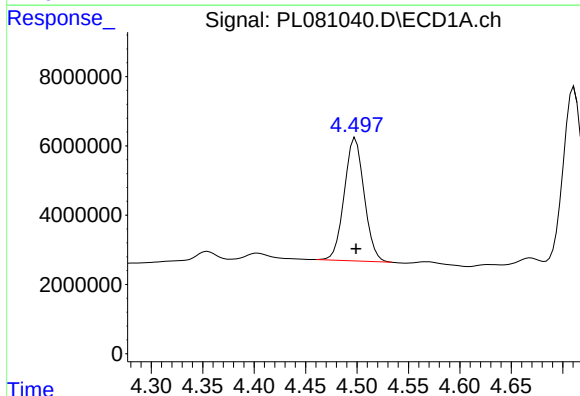


#23 Chlordane-1

R.T.: 4.499 min
Delta R.T.: 0.000 min
Response: 47740494
Conc: 525.88 ng/ml

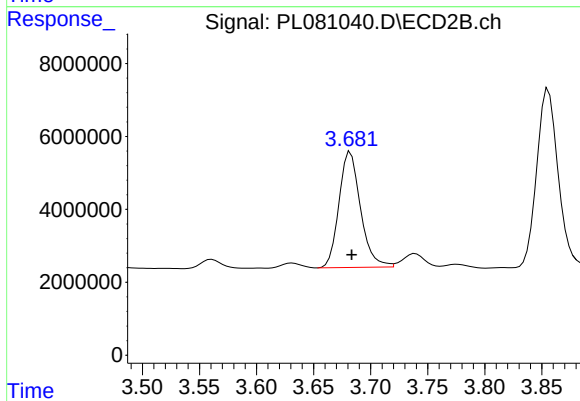

#23 Chlordane-1


R.T.: 3.682 min
Delta R.T.: -0.001 min
Response: 41739831
Conc: 511.97 ng/ml

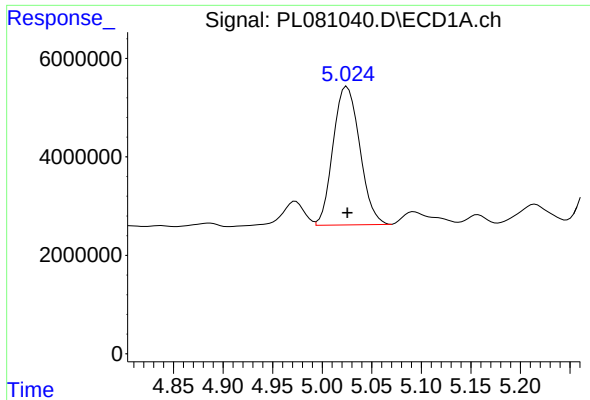

#24 Chlordane-2


R.T.: 5.025 min
Delta R.T.: 0.000 min
Response: 52584829
Conc: 517.08 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL022023CHLOR

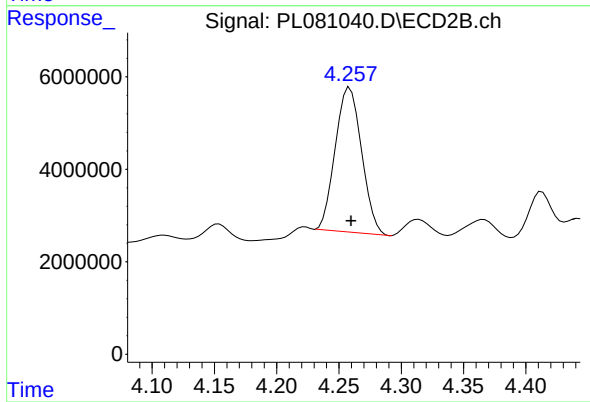


#24 Chlordane-2

R.T.: 4.259 min
Delta R.T.: 0.000 min
Response: 46180581
Conc: 508.06 ng/ml

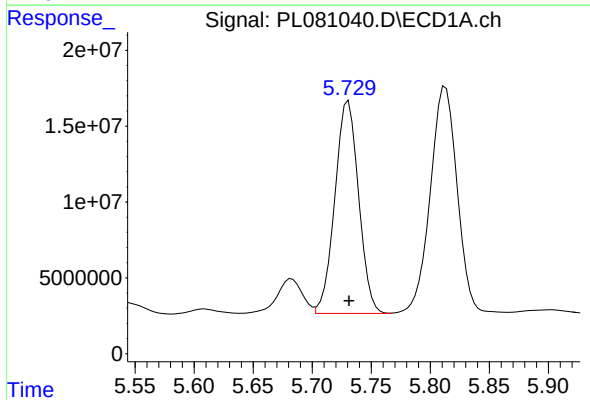


#25 Chlordane-3

R.T.: 5.731 min
Delta R.T.: 0.000 min
Response: 196034379
Conc: 515.80 ng/ml

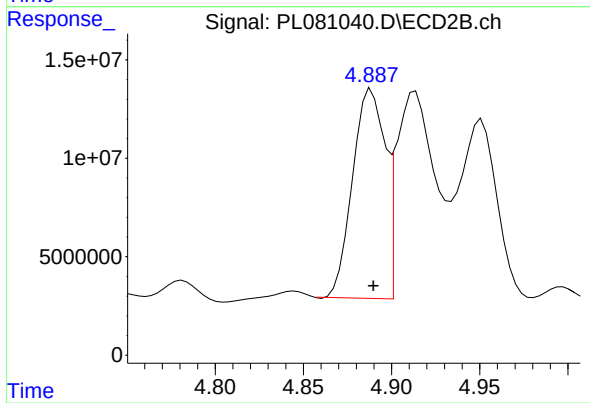

#25 Chlordane-3


R.T.: 4.889 min
Delta R.T.: -0.001 min
Response: 135876847
Conc: 517.09 ng/ml

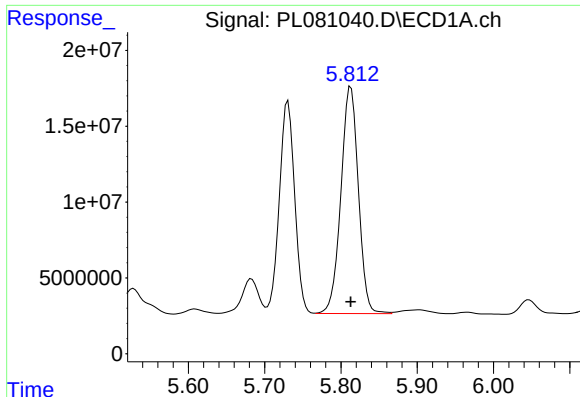

#26 Chlordane-4


R.T.: 5.813 min
Delta R.T.: 0.000 min
Response: 238181943
Conc: 514.01 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL022023CHLOR

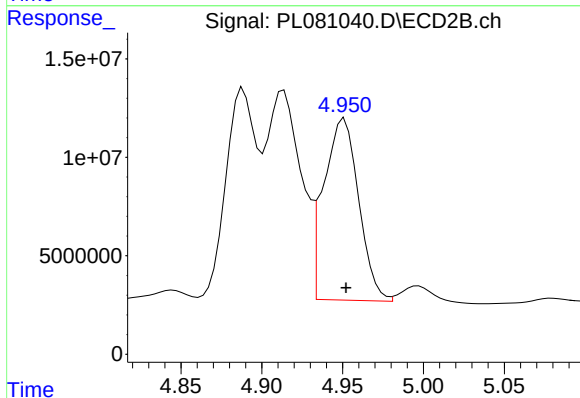


#26 Chlordane-4

R.T.: 4.951 min
Delta R.T.: 0.000 min
Response: 138683670
Conc: 516.87 ng/ml

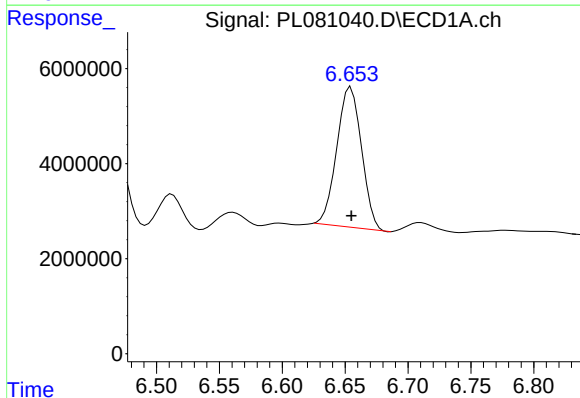


#27 Chlordane-5

R.T.: 6.655 min
Delta R.T.: 0.000 min
Response: 40406777
Conc: 522.62 ng/ml

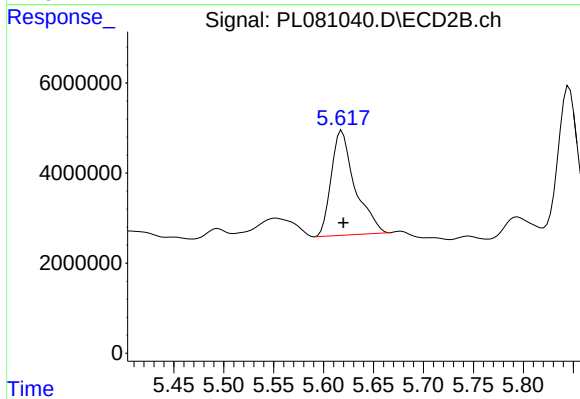

#27 Chlordane-5


R.T.: 5.618 min
Delta R.T.: -0.001 min
Response: 38443060
Conc: 499.25 ng/ml

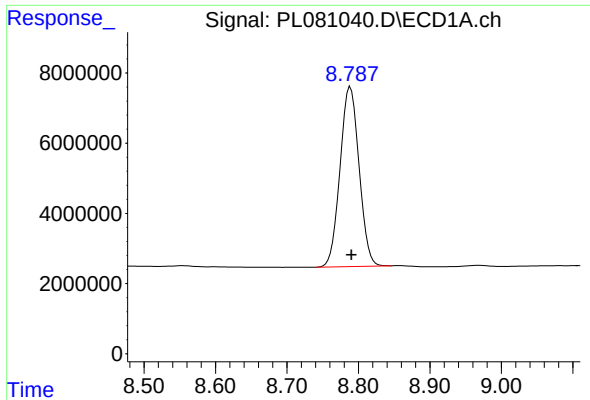

#28 Decachlorobiphenyl

R.T.: 8.789 min
Delta R.T.: -0.002 min
Response: 94684795
Conc: 50.45 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL022023CHLOR

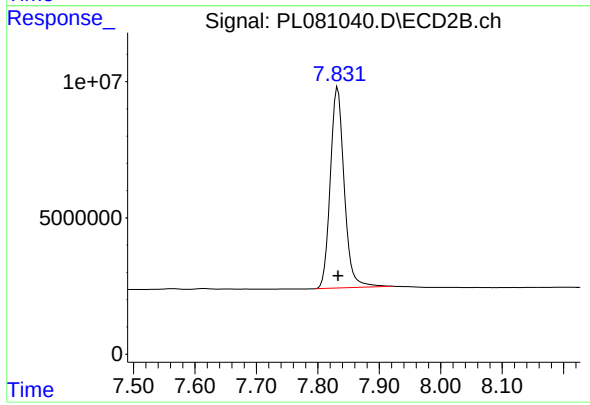

#28 Decachlorobiphenyl

R.T.: 7.832 min
Delta R.T.: 0.000 min
Response: 115803553
Conc: 50.13 ng/ml