

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022024\
Data File : PL088152.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Feb 2024 15:21
Operator : AR\AJ
Sample : P1523-02
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
20240764-COMPOSITE-39N-N-3-02

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 21 00:15:38 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL021524.M
Quant Title : GC Extractables
QLast Update : Fri Feb 16 21:46:54 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.635	2.854	42555324	21259972	15.493	15.158
28)	SA Decachlor...	9.299	8.083	17329030	10045687	8.998	7.890

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022024\
Data File : PL088152.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Feb 2024 15:21
Operator : AR\AJ
Sample : P1523-02
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
20240764-COMPOSITE-39N-N-3-02

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 21 00:15:38 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL021524.M
Quant Title : GC Extractables
QLast Update : Fri Feb 16 21:46:54 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

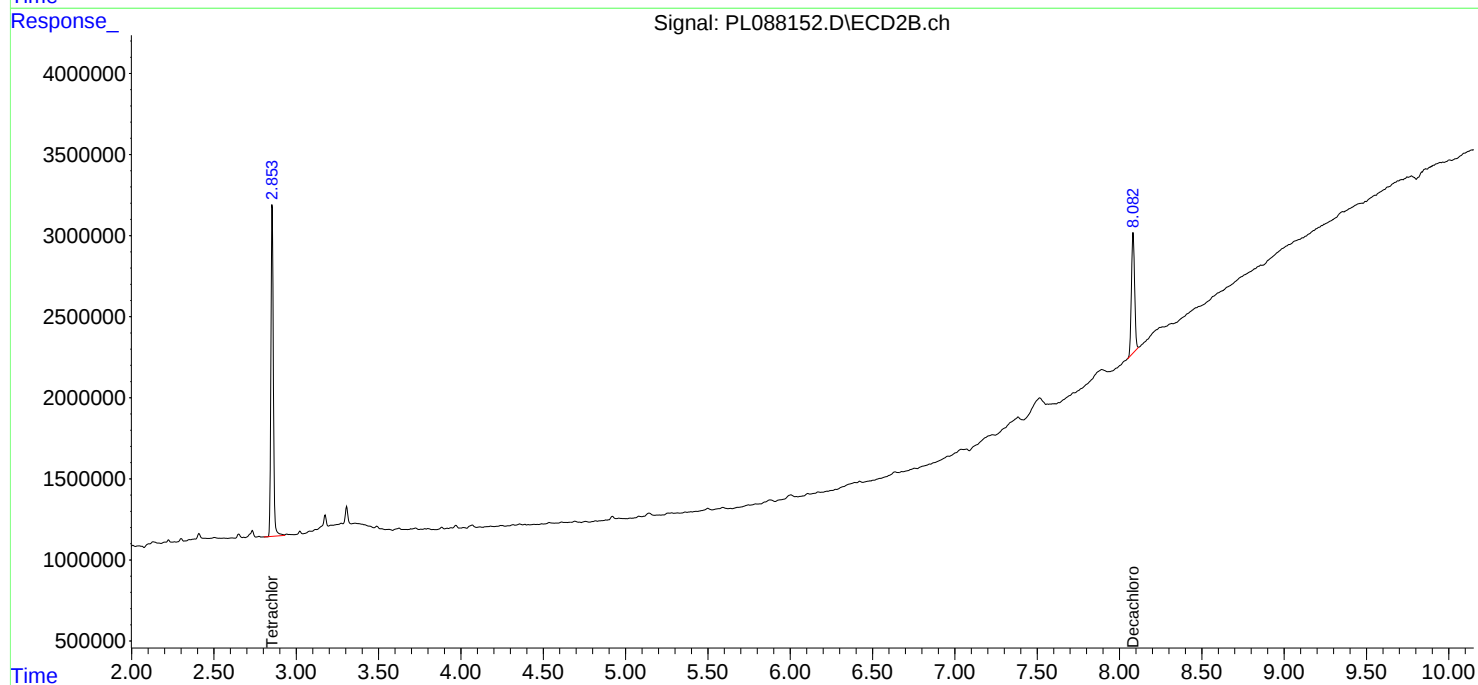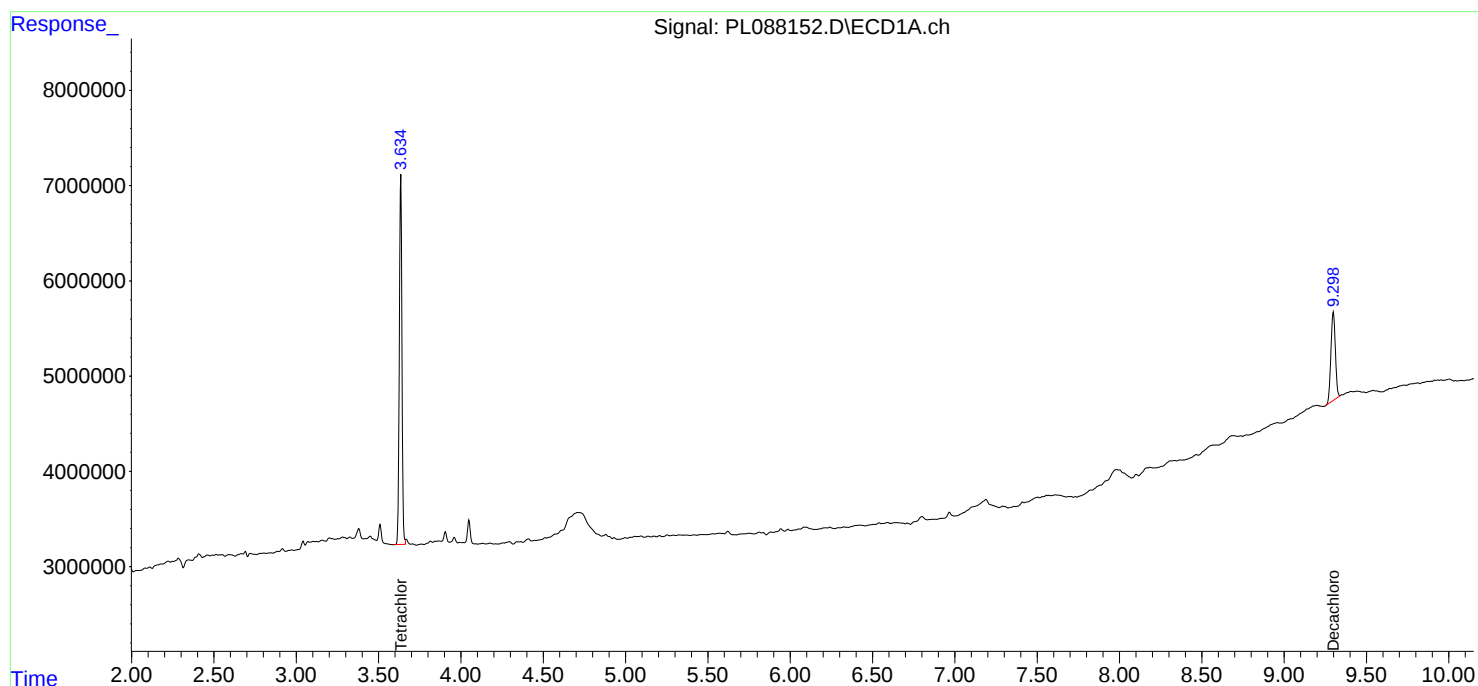


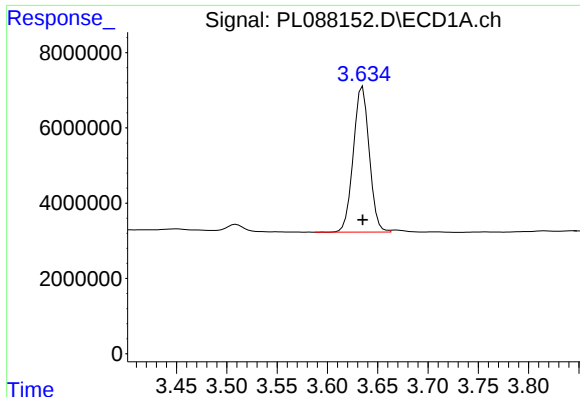

#1 Tetrachloro-m-xylene


R.T.: 3.635 min
Delta R.T.: 0.000 min
Response: 42555324
Conc: 15.49 ng/ml

Instrument :
ECD_L
ClientSampleId :
20240764-COMPOSITE-39N-N-3-02

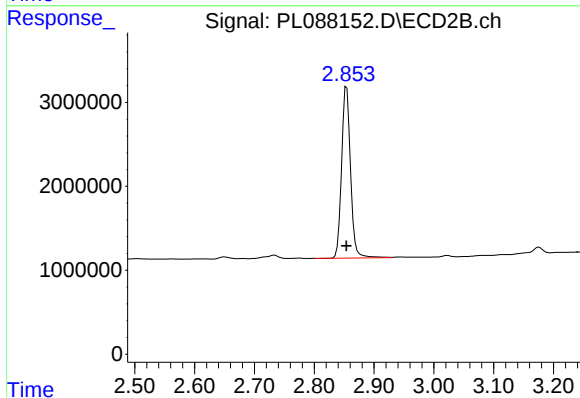


#1 Tetrachloro-m-xylene

R.T.: 2.854 min
Delta R.T.: 0.000 min
Response: 21259972
Conc: 15.16 ng/ml

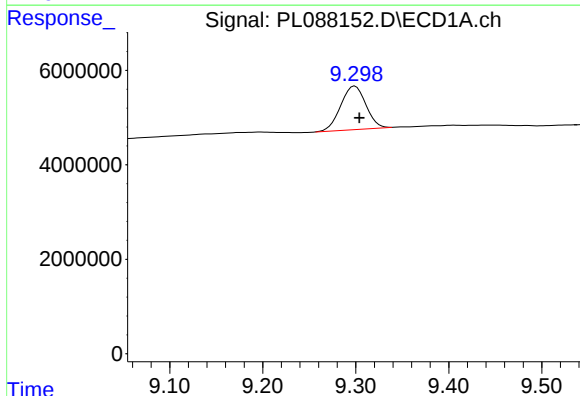

#28 Decachlorobiphenyl

R.T.: 9.299 min
Delta R.T.: -0.005 min
Response: 17329030
Conc: 9.00 ng/ml

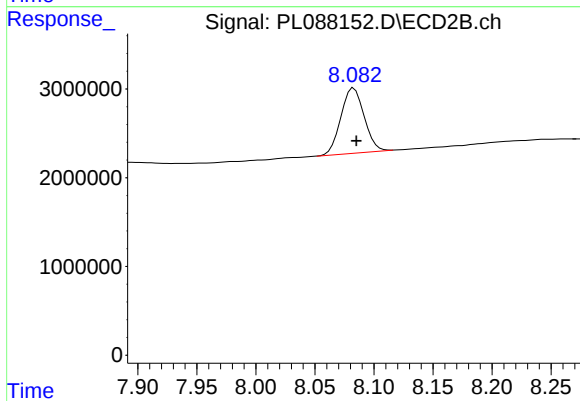

#28 Decachlorobiphenyl

R.T.: 8.083 min
Delta R.T.: -0.002 min
Response: 10045687
Conc: 7.89 ng/ml