

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022024\
 Data File : PL088156.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Feb 2024 16:16
 Operator : AR\AJ
 Sample : P1523-06
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 20240766-AMENDED-COMP-39N-N-3-01

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 02/21/2024
 Supervised By :Ankita Jodhani 02/21/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 21 00:16:46 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL021524.M
 Quant Title : GC Extractables
 QLast Update : Fri Feb 16 21:46:54 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.634	2.853	23057779	11113415	8.395	7.924m
2) SA Decachlor...	9.298	8.083	13856994	7781897	7.195	6.112

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022024\
Data File : PL088156.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Feb 2024 16:16
Operator : AR\AJ
Sample : P1523-06
Misc :
ALS Vial : 13 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
20240766-AMENDED-COMP-39N-N-3-01


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 02/21/2024
Supervised By : Ankita Jodhani 02/21/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 21 00:16:46 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL021524.M
Quant Title : GC Extractables
QLast Update : Fri Feb 16 21:46:54 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

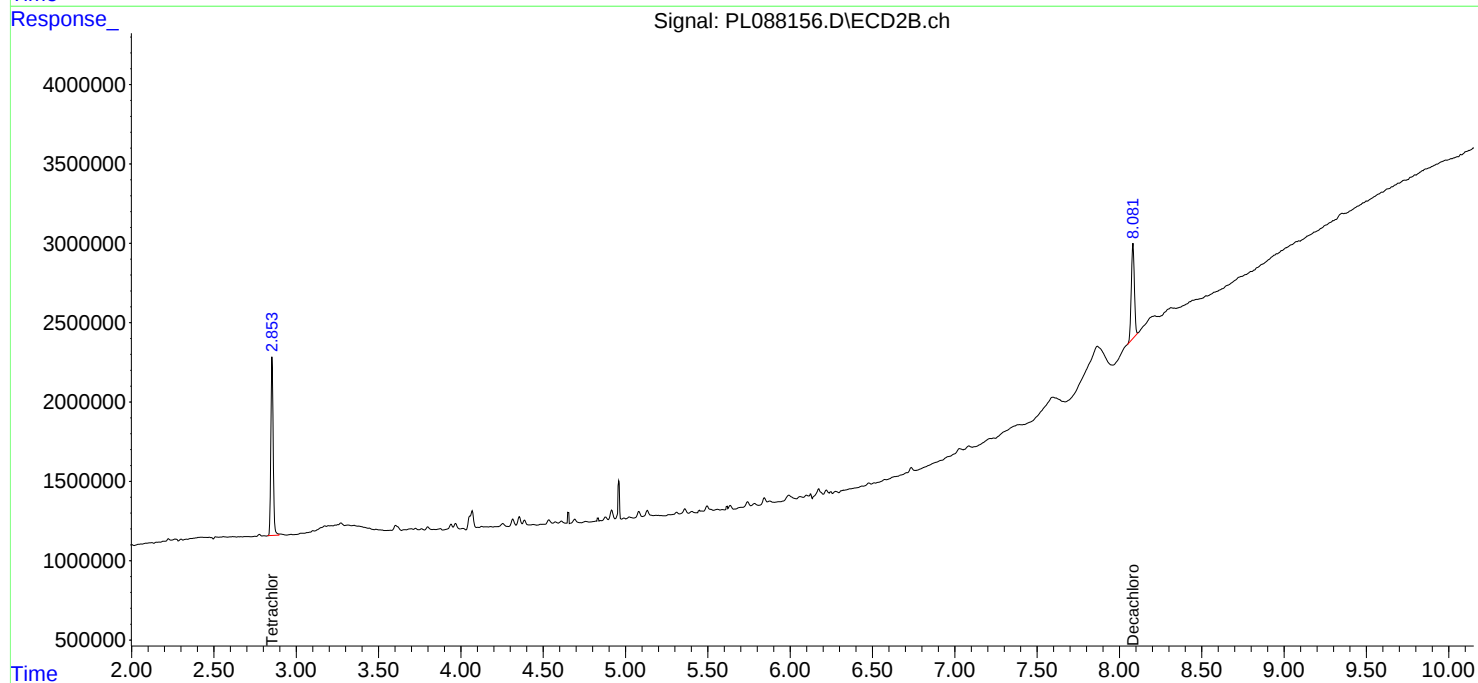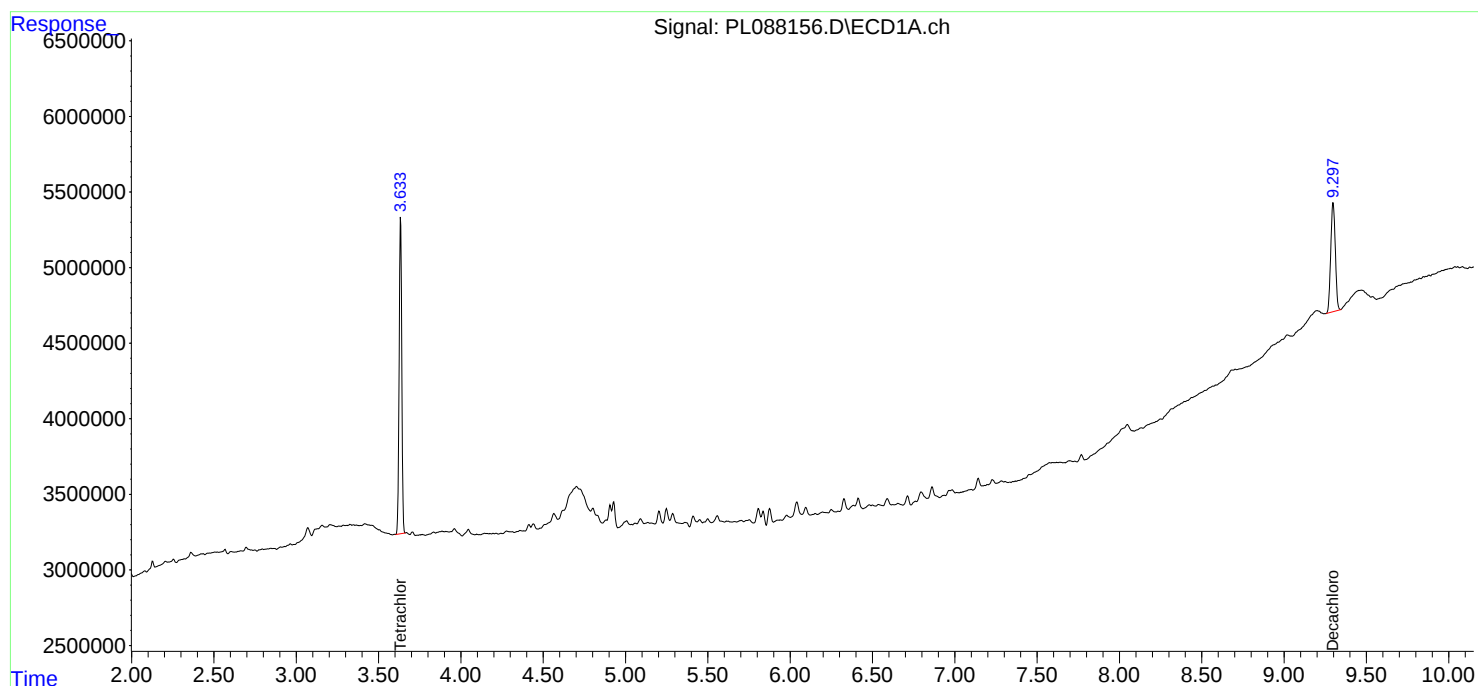

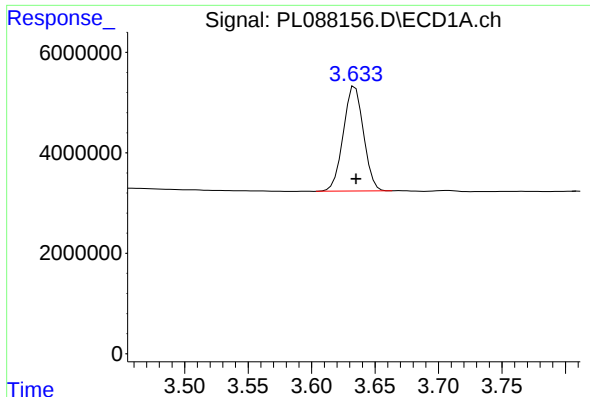


#1 Tetrachloro-m-xylene

R.T.: 3.634 min
Delta R.T.: 0.000 min
Response: 23057779
Conc: 8.39 ng/ml

Instrument :
ECD_L
ClientSampleId :
20240766-AMENDED-COMP-39N-N-3-01


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 02/21/2024
Supervised By :Ankita Jodhani 02/21/2024

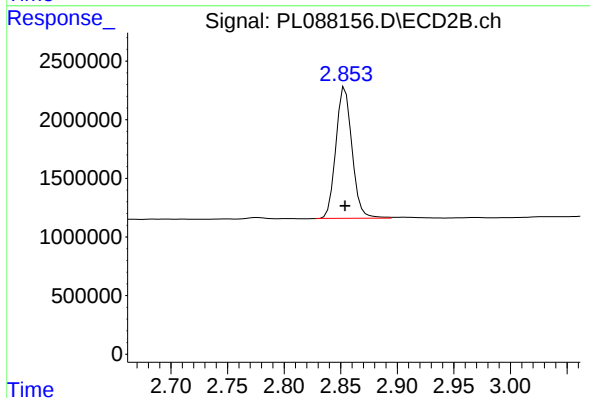


#1 Tetrachloro-m-xylene

R.T.: 2.853 min
Delta R.T.: -0.001 min
Response: 11113415
Conc: 7.92 ng/ml m

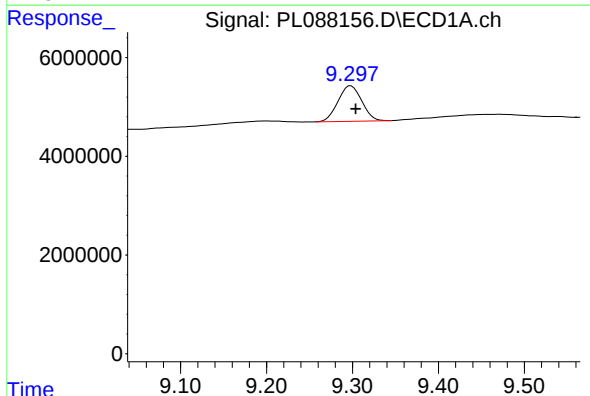

#28 Decachlorobiphenyl

R.T.: 9.298 min
Delta R.T.: -0.006 min
Response: 13856994
Conc: 7.19 ng/ml

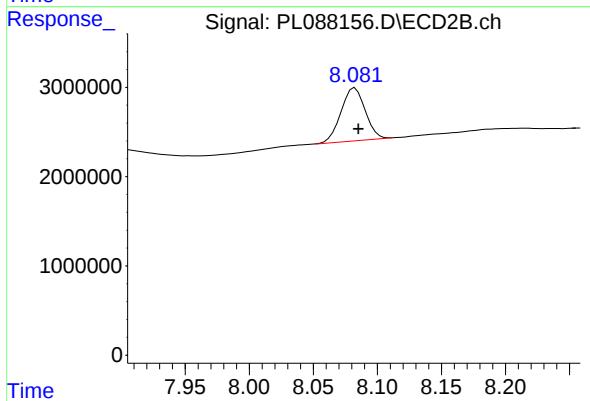

#28 Decachlorobiphenyl

R.T.: 8.083 min
Delta R.T.: -0.003 min
Response: 7781897
Conc: 6.11 ng/ml