

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022119\
 Data File : PL045032.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Feb 2019 21:59
 Operator : AJ\SJ
 Sample : K1547-03
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-1-S

Manual Integrations
 APPROVED

Sohil
 2/22/2019 9:29:16 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 22 00:04:56 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL020619.M
 Quant Title : GC Extractables
 QLast Update : Thu Feb 07 01:39:50 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.365	3.984	60380428	20257441	8.485	8.623
28)	SA Decachlor...	8.050	9.042	86831768	26842836	11.905	12.119
Target Compounds							
12)	B 4,4'-DDE	5.486	6.320	8604338	2898520	0.992	1.214
17)	MA 4,4'-DDT	6.230	7.108	3229626	1123501	0.450m	0.573m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022119\
Data File : PL045032.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Feb 2019 21:59
Operator : AJ\SJ
Sample : K1547-03
Misc :
ALS Vial : 30 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
TP-1-S


Manual Integrations
APPROVED

Sohil
2/22/2019 9:29:16 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 22 00:04:56 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL020619.M
Quant Title : GC Extractables
QLast Update : Thu Feb 07 01:39:50 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

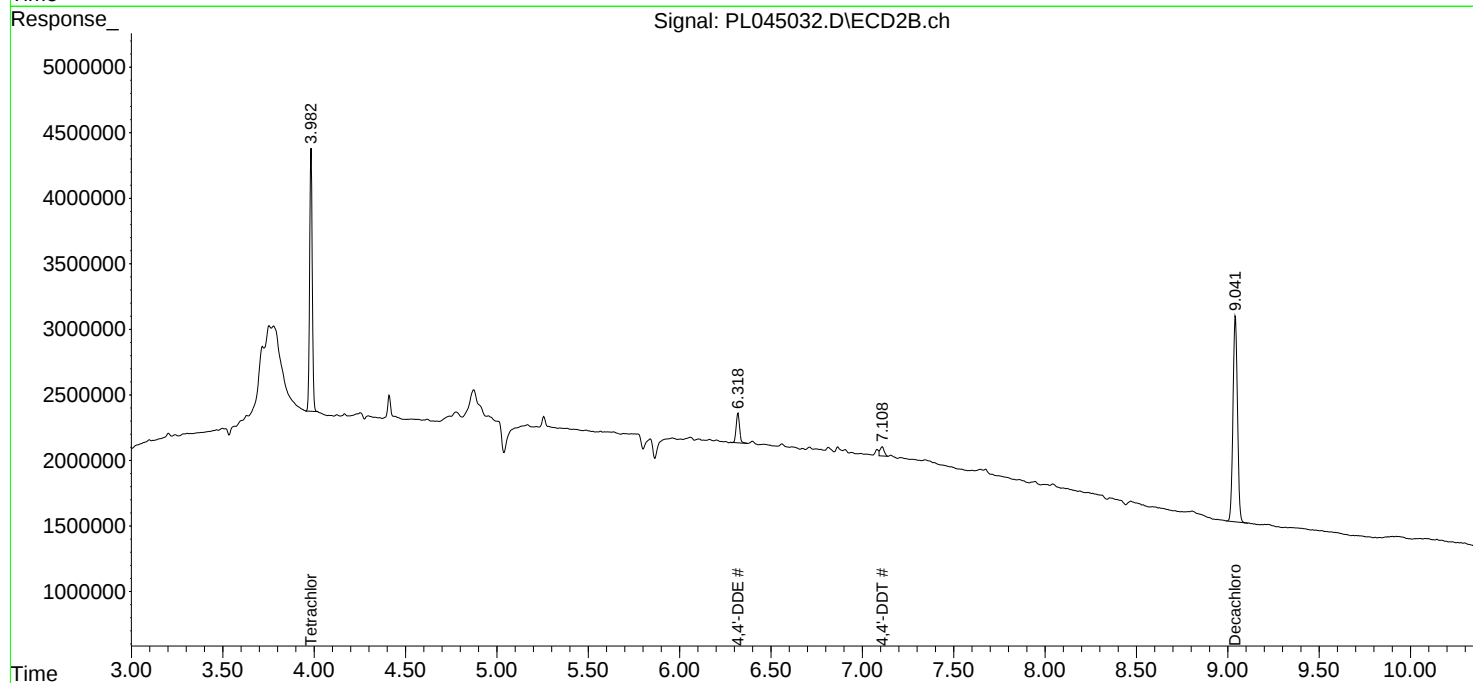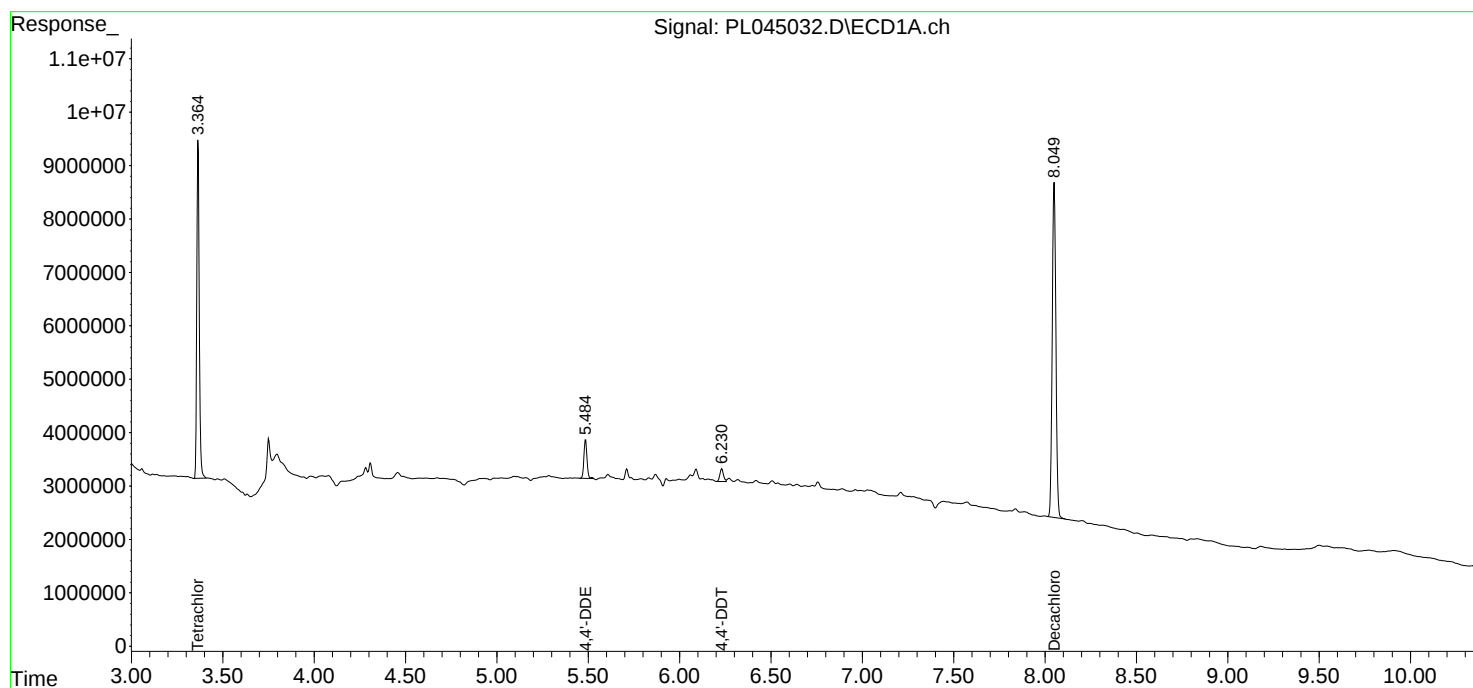

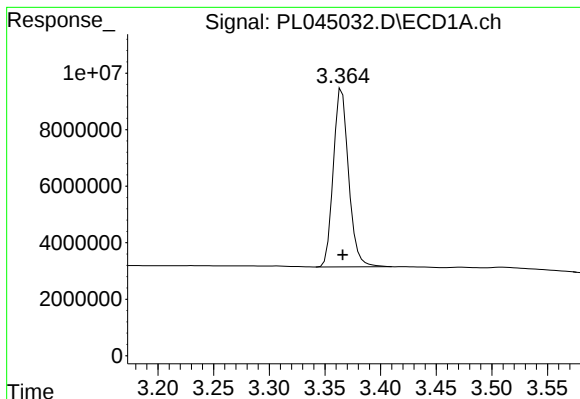


#1 Tetrachloro-m-xylene

R.T.: 3.365 min
Delta R.T.: 0.000 min
Response: 60380428
Conc: 8.49 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-1-S


Manual Integrations
APPROVED

Sohil
2/22/2019 9:29:16 AM

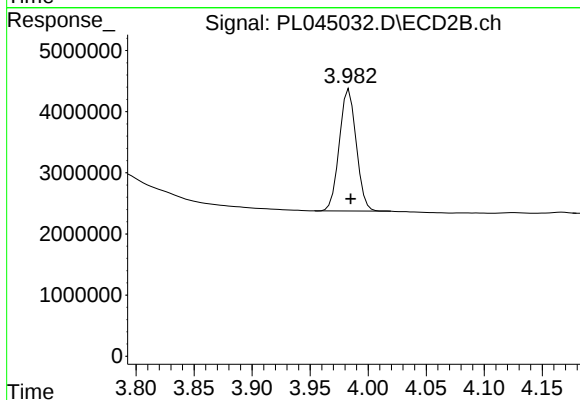


#1 Tetrachloro-m-xylene

R.T.: 3.984 min
Delta R.T.: -0.001 min
Response: 20257441
Conc: 8.62 ng/ml

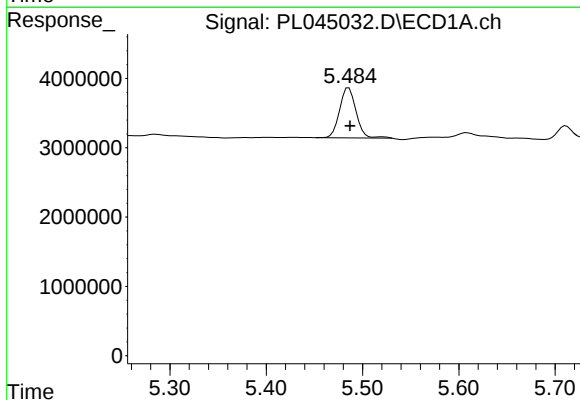


#12 4,4'-DDE

R.T.: 5.486 min
Delta R.T.: -0.001 min
Response: 8604338
Conc: 0.99 ng/ml

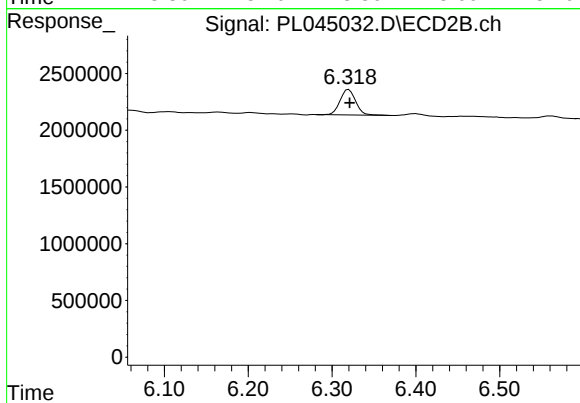

#12 4,4'-DDE

R.T.: 6.320 min
Delta R.T.: -0.001 min
Response: 2898520
Conc: 1.21 ng/ml

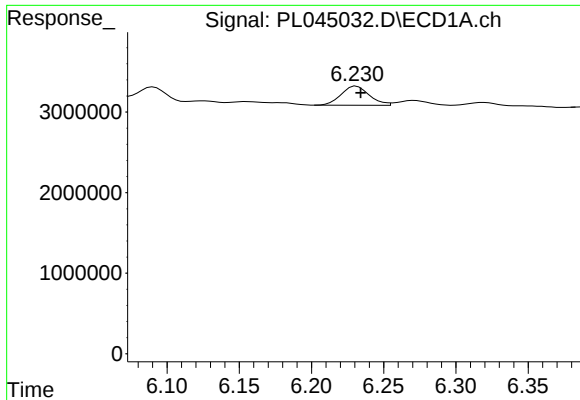


#17 4,4'-DDT

R.T.: 6.230 min
Delta R.T.: -0.004 min
Response: 3229626
Conc: 0.45 ng/ml m

Instrument :
ECD_L
ClientSampleId :
TP-1-S


Manual Integrations
APPROVED

Sohil
2/22/2019 9:29:16 AM

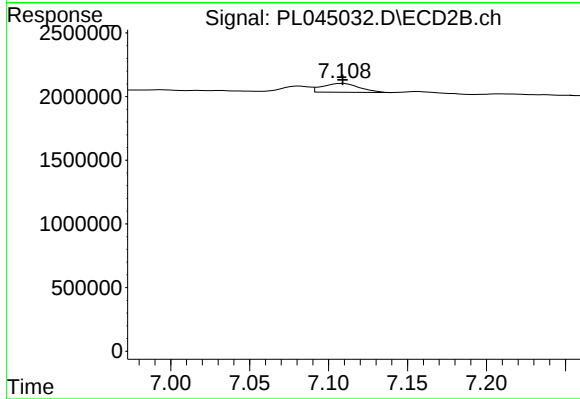


#17 4,4'-DDT

R.T.: 7.108 min
Delta R.T.: 0.000 min
Response: 1123501
Conc: 0.57 ng/ml m

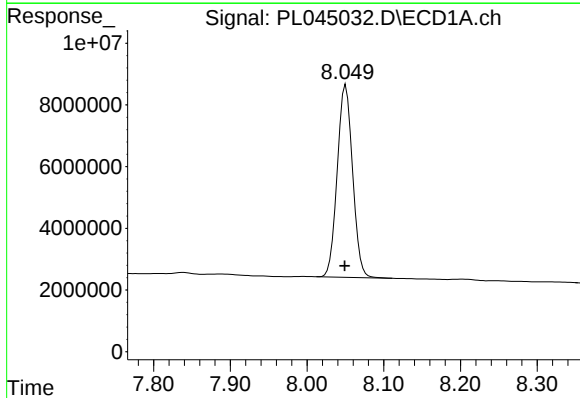

#28 Decachlorobiphenyl

R.T.: 8.050 min
Delta R.T.: 0.001 min
Response: 86831768
Conc: 11.91 ng/ml

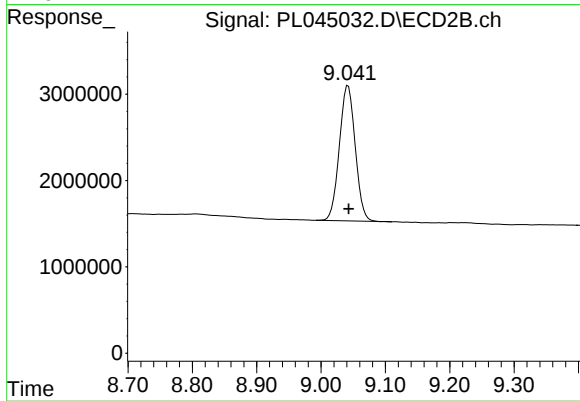

#28 Decachlorobiphenyl

R.T.: 9.042 min
Delta R.T.: 0.000 min
Response: 26842836
Conc: 12.12 ng/ml