

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022121\
 Data File : PL064846.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Feb 2021 14:05
 Operator : AR\AJ
 Sample : INDA201
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 22 03:40:44 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022121CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Feb 22 03:39:50 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.423	4.098	30685680	25375350	10.223	10.257
27)	SA Decachlor...	8.142	9.251	61594559	47844821	21.677	21.180
Target Compounds							
2)	A alpha-BHC	3.856	4.500	44582497	30616557	9.911	9.675
3)	MA gamma-BHC...	4.136	4.792	41845534	29814490	9.982	9.896
4)	MA Heptachlor	4.433	5.303	42267797	32525256	10.243	10.392
9)	A Endosulfan I	5.453	6.369	35031282	24976858	10.289	10.423
13)	MA Dieldrin	5.695	6.629	73975489	49943832	20.162	20.132
14)	MA Endrin	5.949	6.851	65803516	41367375	20.586	20.382
16)	A 4,4'-DDD	6.079	6.970	57003919	37153056	20.170	19.844
17)	MA 4,4'-DDT	6.318	7.269	50359430	36239281	19.219	19.728
20)	A Methoxychlor	6.865	7.731	150.3E6	113.6E6	103.845	102.879


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022121\
Data File : PL064846.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Feb 2021 14:05
Operator : AR\AJ
Sample : INDA201
Misc :
ALS Vial : 11 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 22 03:40:44 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022121CLP.M
Quant Title : GC Extractables
QLast Update : Mon Feb 22 03:39:50 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

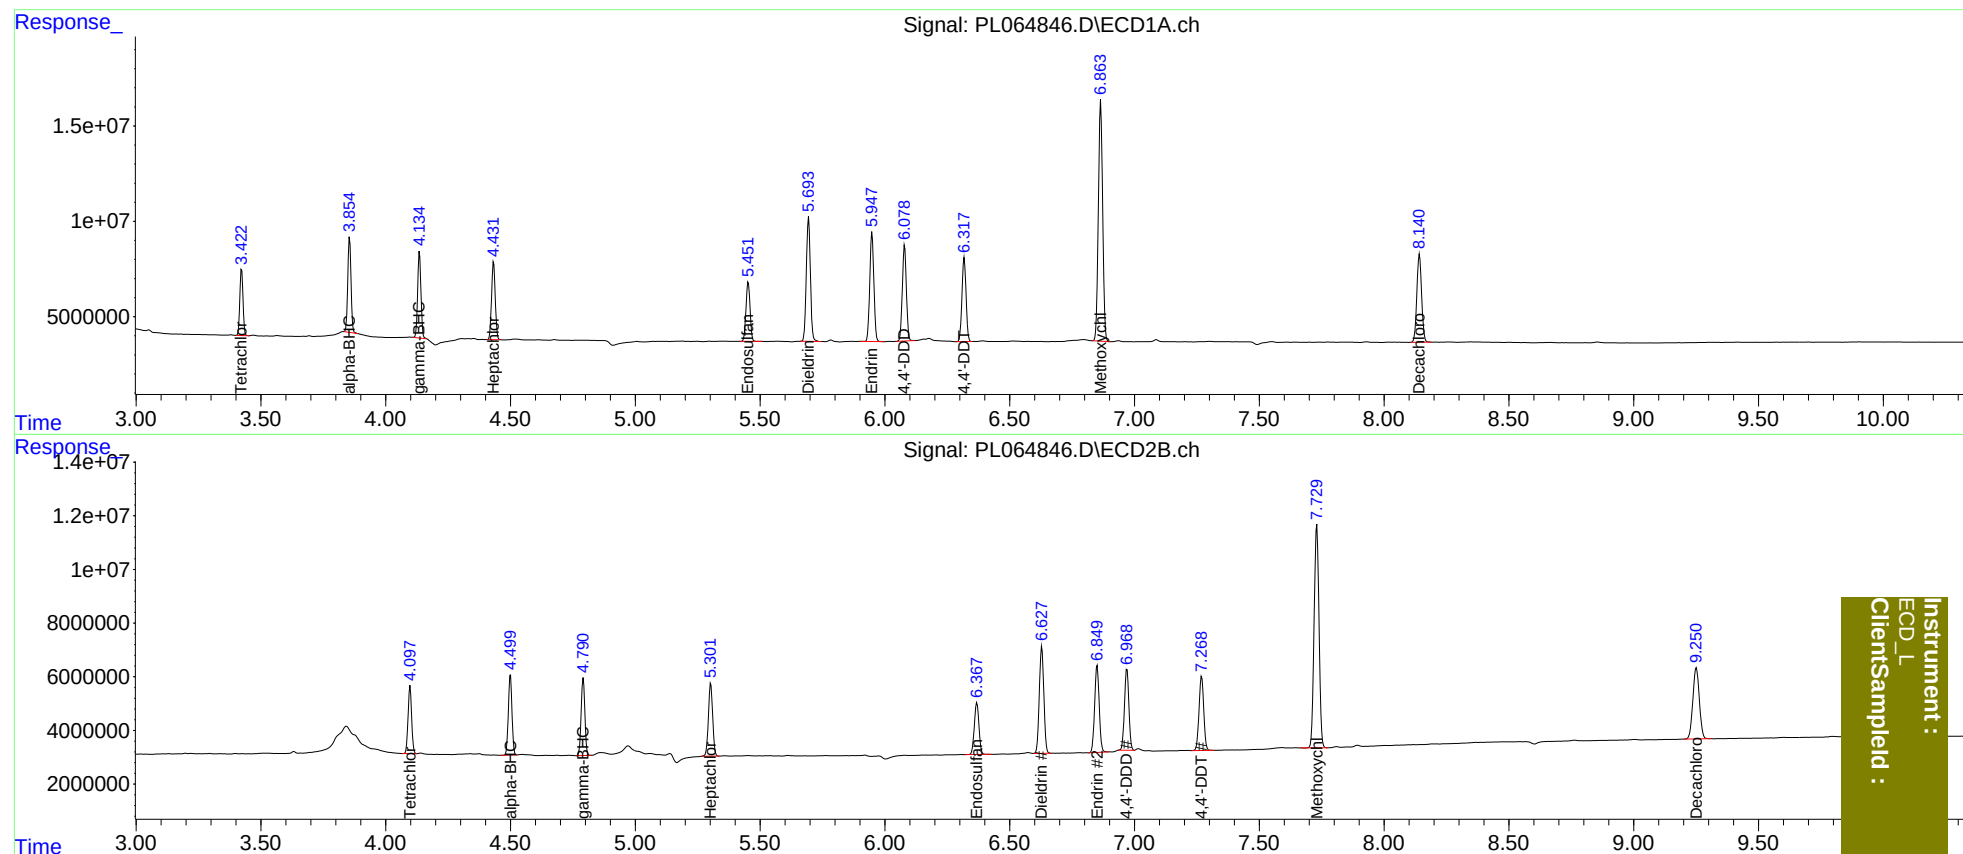


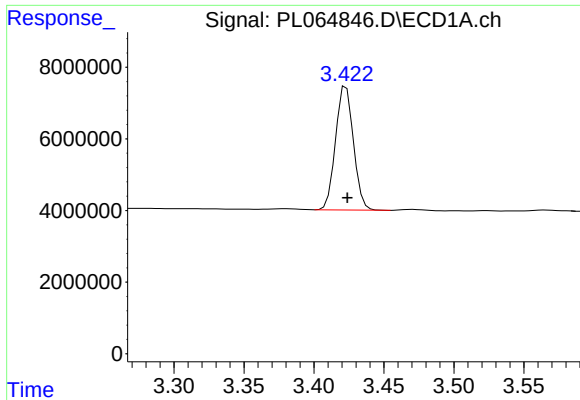

#1 Tetrachloro-m-xylene


R.T.: 3.423 min
Delta R.T.: 0.000 min
Response: 30685680
Conc: 10.22 ng/ml

Instrument :
ECD_L
ClientSampleId :

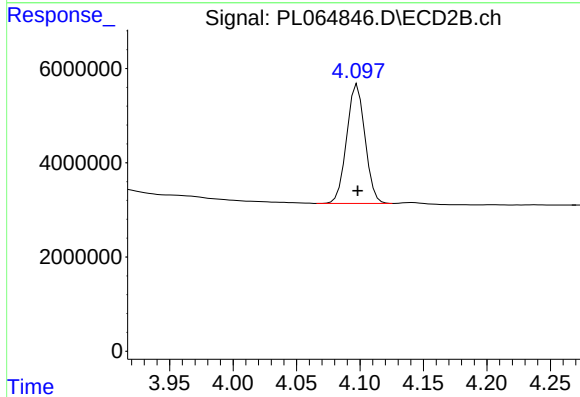


#1 Tetrachloro-m-xylene

R.T.: 4.098 min
Delta R.T.: 0.000 min
Response: 25375350
Conc: 10.26 ng/ml

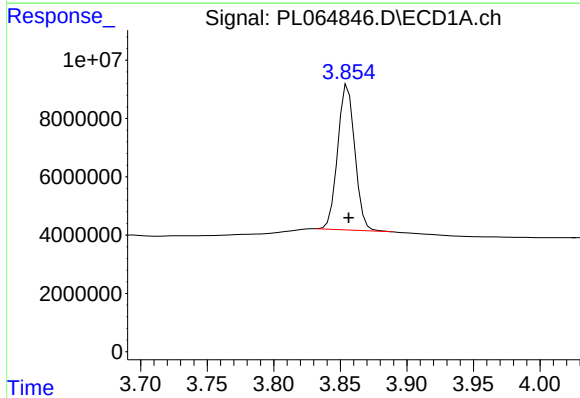


#2 alpha-BHC

R.T.: 3.856 min
Delta R.T.: 0.000 min
Response: 44582497
Conc: 9.91 ng/ml

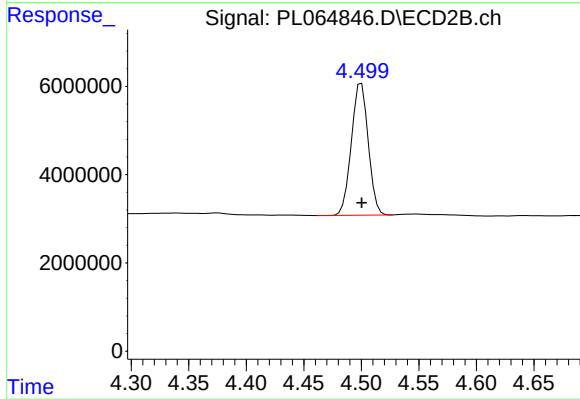

#2 alpha-BHC


R.T.: 4.500 min
Delta R.T.: 0.000 min
Response: 30616557
Conc: 9.68 ng/ml

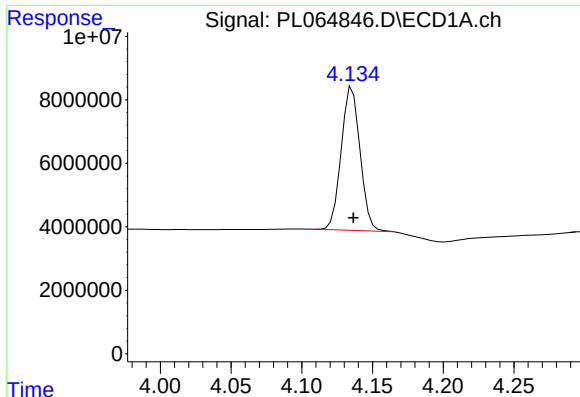

#3 gamma-BHC (Lindane)


R.T.: 4.136 min
Delta R.T.: 0.000 min
Response: 41845534
Conc: 9.98 ng/ml

Instrument :
ECD_L
ClientSampleId :

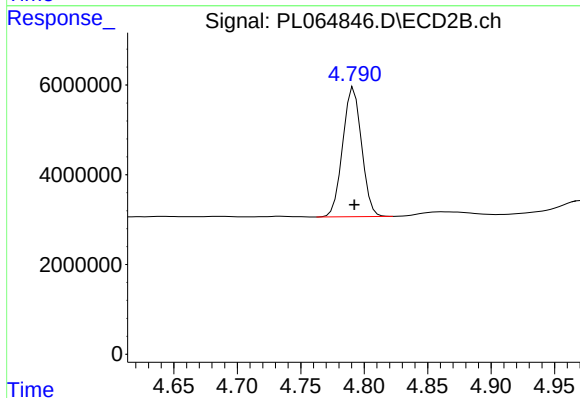


#3 gamma-BHC (Lindane)

R.T.: 4.792 min
Delta R.T.: 0.000 min
Response: 29814490
Conc: 9.90 ng/ml

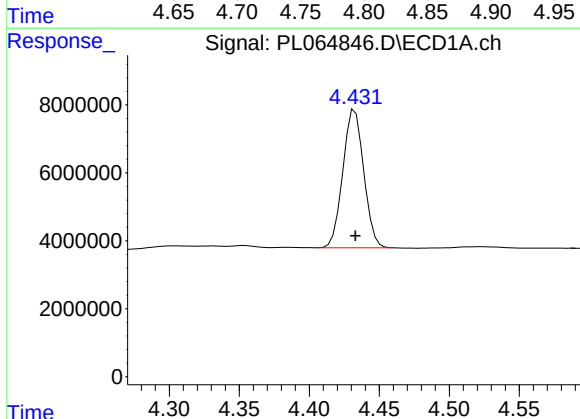


#4 Heptachlor

R.T.: 4.433 min
Delta R.T.: 0.000 min
Response: 42267797
Conc: 10.24 ng/ml

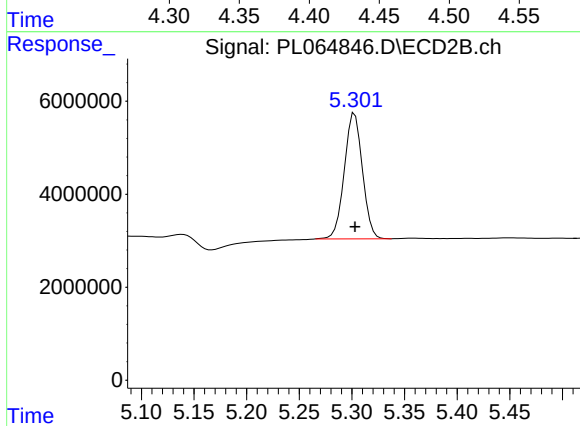

#4 Heptachlor


R.T.: 5.303 min
Delta R.T.: 0.000 min
Response: 32525256
Conc: 10.39 ng/ml

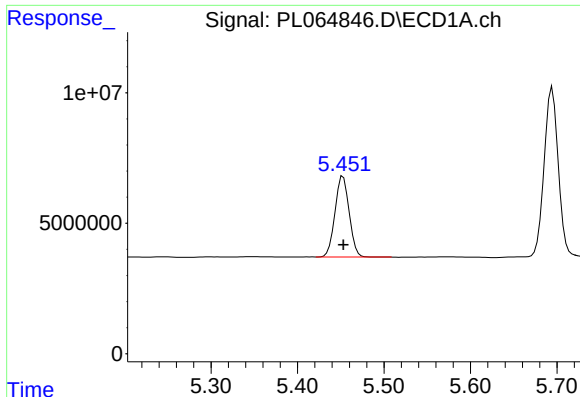

#9 Endosulfan I


R.T.: 5.453 min
Delta R.T.: 0.000 min
Response: 35031282
Conc: 10.29 ng/ml

Instrument :
ECD_L
ClientSampleId :

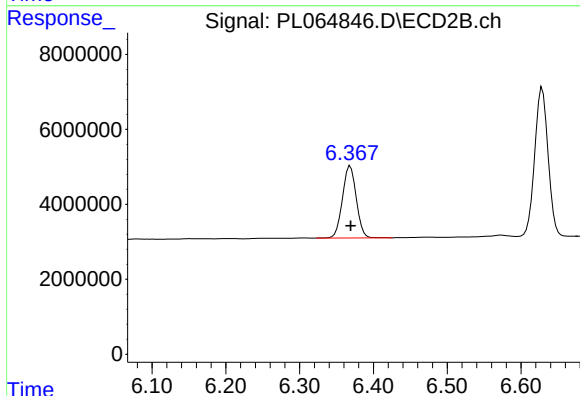


#9 Endosulfan I

R.T.: 6.369 min
Delta R.T.: 0.000 min
Response: 24976858
Conc: 10.42 ng/ml

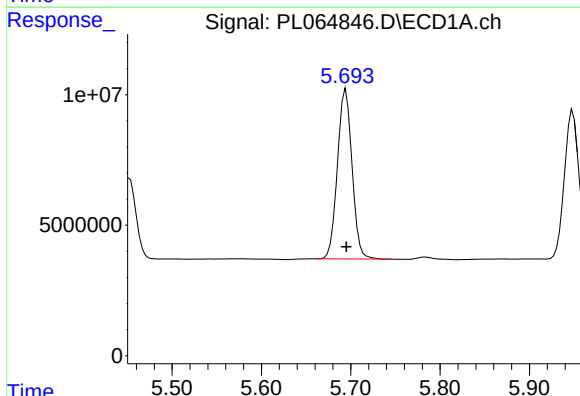


#13 Dieldrin

R.T.: 5.695 min
Delta R.T.: 0.000 min
Response: 73975489
Conc: 20.16 ng/ml

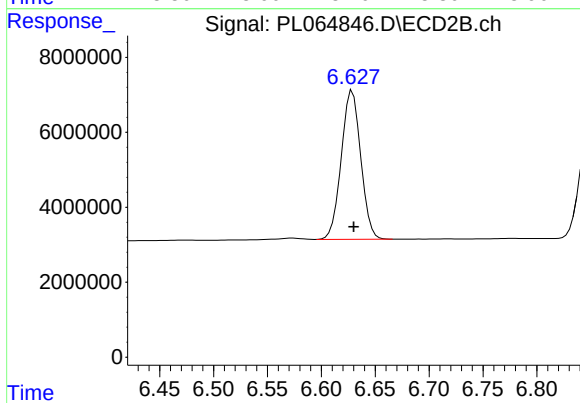

#13 Dieldrin


R.T.: 6.629 min
Delta R.T.: -0.001 min
Response: 49943832
Conc: 20.13 ng/ml

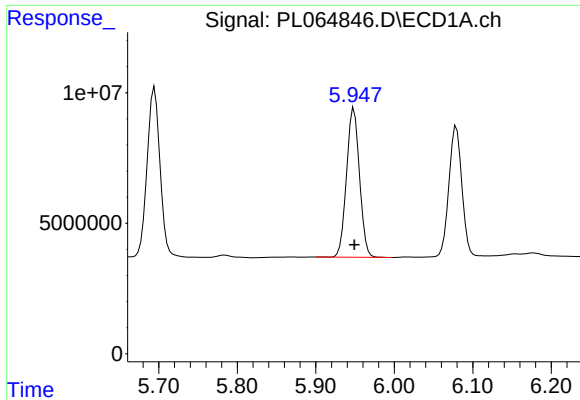

#14 Endrin


R.T.: 5.949 min
Delta R.T.: 0.000 min
Response: 65803516
Conc: 20.59 ng/ml

Instrument :
ECD_L
ClientSampleId :

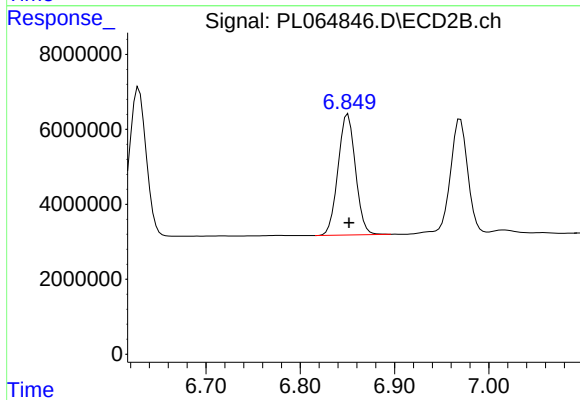


#14 Endrin

R.T.: 6.851 min
Delta R.T.: -0.001 min
Response: 41367375
Conc: 20.38 ng/ml

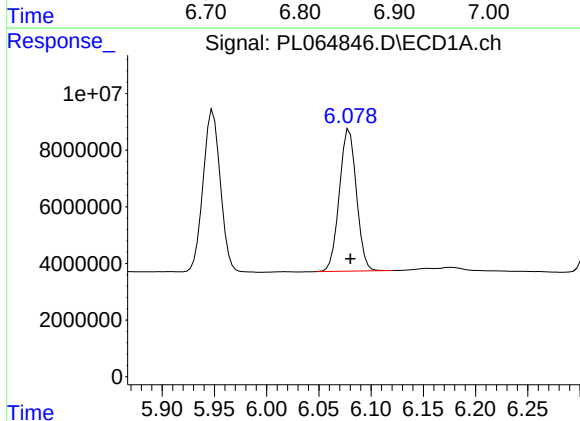


#16 4,4'-DDD

R.T.: 6.079 min
Delta R.T.: -0.001 min
Response: 57003919
Conc: 20.17 ng/ml

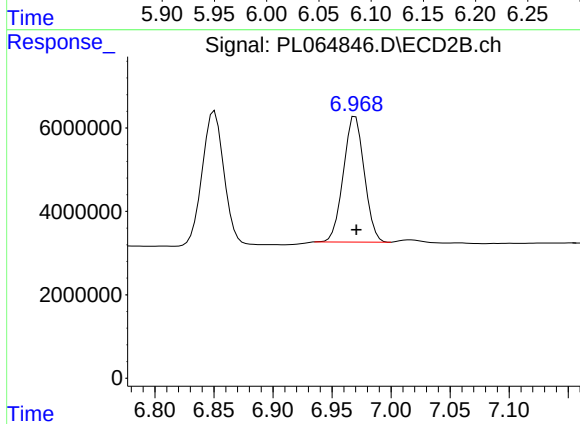

#16 4,4'-DDD


R.T.: 6.970 min
Delta R.T.: 0.000 min
Response: 37153056
Conc: 19.84 ng/ml

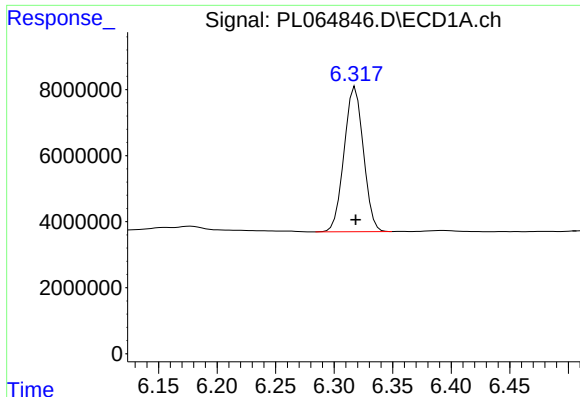

#17 4,4'-DDT


R.T.: 6.318 min
Delta R.T.: 0.000 min
Response: 50359430
Conc: 19.22 ng/ml

Instrument :
ECD_L
ClientSampleId :

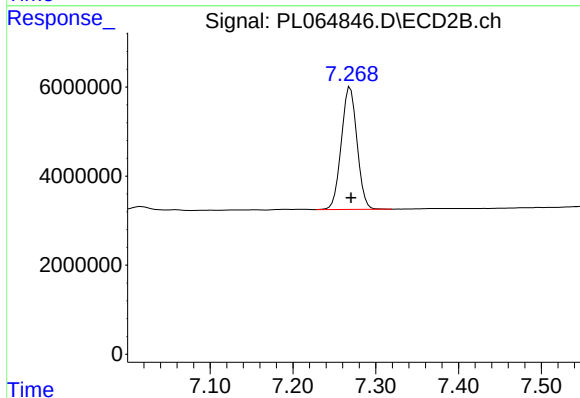


#17 4,4'-DDT

R.T.: 7.269 min
Delta R.T.: -0.001 min
Response: 36239281
Conc: 19.73 ng/ml

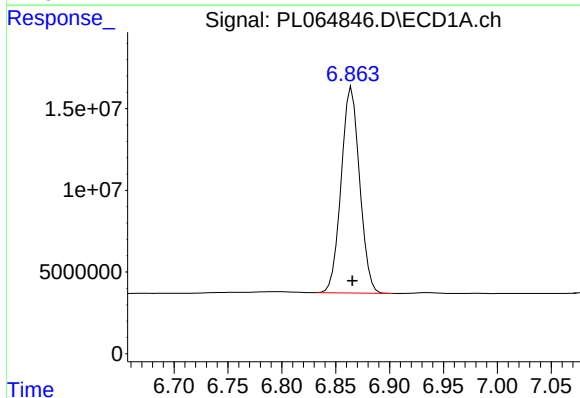


#20 Methoxychlor

R.T.: 6.865 min
Delta R.T.: 0.000 min
Response: 150298315
Conc: 103.84 ng/ml

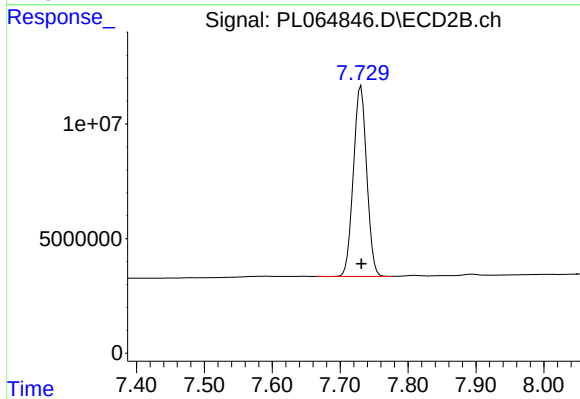

#20 Methoxychlor


R.T.: 7.731 min
Delta R.T.: 0.000 min
Response: 113583596
Conc: 102.88 ng/ml

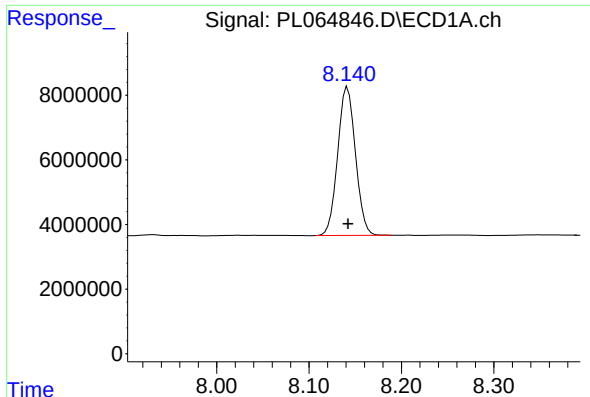

#27 Decachlorobiphenyl

R.T.: 8.142 min
Delta R.T.: 0.000 min
Response: 61594559
Conc: 21.68 ng/ml

Instrument :
ECD_L
ClientSampleId :

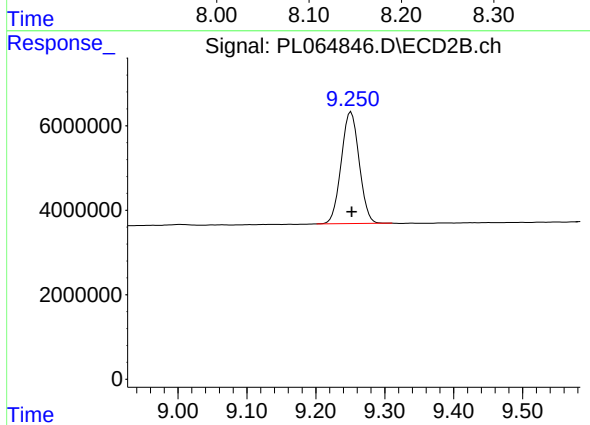

#27 Decachlorobiphenyl

R.T.: 9.251 min
Delta R.T.: -0.001 min
Response: 47844821
Conc: 21.18 ng/ml