

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022121\
 Data File : PL064848.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Feb 2021 14:34
 Operator : AR\AJ
 Sample : INDA301
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 22 03:40:55 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022121CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Feb 22 03:39:50 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.424	4.098	60035188	49480574	20.000	20.000
27)	SA Decachlor...	8.142	9.252	113.7E6	90359503	40.000	40.000
Target Compounds							
2)	A alpha-BHC	3.856	4.500	89966477	63289468	20.000	20.000
3)	MA gamma-BHC...	4.136	4.792	83841475	60255625	20.000	20.000
4)	MA Heptachlor	4.433	5.303	82527667	62593772	20.000	20.000
9)	A Endosulfan I	5.453	6.369	68096646	47926090	20.000	20.000
13)	MA Dieldrin	5.695	6.630	146.8E6	99234092	40.000	40.000
14)	MA Endrin	5.949	6.852	127.9E6	81182571	40.000	40.000
16)	A 4,4'-DDD	6.080	6.971	113.0E6	74889452	40.000	40.000
17)	MA 4,4'-DDT	6.319	7.270	104.8E6	73477564	40.000	40.000
20)	A Methoxychlor	6.865	7.731	289.5E6	220.8E6	200.000	200.000


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022121\
Data File : PL064848.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Feb 2021 14:34
Operator : AR\AJ
Sample : INDA301
Misc :
ALS Vial : 13 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 22 03:40:55 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022121CLP.M
Quant Title : GC Extractables
QLast Update : Mon Feb 22 03:39:50 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

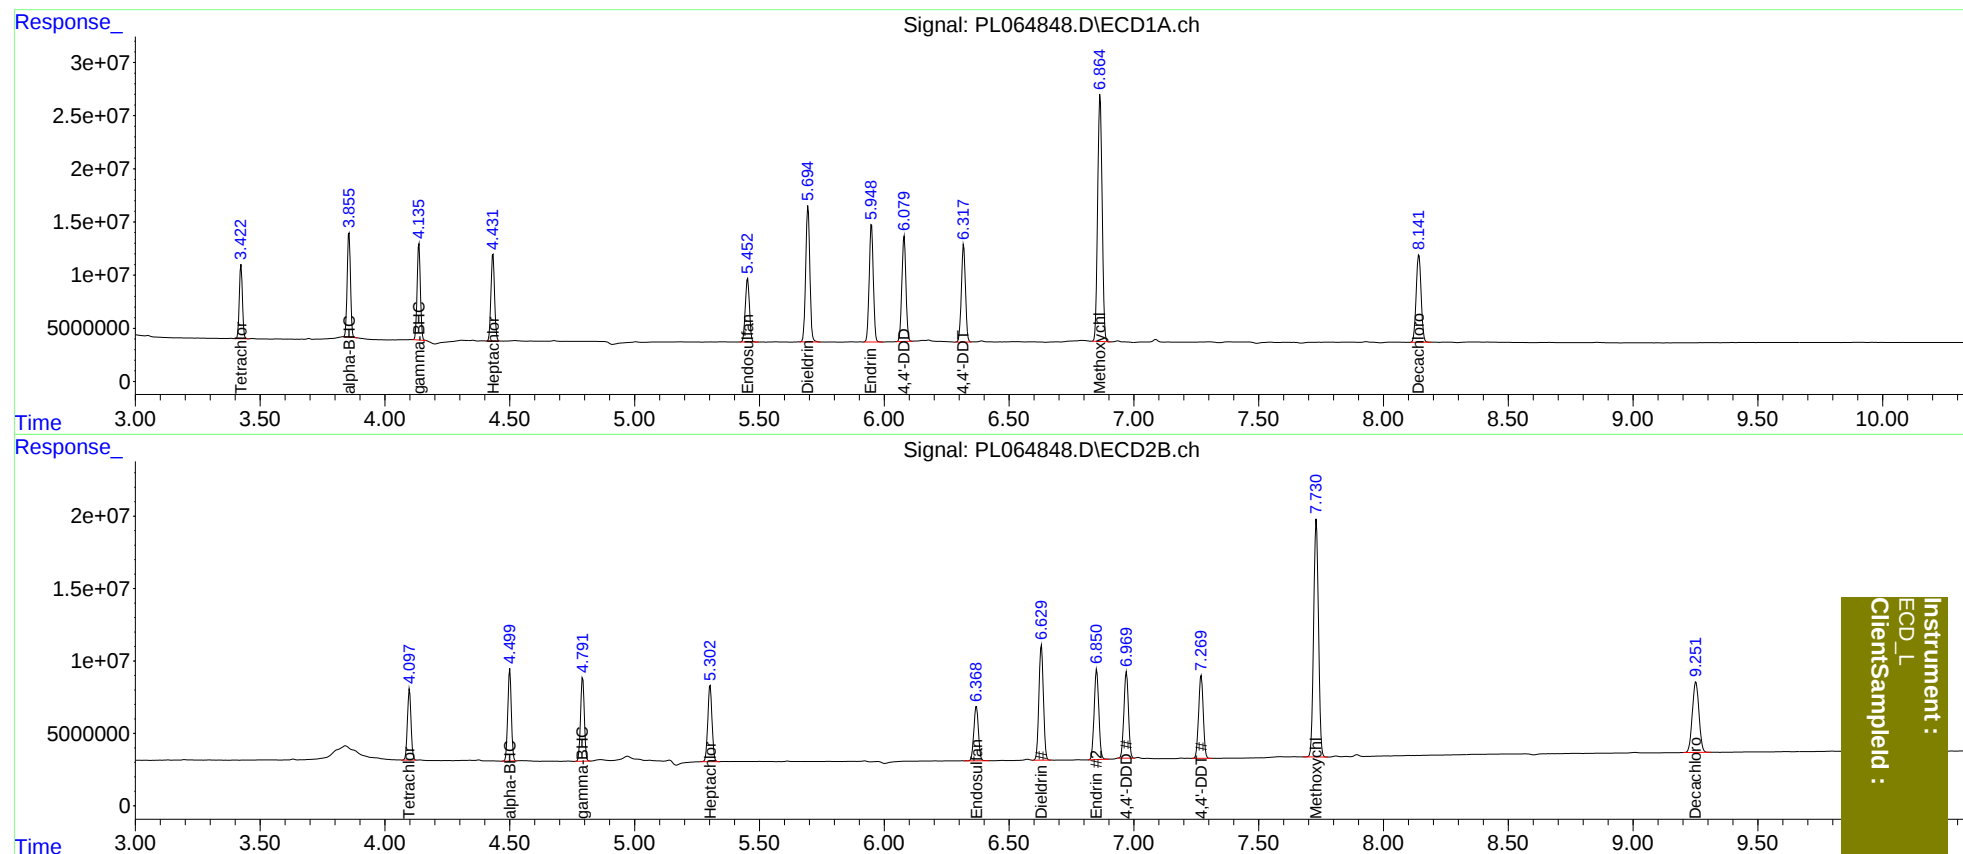


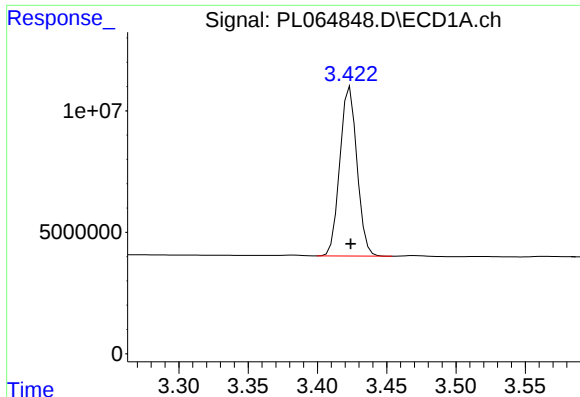

#1 Tetrachloro-m-xylene


R.T.: 3.424 min
Delta R.T.: 0.000 min
Response: 60035188
Conc: 20.00 ng/ml

Instrument :
ECD_L
ClientSampleId :

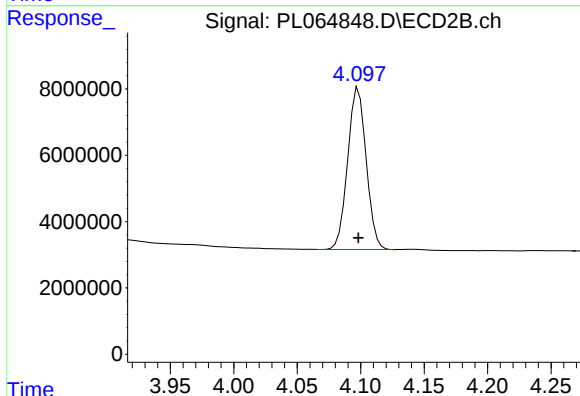


#1 Tetrachloro-m-xylene

R.T.: 4.098 min
Delta R.T.: 0.000 min
Response: 49480574
Conc: 20.00 ng/ml

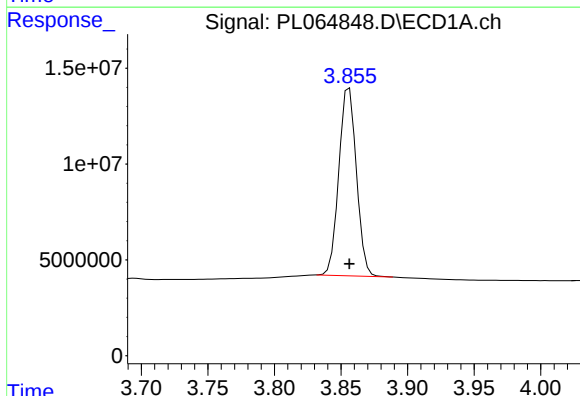


#2 alpha-BHC

R.T.: 3.856 min
Delta R.T.: 0.000 min
Response: 89966477
Conc: 20.00 ng/ml

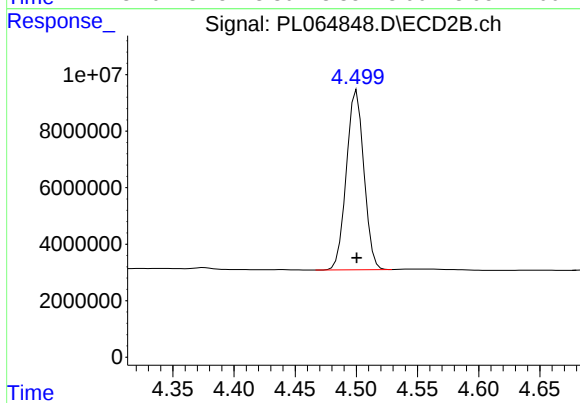

#2 alpha-BHC


R.T.: 4.500 min
Delta R.T.: 0.000 min
Response: 63289468
Conc: 20.00 ng/ml

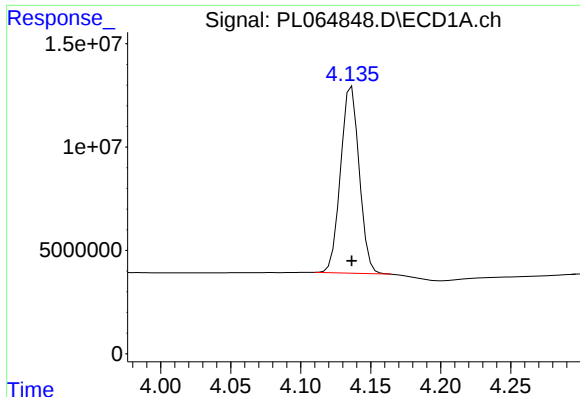

#3 gamma-BHC (Lindane)


R.T.: 4.136 min
Delta R.T.: 0.000 min
Response: 83841475
Conc: 20.00 ng/ml

Instrument :
ECD_L
ClientSampleId :

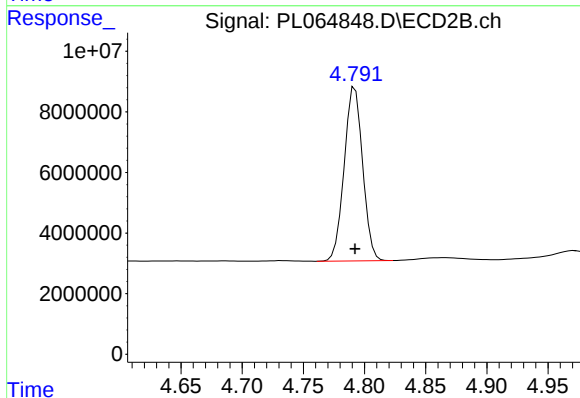


#3 gamma-BHC (Lindane)

R.T.: 4.792 min
Delta R.T.: 0.000 min
Response: 60255625
Conc: 20.00 ng/ml

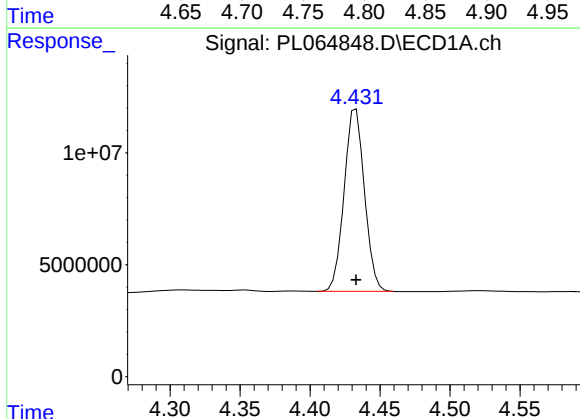


#4 Heptachlor

R.T.: 4.433 min
Delta R.T.: 0.000 min
Response: 82527667
Conc: 20.00 ng/ml

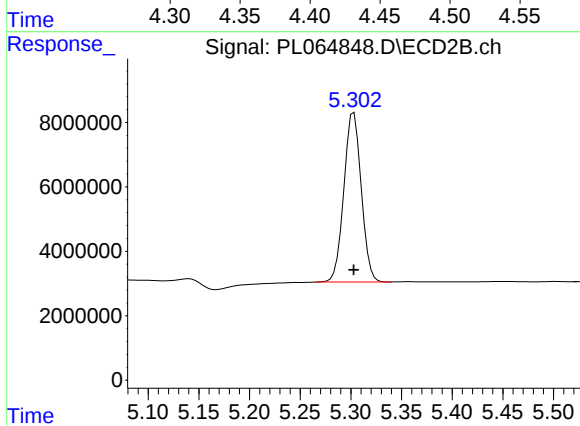

#4 Heptachlor


R.T.: 5.303 min
Delta R.T.: 0.000 min
Response: 62593772
Conc: 20.00 ng/ml

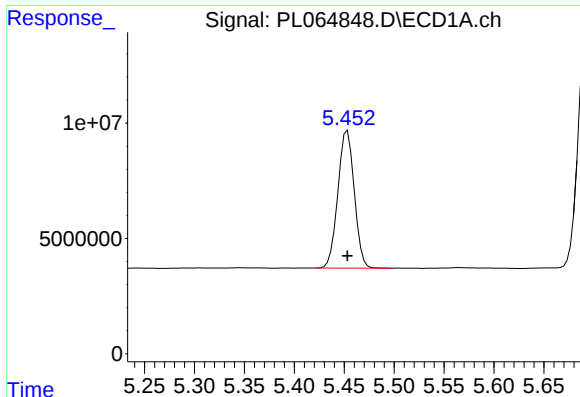

#9 Endosulfan I


R.T.: 5.453 min
Delta R.T.: 0.000 min
Response: 68096646
Conc: 20.00 ng/ml

Instrument :
ECD_L
ClientSampleId :

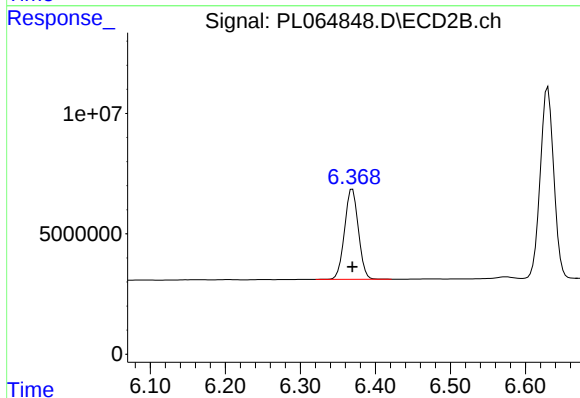


#9 Endosulfan I

R.T.: 6.369 min
Delta R.T.: 0.000 min
Response: 47926090
Conc: 20.00 ng/ml

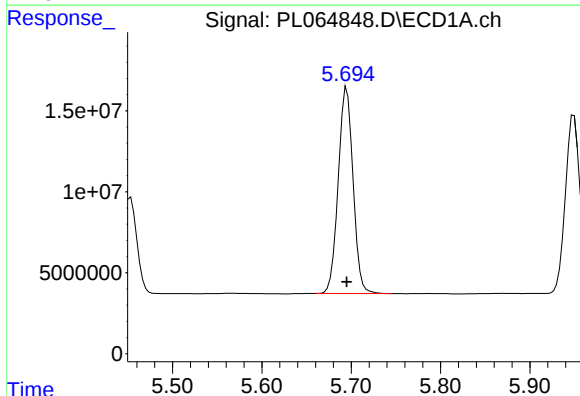


#13 Dieldrin

R.T.: 5.695 min
Delta R.T.: 0.000 min
Response: 146764530
Conc: 40.00 ng/ml

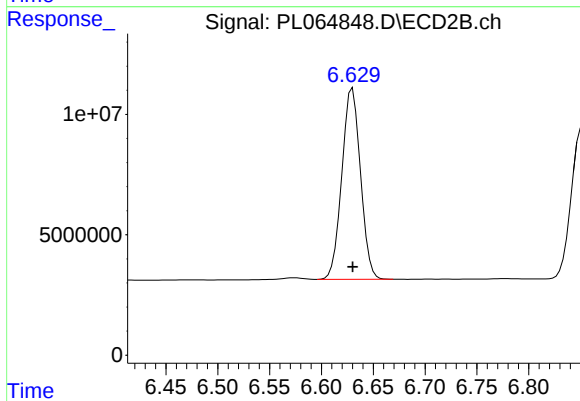

#13 Dieldrin


R.T.: 6.630 min
Delta R.T.: 0.000 min
Response: 99234092
Conc: 40.00 ng/ml

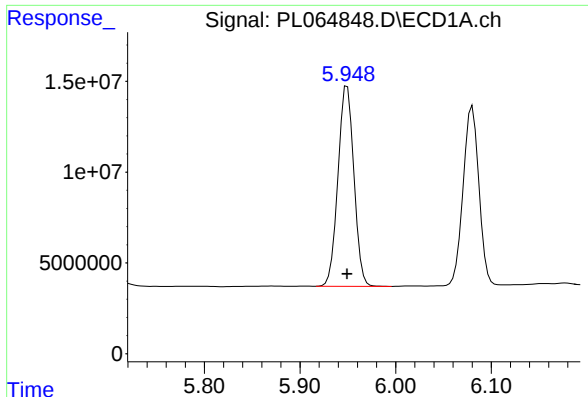

#14 Endrin


R.T.: 5.949 min
Delta R.T.: 0.000 min
Response: 127858076
Conc: 40.00 ng/ml

Instrument :
ECD_L
ClientSampleId :

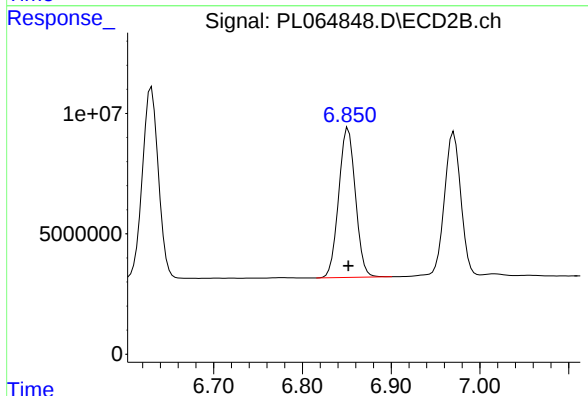


#14 Endrin

R.T.: 6.852 min
Delta R.T.: 0.000 min
Response: 81182571
Conc: 40.00 ng/ml

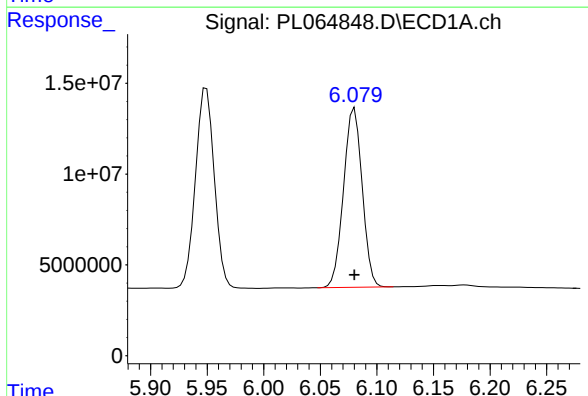


#16 4,4'-DDD

R.T.: 6.080 min
Delta R.T.: 0.000 min
Response: 113048089
Conc: 40.00 ng/ml

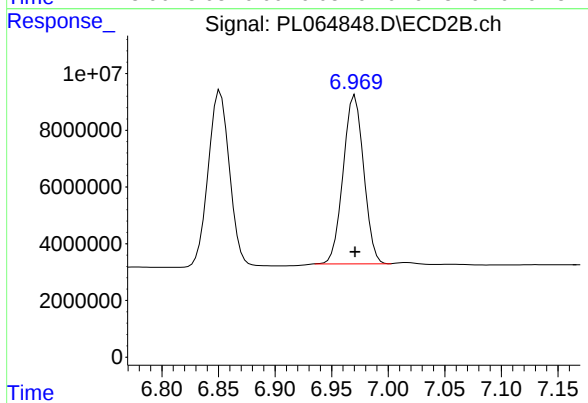

#16 4,4'-DDD


R.T.: 6.971 min
Delta R.T.: 0.000 min
Response: 74889452
Conc: 40.00 ng/ml

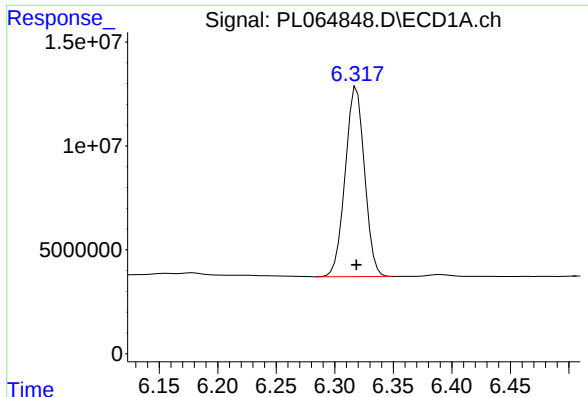

#17 4,4'-DDT


R.T.: 6.319 min
Delta R.T.: 0.000 min
Response: 104814046
Conc: 40.00 ng/ml

Instrument :
ECD_L
ClientSampleId :

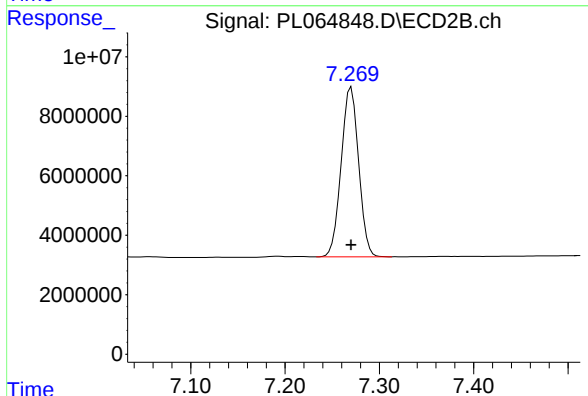


#17 4,4'-DDT

R.T.: 7.270 min
Delta R.T.: 0.000 min
Response: 73477564
Conc: 40.00 ng/ml

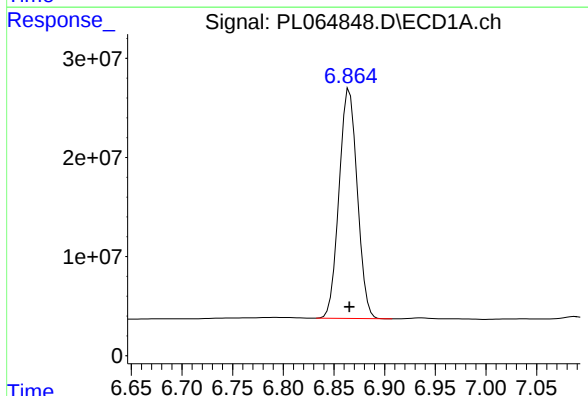


#20 Methoxychlor

R.T.: 6.865 min
Delta R.T.: 0.000 min
Response: 289467401
Conc: 200.00 ng/ml

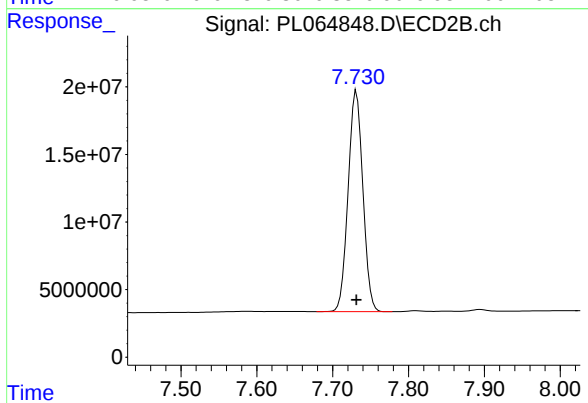

#20 Methoxychlor

R.T.: 7.731 min
Delta R.T.: 0.000 min
Response: 220810213
Conc: 200.00 ng/ml

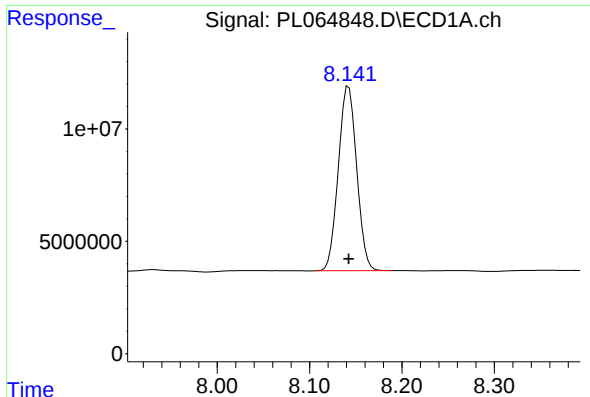

#27 Decachlorobiphenyl


R.T.: 8.142 min

Delta R.T.: 0.000 min

Response: 113656263

Conc: 40.00 ng/ml

Instrument :
ECD_L
ClientSampleId :

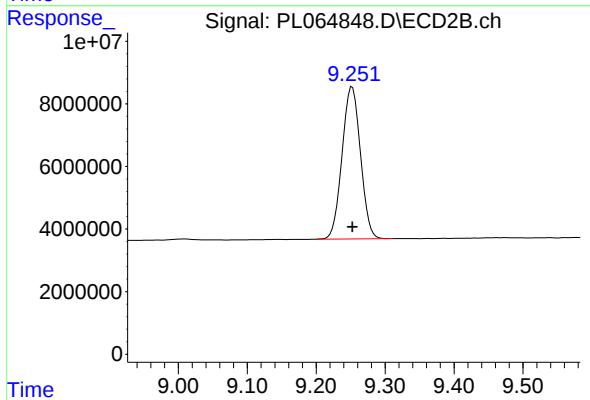

#27 Decachlorobiphenyl

R.T.: 9.252 min

Delta R.T.: 0.000 min

Response: 90359503

Conc: 40.00 ng/ml