

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022121\
 Data File : PL064850.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Feb 2021 15:02
 Operator : AR\AJ
 Sample : INDA401
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 22 03:41:07 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022121CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Feb 22 03:39:50 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.423	4.098	120.6E6	100.0E6	40.185	40.427
27)	SA Decachlor...	8.142	9.252	217.4E6	172.7E6	76.512	76.443
Target Compounds							
2)	A alpha-BHC	3.856	4.500	189.7E6	136.5E6	42.172	43.128
3)	MA gamma-BHC...	4.136	4.792	174.5E6	126.5E6	41.617	41.974
4)	MA Heptachlor	4.433	5.303	167.9E6	127.2E6	40.687	40.632
9)	A Endosulfan I	5.453	6.369	136.6E6	96706612	40.115	40.357
13)	MA Dieldrin	5.695	6.629	302.2E6	207.7E6	82.366	83.712
14)	MA Endrin	5.949	6.851	261.2E6	167.9E6	81.721	82.749
16)	A 4,4'-DDD	6.080	6.970	233.3E6	157.2E6	82.557	83.989
17)	MA 4,4'-DDT	6.319	7.270	224.5E6	156.3E6	85.664	85.091
20)	A Methoxychlor	6.866	7.731	568.8E6	445.3E6	392.978	403.303


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022121\
Data File : PL064850.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Feb 2021 15:02
Operator : AR\AJ
Sample : INDA401
Misc :
ALS Vial : 15 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 22 03:41:07 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022121CLP.M
Quant Title : GC Extractables
QLast Update : Mon Feb 22 03:39:50 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

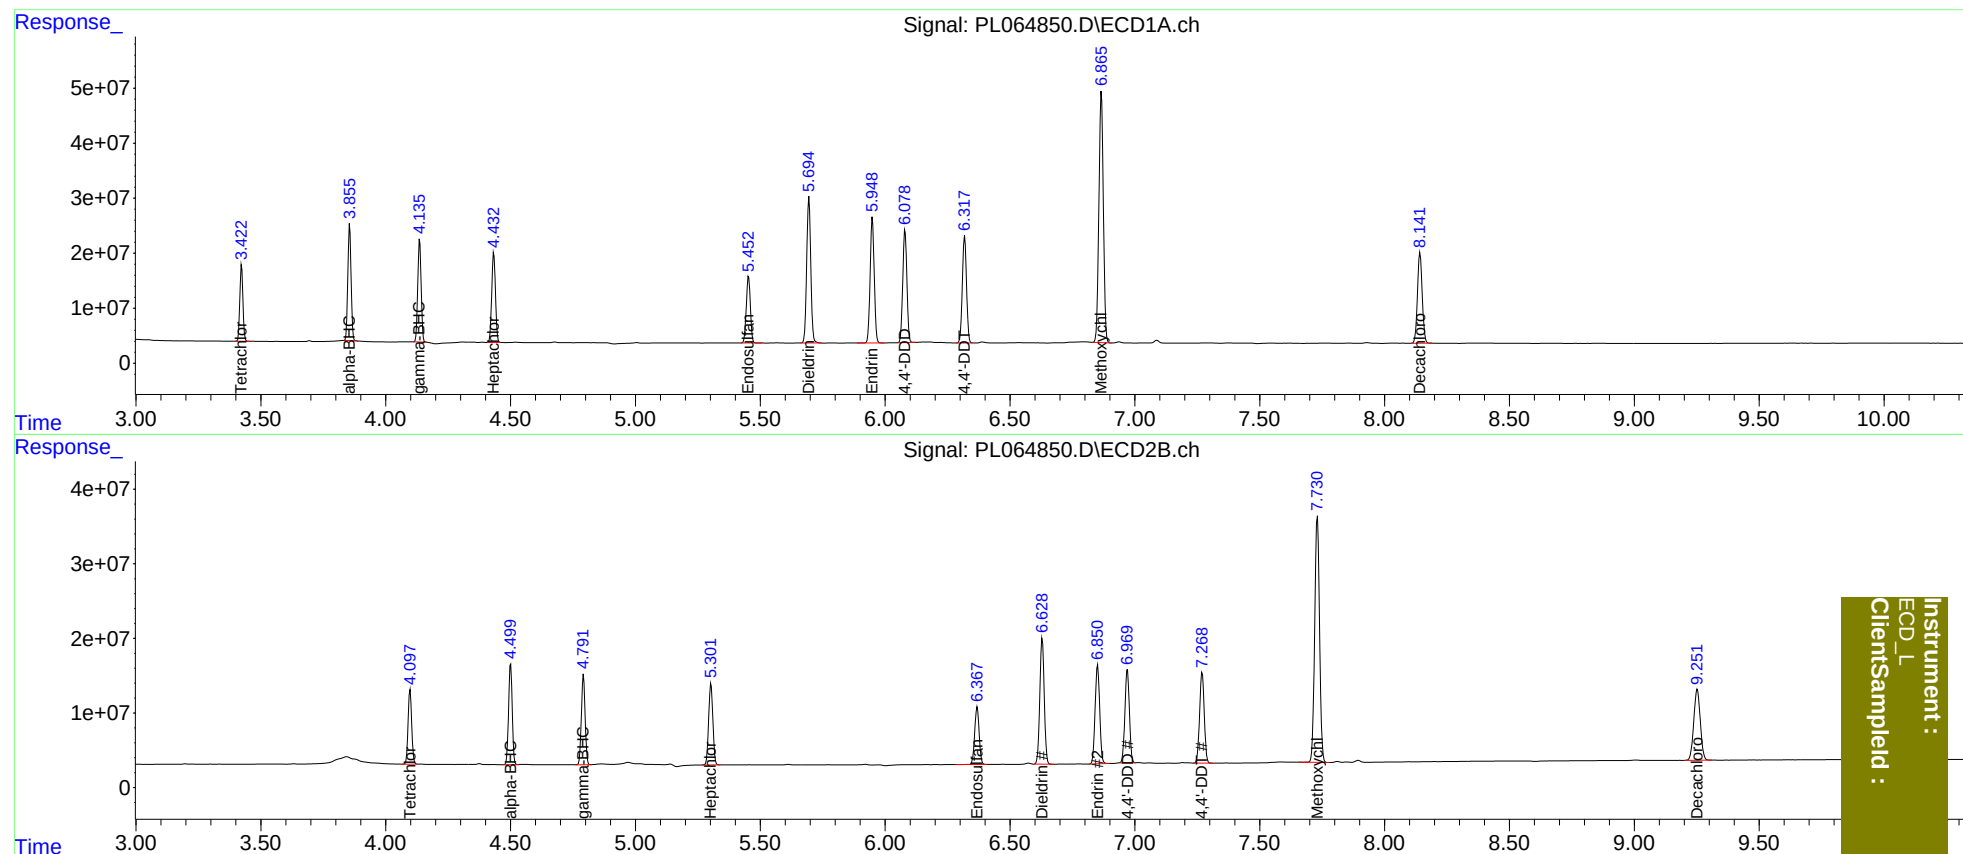


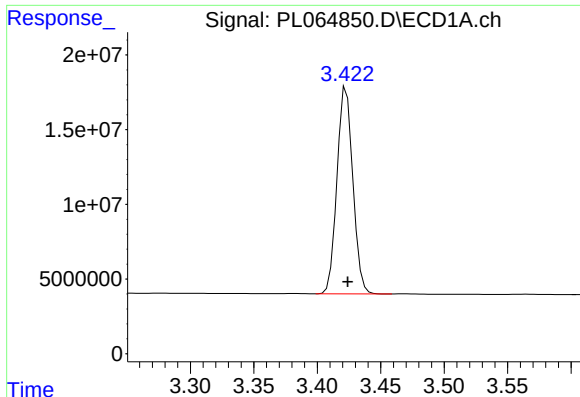

#1 Tetrachloro-m-xylene


R.T.: 3.423 min
Delta R.T.: 0.000 min
Response: 120625578
Conc: 40.18 ng/ml

Instrument :
ECD_L
ClientSampleId :

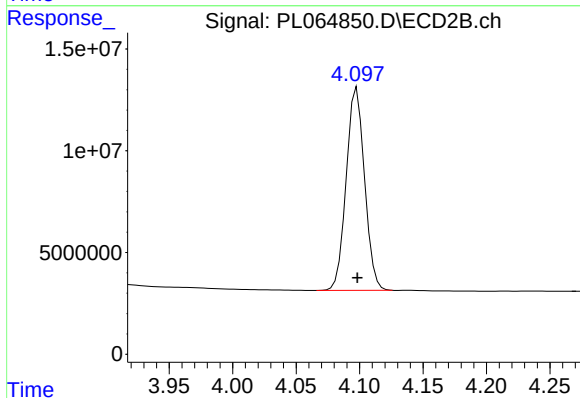


#1 Tetrachloro-m-xylene

R.T.: 4.098 min
Delta R.T.: 0.000 min
Response: 100017475
Conc: 40.43 ng/ml

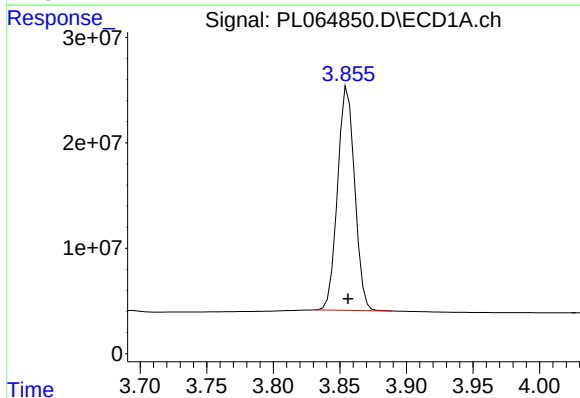


#2 alpha-BHC

R.T.: 3.856 min
Delta R.T.: 0.000 min
Response: 189704145
Conc: 42.17 ng/ml

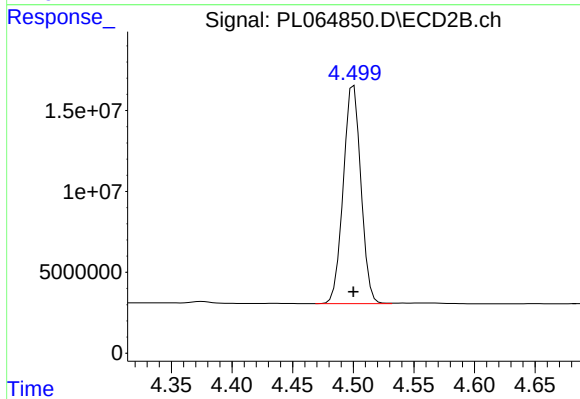

#2 alpha-BHC


R.T.: 4.500 min
Delta R.T.: 0.000 min
Response: 136477008
Conc: 43.13 ng/ml

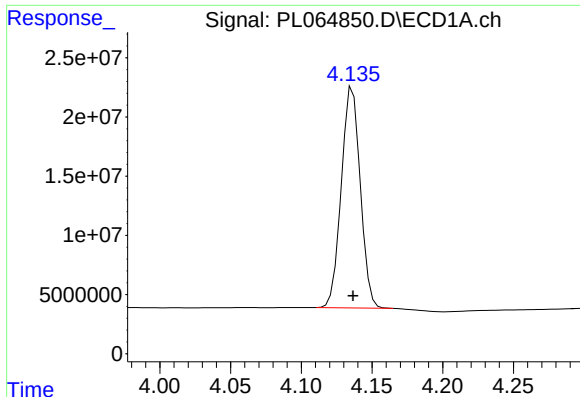

#3 gamma-BHC (Lindane)


R.T.: 4.136 min
Delta R.T.: 0.000 min
Response: 174462178
Conc: 41.62 ng/ml

Instrument :
ECD_L
ClientSampleId :

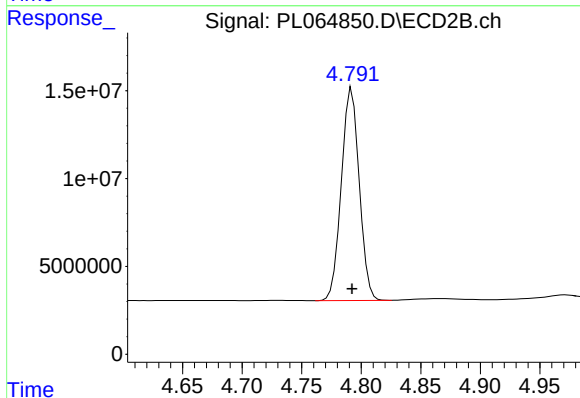


#3 gamma-BHC (Lindane)

R.T.: 4.792 min
Delta R.T.: 0.000 min
Response: 126458900
Conc: 41.97 ng/ml

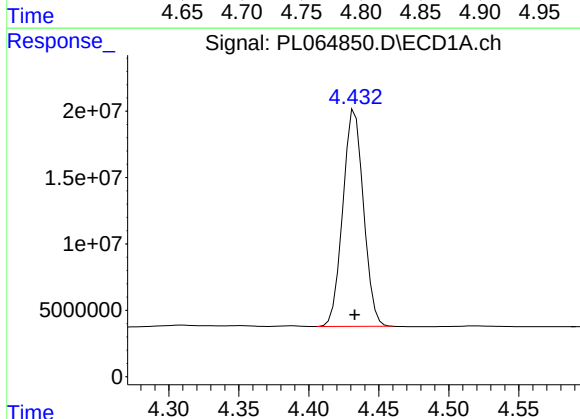


#4 Heptachlor

R.T.: 4.433 min
Delta R.T.: 0.000 min
Response: 167890319
Conc: 40.69 ng/ml

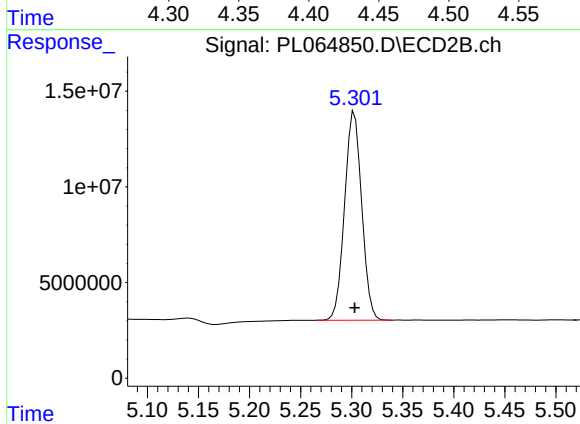

#4 Heptachlor


R.T.: 5.303 min
Delta R.T.: 0.000 min
Response: 127164289
Conc: 40.63 ng/ml

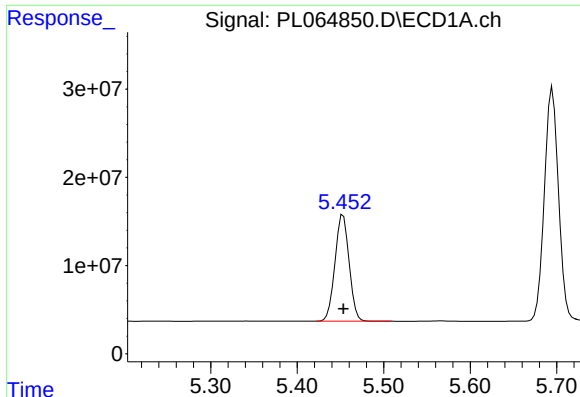

#9 Endosulfan I


R.T.: 5.453 min
Delta R.T.: 0.000 min
Response: 136583347
Conc: 40.11 ng/ml

Instrument :
ECD_L
ClientSampleId :

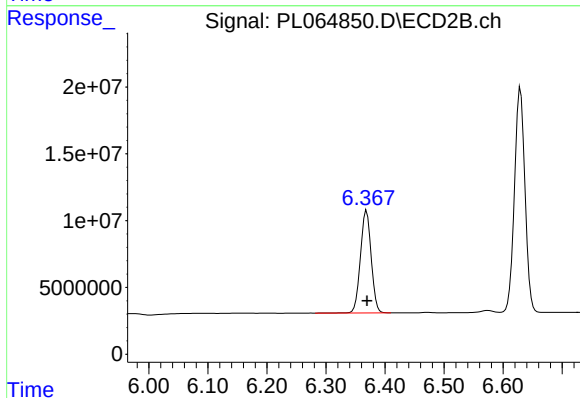


#9 Endosulfan I

R.T.: 6.369 min
Delta R.T.: 0.000 min
Response: 96706612
Conc: 40.36 ng/ml

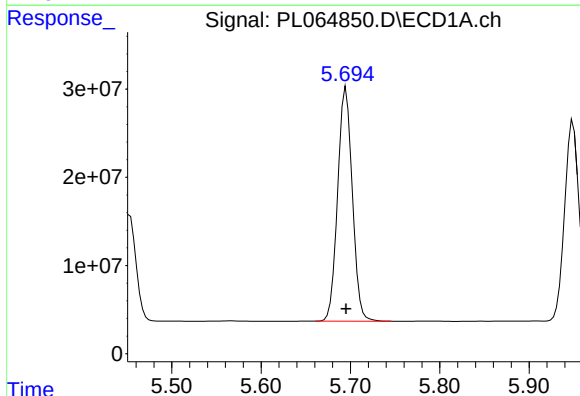


#13 Dieldrin

R.T.: 5.695 min
Delta R.T.: 0.000 min
Response: 302208724
Conc: 82.37 ng/ml

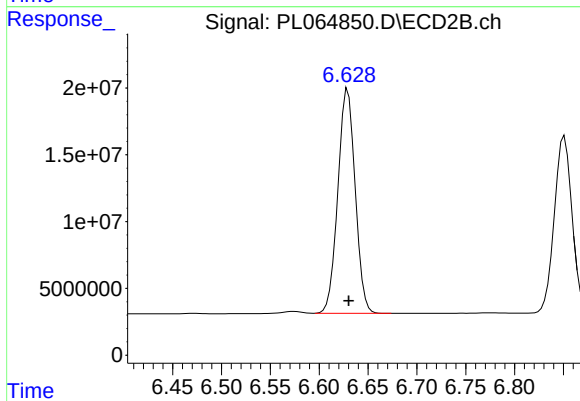

#13 Dieldrin


R.T.: 6.629 min
Delta R.T.: 0.000 min
Response: 207677431
Conc: 83.71 ng/ml

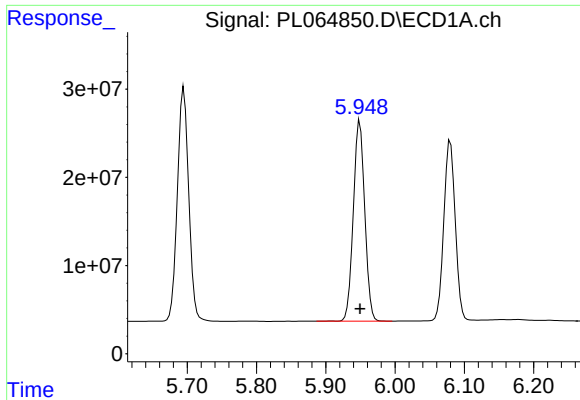

#14 Endrin


R.T.: 5.949 min
Delta R.T.: 0.000 min
Response: 261218547
Conc: 81.72 ng/ml

Instrument :
ECD_L
ClientSampleId :

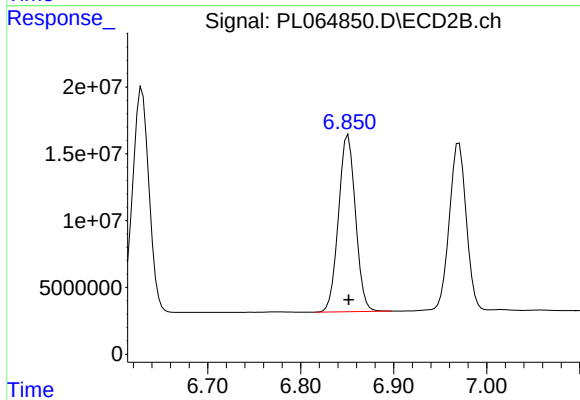


#14 Endrin

R.T.: 6.851 min
Delta R.T.: 0.000 min
Response: 167944675
Conc: 82.75 ng/ml

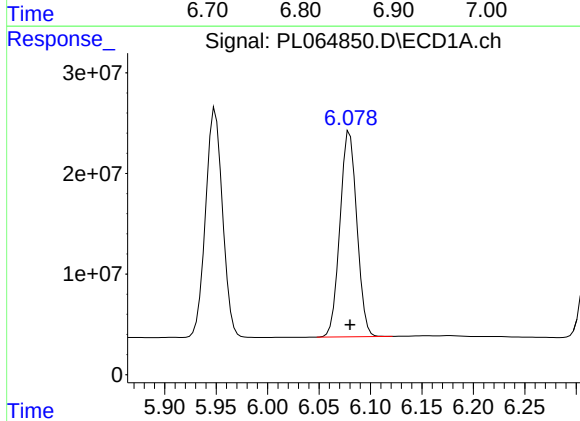


#16 4,4'-DDD

R.T.: 6.080 min
Delta R.T.: 0.000 min
Response: 233323188
Conc: 82.56 ng/ml

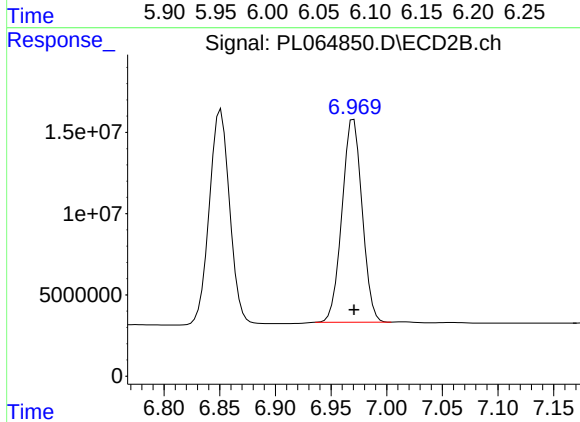

#16 4,4'-DDD


R.T.: 6.970 min
Delta R.T.: 0.000 min
Response: 157248189
Conc: 83.99 ng/ml

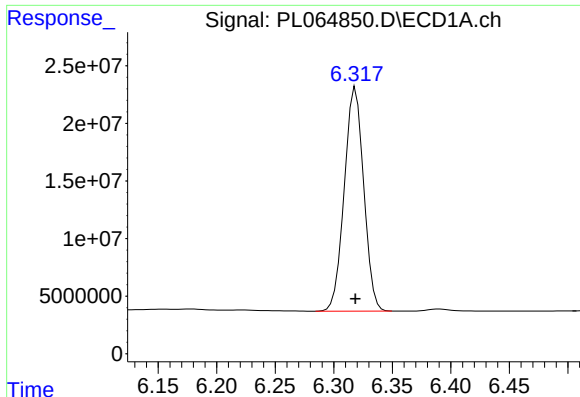

#17 4,4'-DDT


R.T.: 6.319 min
Delta R.T.: 0.000 min
Response: 224469715
Conc: 85.66 ng/ml

Instrument :
ECD_L
ClientSampleId :

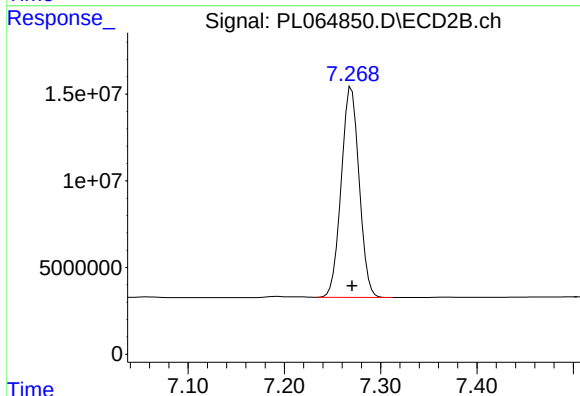


#17 4,4'-DDT

R.T.: 7.270 min
Delta R.T.: 0.000 min
Response: 156306703
Conc: 85.09 ng/ml

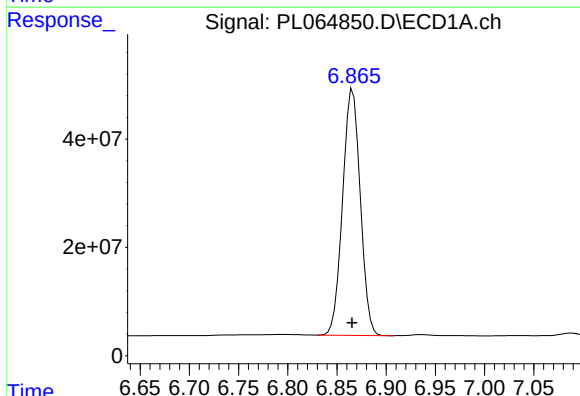


#20 Methoxychlor

R.T.: 6.866 min
Delta R.T.: 0.000 min
Response: 568772072
Conc: 392.98 ng/ml

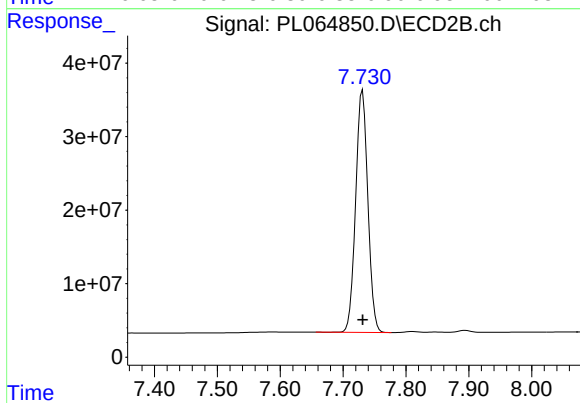

#20 Methoxychlor


R.T.: 7.731 min
Delta R.T.: 0.000 min
Response: 445266968
Conc: 403.30 ng/ml

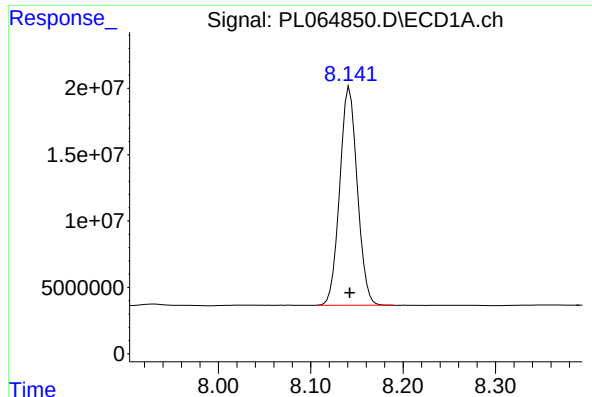

#27 Decachlorobiphenyl

R.T.: 8.142 min
Delta R.T.: 0.000 min
Response: 217402177
Conc: 76.51 ng/ml

Instrument :
ECD_L
ClientSampleId :

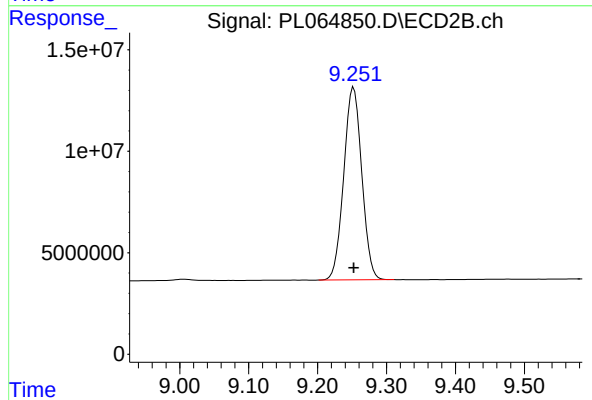

#27 Decachlorobiphenyl

R.T.: 9.252 min
Delta R.T.: 0.000 min
Response: 172682837
Conc: 76.44 ng/ml