

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022121\
 Data File : PL064852.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Feb 2021 15:31
 Operator : AR\AJ
 Sample : INDA501
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 22 03:41:18 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022121CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Feb 22 03:39:50 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.423	4.098	234.3E6	194.2E6	78.040	78.514
27)	SA Decachlor...	8.143	9.253	406.4E6	322.8E6	143.025	142.914
Target Compounds							
2)	A alpha-BHC	3.856	4.500	384.6E6	281.2E6	85.493	88.865
3)	MA gamma-BHC...	4.136	4.793	351.2E6	257.5E6	83.769	85.466
4)	MA Heptachlor	4.433	5.303	331.6E6	254.2E6	80.352	81.223
9)	A Endosulfan I	5.453	6.369	267.2E6	191.0E6	78.490	79.707
13)	MA Dieldrin	5.695	6.630	599.9E6	422.3E6	163.513	170.243
14)	MA Endrin	5.949	6.852	518.4E6	342.7E6	162.169	168.861
16)	A 4,4'-DDD	6.080	6.971	462.6E6	320.5E6	163.680	171.212
17)	MA 4,4'-DDT	6.319	7.271	463.5E6	324.6E6	176.889	176.731
20)	A Methoxychlor	6.866	7.732	1079.2E6	872.8E6	745.613	790.521


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022121\
Data File : PL064852.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Feb 2021 15:31
Operator : AR\AJ
Sample : INDA501
Misc :
ALS Vial : 17 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 22 03:41:18 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022121CLP.M
Quant Title : GC Extractables
QLast Update : Mon Feb 22 03:39:50 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

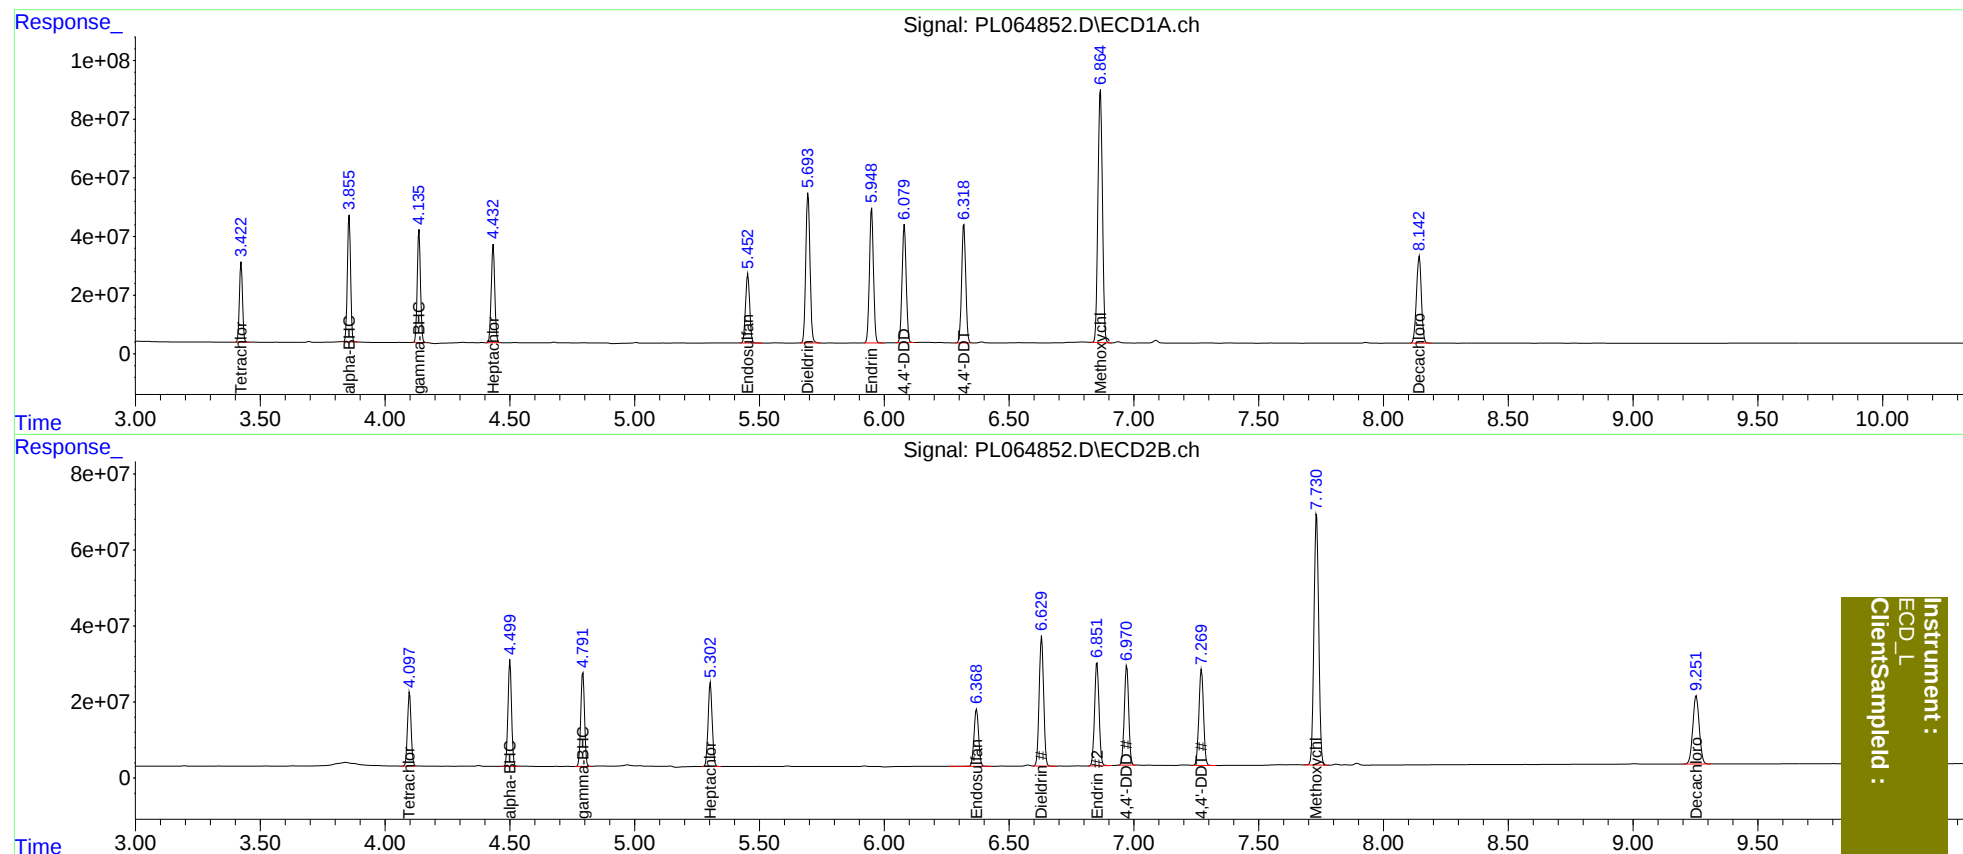


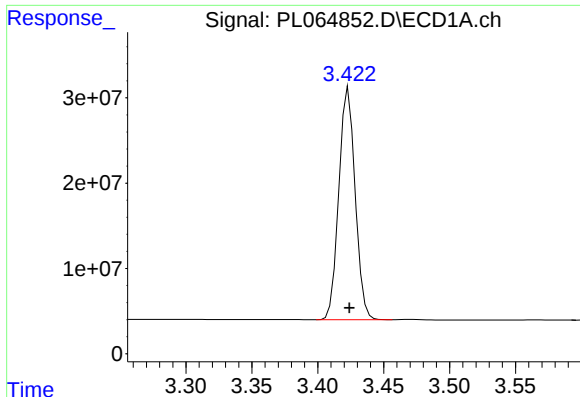

#1 Tetrachloro-m-xylene


R.T.: 3.423 min
Delta R.T.: 0.000 min
Response: 234256236
Conc: 78.04 ng/ml

Instrument :
ECD_L
ClientSampleId :

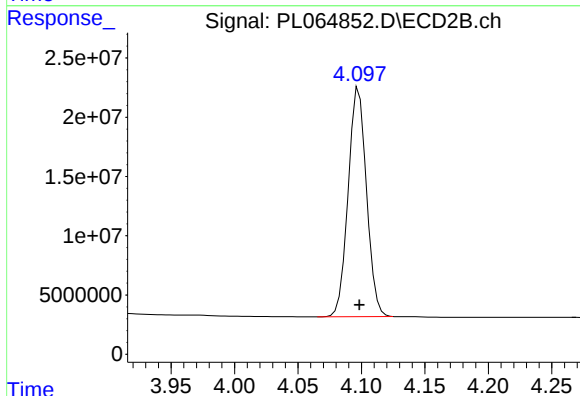


#1 Tetrachloro-m-xylene

R.T.: 4.098 min
Delta R.T.: 0.000 min
Response: 194245973
Conc: 78.51 ng/ml

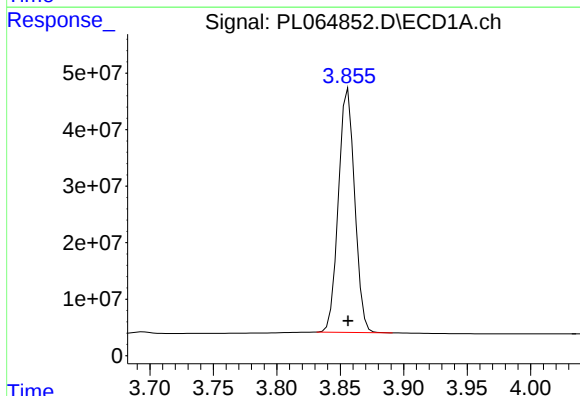


#2 alpha-BHC

R.T.: 3.856 min
Delta R.T.: 0.000 min
Response: 384575643
Conc: 85.49 ng/ml

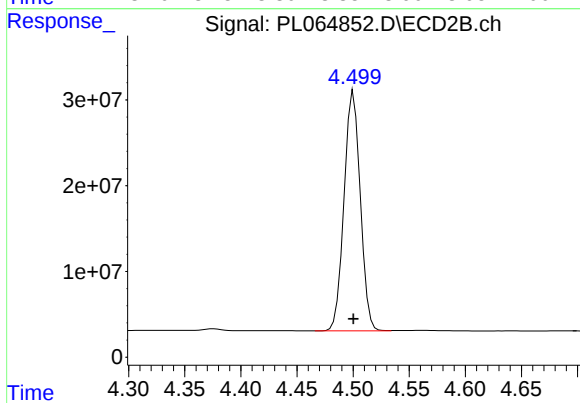

#2 alpha-BHC


R.T.: 4.500 min
Delta R.T.: 0.000 min
Response: 281210759
Conc: 88.86 ng/ml

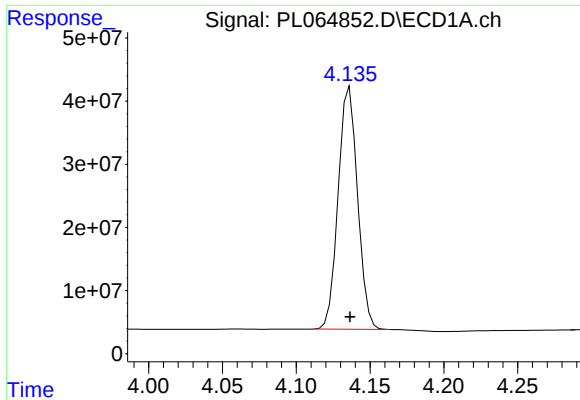

#3 gamma-BHC (Lindane)


R.T.: 4.136 min
Delta R.T.: 0.000 min
Response: 351164328
Conc: 83.77 ng/ml

Instrument :
ECD_L
ClientSampleId :

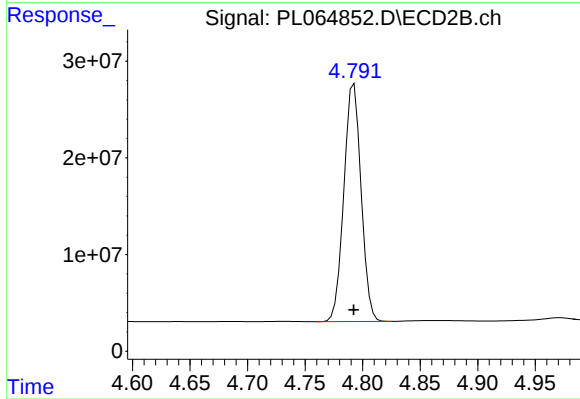


#3 gamma-BHC (Lindane)

R.T.: 4.793 min
Delta R.T.: 0.000 min
Response: 257491042
Conc: 85.47 ng/ml

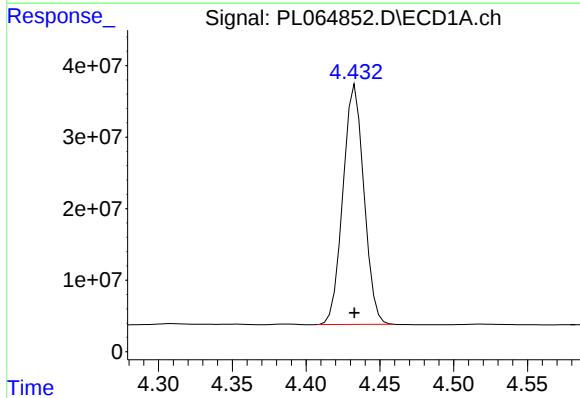


#4 Heptachlor

R.T.: 4.433 min
Delta R.T.: 0.000 min
Response: 331562359
Conc: 80.35 ng/ml

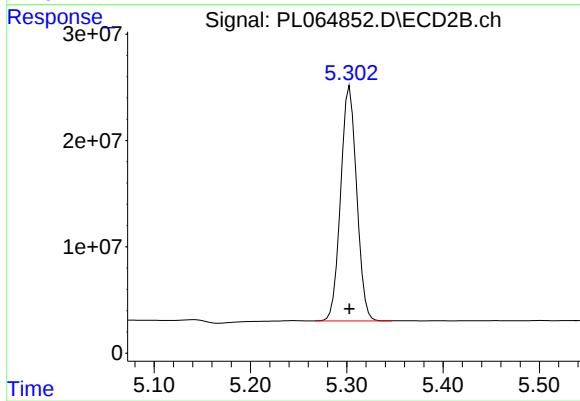

#4 Heptachlor


R.T.: 5.303 min
Delta R.T.: 0.000 min
Response: 254202925
Conc: 81.22 ng/ml

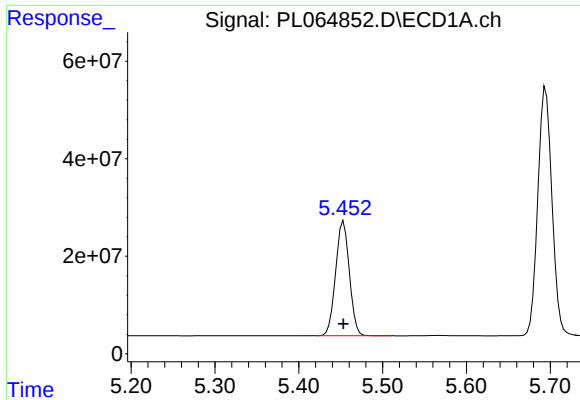

#9 Endosulfan I


R.T.: 5.453 min
Delta R.T.: 0.000 min
Response: 267245130
Conc: 78.49 ng/ml

Instrument :
ECD_L
ClientSampleId :

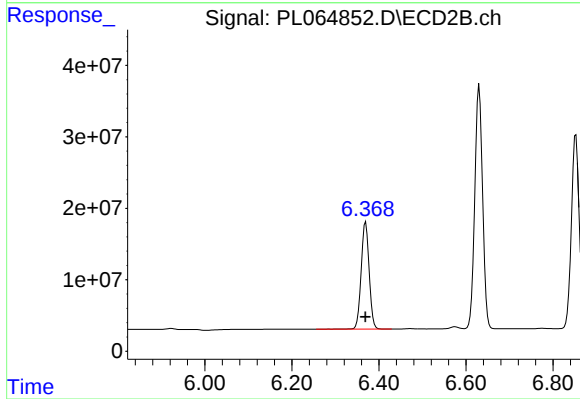


#9 Endosulfan I

R.T.: 6.369 min
Delta R.T.: 0.000 min
Response: 191002023
Conc: 79.71 ng/ml

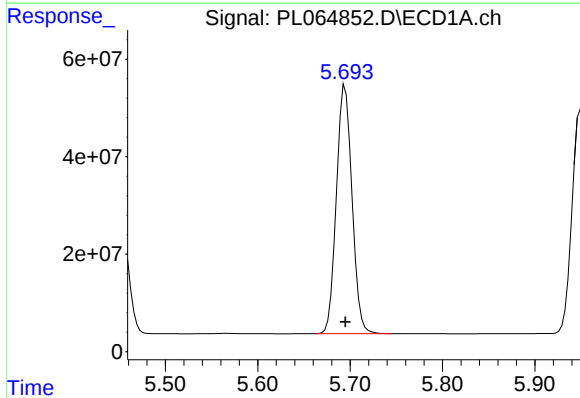


#13 Dieldrin

R.T.: 5.695 min
Delta R.T.: 0.000 min
Response: 599947165
Conc: 163.51 ng/ml

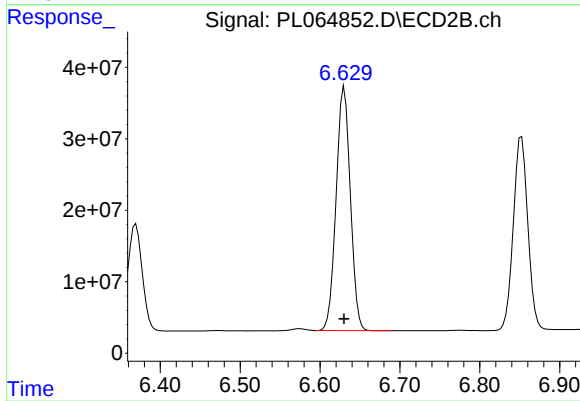

#13 Dieldrin


R.T.: 6.630 min
Delta R.T.: 0.000 min
Response: 422347765
Conc: 170.24 ng/ml

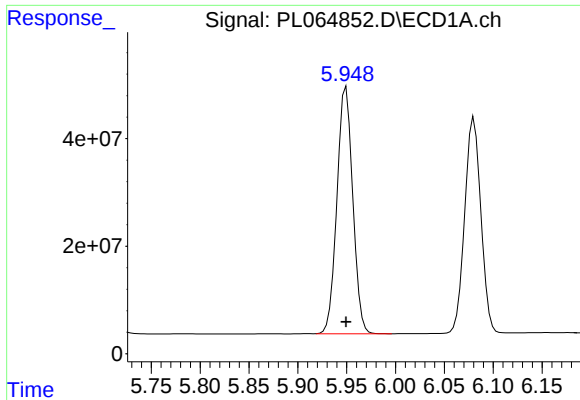

#14 Endrin


R.T.: 5.949 min
Delta R.T.: 0.000 min
Response: 518365205
Conc: 162.17 ng/ml

Instrument :
ECD_L
ClientSampleId :

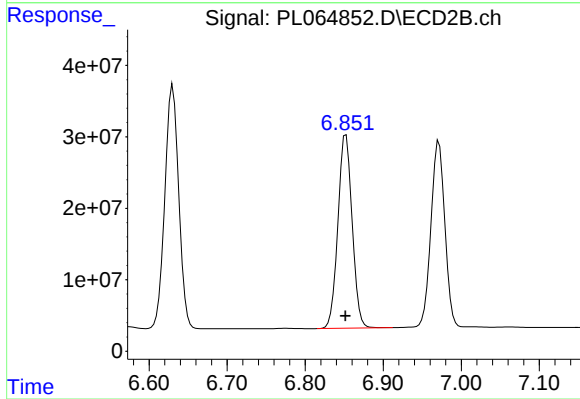


#14 Endrin

R.T.: 6.852 min
Delta R.T.: 0.000 min
Response: 342714071
Conc: 168.86 ng/ml

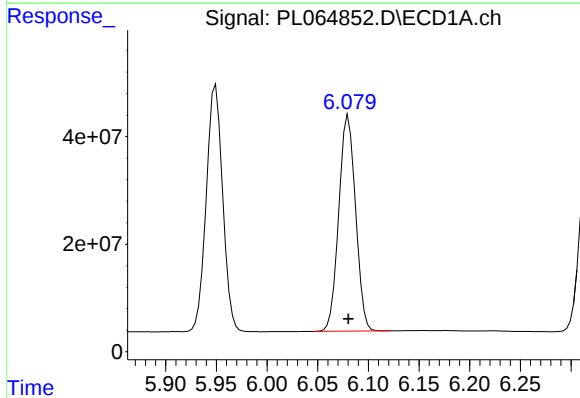


#16 4,4'-DDD

R.T.: 6.080 min
Delta R.T.: 0.000 min
Response: 462591886
Conc: 163.68 ng/ml

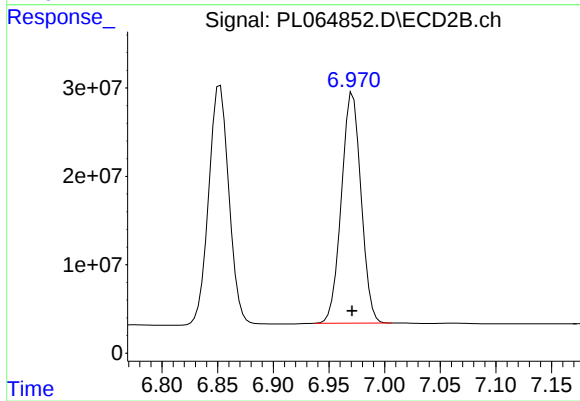

#16 4,4'-DDD


R.T.: 6.971 min
Delta R.T.: 0.000 min
Response: 320549400
Conc: 171.21 ng/ml

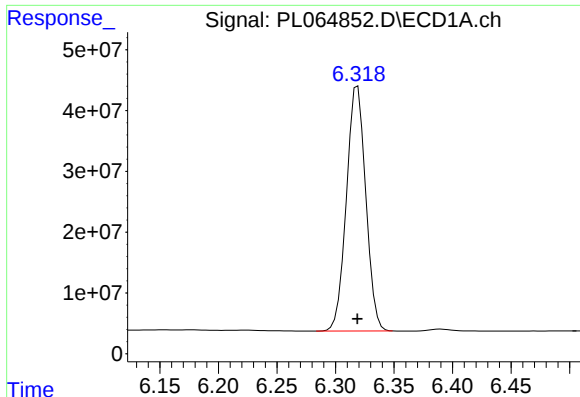

#17 4,4'-DDT


R.T.: 6.319 min
Delta R.T.: 0.000 min
Response: 463511828
Conc: 176.89 ng/ml

Instrument :
ECD_L
ClientSampleId :

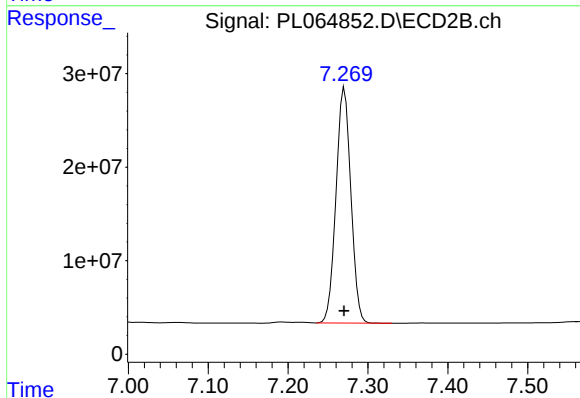


#17 4,4'-DDT

R.T.: 7.271 min
Delta R.T.: 0.000 min
Response: 324643869
Conc: 176.73 ng/ml

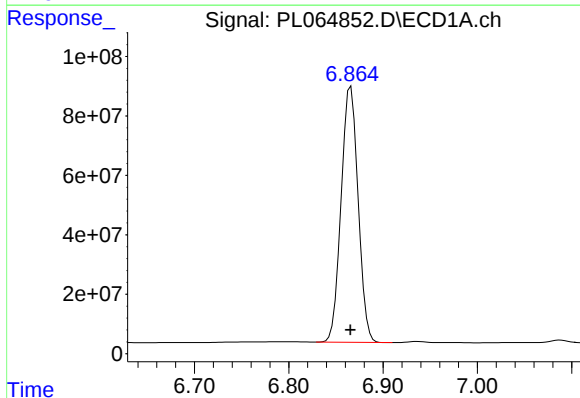


#20 Methoxychlor

R.T.: 6.866 min
Delta R.T.: 0.000 min
Response: 1079153367
Conc: 745.61 ng/ml

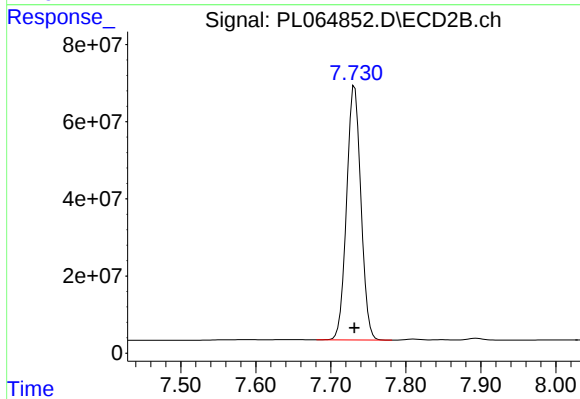

#20 Methoxychlor


R.T.: 7.732 min
Delta R.T.: 0.000 min
Response: 872775940
Conc: 790.52 ng/ml

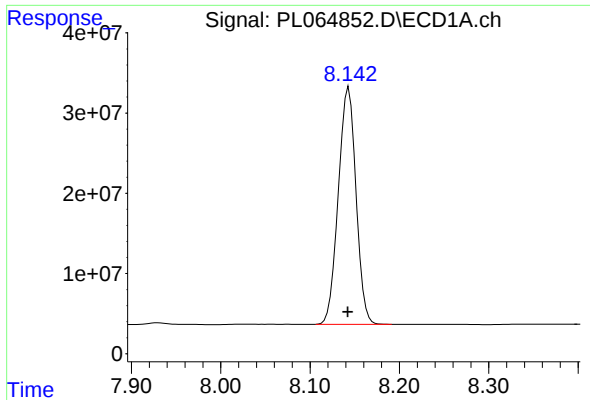

#27 Decachlorobiphenyl

R.T.: 8.143 min
Delta R.T.: 0.000 min
Response: 406392506
Conc: 143.03 ng/ml

Instrument :
ECD_L
ClientSampleId :

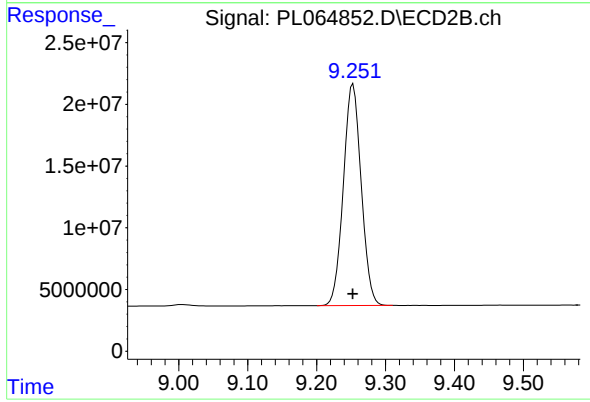

#27 Decachlorobiphenyl

R.T.: 9.253 min
Delta R.T.: 0.000 min
Response: 322841500
Conc: 142.91 ng/ml