

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022121\
 Data File : PL064854.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Feb 2021 15:59
 Operator : AR\AJ
 Sample : PIBLK51
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 22 03:56:56 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022121CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Feb 22 03:50:14 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.423	4.098	53328316	44441989	17.686	17.799
27)	SA Decachlor...	8.143	9.252	93288432	73853680	32.619	32.925
Target Compounds							
6)	B beta-BHC	4.352f	4.973	719975	3762734	0.388	2.092 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022121\
Data File : PL064854.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Feb 2021 15:59
Operator : AR\AJ
Sample : PIBLK51
Misc :
ALS Vial : 19 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 22 03:56:56 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022121CLP.M
Quant Title : GC Extractables
QLast Update : Mon Feb 22 03:50:14 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

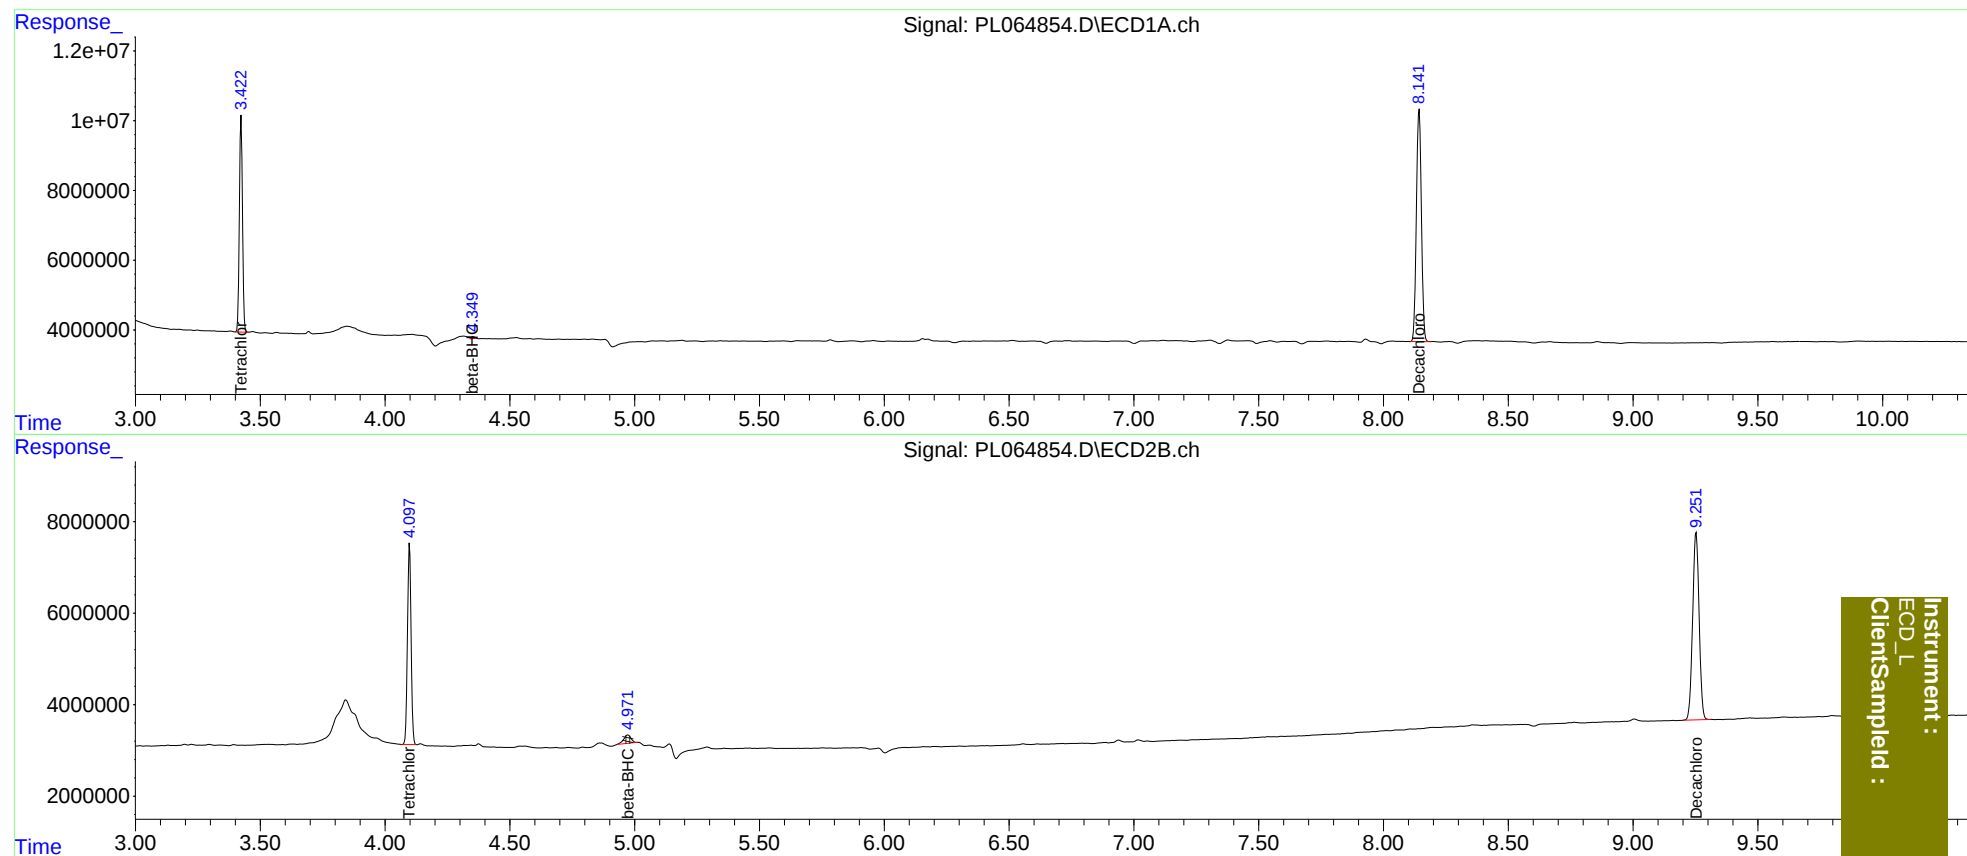


Instrument :
ECD_L
ClientSampleId :

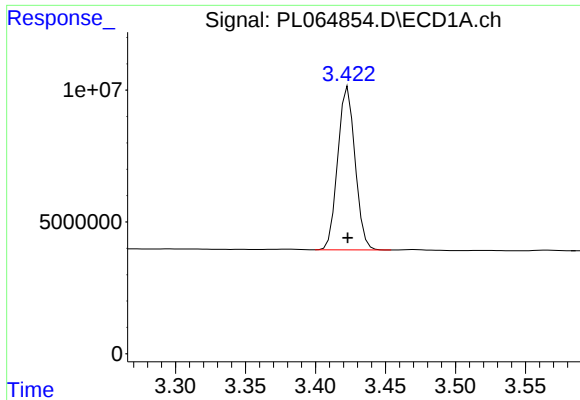

#1 Tetrachloro-m-xylene


R.T.: 3.423 min
Delta R.T.: 0.000 min
Response: 53328316
Conc: 17.69 ng/ml

Instrument :
ECD_L
ClientSampleId :

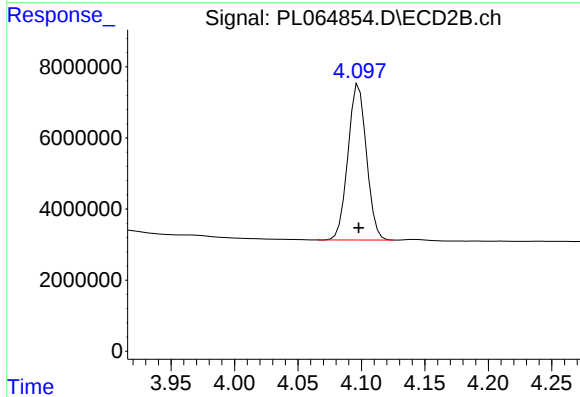


#1 Tetrachloro-m-xylene

R.T.: 4.098 min
Delta R.T.: 0.000 min
Response: 44441989
Conc: 17.80 ng/ml

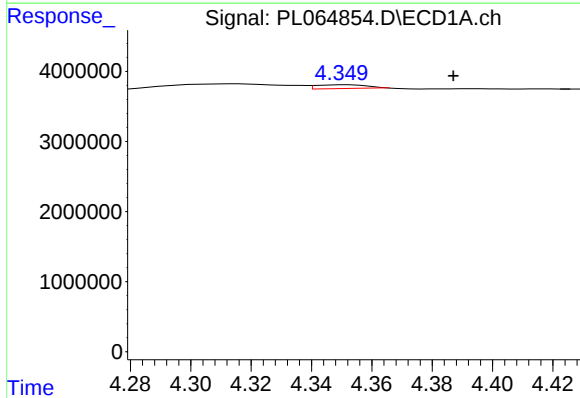


#6 beta-BHC

R.T.: 4.352 min
Delta R.T.: -0.035 min
Response: 719975
Conc: 0.39 ng/ml

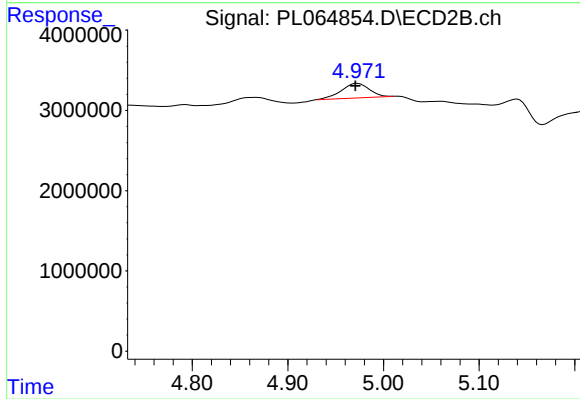

#6 beta-BHC

R.T.: 4.973 min
Delta R.T.: 0.002 min
Response: 3762734
Conc: 2.09 ng/ml

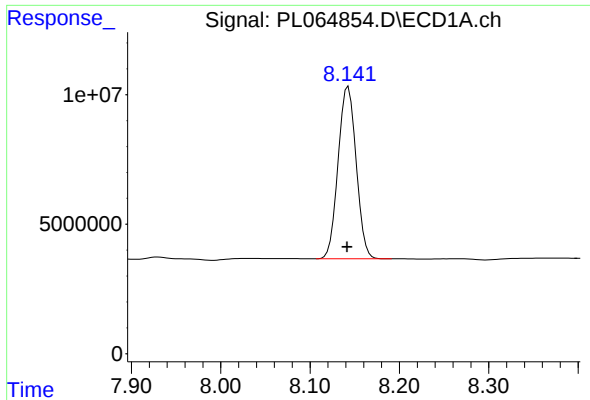

#27 Decachlorobiphenyl


R.T.: 8.143 min

Delta R.T.: 0.001 min

Response: 93288432

Conc: 32.62 ng/ml

Instrument :
ECD_L
ClientSampleId :

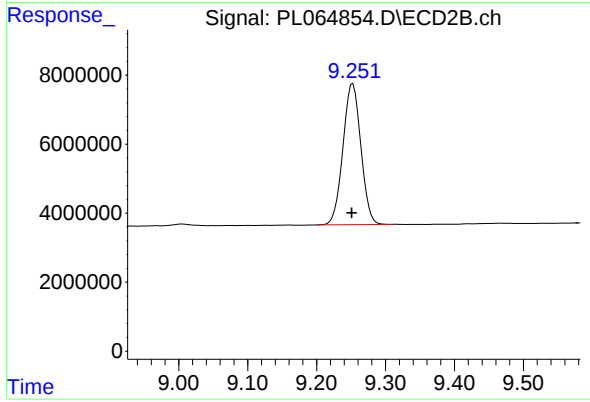

#27 Decachlorobiphenyl

R.T.: 9.252 min

Delta R.T.: 0.002 min

Response: 73853680

Conc: 32.92 ng/ml