

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022121\
 Data File : PL064837.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Feb 2021 11:57
 Operator : AR\AJ
 Sample : RESC51
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 RESC51

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 22 03:56:31 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022121CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Feb 22 03:50:14 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.423	4.098	57784705	47901473	19.164	19.184
2)	SA Decachlor...	8.142	9.250	109.1E6	87302947	38.143	38.921
Target Compounds							
2)	A alpha-BHC	3.856	4.499	41749223	29097439	9.123	9.043
3)	MA gamma-BHC...	4.136	4.791	40117937	28126712	9.457	9.226
4)	MA Heptachlor	4.432	5.302	38628709	30410089	9.263	9.500
5)	MB Aldrin	4.677	5.612	36352516	26177260	9.492	9.578
6)	B beta-BHC	4.387	4.970	18065017	19184199	9.742	10.664
7)	B delta-BHC	4.588	5.191	39759943	25887878	9.381	9.217
8)	B Heptachlo...	5.117	6.007	34748958	21442606	9.600	9.164
9)	A Endosulfan I	5.452	6.368	31622525	22273292	9.255	9.178
10)	B trans-Chl...	5.342	6.242	35917701	25700722	9.593	9.628
11)	B cis-Chlor...	5.400	6.314	34522990	25030610	9.515	9.505
12)	B 4,4'-DDE	5.566	6.471	64196544	44475270	18.684	18.611
13)	MA Dieldrin	5.694	6.629	67848461	46136116	18.394	18.311
14)	MA Endrin	5.948	6.850	61163620	39103093	18.924	18.947
15)	B Endosulfa...	6.221	7.065	56312689	38177584	19.122	19.069
16)	A 4,4'-DDD	6.079	6.969	51798861	34092449	18.231	18.064
17)	MA 4,4'-DDT	6.318	7.268	47763009	34102016	18.230	18.322
18)	B Endrin al...	6.390	7.191	49632269	34390560	19.776	19.597
19)	B Endosulfa...	6.602	7.414	60232540	39826770	19.589	19.592
20)	A Methoxychlor	6.864	7.730	139.0E6	107.2E6	96.968	96.814
21)	B Endrin ke...	7.088	7.893	62451505	40480370	20.166	19.770

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022121\
Data File : PL064837.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Feb 2021 11:57
Operator : AR\AJ
Sample : RESC51
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 22 03:56:31 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022121CLP.M
Quant Title : GC Extractables
QLast Update : Mon Feb 22 03:50:14 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

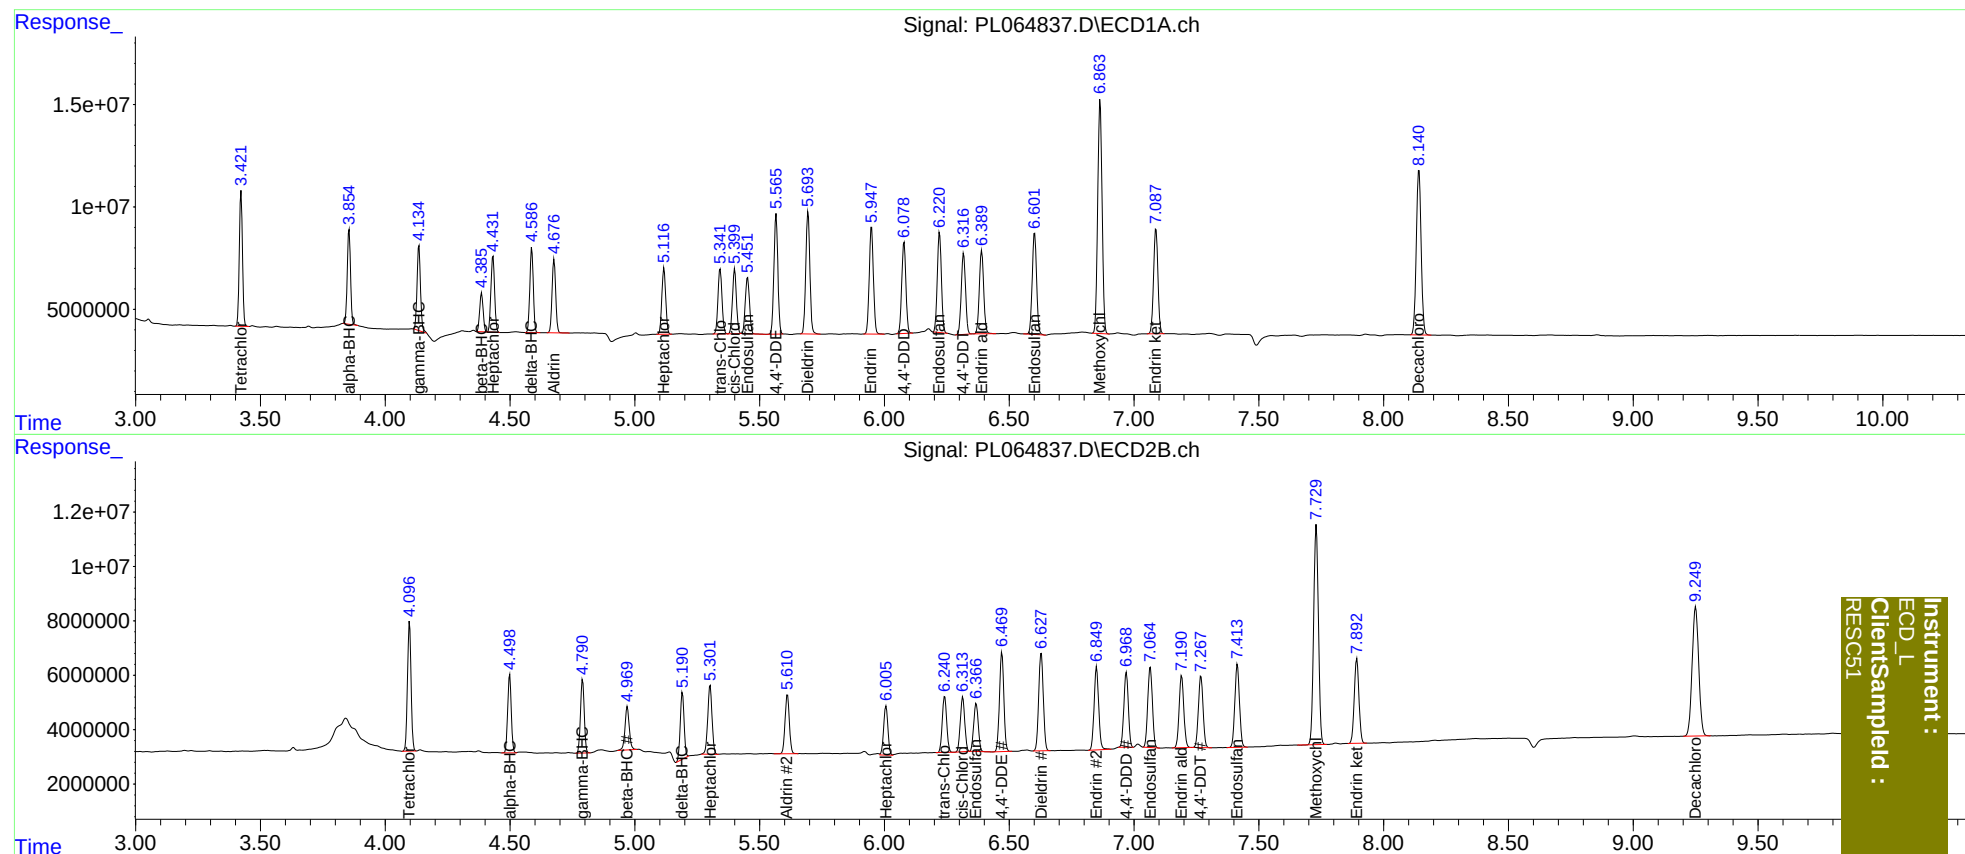

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022121\
Data File : PL064837.D
Acq On : 21 Feb 2021 11:57
Operator : AR\AJ
Sample : RESC51
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
RESC51

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e

Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022121CLP.M
Title : GC Extractables
Last Update : Mon Feb 22 03:50:14 2021
Integrator: ChemStation

RT#1	RT#2	Resolution
3.423	3.856	100.00%
3.856	4.136	100.00%
4.136	4.387	100.00%
4.387	4.432	100.00%
4.432	4.588	100.00%
4.588	4.677	100.00%
4.677	5.117	100.00%
5.117	5.342	100.00%
5.342	5.400	100.00%
5.400	5.452	100.00%
5.452	5.566	100.00%
5.566	5.694	100.00%
5.694	5.948	100.00%
5.948	6.079	100.00%
6.079	6.221	100.00%
6.221	6.318	100.00%
6.318	6.390	100.00%
6.390	6.602	100.00%
6.602	6.864	100.00%
6.864	7.088	100.00%
7.088	8.142	100.00%

Signal #2

4.098	4.499	100.00%
4.499	4.791	100.00%
4.791	4.970	100.00%
4.970	5.191	100.00%
5.191	5.302	100.00%
5.302	5.612	100.00%
5.612	6.007	100.00%
6.007	6.242	100.00%
6.242	6.314	100.00%
6.314	6.368	100.00%
6.368	6.471	100.00%
6.471	6.629	100.00%
6.629	6.850	100.00%
6.850	6.969	100.00%
6.969	7.065	100.00%
7.065	7.191	100.00%
7.191	7.268	100.00%
7.268	7.414	100.00%
7.414	7.730	100.00%
7.730	7.893	100.00%
7.893	9.250	100.00%