

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022122\
 Data File : PL072866.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Feb 2022 23:33
 Operator : AR\AJ
 Sample : N1602-12
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 SPLP-LEACHATE-AMENDED-3-COMP

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 02/22/2022
 Supervised By : Ankita Jodhani 02/22/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 22 02:35:18 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL020722.M
 Quant Title : GC Extractables
 QLast Update : Tue Feb 08 05:14:10 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.551	5.489	10133454	37081864	21.045	21.467
28) SA Decachlor...	10.309	11.377	16266092	36500443	21.486m	23.017

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022122\
Data File : PL072866.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Feb 2022 23:33
Operator : AR\AJ
Sample : N1602-12
Misc :
ALS Vial : 34 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
SPLP-LEACHATE-AMENDED-3-COMP


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 02/22/2022
Supervised By : Ankita Jodhani 02/22/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 22 02:35:18 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL020722.M
Quant Title : GC Extractables
QLast Update : Tue Feb 08 05:14:10 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

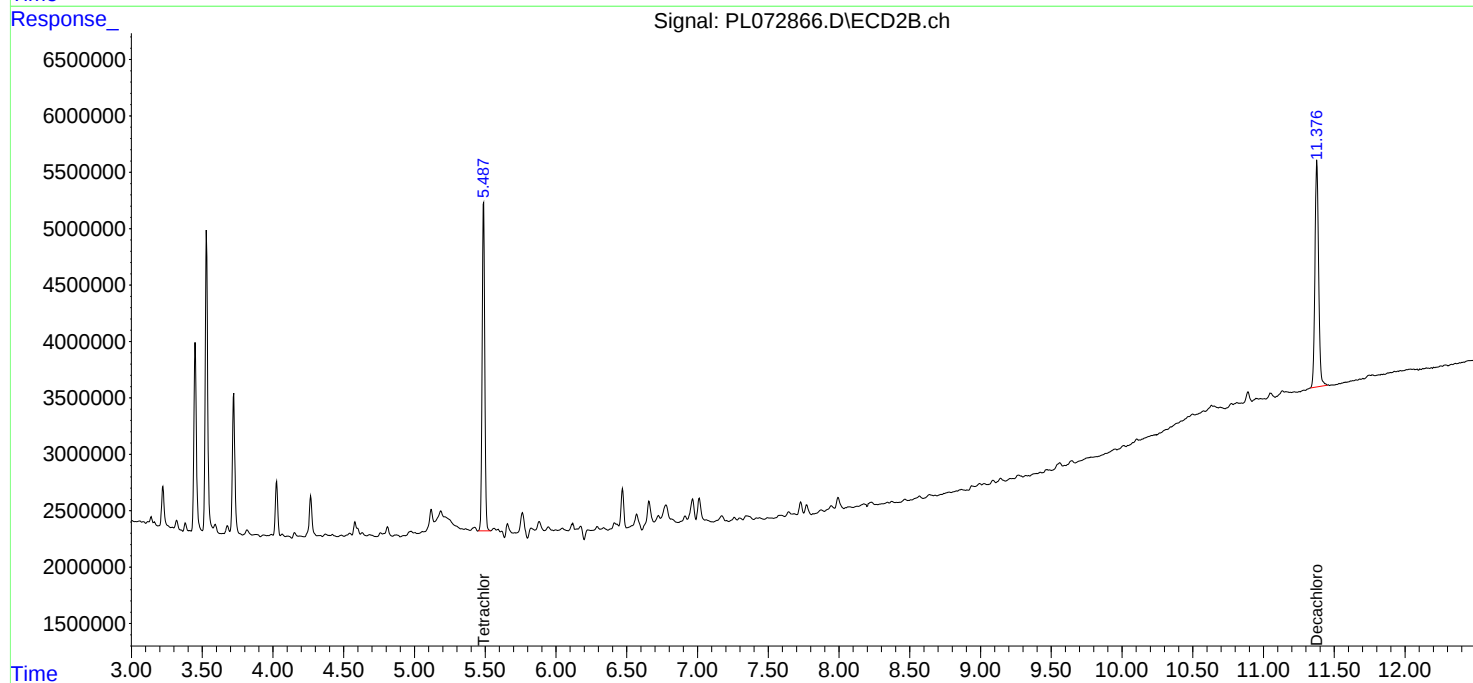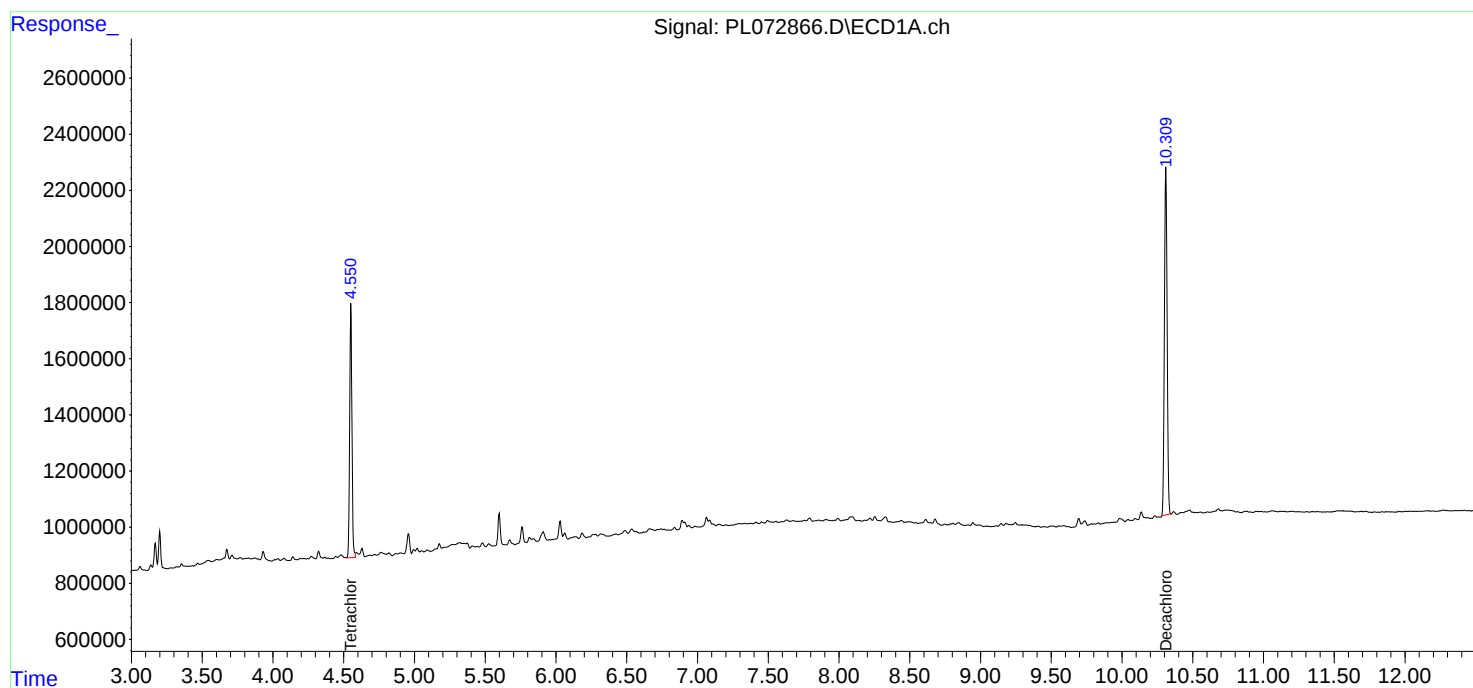

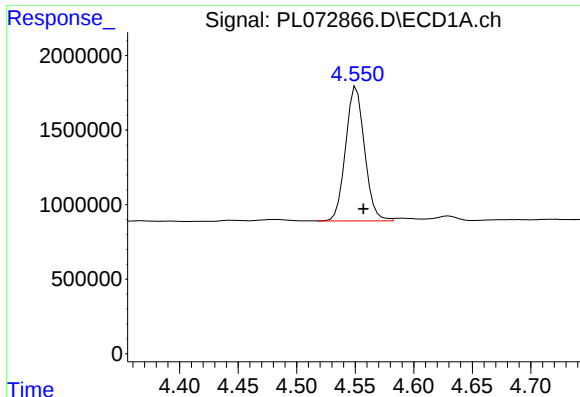


#1 Tetrachloro-m-xylene

R.T.: 4.551 min
Delta R.T.: -0.006 min
Response: 10133454
Conc: 21.05 ng/ml

Instrument :
ECD_L
ClientSampleId :
SPLP-LEACHATE-AMENDED-3-COMP


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 02/22/2022
Supervised By :Ankita Jodhani 02/22/2022

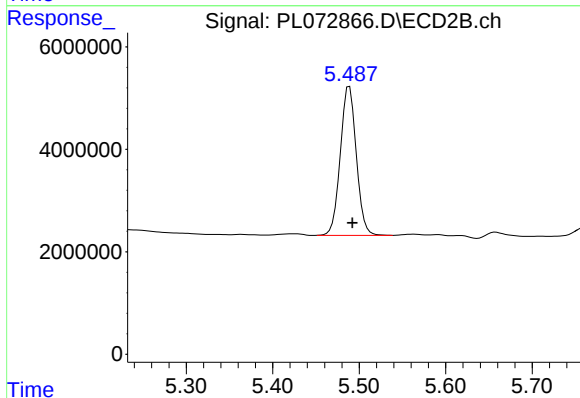


#1 Tetrachloro-m-xylene

R.T.: 5.489 min
Delta R.T.: -0.003 min
Response: 37081864
Conc: 21.47 ng/ml

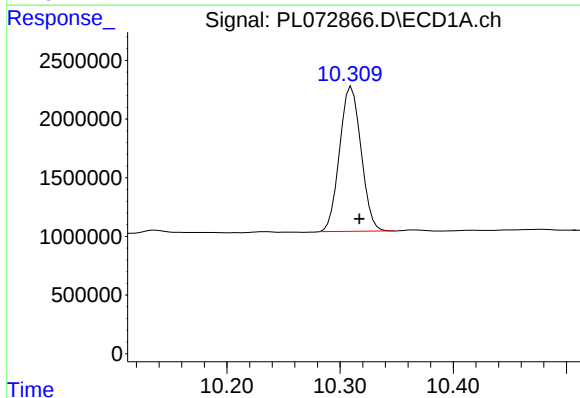

#28 Decachlorobiphenyl

R.T.: 10.309 min
Delta R.T.: -0.008 min
Response: 16266092
Conc: 21.49 ng/ml m

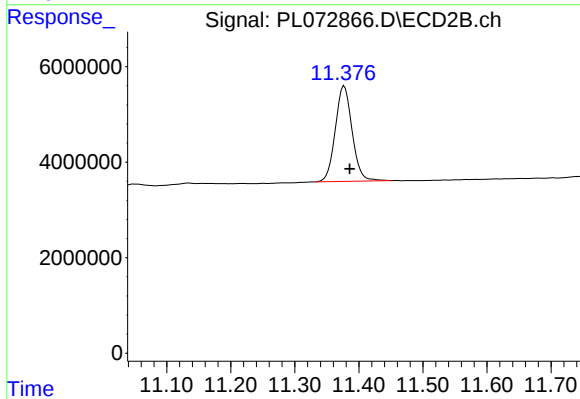

#28 Decachlorobiphenyl

R.T.: 11.377 min
Delta R.T.: -0.009 min
Response: 36500443
Conc: 23.02 ng/ml