

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022123\
 Data File : PL081065.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Feb 2023 10:52
 Operator : AR\AJ
 Sample : PB150915BS
 Misc : CHLOR,BS
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PB150915BS

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 22 03:40:53 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022023.M
 Quant Title : GC Extractables
 QLast Update : Mon Feb 20 18:06:39 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.354	2.685	45080005	52106032	19.339	22.643
28)	SA Decachlor...	8.792	7.833	39055651	47314208	19.976	20.197
Target Compounds							
23)	Chlordane-1	4.501	3.682	18420418	15679729	202.906	192.325
24)	Chlordane-2	5.028	4.259	21910907	18228873	215.454	200.545
25)	Chlordane-3	5.733	4.889	76498249	49681293	201.282	189.065
26)	Chlordane-4	5.815	4.951	94436325	51496582	203.799	191.926
27)	Chlordane-5	6.657	5.619	15808536	15496991	204.469	201.254



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022123\
Data File : PL081065.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Feb 2023 10:52
Operator : AR\AJ
Sample : PB150915BS
Misc : CHLOR,BS
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PB150915BS

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 22 03:40:53 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022023.M
Quant Title : GC Extractables
QLast Update : Mon Feb 20 18:06:39 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

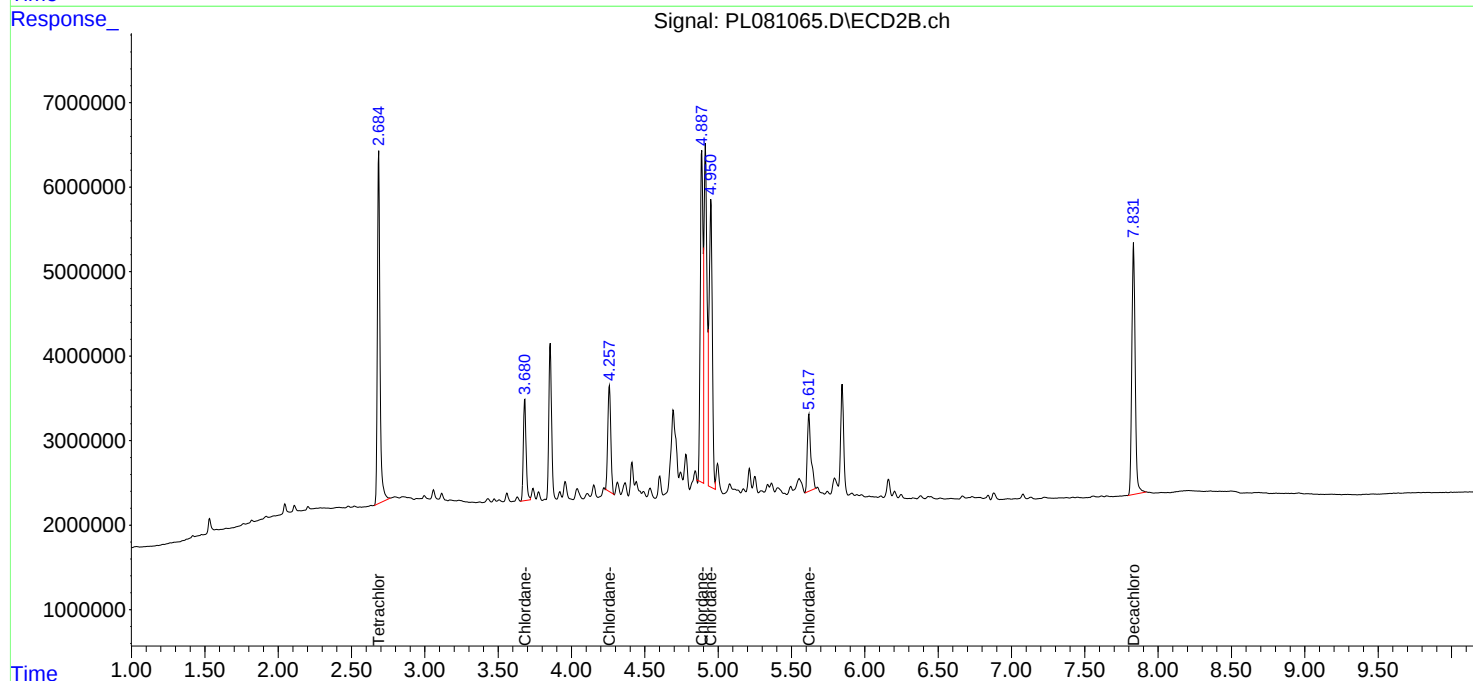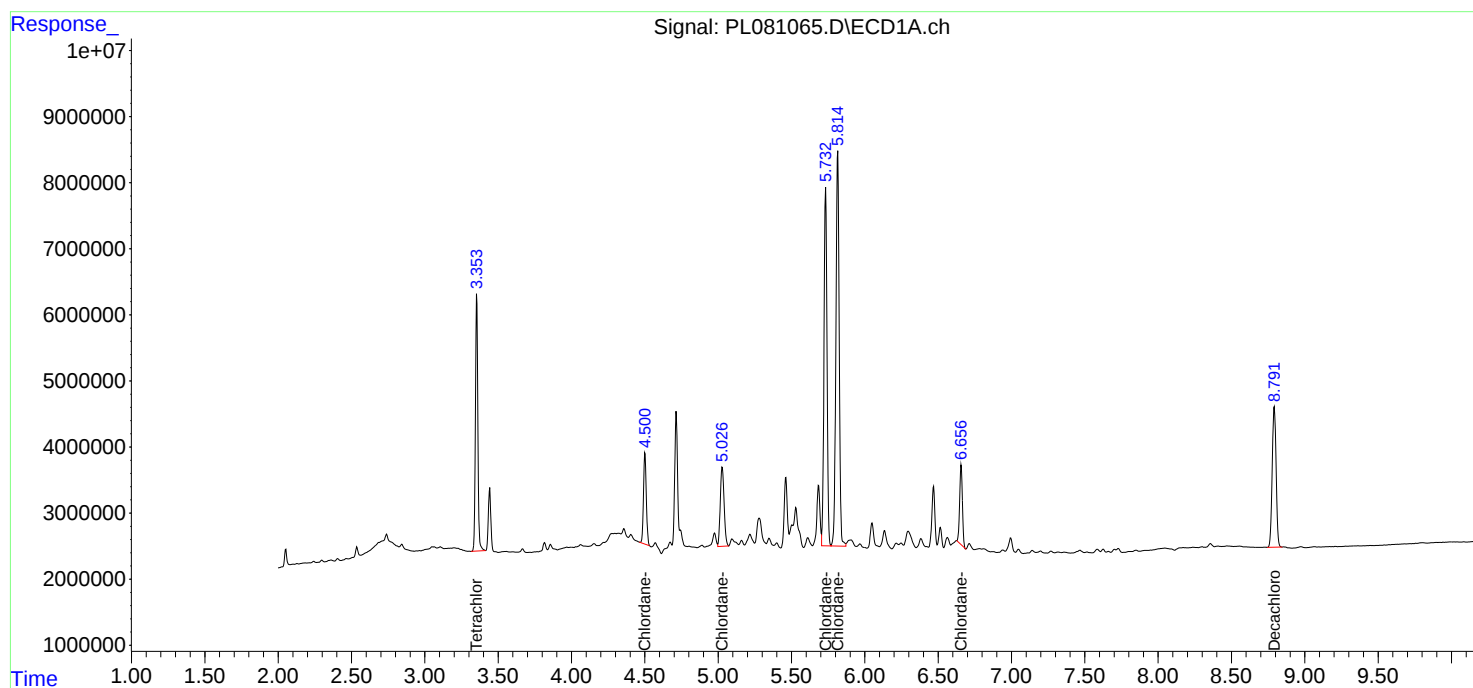


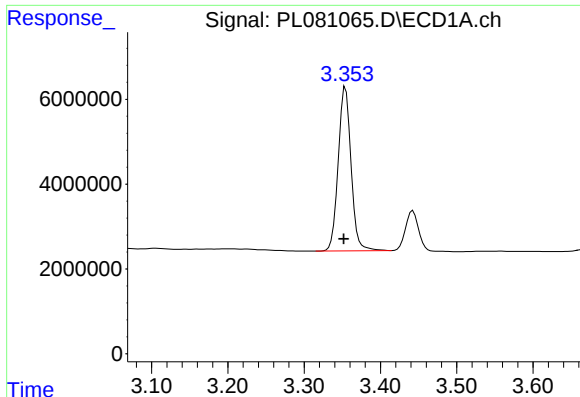

#1 Tetrachloro-m-xylene


R.T.: 3.354 min
Delta R.T.: 0.002 min
Response: 45080005
Conc: 19.34 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB150915BS

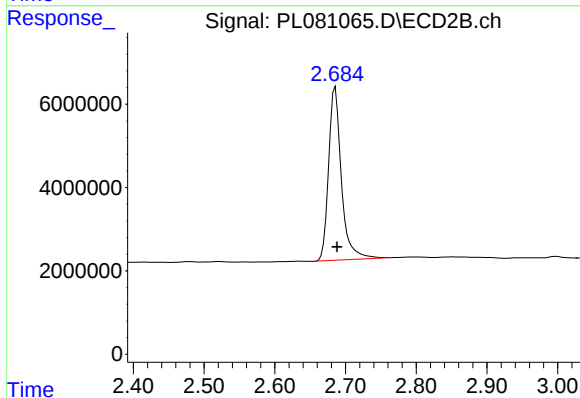


#1 Tetrachloro-m-xylene

R.T.: 2.685 min
Delta R.T.: -0.002 min
Response: 52106032
Conc: 22.64 ng/ml

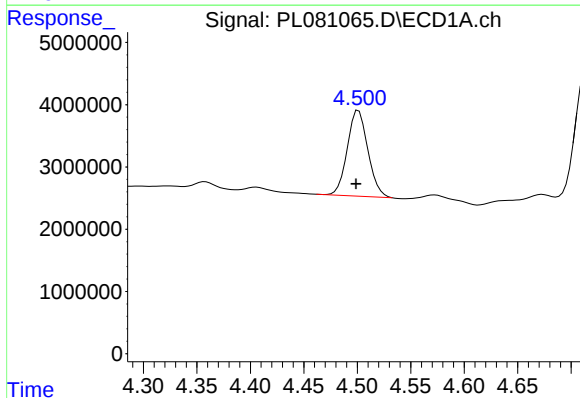


#23 Chlordane-1

R.T.: 4.501 min
Delta R.T.: 0.002 min
Response: 18420418
Conc: 202.91 ng/ml

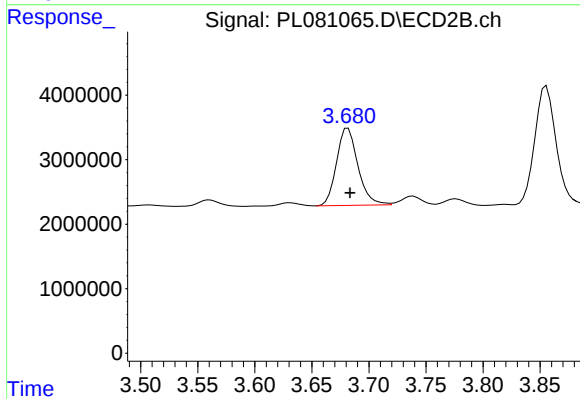

#23 Chlordane-1


R.T.: 3.682 min
Delta R.T.: -0.002 min
Response: 15679729
Conc: 192.32 ng/ml

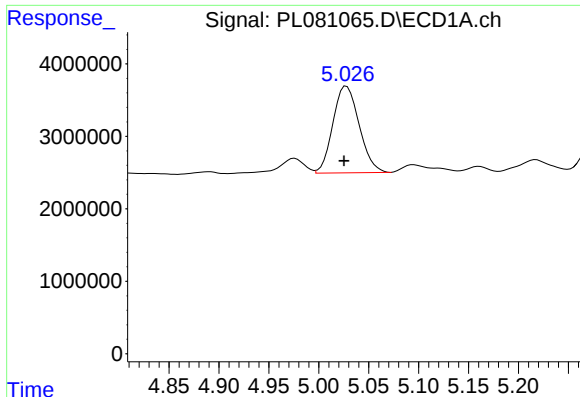

#24 Chlordane-2


R.T.: 5.028 min
Delta R.T.: 0.002 min
Response: 21910907
Conc: 215.45 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB150915BS

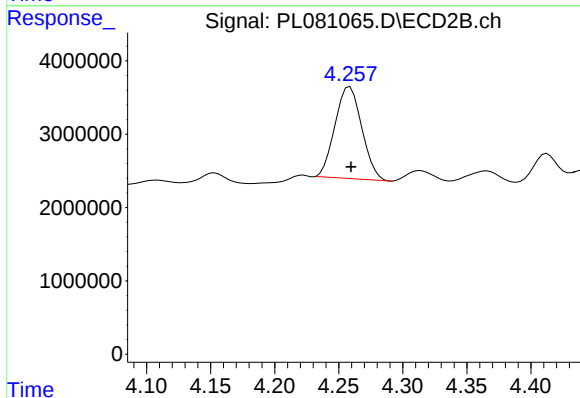


#24 Chlordane-2

R.T.: 4.259 min
Delta R.T.: 0.000 min
Response: 18228873
Conc: 200.54 ng/ml

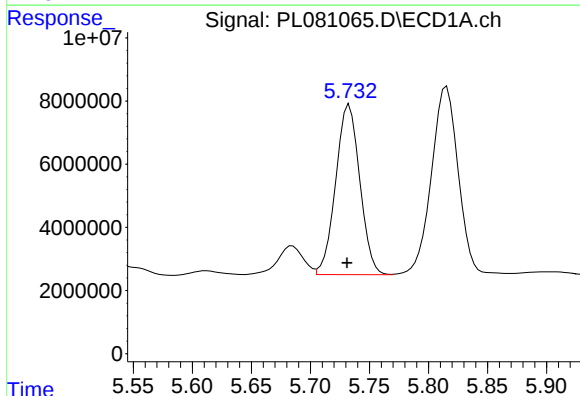


#25 Chlordane-3

R.T.: 5.733 min
Delta R.T.: 0.002 min
Response: 76498249
Conc: 201.28 ng/ml

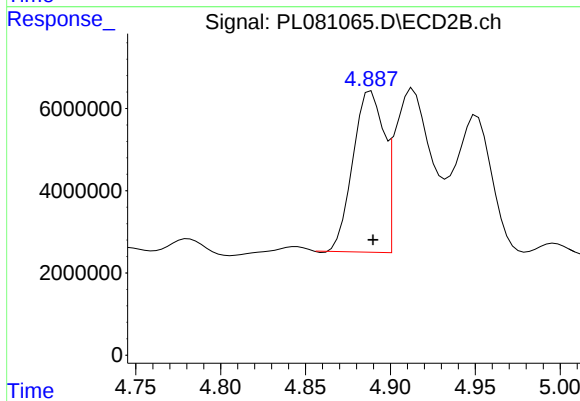

#25 Chlordane-3


R.T.: 4.889 min
Delta R.T.: -0.001 min
Response: 49681293
Conc: 189.07 ng/ml

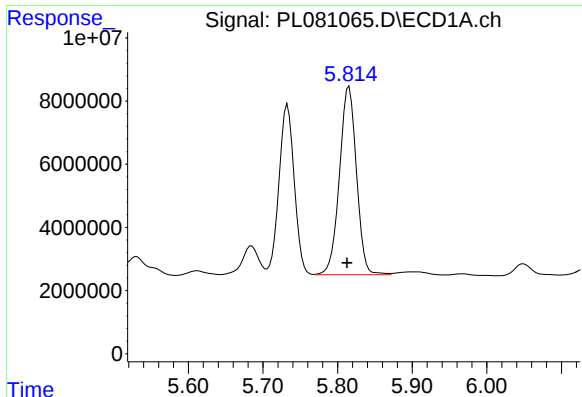

#26 Chlordane-4


R.T.: 5.815 min
Delta R.T.: 0.003 min
Response: 94436325
Conc: 203.80 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB150915BS

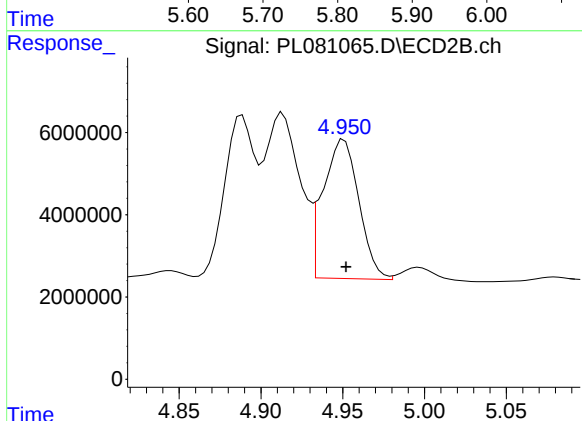


#26 Chlordane-4

R.T.: 4.951 min
Delta R.T.: -0.001 min
Response: 51496582
Conc: 191.93 ng/ml

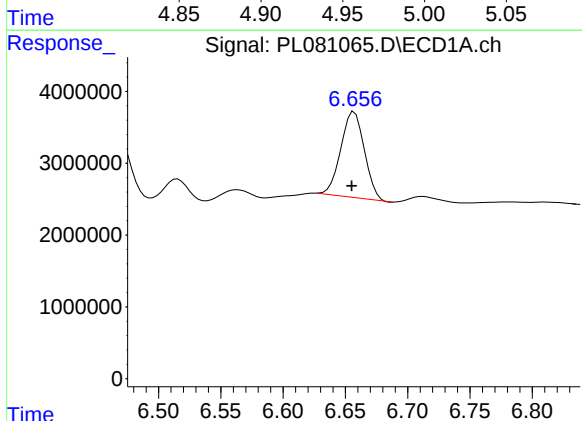


#27 Chlordane-5

R.T.: 6.657 min
Delta R.T.: 0.002 min
Response: 15808536
Conc: 204.47 ng/ml

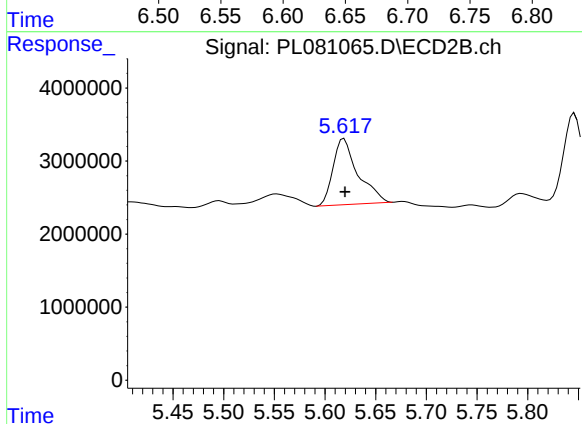

#27 Chlordane-5


R.T.: 5.619 min
Delta R.T.: 0.000 min
Response: 15496991
Conc: 201.25 ng/ml

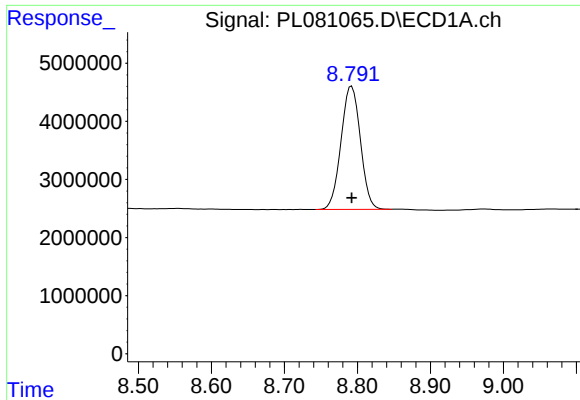

#28 Decachlorobiphenyl

R.T.: 8.792 min
Delta R.T.: 0.000 min
Response: 39055651
Conc: 19.98 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB150915BS

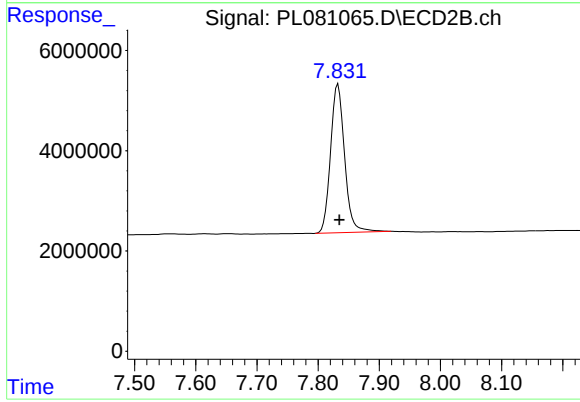

#28 Decachlorobiphenyl

R.T.: 7.833 min
Delta R.T.: -0.002 min
Response: 47314208
Conc: 20.20 ng/ml