

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022125\
 Data File : PL094335.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Feb 2025 12:59
 Operator : AR\AJ
 Sample : PCHLORICC050
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 21 13:17:05 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022125.M
 Quant Title : GC Extractables
 QLast Update : Fri Feb 21 13:07:33 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.535	2.769	13511945	19206372	5.439	5.018
28)	SA Decachlor...	9.047	7.903	12515192	21765591	5.876	5.587
Target Compounds							
23)	Chlordane-1	4.696	3.765	7124050	7218119	56.966	53.147
24)	Chlordane-2	5.226	4.343	7191227	8938123	57.342	56.687
25)	Chlordane-3	5.935	4.971	25920643	24761347	59.199	52.121
26)	Chlordane-4	6.016	5.034	32071300	24554628	60.508	52.238
27)	Chlordane-5	6.866	5.929	5280748	8294395	53.417	50.660



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022125\
Data File : PL094335.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Feb 2025 12:59
Operator : AR\AJ
Sample : PCHLORICC050
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 21 13:17:05 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022125.M
Quant Title : GC Extractables
QLast Update : Fri Feb 21 13:07:33 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

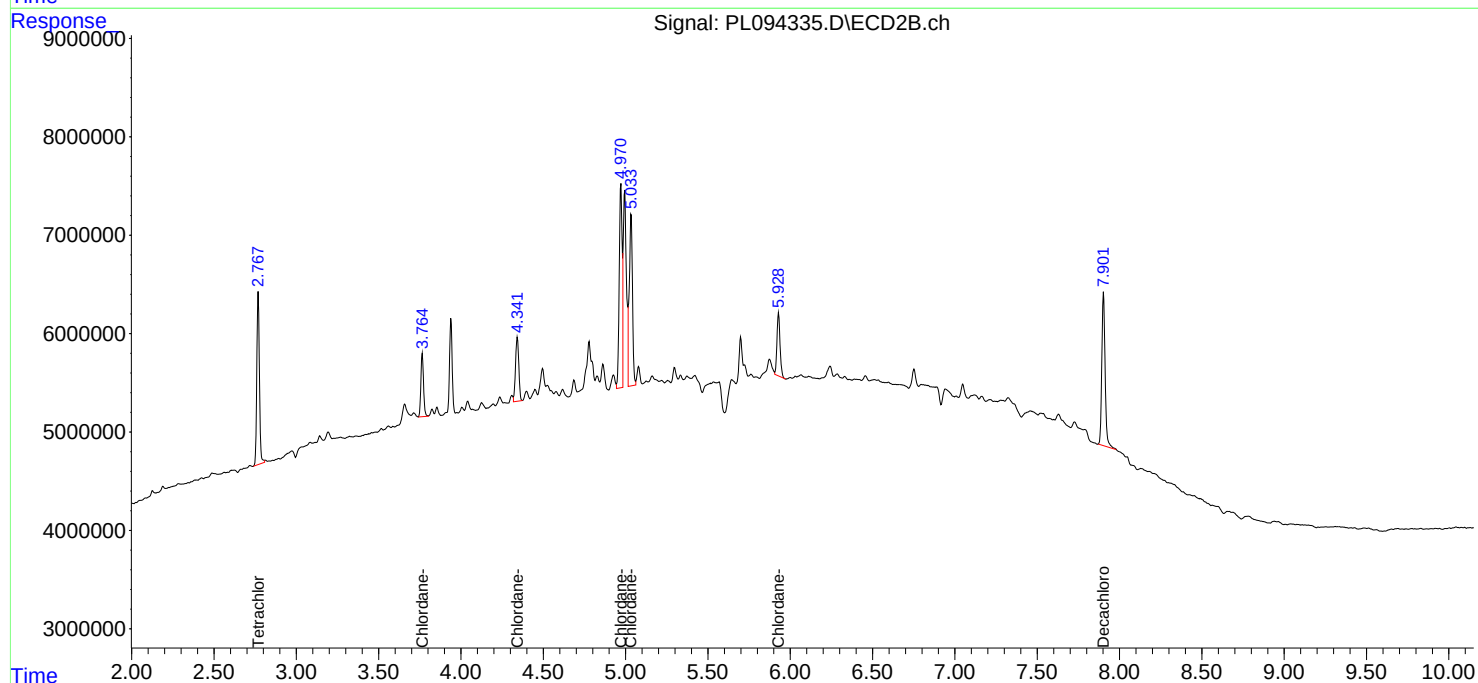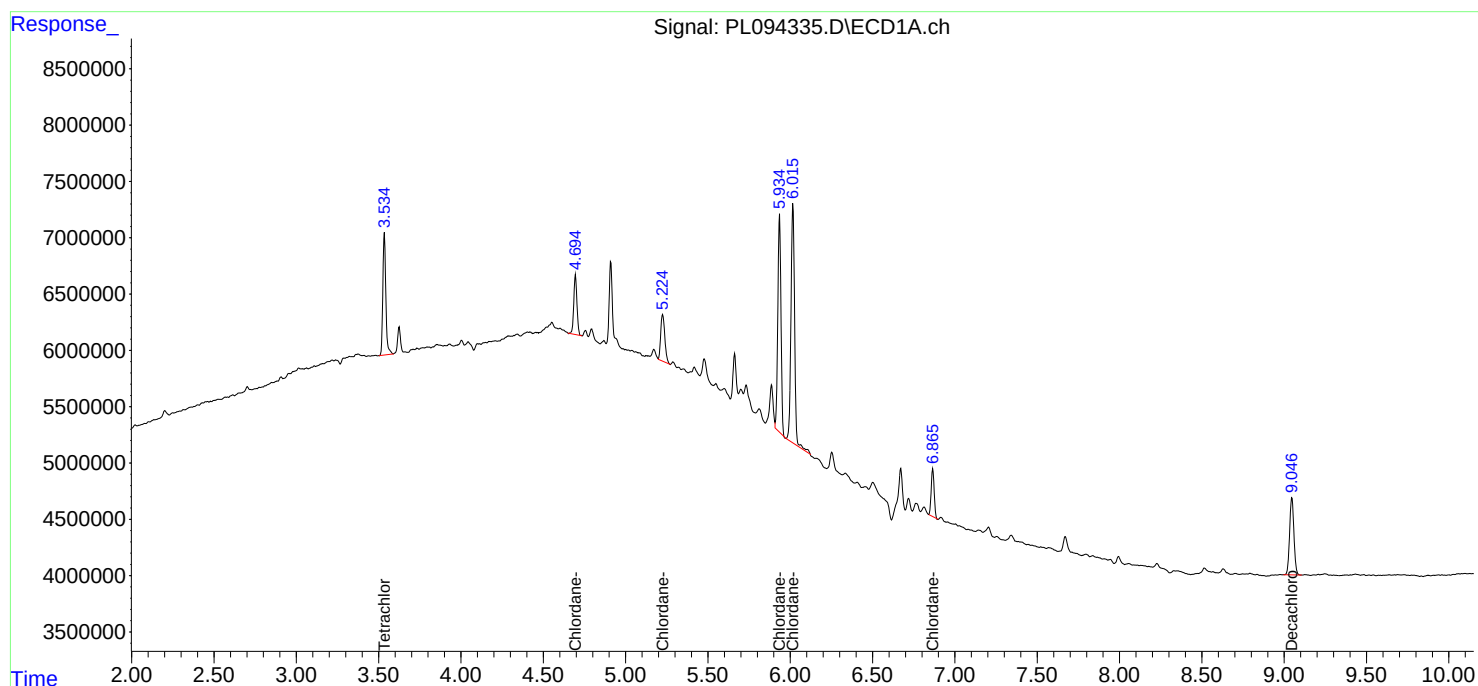


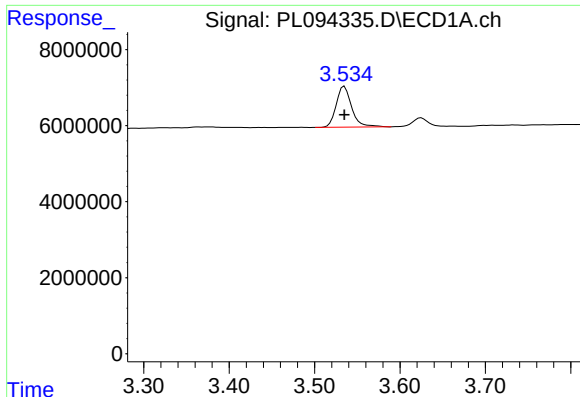

#1 Tetrachloro-m-xylene


R.T.: 3.535 min
Delta R.T.: 0.000 min
Response: 13511945
Conc: 5.44 ng/ml

Instrument :
ECD_L
ClientSampleId :

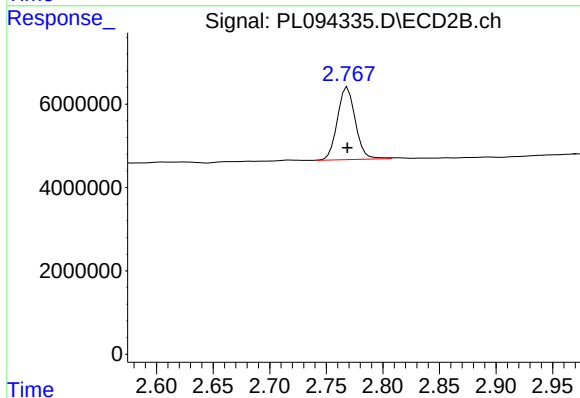


#1 Tetrachloro-m-xylene

R.T.: 2.769 min
Delta R.T.: 0.000 min
Response: 19206372
Conc: 5.02 ng/ml

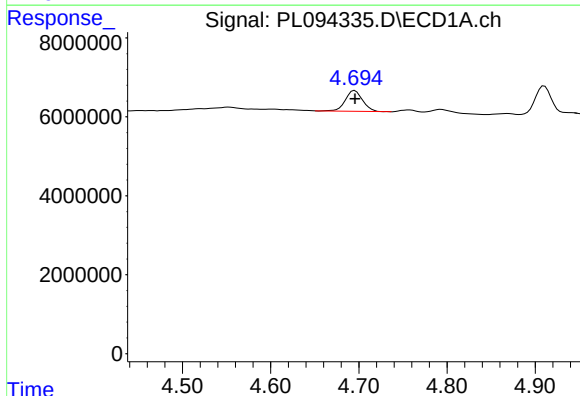


#23 Chlordane-1

R.T.: 4.696 min
Delta R.T.: 0.000 min
Response: 7124050
Conc: 56.97 ng/ml

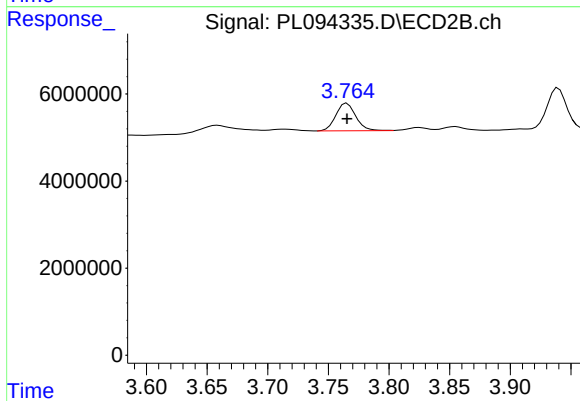

#23 Chlordane-1


R.T.: 3.765 min
Delta R.T.: 0.000 min
Response: 7218119
Conc: 53.15 ng/ml

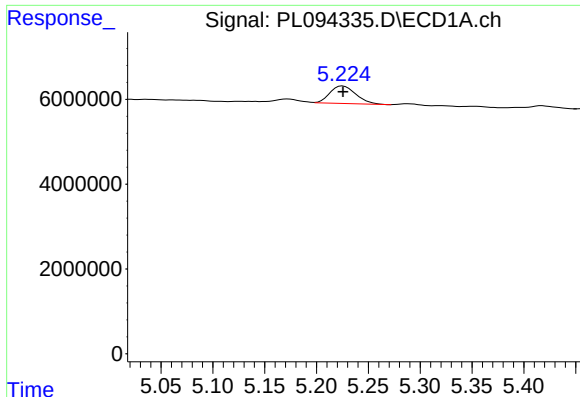

#24 Chlordane-2


R.T.: 5.226 min
Delta R.T.: 0.000 min
Response: 7191227
Conc: 57.34 ng/ml

Instrument :
ECD_L
ClientSampleId :

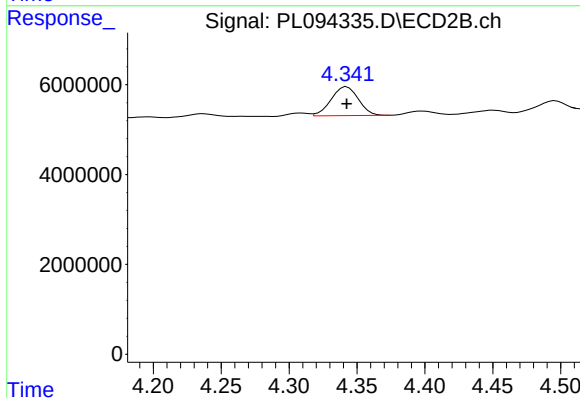


#24 Chlordane-2

R.T.: 4.343 min
Delta R.T.: 0.000 min
Response: 8938123
Conc: 56.69 ng/ml

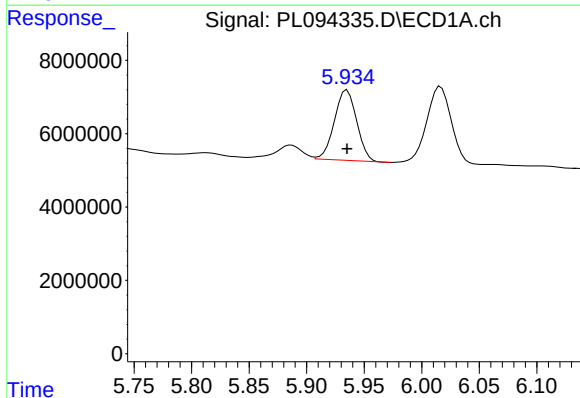


#25 Chlordane-3

R.T.: 5.935 min
Delta R.T.: 0.000 min
Response: 25920643
Conc: 59.20 ng/ml

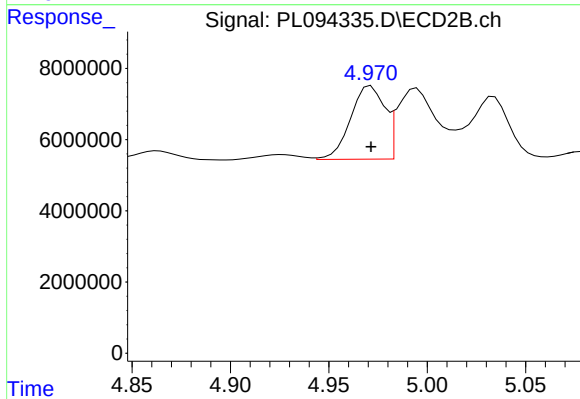

#25 Chlordane-3


R.T.: 4.971 min
Delta R.T.: 0.000 min
Response: 24761347
Conc: 52.12 ng/ml

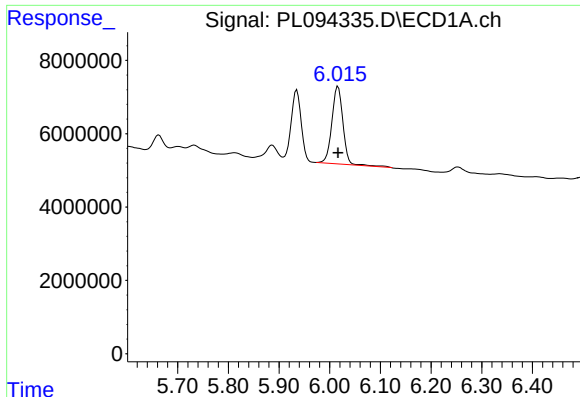

#26 Chlordane-4


R.T.: 6.016 min
Delta R.T.: 0.000 min
Response: 32071300
Conc: 60.51 ng/ml

Instrument :
ECD_L
ClientSampleId :

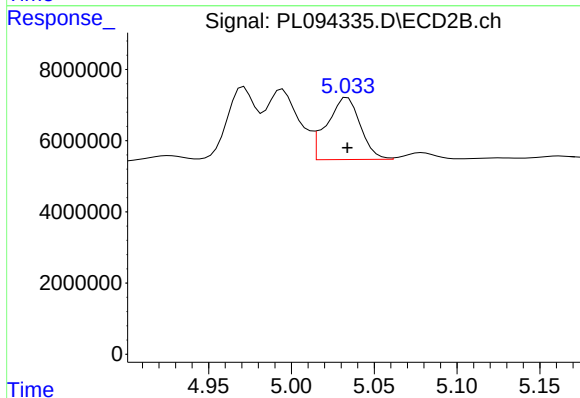


#26 Chlordane-4

R.T.: 5.034 min
Delta R.T.: 0.000 min
Response: 24554628
Conc: 52.24 ng/ml

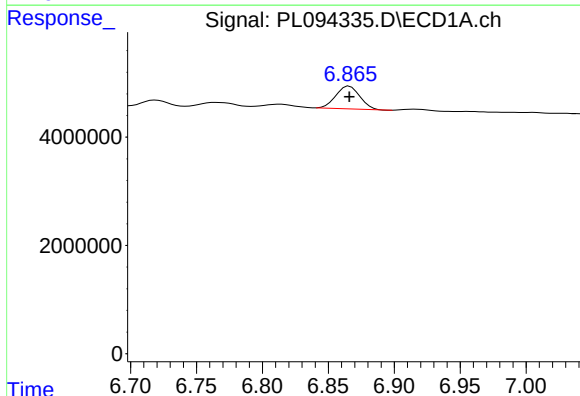


#27 Chlordane-5

R.T.: 6.866 min
Delta R.T.: 0.000 min
Response: 5280748
Conc: 53.42 ng/ml

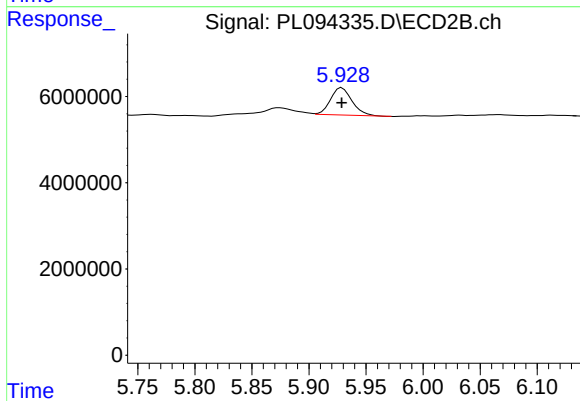

#27 Chlordane-5


R.T.: 5.929 min
Delta R.T.: 0.000 min
Response: 8294395
Conc: 50.66 ng/ml

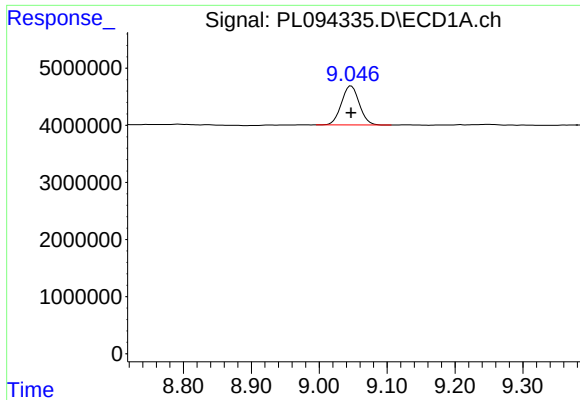

#28 Decachlorobiphenyl

R.T.: 9.047 min
Delta R.T.: 0.000 min
Response: 12515192
Conc: 5.88 ng/ml

Instrument :
ECD_L
ClientSampleId :

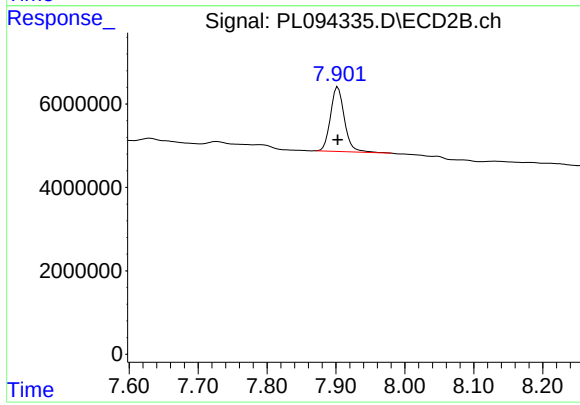

#28 Decachlorobiphenyl

R.T.: 7.903 min
Delta R.T.: 0.000 min
Response: 21765591
Conc: 5.59 ng/ml