

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022125\
 Data File : PL094332.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Feb 2025 12:18
 Operator : AR\AJ
 Sample : PCHLORICC750
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 21 13:13:10 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022125.M
 Quant Title : GC Extractables
 QLast Update : Fri Feb 21 13:07:33 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.536	2.770	178.4E6	284.2E6	73.665	73.722
28)	SA Decachlor...	9.048	7.904	147.8E6	278.4E6	74.122	74.212
Target Compounds							
23)	Chlordane-1	4.697	3.766	88202803	98915911	738.051	737.902
24)	Chlordane-2	5.227	4.342	87621193	111.5E6	736.762	737.660
25)	Chlordane-3	5.937	4.972	305.5E6	346.8E6	739.667	734.870
26)	Chlordane-4	6.018	5.035	366.0E6	343.3E6	738.316	730.399
27)	Chlordane-5	6.867	5.929	71018139	121.5E6	742.412	739.548



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022125\
Data File : PL094332.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Feb 2025 12:18
Operator : AR\AJ
Sample : PCHLORICC750
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 21 13:13:10 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022125.M
Quant Title : GC Extractables
QLast Update : Fri Feb 21 13:07:33 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

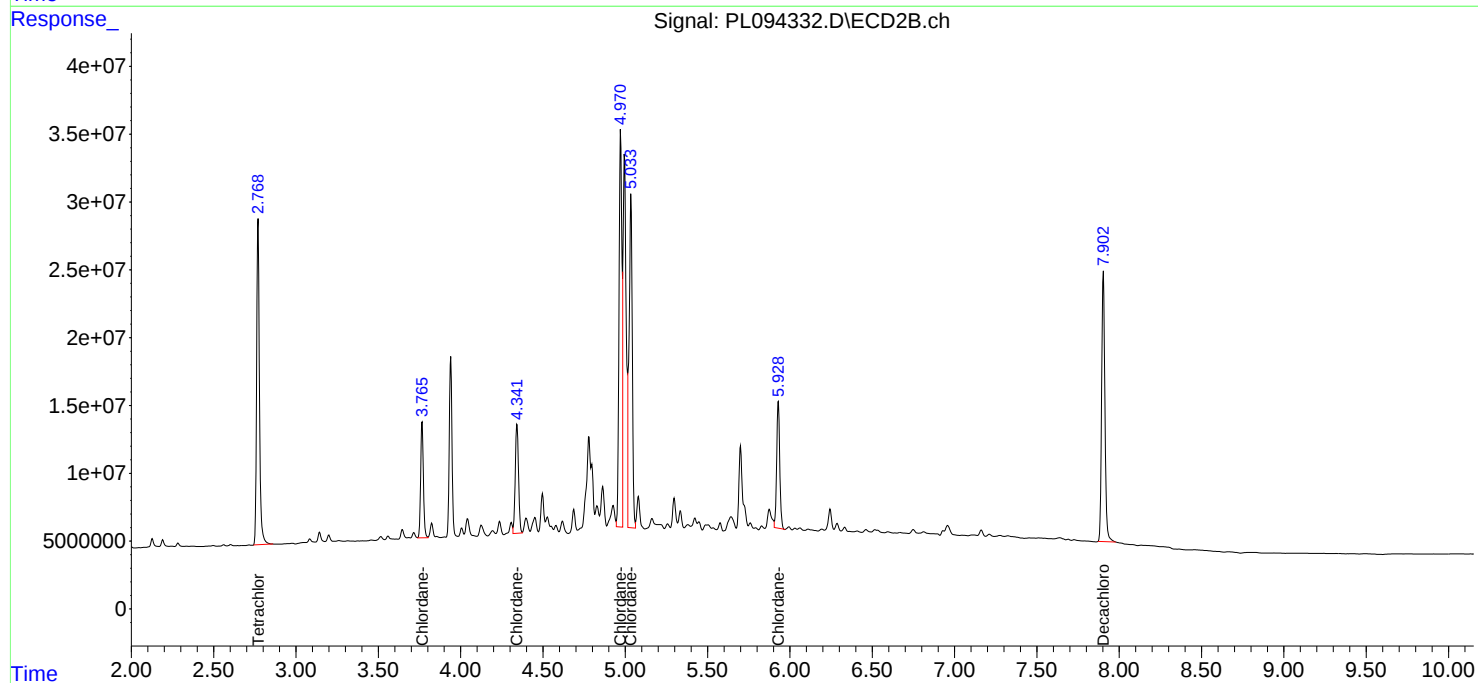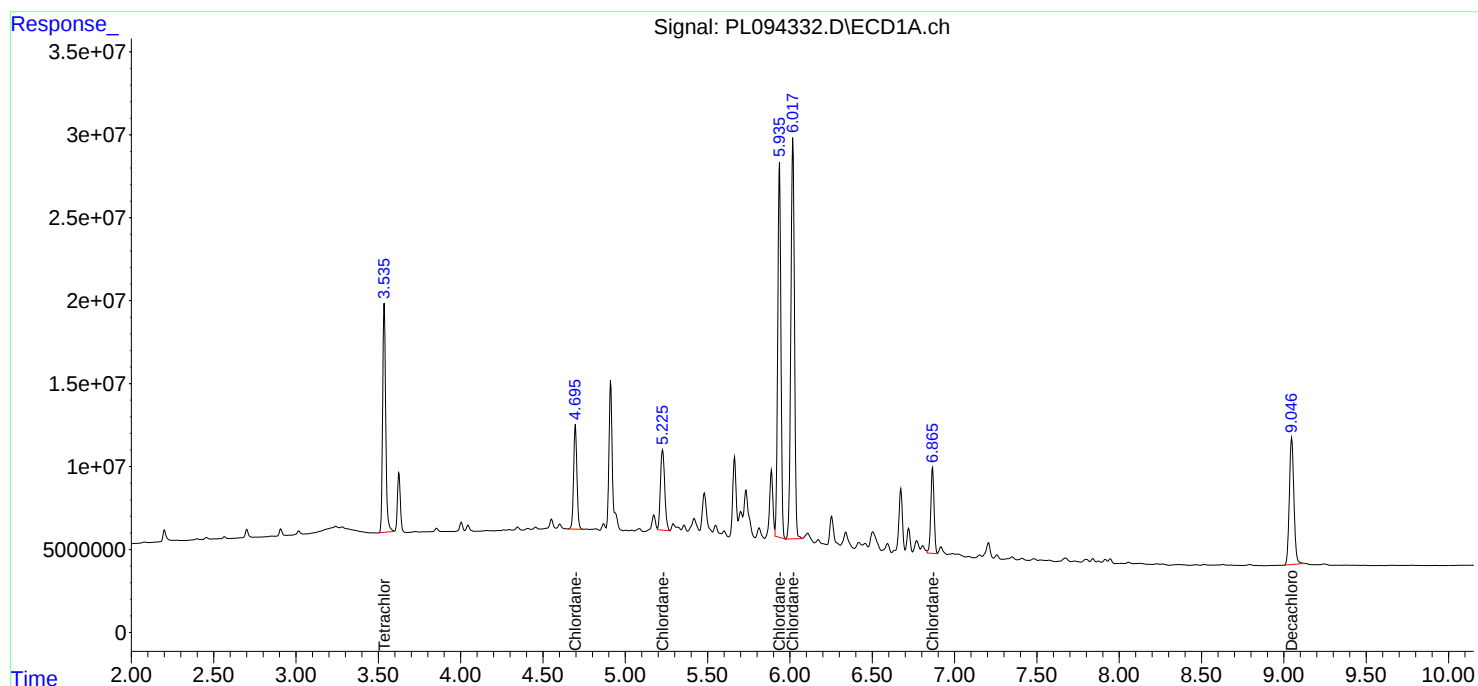


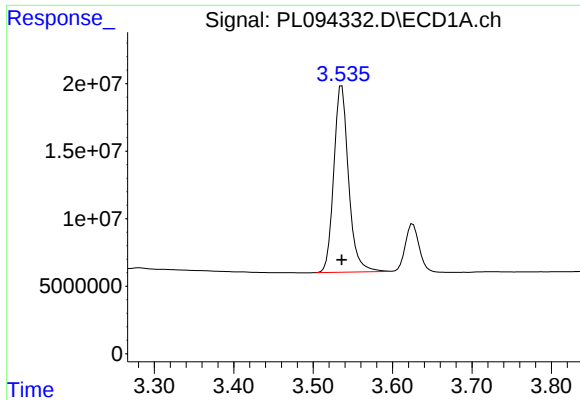

#1 Tetrachloro-m-xylene


R.T.: 3.536 min
Delta R.T.: 0.000 min
Response: 178352872
Conc: 73.66 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

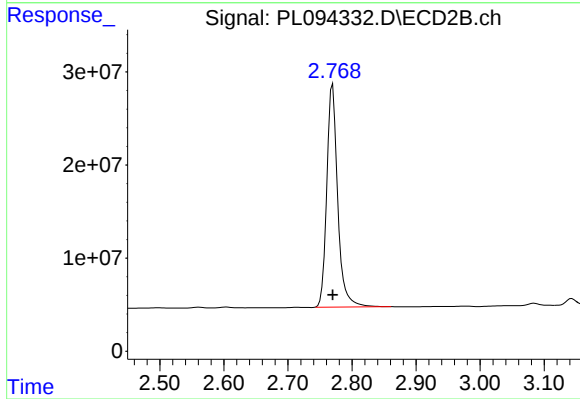


#1 Tetrachloro-m-xylene

R.T.: 2.770 min
Delta R.T.: 0.000 min
Response: 284218464
Conc: 73.72 ng/ml

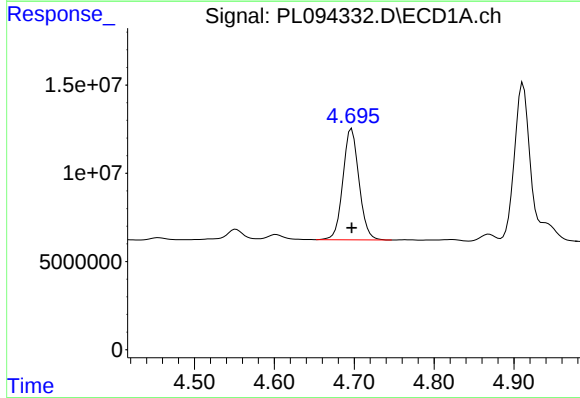


#23 Chlordane-1

R.T.: 4.697 min
Delta R.T.: 0.000 min
Response: 88202803
Conc: 738.05 ng/ml

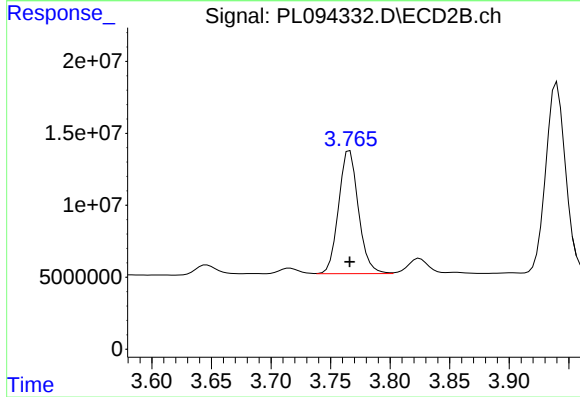

#23 Chlordane-1


R.T.: 3.766 min
Delta R.T.: 0.000 min
Response: 98915911
Conc: 737.90 ng/ml

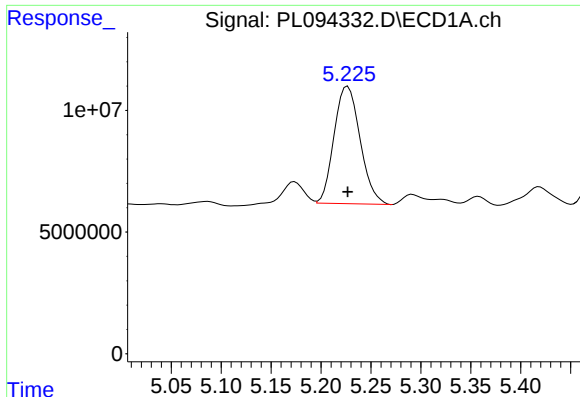

#24 Chlordane-2


R.T.: 5.227 min
Delta R.T.: 0.000 min
Response: 87621193
Conc: 736.76 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

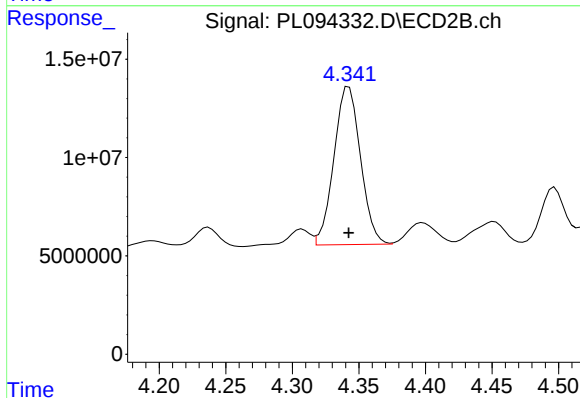


#24 Chlordane-2

R.T.: 4.342 min
Delta R.T.: 0.000 min
Response: 111450063
Conc: 737.66 ng/ml

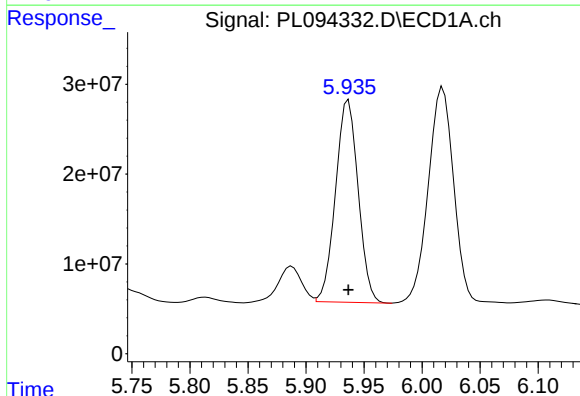


#25 Chlordane-3

R.T.: 5.937 min
Delta R.T.: 0.000 min
Response: 305548347
Conc: 739.67 ng/ml

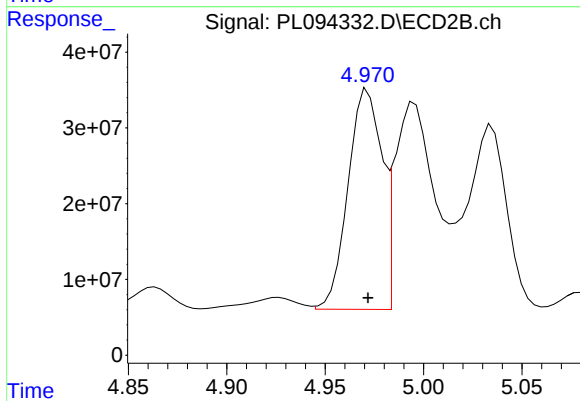

#25 Chlordane-3


R.T.: 4.972 min
Delta R.T.: 0.000 min
Response: 346806789
Conc: 734.87 ng/ml

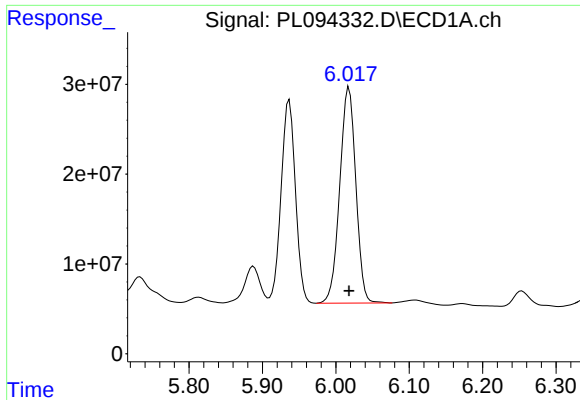

#26 Chlordane-4


R.T.: 6.018 min
Delta R.T.: 0.000 min
Response: 366010828
Conc: 738.32 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

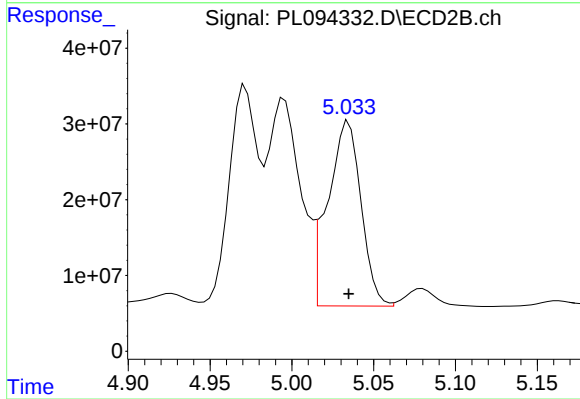


#26 Chlordane-4

R.T.: 5.035 min
Delta R.T.: 0.000 min
Response: 343281182
Conc: 730.40 ng/ml

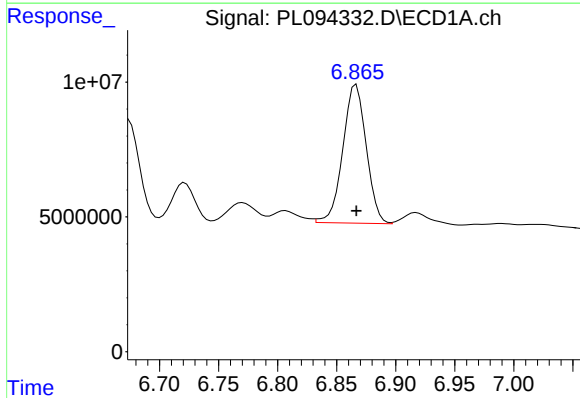


#27 Chlordane-5

R.T.: 6.867 min
Delta R.T.: 0.000 min
Response: 71018139
Conc: 742.41 ng/ml

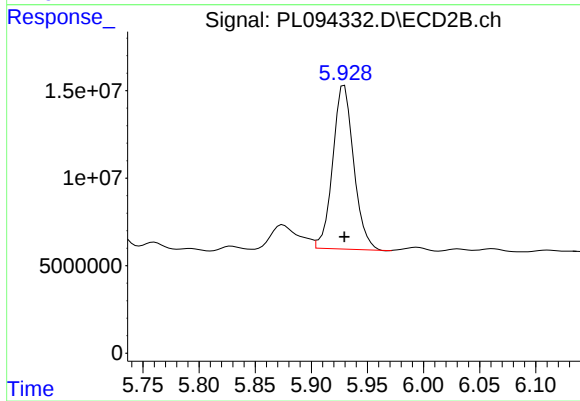

#27 Chlordane-5


R.T.: 5.929 min
Delta R.T.: 0.000 min
Response: 121523395
Conc: 739.55 ng/ml

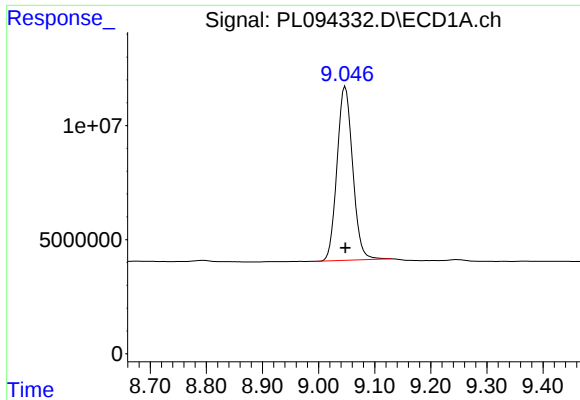

#28 Decachlorobiphenyl

R.T.: 9.048 min
Delta R.T.: 0.000 min
Response: 147805432
Conc: 74.12 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

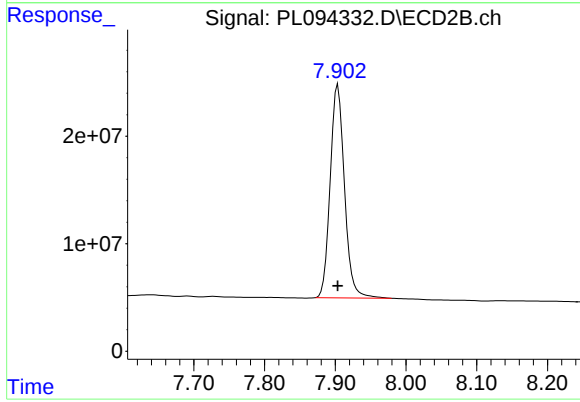

#28 Decachlorobiphenyl

R.T.: 7.904 min
Delta R.T.: 0.000 min
Response: 278394435
Conc: 74.21 ng/ml