

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022125\
 Data File : PL094334.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Feb 2025 12:45
 Operator : AR\AJ
 Sample : PCHLORICC250
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 21 13:15:10 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022125.M
 Quant Title : GC Extractables
 QLast Update : Fri Feb 21 13:07:33 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.535	2.769	61412668	93291989	25.273	24.394
28)	SA Decachlor...	9.049	7.904	54080317	96786740	26.557	25.596
Target Compounds							
23)	Chlordane-1	4.696	3.765	31072121	33139081	257.426	247.905
24)	Chlordane-2	5.226	4.342	31609651	39089932	261.658	256.488
25)	Chlordane-3	5.936	4.972	107.9E6	116.1E6	258.310	246.981
26)	Chlordane-4	6.019	5.035	130.4E6	112.3E6	259.623	241.619
27)	Chlordane-5	6.867	5.930	25426998	39945223	261.673	244.783



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022125\
Data File : PL094334.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Feb 2025 12:45
Operator : AR\AJ
Sample : PCHLORICC250
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 21 13:15:10 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022125.M
Quant Title : GC Extractables
QLast Update : Fri Feb 21 13:07:33 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

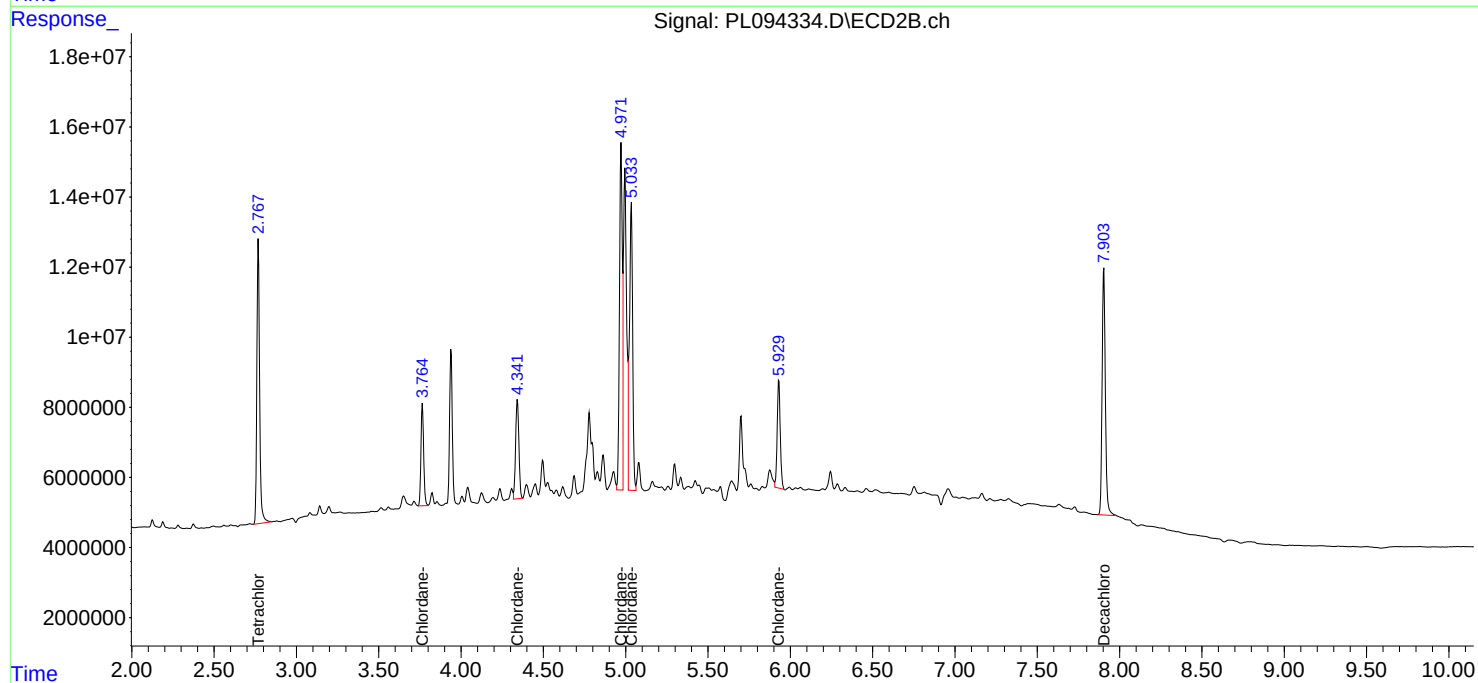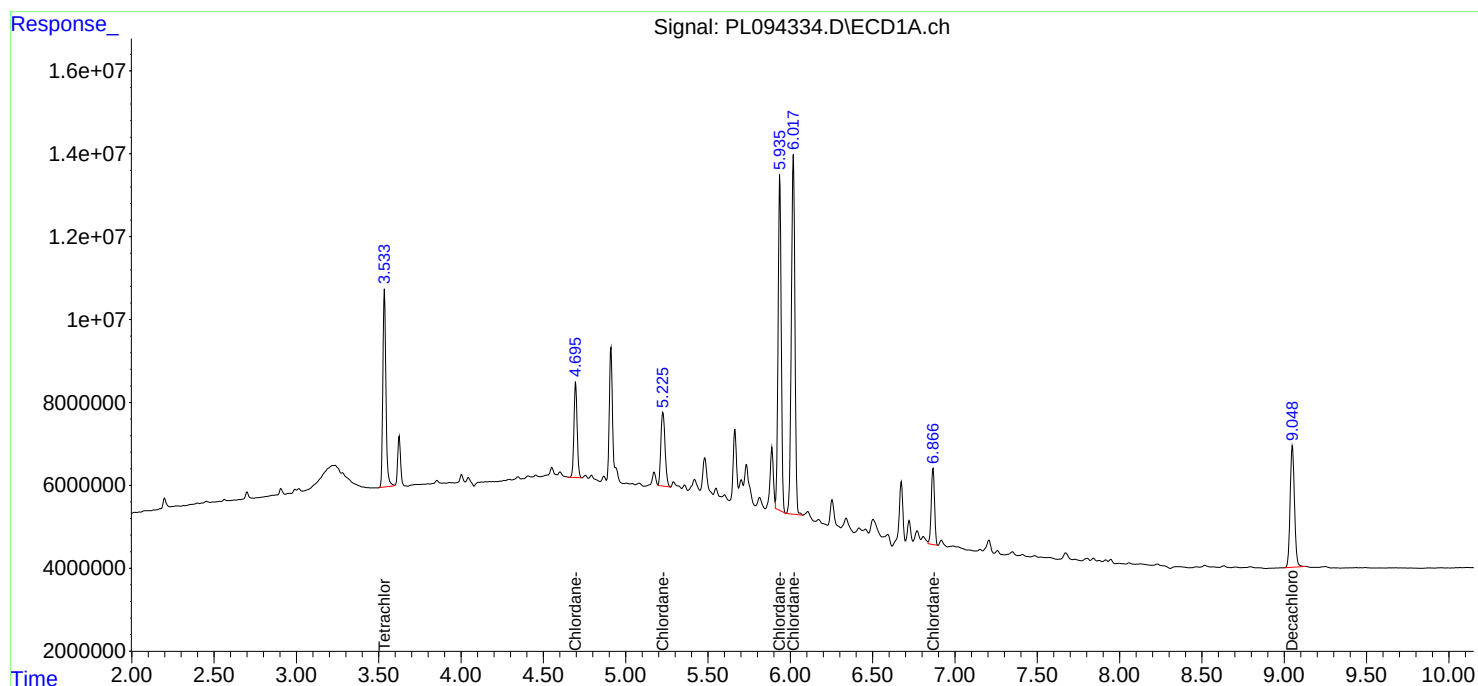


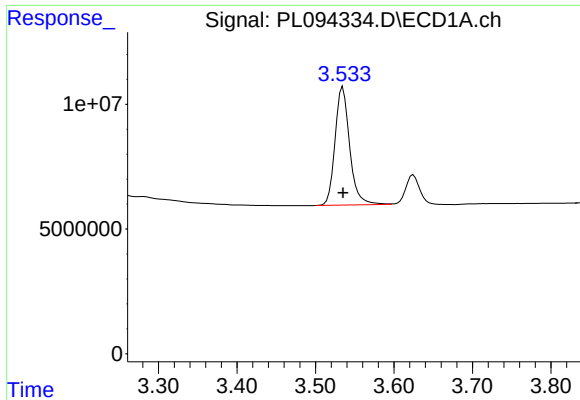

#1 Tetrachloro-m-xylene


R.T.: 3.535 min
Delta R.T.: 0.000 min
Response: 61412668
Conc: 25.27 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

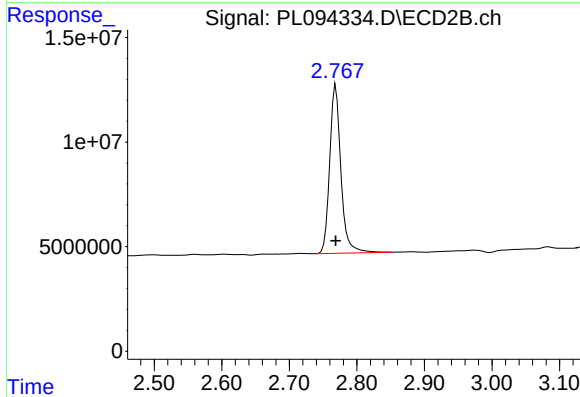


#1 Tetrachloro-m-xylene

R.T.: 2.769 min
Delta R.T.: 0.000 min
Response: 93291989
Conc: 24.39 ng/ml

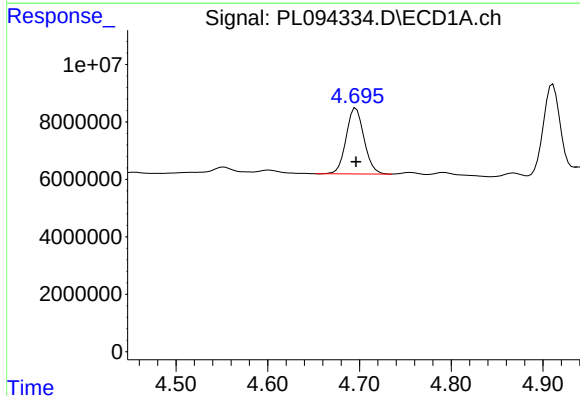


#23 Chlordane-1

R.T.: 4.696 min
Delta R.T.: 0.000 min
Response: 31072121
Conc: 257.43 ng/ml

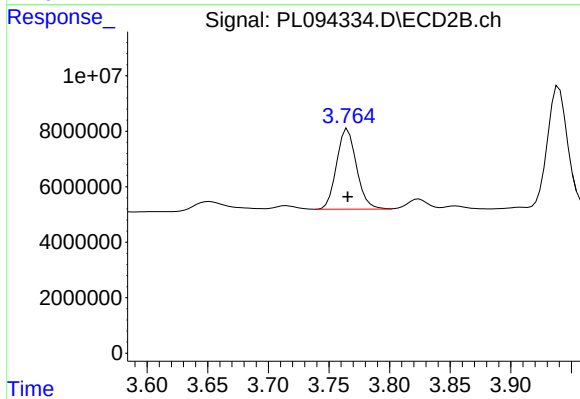

#23 Chlordane-1


R.T.: 3.765 min
Delta R.T.: 0.000 min
Response: 33139081
Conc: 247.90 ng/ml

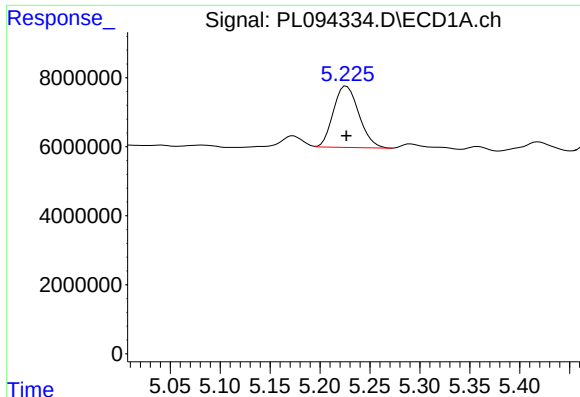

#24 Chlordane-2


R.T.: 5.226 min
Delta R.T.: 0.000 min
Response: 31609651
Conc: 261.66 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

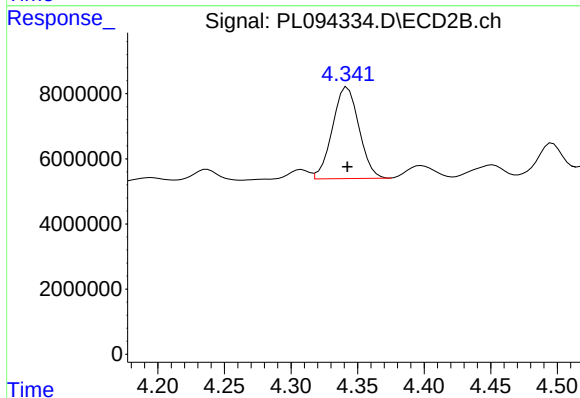


#24 Chlordane-2

R.T.: 4.342 min
Delta R.T.: 0.000 min
Response: 39089932
Conc: 256.49 ng/ml

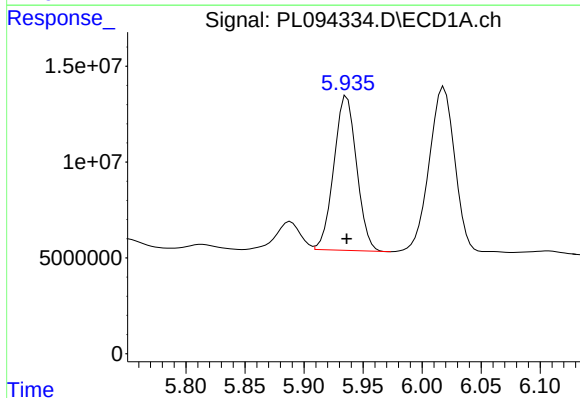


#25 Chlordane-3

R.T.: 5.936 min
Delta R.T.: 0.000 min
Response: 107900871
Conc: 258.31 ng/ml

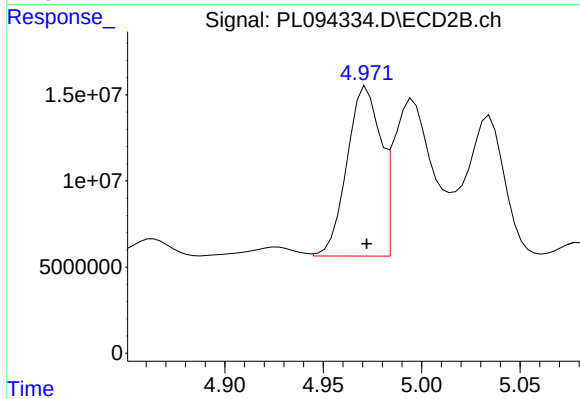

#25 Chlordane-3


R.T.: 4.972 min
Delta R.T.: 0.000 min
Response: 116090462
Conc: 246.98 ng/ml

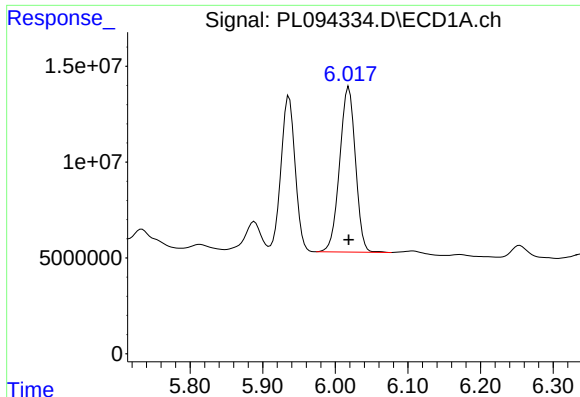

#26 Chlordane-4


R.T.: 6.019 min
Delta R.T.: 0.000 min
Response: 130377884
Conc: 259.62 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

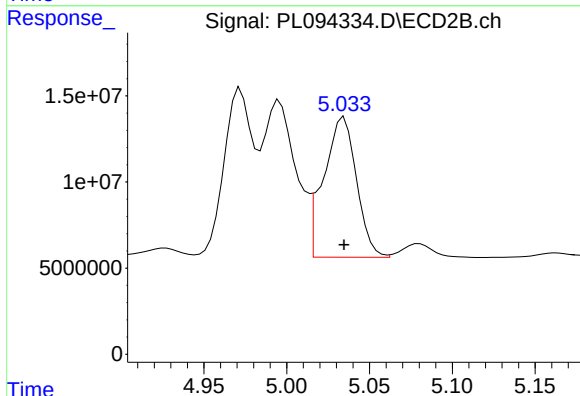


#26 Chlordane-4

R.T.: 5.035 min
Delta R.T.: 0.000 min
Response: 112303671
Conc: 241.62 ng/ml

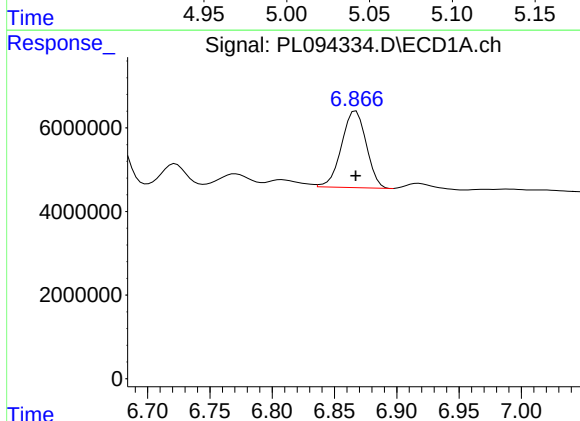


#27 Chlordane-5

R.T.: 6.867 min
Delta R.T.: 0.000 min
Response: 25426998
Conc: 261.67 ng/ml

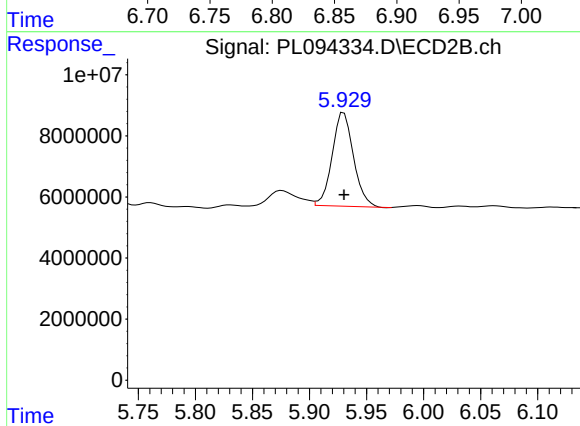

#27 Chlordane-5


R.T.: 5.930 min
Delta R.T.: 0.000 min
Response: 39945223
Conc: 244.78 ng/ml

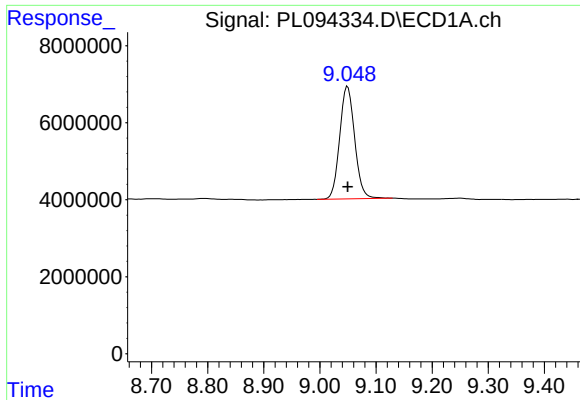

#28 Decachlorobiphenyl

R.T.: 9.049 min
Delta R.T.: 0.000 min
Response: 54080317
Conc: 26.56 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

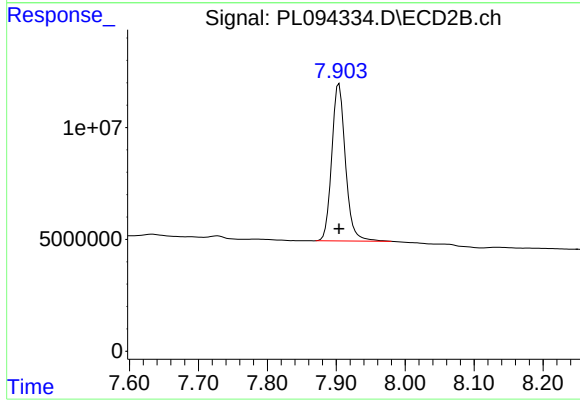

#28 Decachlorobiphenyl

R.T.: 7.904 min
Delta R.T.: 0.000 min
Response: 96786740
Conc: 25.60 ng/ml