

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022125\
 Data File : PL094349.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Feb 2025 16:38
 Operator : AR\AJ
 Sample : Q1395-01
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 BEL-25-0005

Manual Integrations APPROVED

Reviewed By :Abdul
 Mirza

02/22/2025
 Supervised By :Ankita
 Jodhani

02/24/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 22 00:23:00 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022125.M
 Quant Title : GC Extractables
 QLast Update : Fri Feb 21 14:52:19 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.536	2.774	22088035	25951823	8.699m	8.132
28)	SA Decachlor...	9.061	7.920	23026119	30307477	10.824m	7.881 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022125\
Data File : PL094349.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Feb 2025 16:38
Operator : AR\AJ
Sample : Q1395-01
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
BEL-25-0005

Manual Integrations
APPROVED



Reviewed By :Abdul
Mirza


02/22/2025
Supervised By :Ankita
Jodhani

02/24/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 22 00:23:00 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022125.M
Quant Title : GC Extractables
QLast Update : Fri Feb 21 14:52:19 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

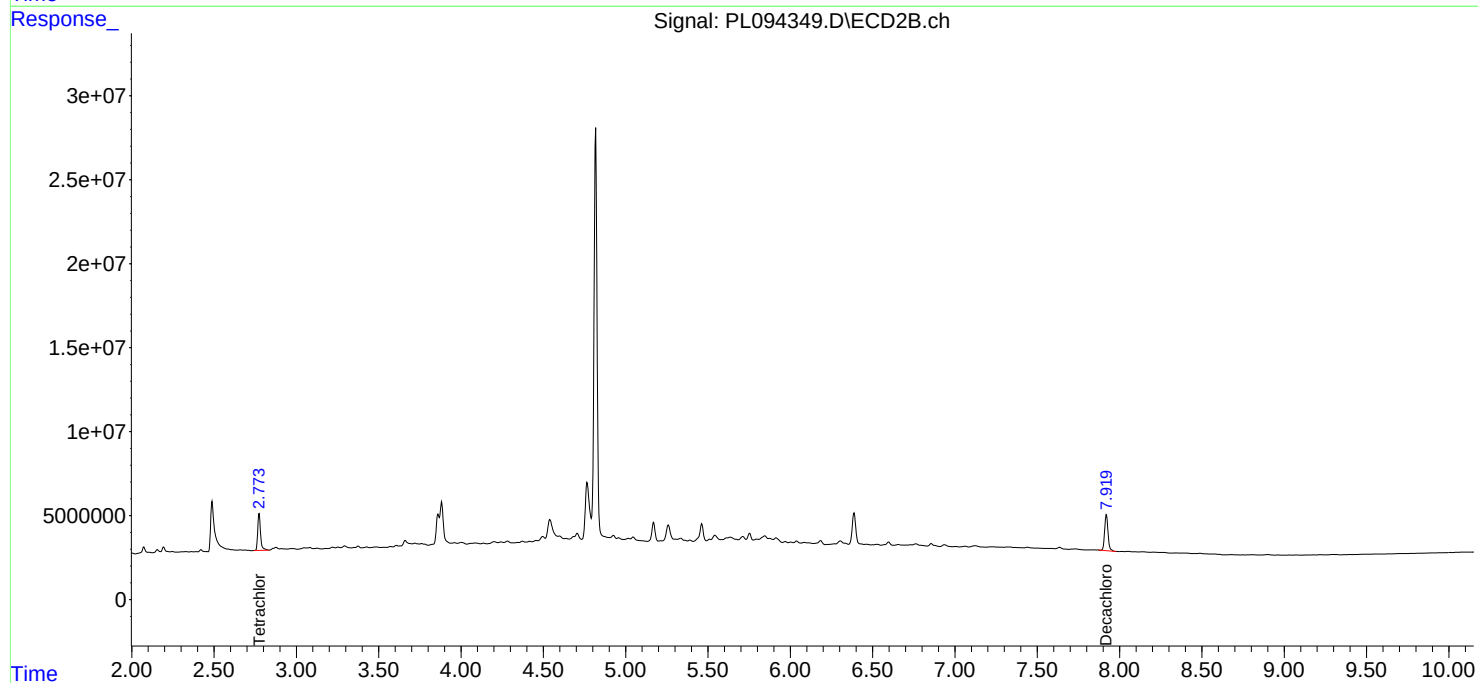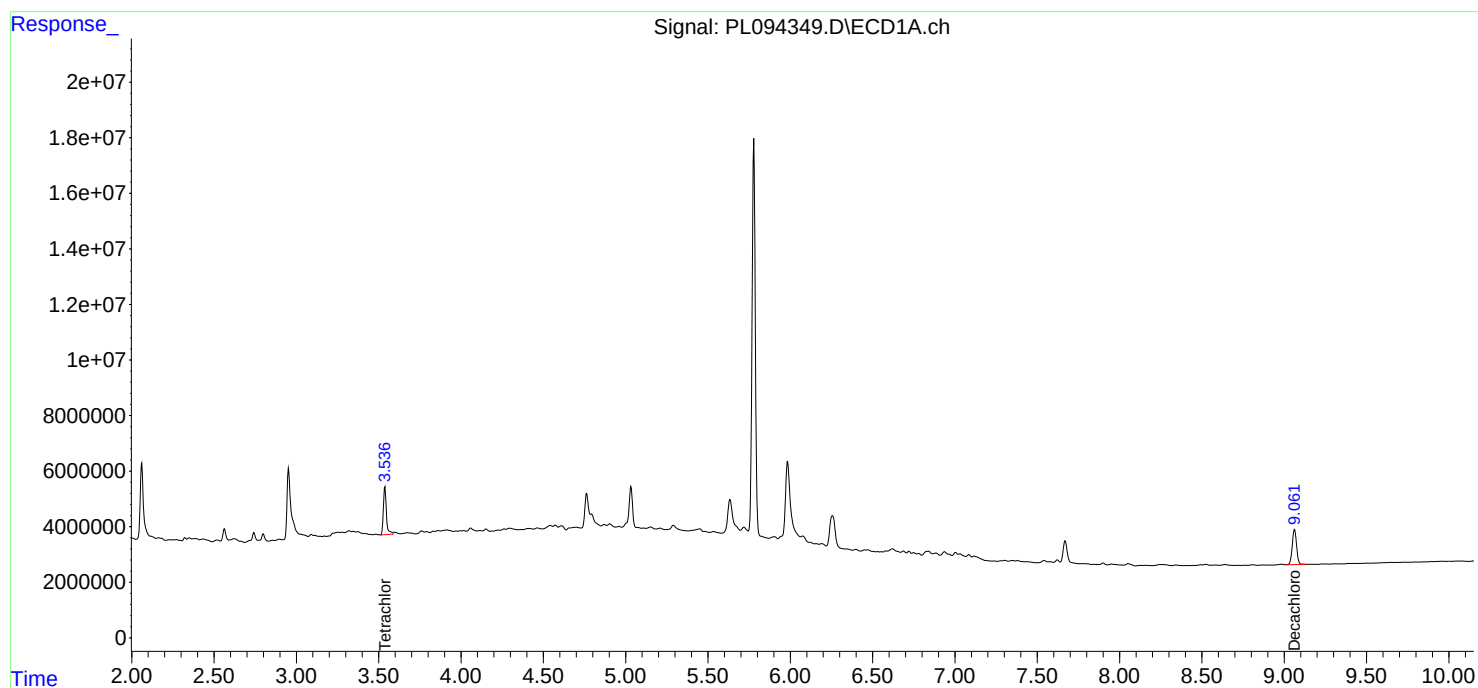

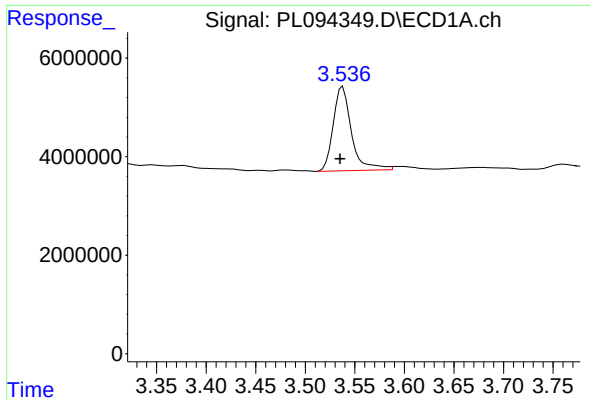

#1 Tetrachloro-m-xylene

R.T.: 3.536 min
Delta R.T.: 0.001 min
Response: 22088035
Conc: 8.70 ng/ml


Instrument :
ECD_L
ClientSampleId :
BEL-25-0005

Manual Integrations
APPROVED

Reviewed By :Abdul
Mirza


02/22/2025
Supervised By :Ankita
Jodhani

02/24/2025

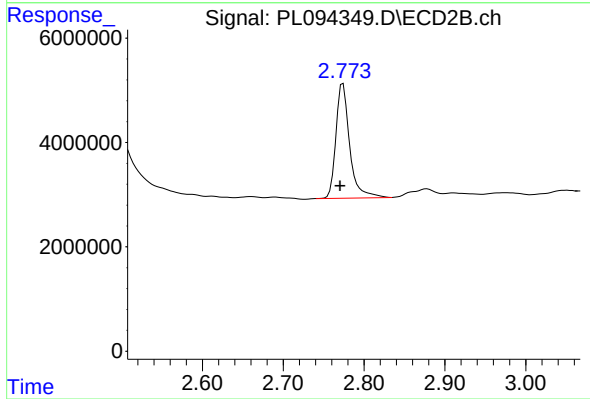


#1 Tetrachloro-m-xylene

R.T.: 2.774 min
Delta R.T.: 0.004 min
Response: 25951823
Conc: 8.13 ng/ml

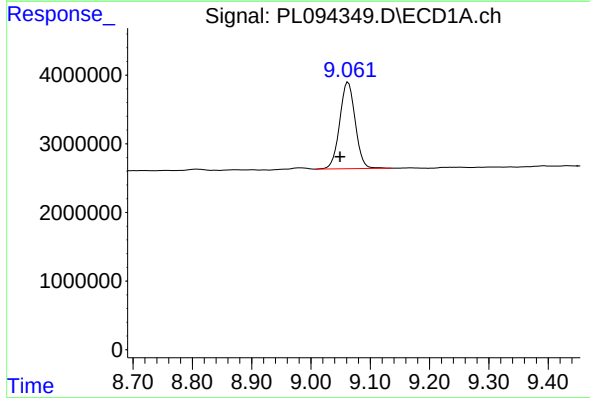

#28 Decachlorobiphenyl

R.T.: 9.061 min
Delta R.T.: 0.012 min
Response: 23026119
Conc: 10.82 ng/ml m

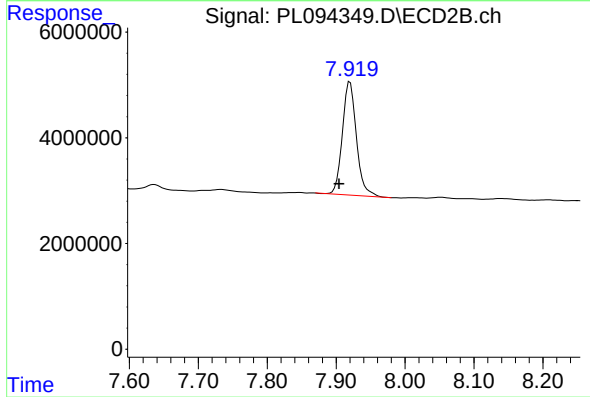

#28 Decachlorobiphenyl

R.T.: 7.920 min
Delta R.T.: 0.016 min
Response: 30307477
Conc: 7.88 ng/ml