

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022125\
 Data File : PL094359.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Feb 2025 18:55
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 I.BLK

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 02/24/2025
 Supervised By : Ankita Jodhani 02/24/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 22 00:27:23 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022125.M
 Quant Title : GC Extractables
 QLast Update : Fri Feb 21 14:52:19 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.535	2.768	65438971	80297129	25.773	25.162m
2)	SA Decachlor...	9.046	7.902	50790380	75990005	23.876	19.760

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022125\
Data File : PL094359.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Feb 2025 18:55
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
I.BLK


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 02/24/2025
Supervised By : Ankita Jodhani 02/24/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 22 00:27:23 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022125.M
Quant Title : GC Extractables
QLast Update : Fri Feb 21 14:52:19 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

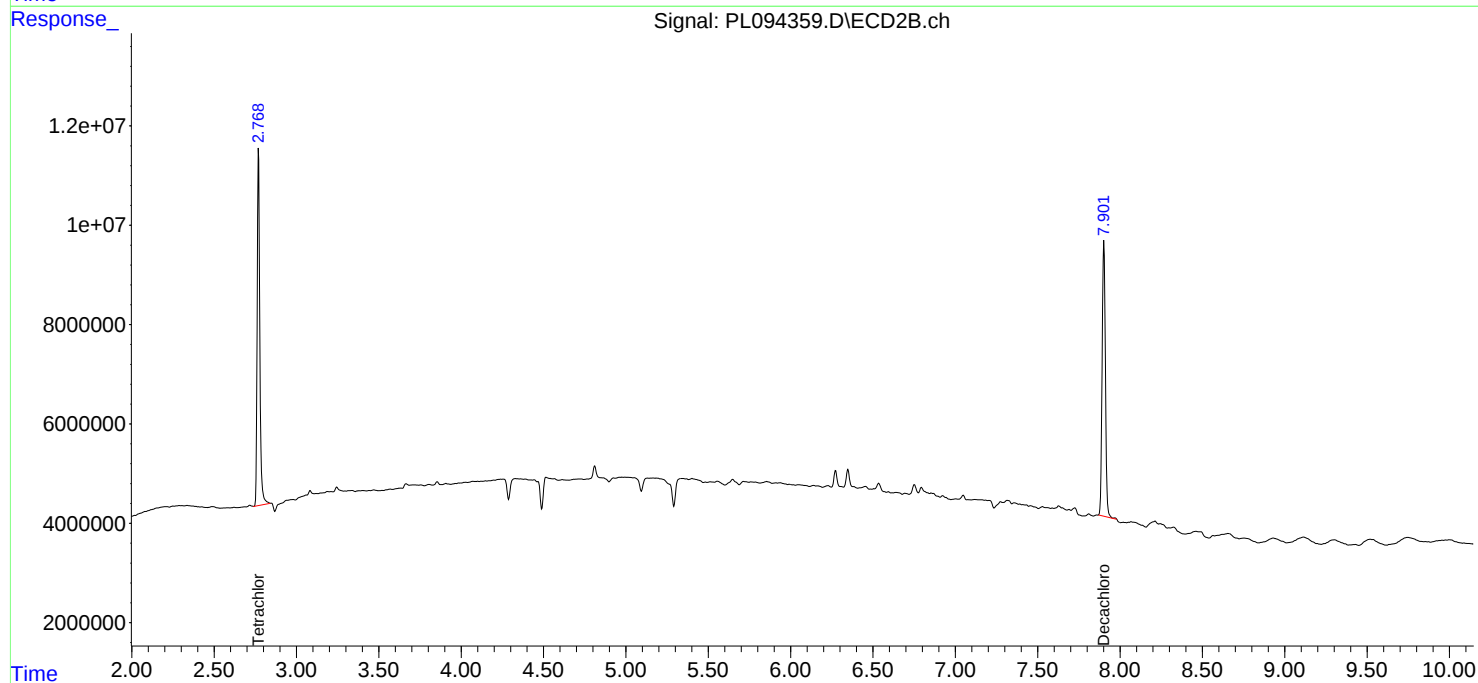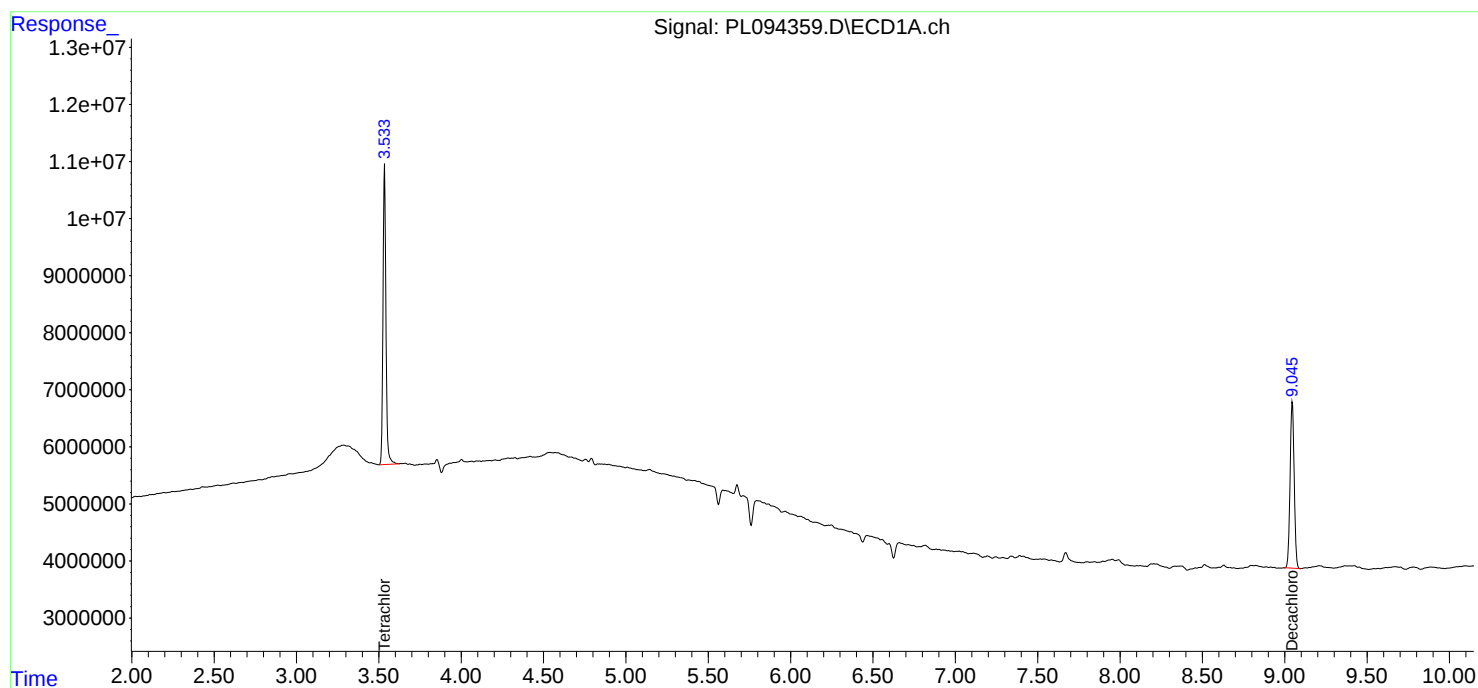

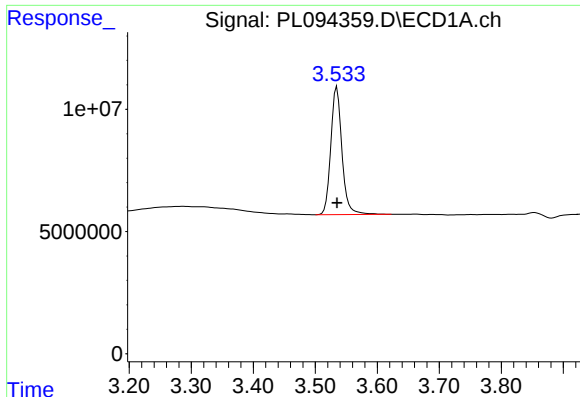


#1 Tetrachloro-m-xylene

R.T.: 3.535 min
Delta R.T.: 0.000 min
Response: 65438971
Conc: 25.77 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 02/24/2025
Supervised By :Ankita Jodhani 02/24/2025

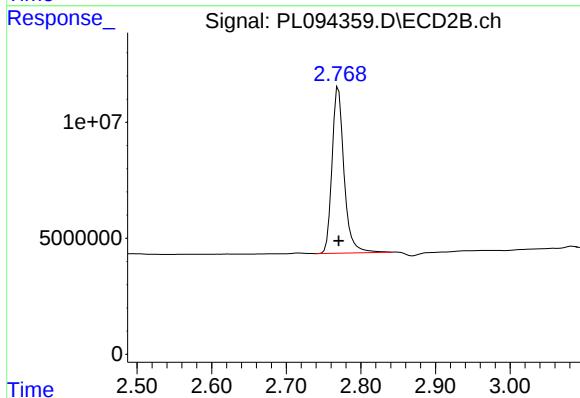


#1 Tetrachloro-m-xylene

R.T.: 2.768 min
Delta R.T.: -0.002 min
Response: 80297129
Conc: 25.16 ng/ml m

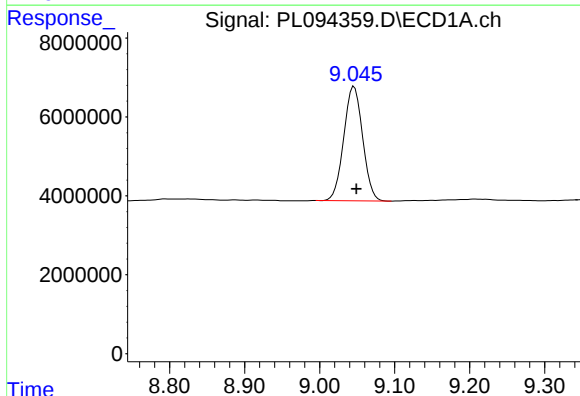

#28 Decachlorobiphenyl

R.T.: 9.046 min
Delta R.T.: -0.003 min
Response: 50790380
Conc: 23.88 ng/ml

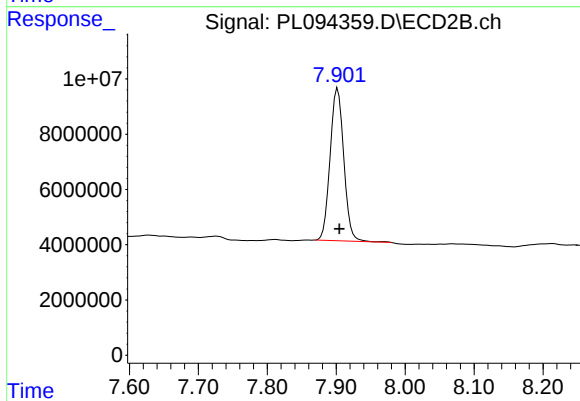

#28 Decachlorobiphenyl

R.T.: 7.902 min
Delta R.T.: -0.002 min
Response: 75990005
Conc: 19.76 ng/ml