

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022125\
 Data File : PL094361.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Feb 2025 19:36
 Operator : AR\AJ
 Sample : Q1393-05
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PURGE-WATER-COMP

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 02/22/2025
 Supervised By :Ankita Jodhani 02/24/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 22 00:28:39 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022125.M
 Quant Title : GC Extractables
 QLast Update : Fri Feb 21 14:52:19 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.534	2.769	27477866	75350284	10.822m	23.612m#
2)	SA Decachlor...	9.046	7.902	46337684	70637930	21.783	18.368

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022125\
Data File : PL094361.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Feb 2025 19:36
Operator : AR\AJ
Sample : Q1393-05
Misc :
ALS Vial : 38 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
PURGE-WATER-COMP


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 02/22/2025
Supervised By : Ankita Jodhani 02/24/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 22 00:28:39 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022125.M
Quant Title : GC Extractables
QLast Update : Fri Feb 21 14:52:19 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

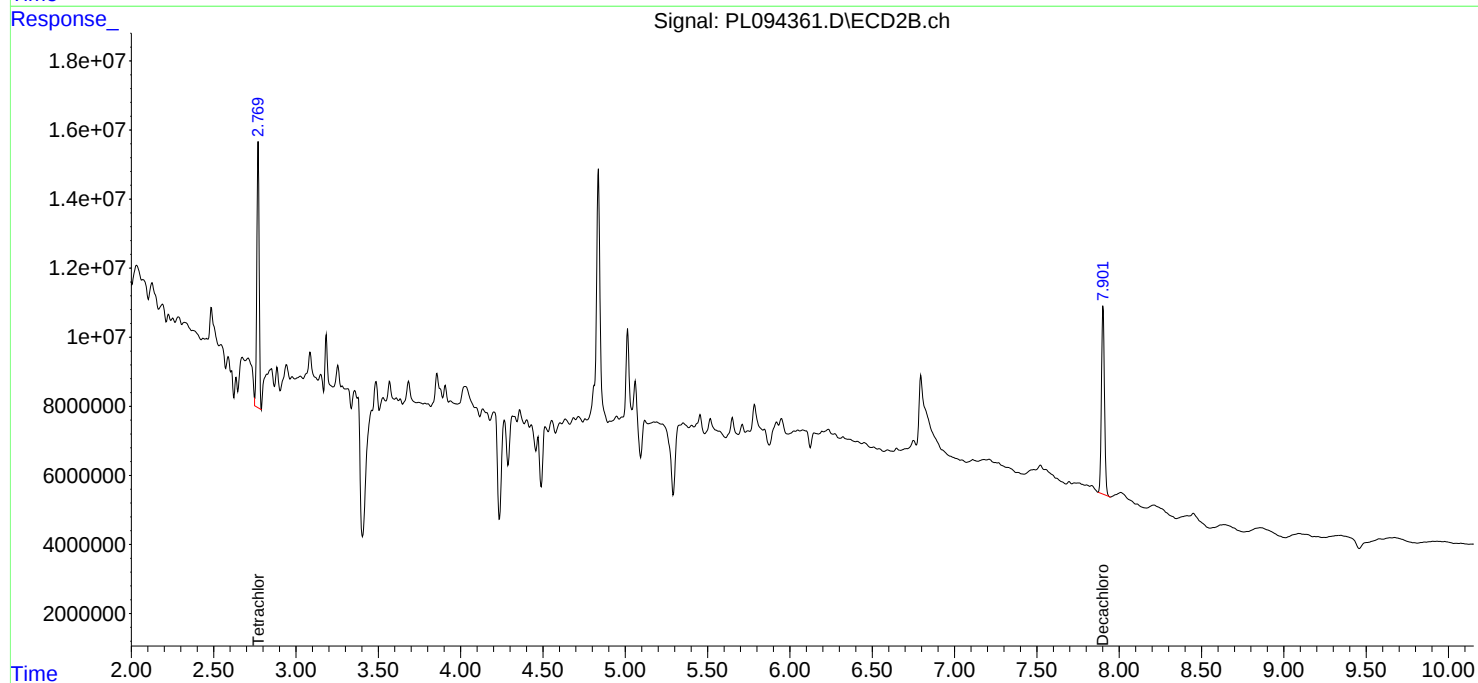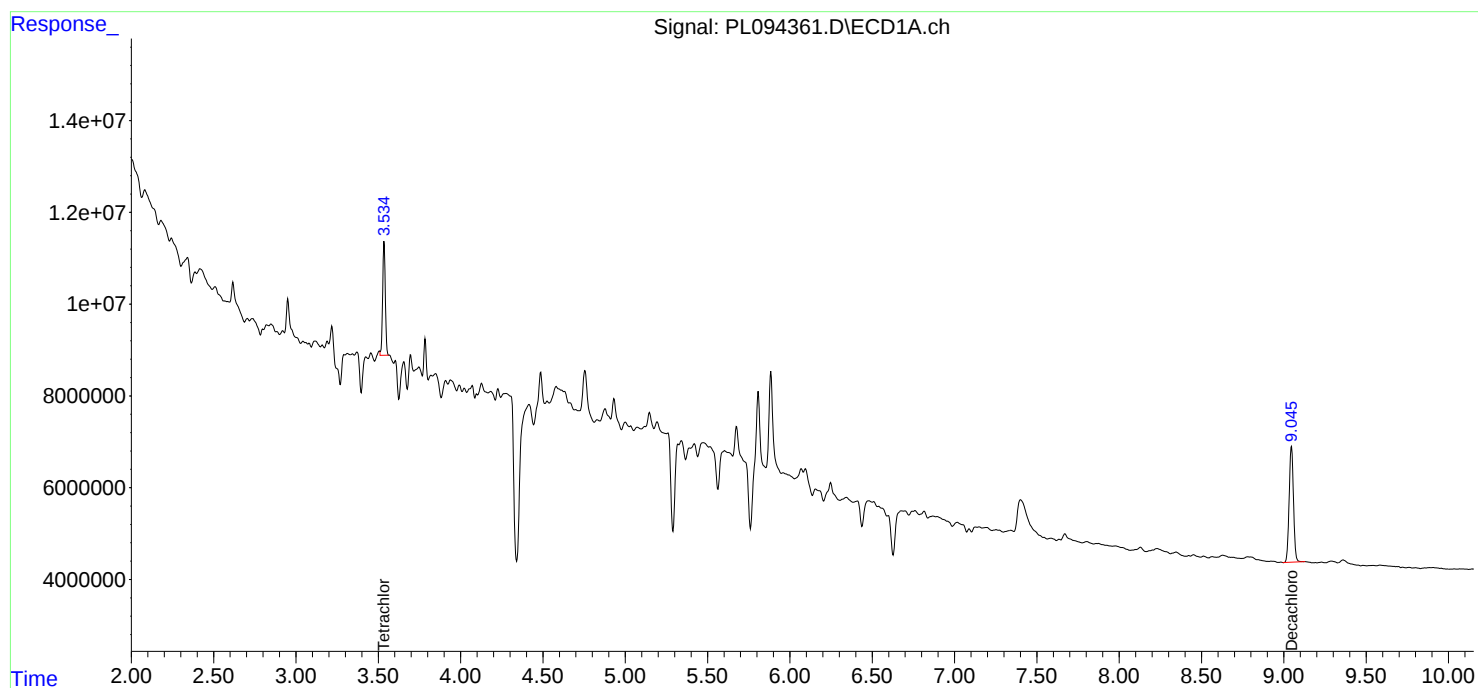

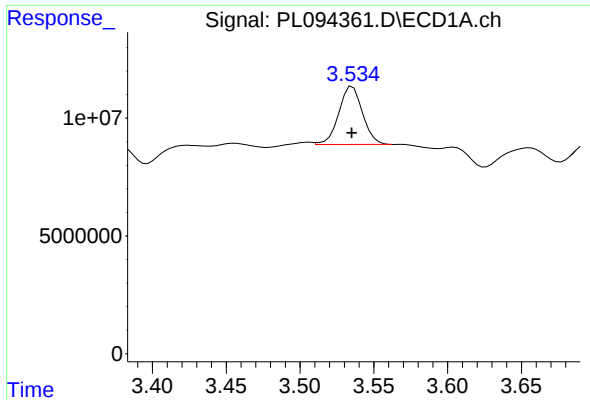


#1 Tetrachloro-m-xylene

R.T.: 3.534 min
Delta R.T.: 0.000 min
Response: 27477866
Conc: 10.82 ng/ml

Instrument :
ECD_L
ClientSampleId :
PURGE-WATER-COMP


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 02/22/2025
Supervised By :Ankita Jodhani 02/24/2025

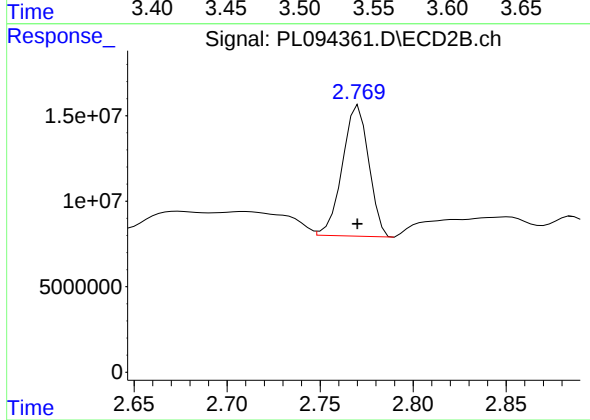


#1 Tetrachloro-m-xylene

R.T.: 2.769 min
Delta R.T.: 0.000 min
Response: 75350284
Conc: 23.61 ng/ml m

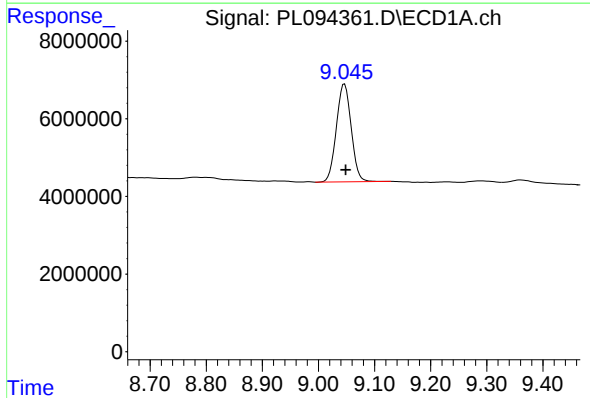

#28 Decachlorobiphenyl

R.T.: 9.046 min
Delta R.T.: -0.002 min
Response: 46337684
Conc: 21.78 ng/ml

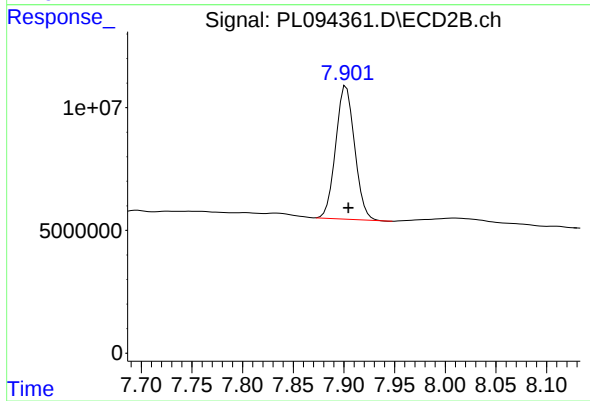

#28 Decachlorobiphenyl

R.T.: 7.902 min
Delta R.T.: -0.002 min
Response: 70637930
Conc: 18.37 ng/ml